

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY030520\
 Data File : VY001878.D
 Acq On : 05 Mar 2020 13:51
 Operator : SY/MD
 Sample : L1778-18
 Misc : 8.84G/5ML/MSVOA Y/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 S6

Quant Time: Mar 06 05:27:53 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y030420S.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 05 04:05:33 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.81	168	140052	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.71	114	271220	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.50	117	238074	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.43	152	93451	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.16	65	86350	57.75	ug/l	0.00
Spiked Amount	50.000		Recovery	=	115.50%	
35) Dibromofluoromethane	7.74	113	78438	52.96	ug/l	0.00
Spiked Amount	50.000		Recovery	=	105.92%	
50) Toluene-d8	10.19	98	327391	52.42	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.84%	
62) 4-Bromofluorobenzene	12.49	95	101676	46.82	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.64%	


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY030520\
Data File : VY001878.D
Acq On : 05 Mar 2020 13:51
Operator : SY/MD
Sample : L1778-18
Misc : 8.84G/5ML/MSVOA Y/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
S6

Quant Time: Mar 06 05:27:53 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y030420S.M
Quant Title : SW846 8260
QLast Update : Thu Mar 05 04:05:33 2020
Response via : Initial Calibration

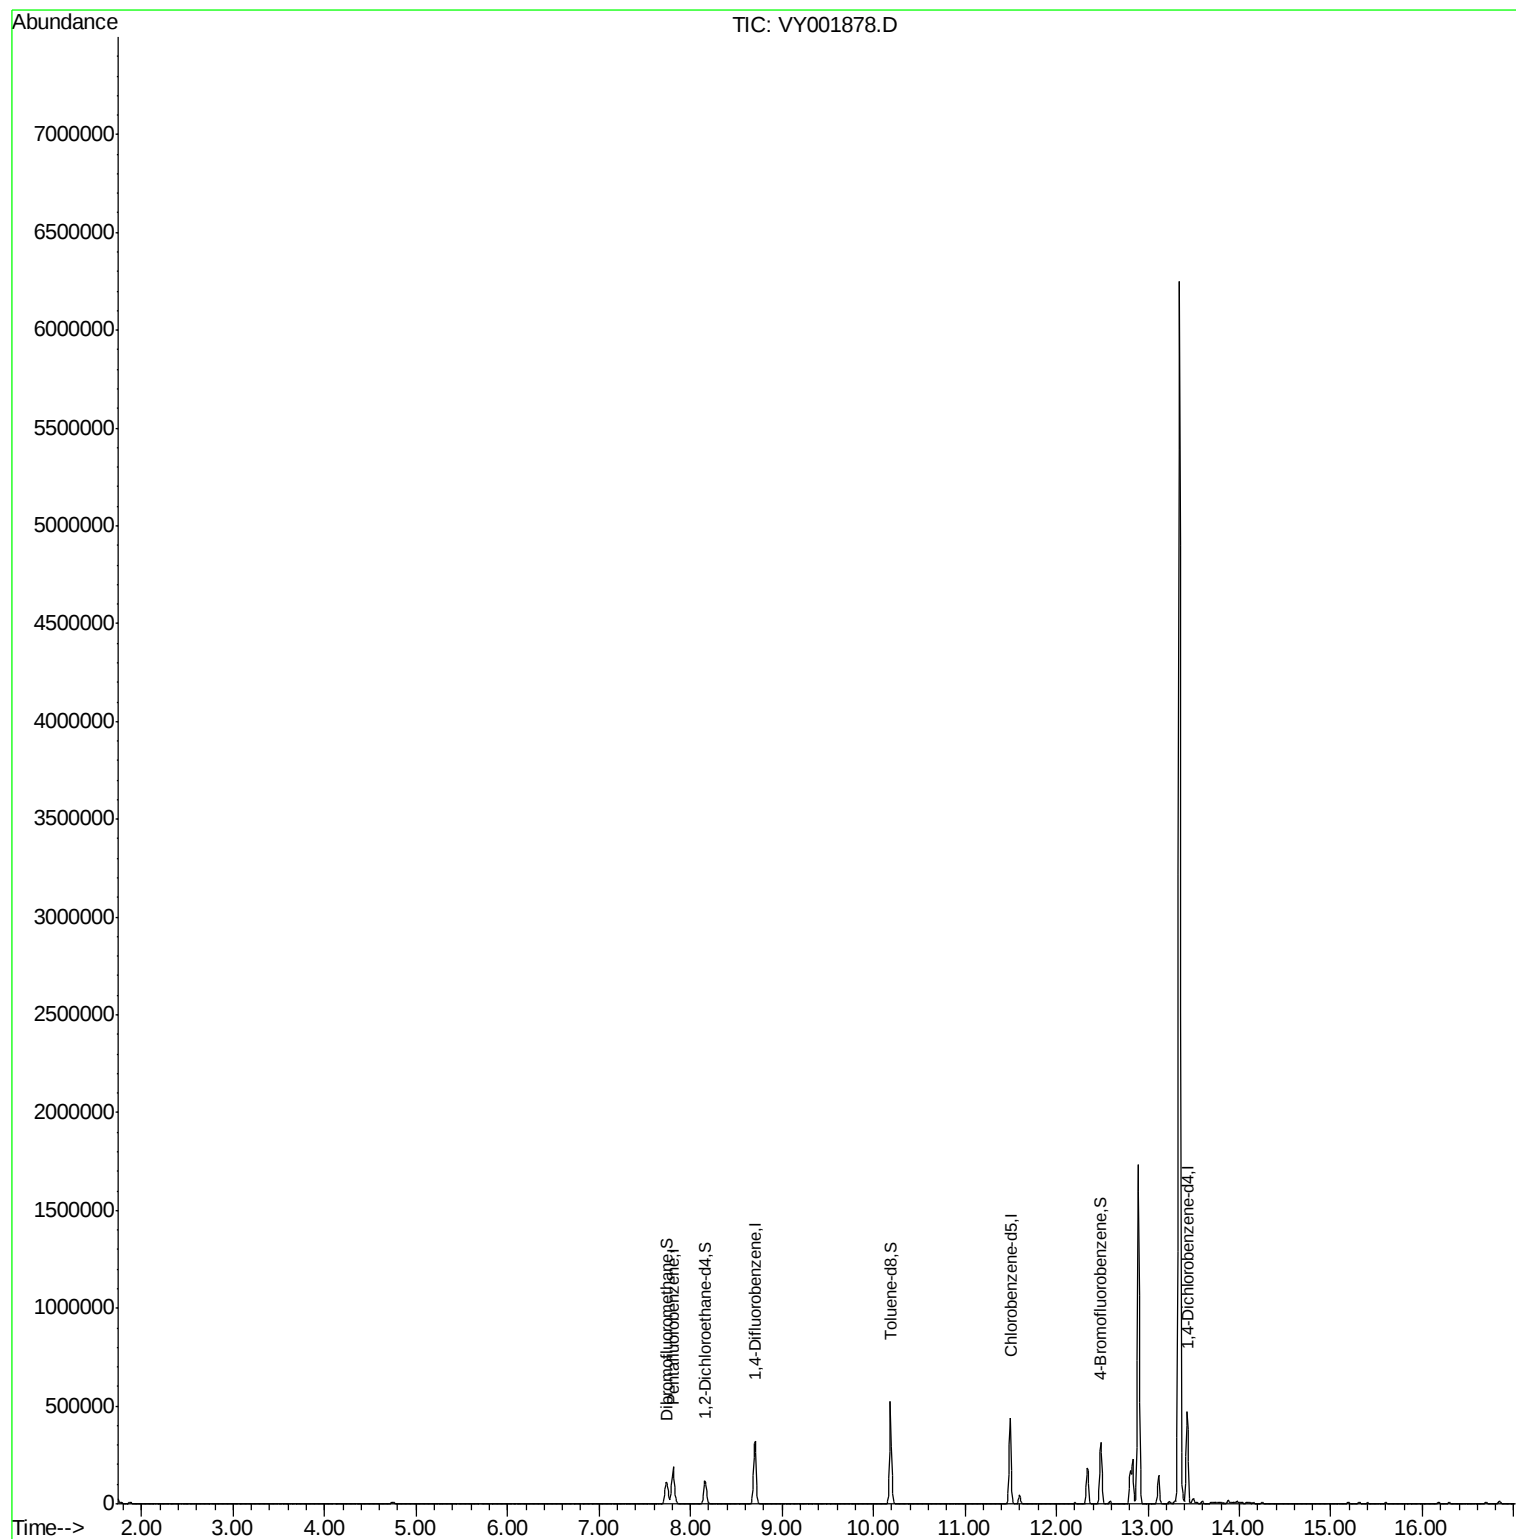



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.81 min Scan# 996

Delta R.T. -0.01 min

Lab File: VY001878.D

Acq: 05 Mar 2020 13:51

Instrument :

MSVOA_Y

ClientSampled :


S6

Tot Ion:168 Resp: 140052

Ion Ratio Lower Upper




168 100

99 58.6 46.7 70.1

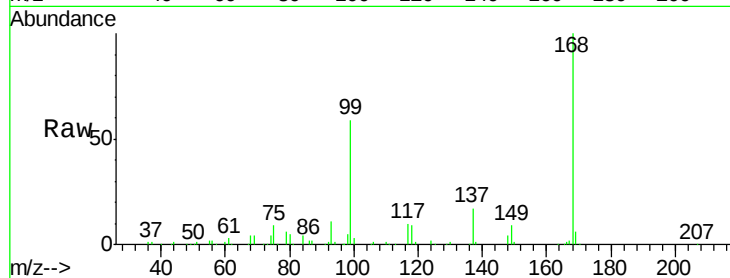

Abundance Ion 167.90 (167.60 to 168.60): VY001845.D (-986) (-)

Ion 98.90 (98.60 to 99.60): VY001845.D (-986) (-)

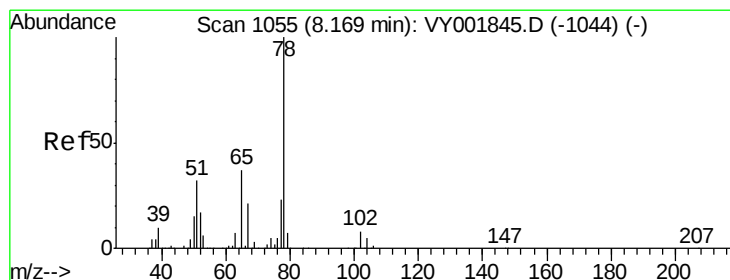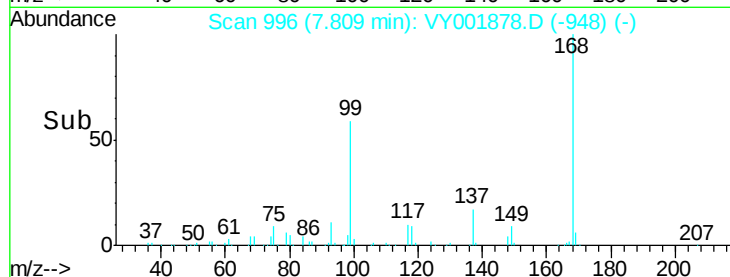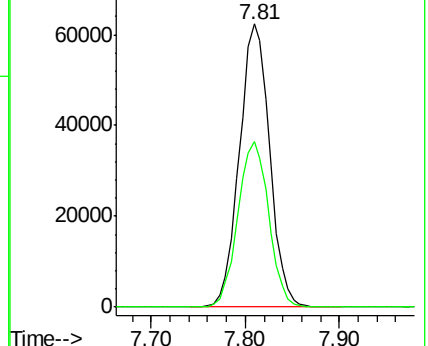

#33

1,2-Dichloroethane-d4

Concen: 57.753 ug/l

RT: 8.16 min Scan# 1054

Delta R.T. -0.01 min

Lab File: VY001878.D


Acq: 05 Mar 2020 13:51

Tgt Ion: 65 Resp: 86350

Ion Ratio Lower Upper



65 100

67 55.2 0.0 110.8

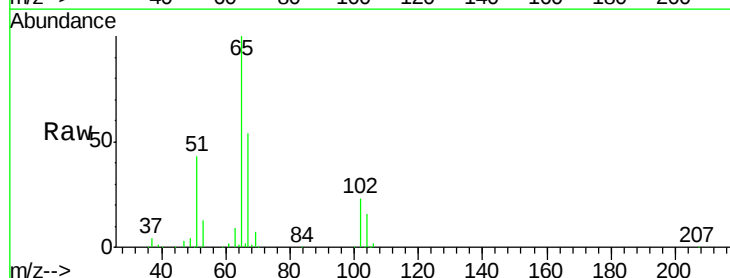

Abundance Ion 64.90 (64.60 to 65.60): VY001845.D (-1044) (-)

Ion 66.90 (66.60 to 67.60): VY001845.D (-1044) (-)

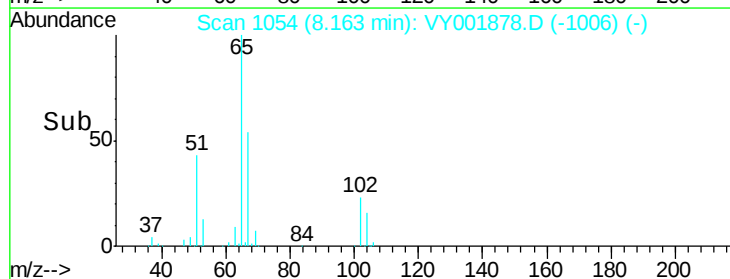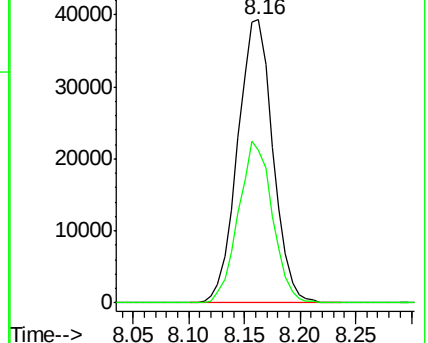



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.71 min Scan# 1143

Delta R.T. -0.01 min

Lab File: VY001878.D

Acq: 05 Mar 2020 13:51

Instrument :

MSVOA_Y

ClientSampleId :

S6


Tot Ion:114 Resp: 271220

Ion Ratio Lower Upper

114 100

63 20.8 0.0 39.4




88 15.7 0.0 30.4

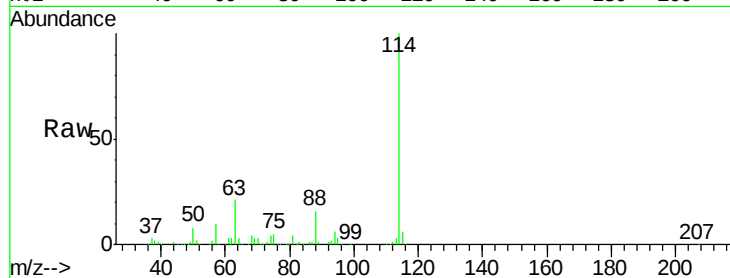

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VY0

Ion 87.90 (87.60 to 88.60): VY0

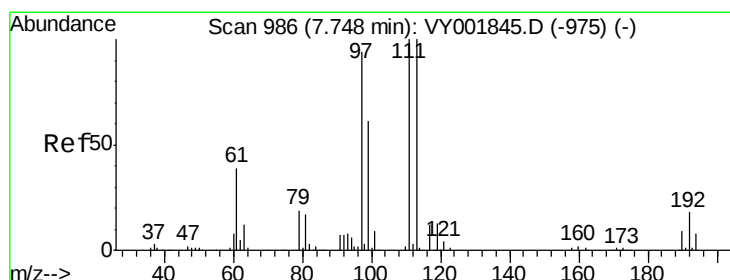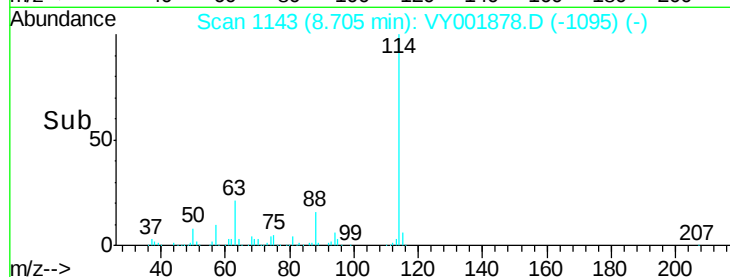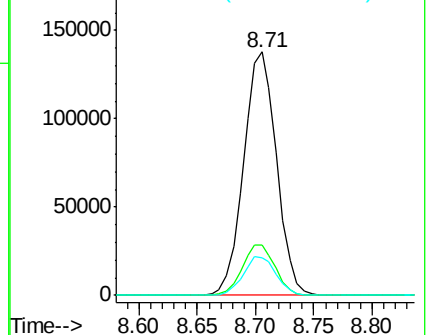

#35

Dibromofluoromethane

Concen: 52.963 ug/l

RT: 7.74 min Scan# 985

Delta R.T. -0.01 min

Lab File: VY001878.D

Acq: 05 Mar 2020 13:51


Tgt Ion:113 Resp: 78438

Ion Ratio Lower Upper

113 100

111 104.2 81.8 122.8



192 18.0 14.2 21.2

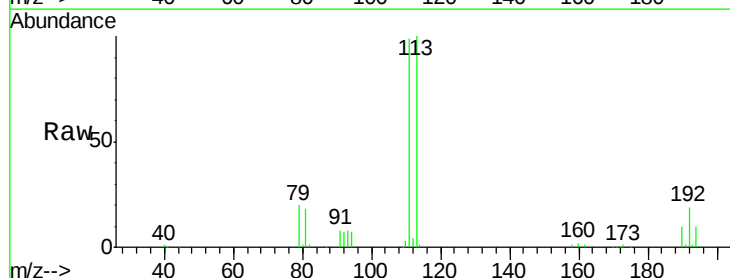


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

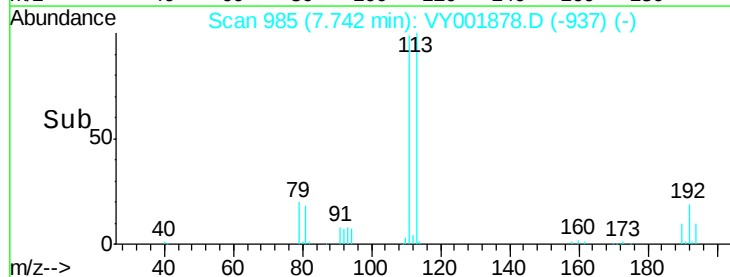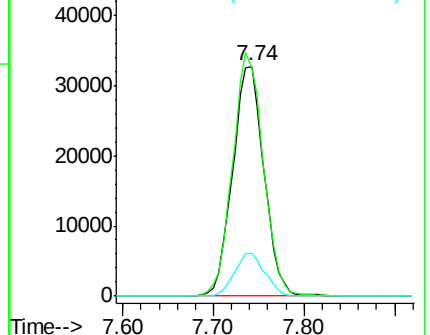

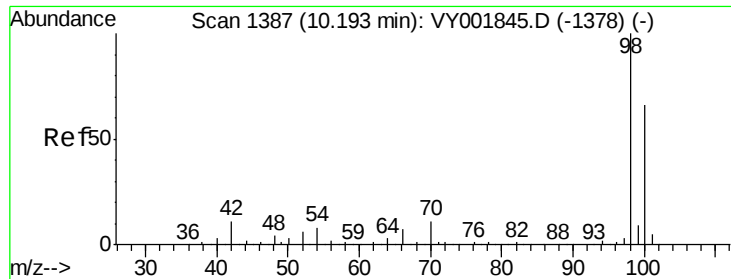

#50

Toluene-d8

Concen: 52.424 ug/l

RT: 10.19 min Scan# 1386

Delta R.T. -0.01 min

Lab File: VY001878.D

Acq: 05 Mar 2020 13:51

Instrument :

MSVOA_Y

ClientSampled :


S6

Tot Ion: 98 Resp: 327391

Ion Ratio Lower Upper

98 100

100 65.7 53.0 79.4

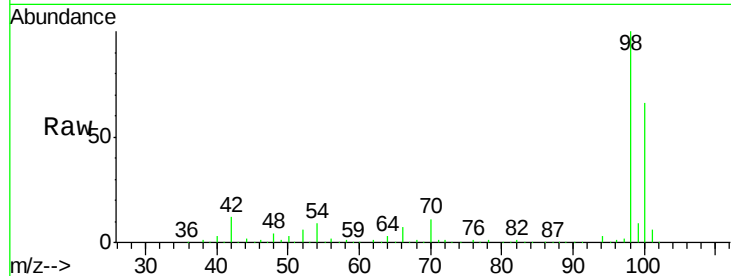

Abundance Ion 98.00 (97.70 to 98.70): VY001845.D (-1378) (-)

Ion 100.00 (99.70 to 100.70): VY001845.D (-1378) (-)

10.19

200000



150000

100000

50000

0

Time-->

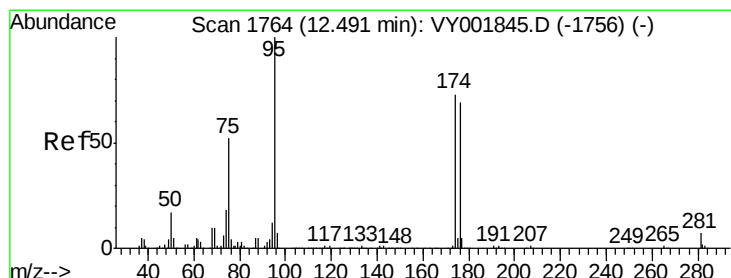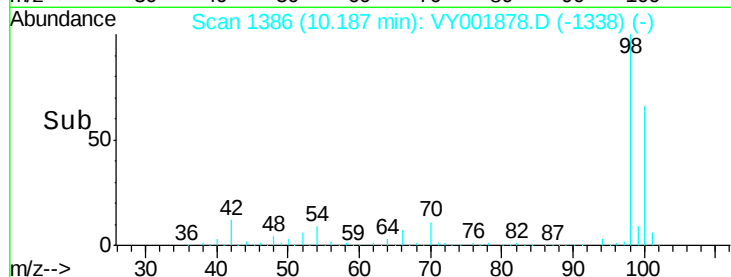

#62

4-Bromofluorobenzene

Concen: 46.823 ug/l

RT: 12.49 min Scan# 1763

Delta R.T. -0.01 min

Lab File: VY001878.D

Acq: 05 Mar 2020 13:51


Tgt Ion: 95 Resp: 101676

Ion Ratio Lower Upper

95 100

174 71.2 0.0 145.0

176 69.6 0.0 137.4

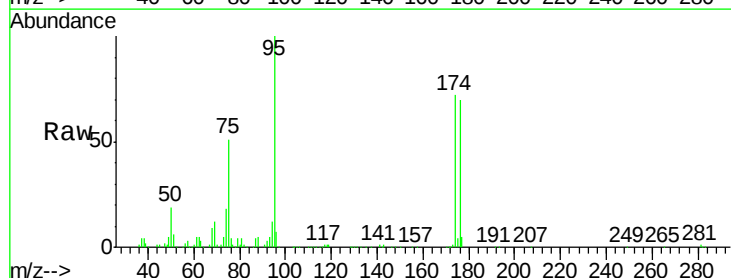

Abundance Ion 94.90 (94.60 to 95.60): VY001845.D (-1756) (-)

Ion 173.80 (173.50 to 174.50): VY001845.D (-1756) (-)

Ion 175.80 (175.50 to 176.50): VY001845.D (-1756) (-)

12.49

80000


60000


40000

20000

0

Time-->




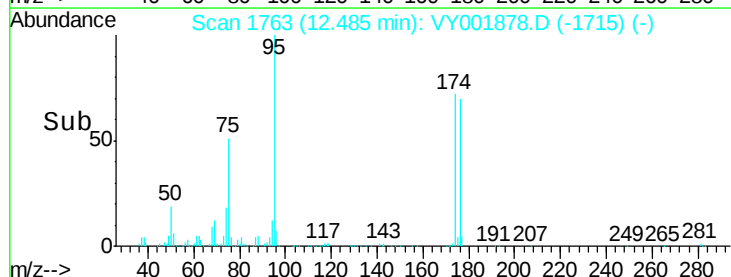


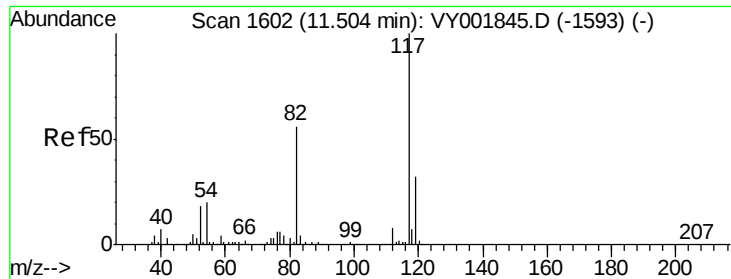

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.50 min Scan# 1601
Delta R.T. -0.01 min
Lab File: VY001878.D
Acq: 05 Mar 2020 13:51

Instrument :
MSVOA_Y
ClientSampleId :
S6

Tot Ion:117 Resp: 238074
Ion Ratio Lower Upper
117 100
82 56.0 44.5 66.7
119 30.7 25.7 38.5

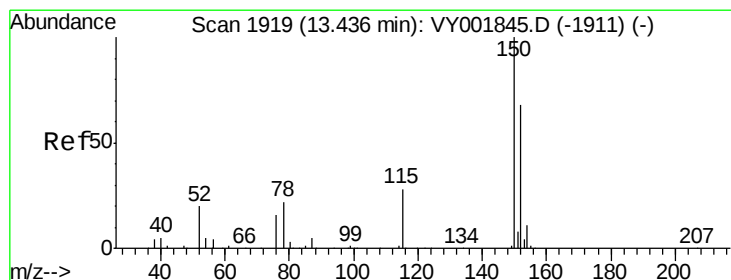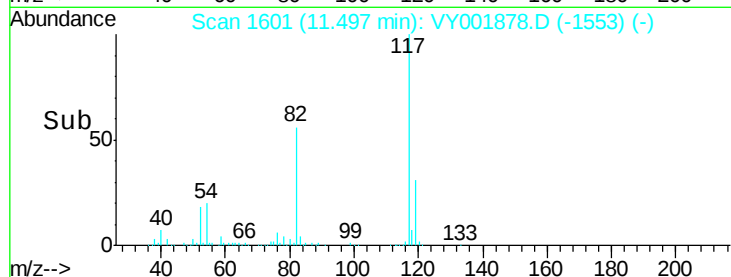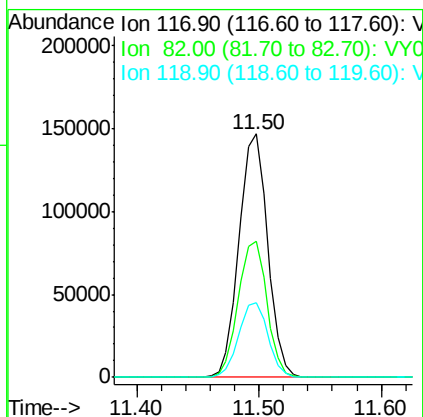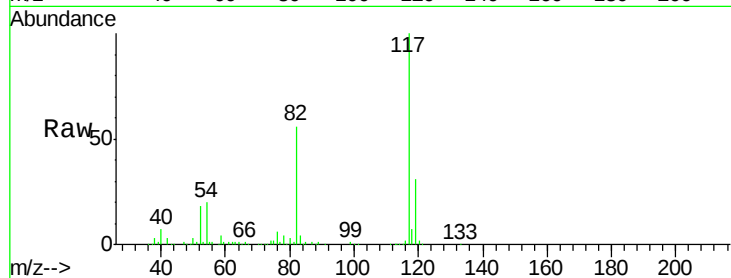

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.43 min Scan# 1918
Delta R.T. -0.01 min
Lab File: VY001878.D
Acq: 05 Mar 2020 13:51

Tgt Ion:152 Resp: 93451
Ion Ratio Lower Upper
152 100
115 61.8 29.9 89.7
150 157.0 0.0 340.6

