

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY030520\
 Data File : VY001883.D
 Acq On : 05 Mar 2020 15:43
 Operator : SY/MD
 Sample : L1783-01RE
 Misc : 9.45G/5ML/MSVOA Y/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 GP-10-030220RE

Quant Time: Mar 06 05:35:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y030420S.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 05 04:05:33 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.82	168	112064	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.71	114	209135	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.50	117	108851	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.44	152	22088	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.16	65	72184	60.34	ug/l	0.00
Spiked Amount	50.000		Recovery	=	120.68%	
35) Dibromofluoromethane	7.74	113	71426	62.55	ug/l	0.00
Spiked Amount	50.000		Recovery	=	125.10%	
50) Toluene-d8	10.19	98	220250	45.74	ug/l	0.00
Spiked Amount	50.000		Recovery	=	91.48%	
62) 4-Bromofluorobenzene	12.49	95	31195	18.63	ug/l	0.00
Spiked Amount	50.000		Recovery	=	37.26%	


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY030520\
Data File : VY001883.D
Acq On : 05 Mar 2020 15:43
Operator : SY/MD
Sample : L1783-01RE
Misc : 9.45G/5ML/MSVOA Y/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
GP-10-030220RE

Quant Time: Mar 06 05:35:49 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y030420S.M
Quant Title : SW846 8260
QLast Update : Thu Mar 05 04:05:33 2020
Response via : Initial Calibration

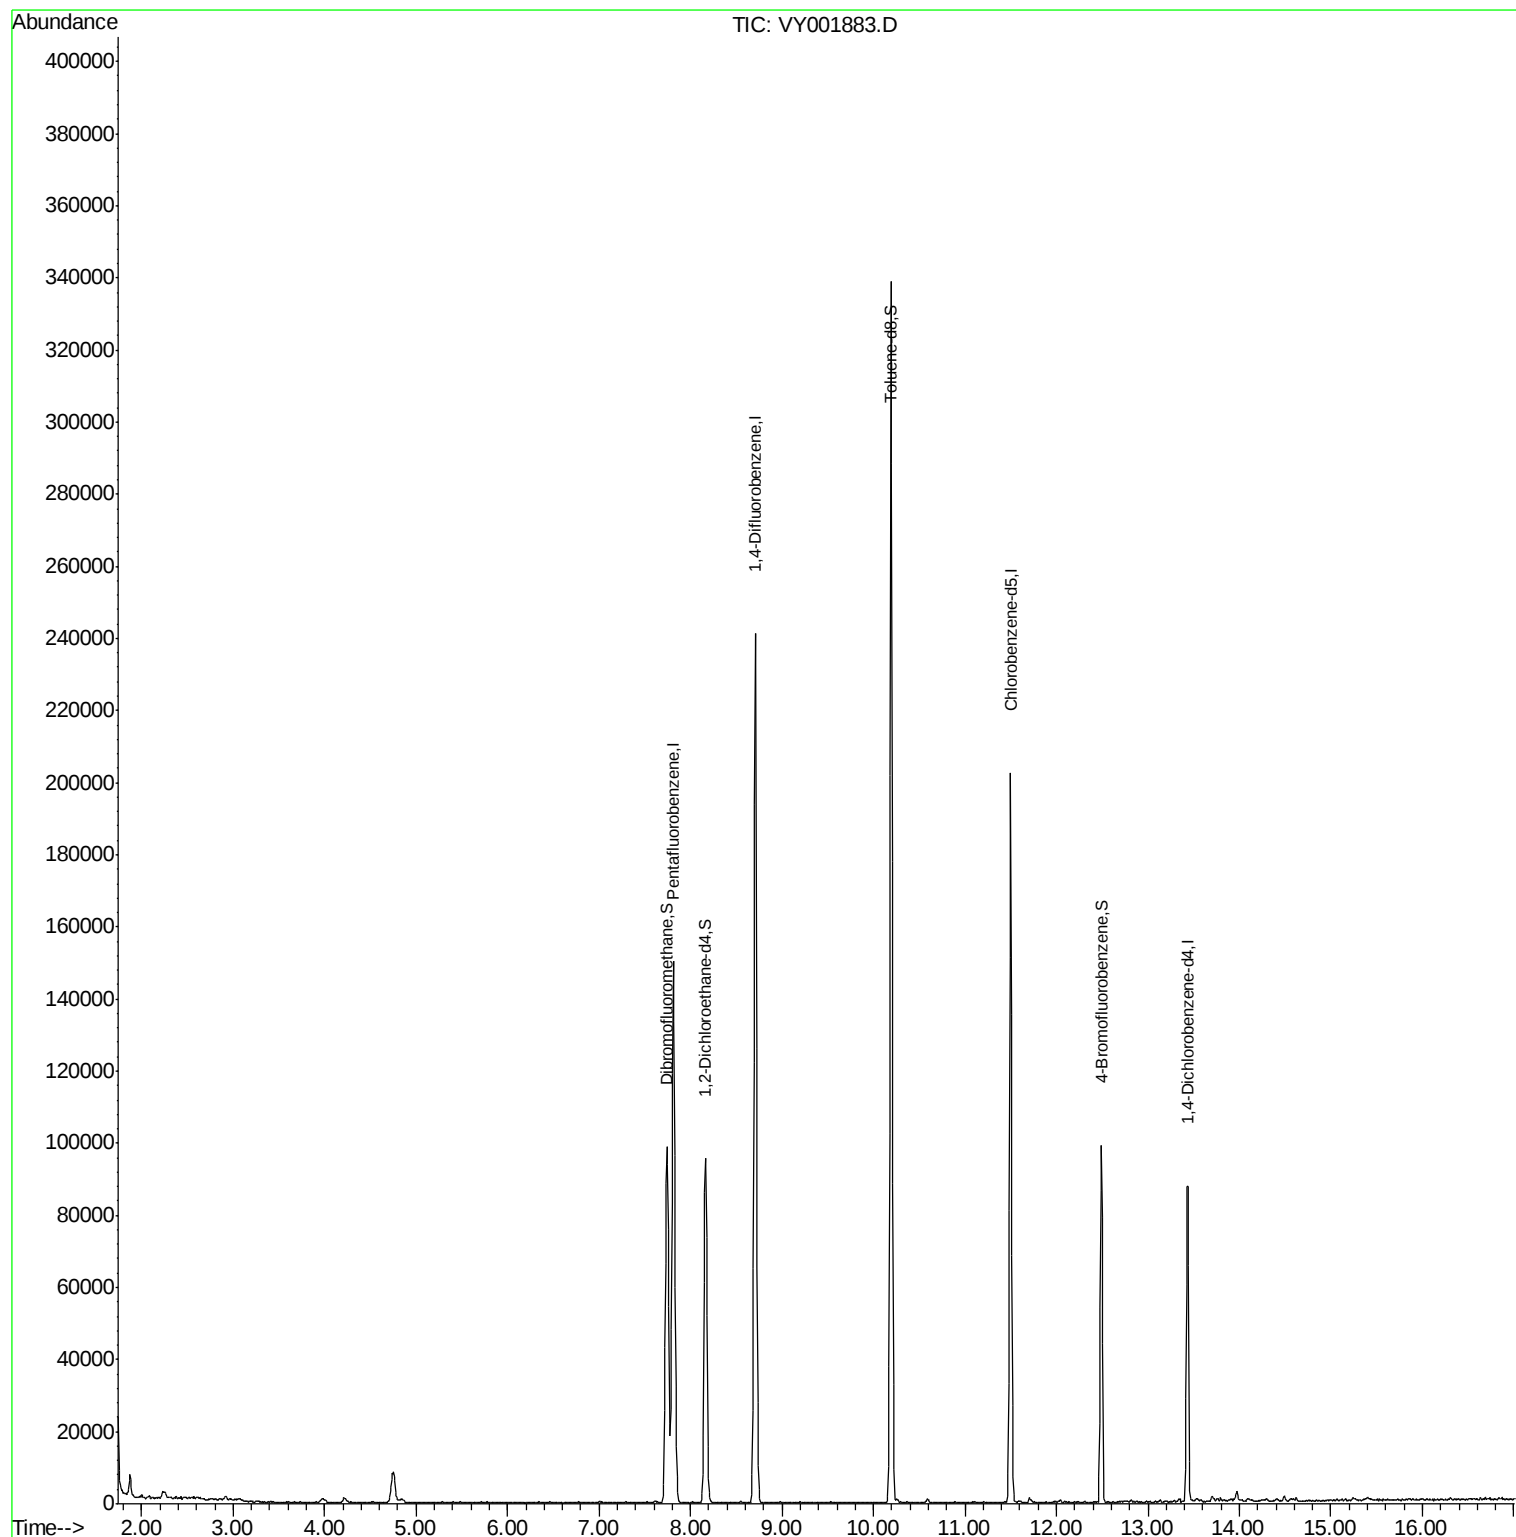



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.82 min Scan# 997

Delta R.T. 0.00 min

Lab File: VY001883.D

Acq: 05 Mar 2020 15:43

Instrument :

MSVOA_Y

ClientSampleId :


GP-10-030220RE

Tot Ion:168 Resp: 112064




Ion Ratio Lower Upper

168 100

99 57.4 46.7 70.1

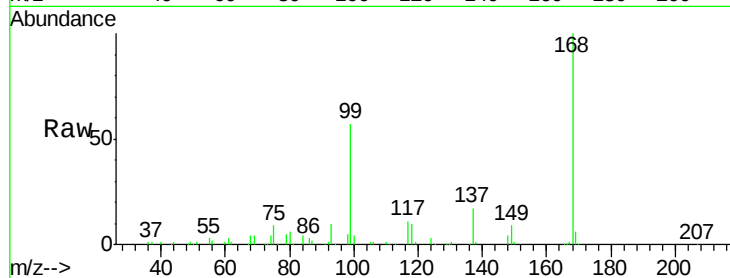

Abundance Ion 167.90 (167.60 to 168.60): VY001845.D (-986) (-)

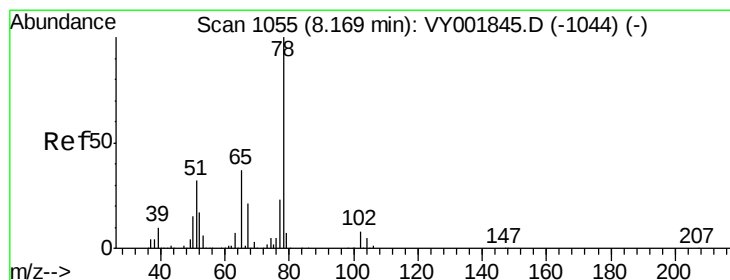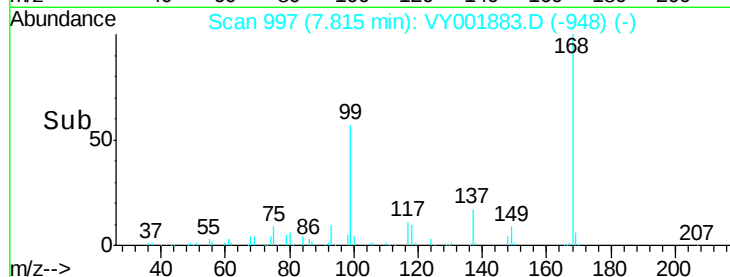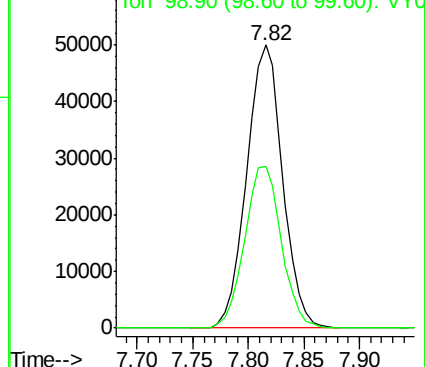

#33

1,2-Dichloroethane-d4

Concen: 60.336 ug/l

RT: 8.16 min Scan# 1054

Delta R.T. -0.01 min

Lab File: VY001883.D


Acq: 05 Mar 2020 15:43

Tgt Ion: 65 Resp: 72184



Ion Ratio Lower Upper

65 100

67 54.8 0.0 110.8

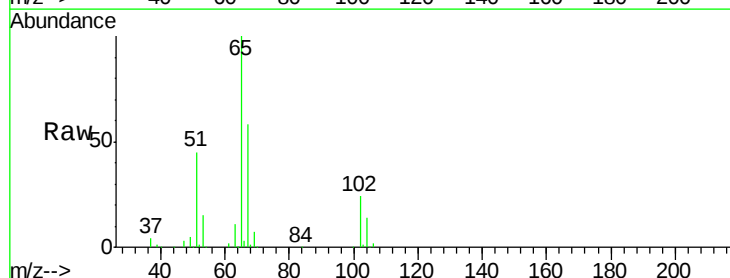

Abundance Ion 64.90 (64.60 to 65.60): VY001845.D (-1044) (-)

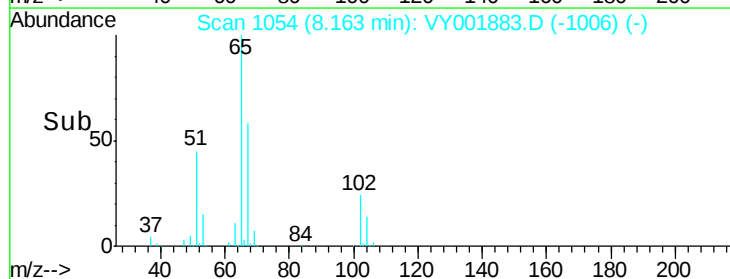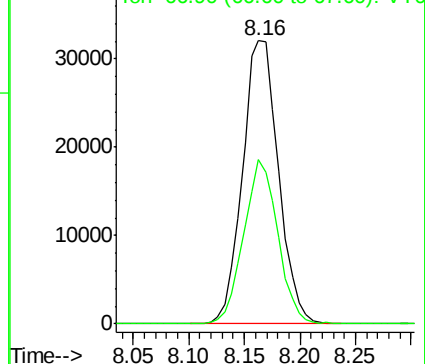



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.71 min Scan# 1144

Delta R.T. 0.00 min

Lab File: VY001883.D

Acq: 05 Mar 2020 15:43

Instrument :

MSVOA_Y

ClientSampleId :

GP-10-030220RE


Tot Ion:114 Resp: 209135

Ion Ratio Lower Upper

114 100

63 20.0 0.0 39.4




88 16.0 0.0 30.4

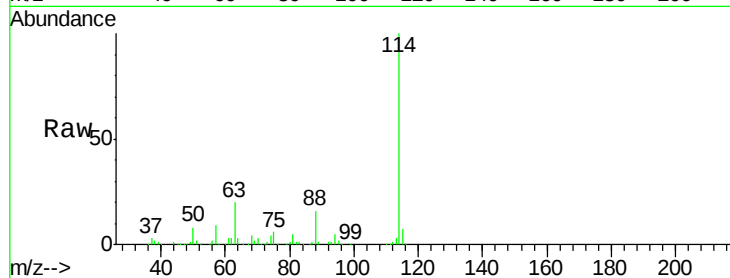

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VY0

Ion 87.90 (87.60 to 88.60): VY0

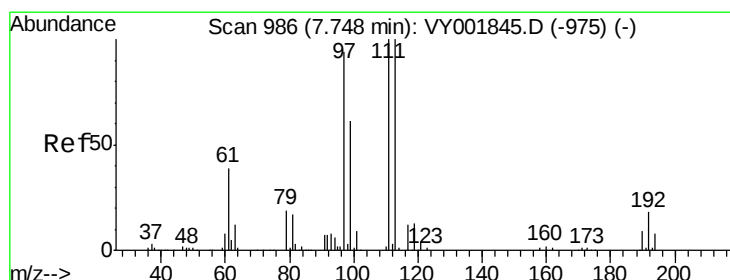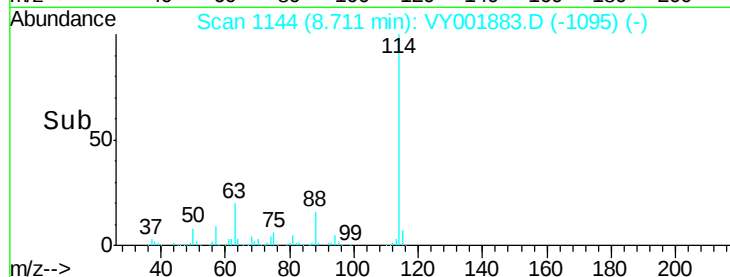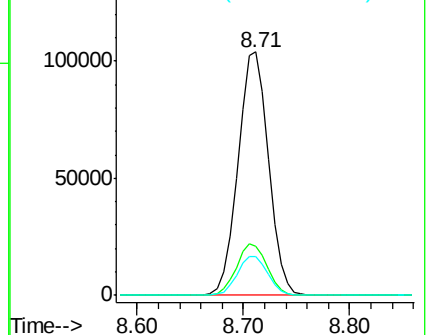

#35

Dibromofluoromethane

Concen: 62.546 ug/l

RT: 7.74 min Scan# 985

Delta R.T. -0.01 min

Lab File: VY001883.D

Acq: 05 Mar 2020 15:43


Tgt Ion:113 Resp: 71426

Ion Ratio Lower Upper

113 100

111 102.3 81.8 122.8



192 17.7 14.2 21.2

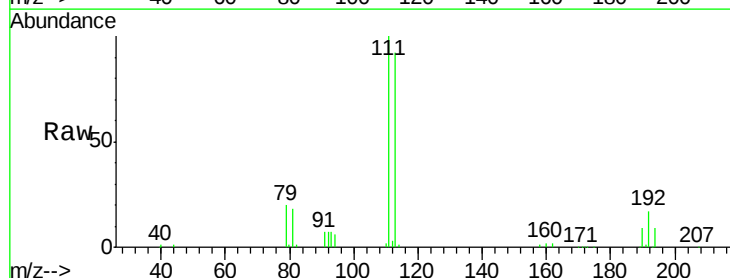


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

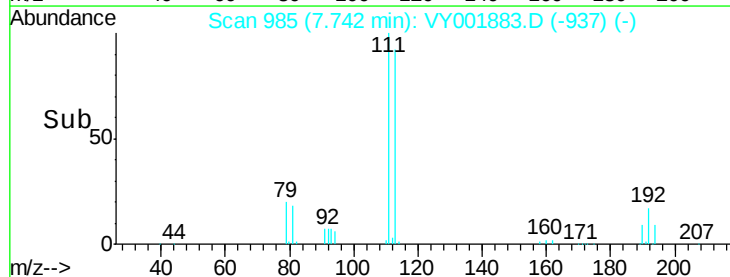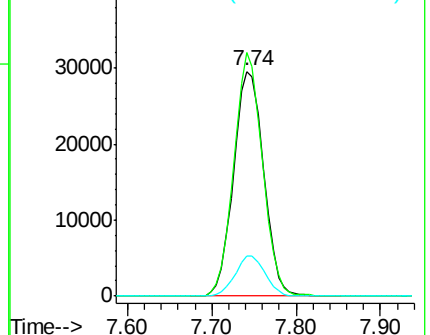

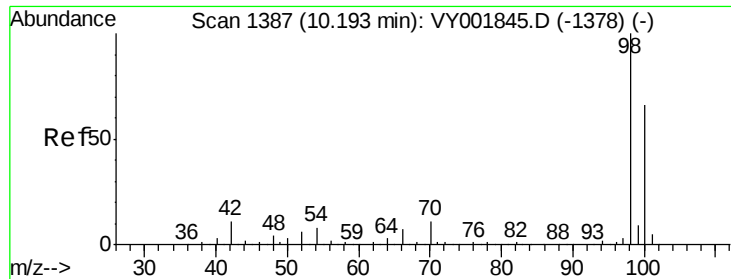

#50

Toluene-d8

Concen: 45.738 ug/l

RT: 10.19 min Scan# 1387

Delta R.T. 0.00 min

Lab File: VY001883.D

Acq: 05 Mar 2020 15:43

Instrument :

MSVOA_Y

ClientSampleId :


GP-10-030220RE

Tot Ion: 98 Resp: 220250

Ion Ratio Lower Upper

98 100

100 65.0 53.0 79.4

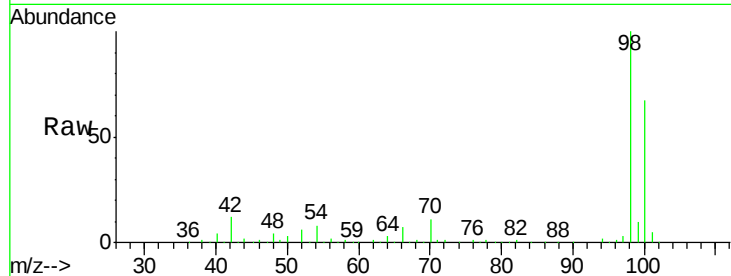

Abundance Ion 98.00 (97.70 to 98.70): VY001845.D (-1378) (-)

Ion 100.00 (99.70 to 100.70): VY001883.D (-1338) (-)

10.19



150000

100000

50000

0

Time-->

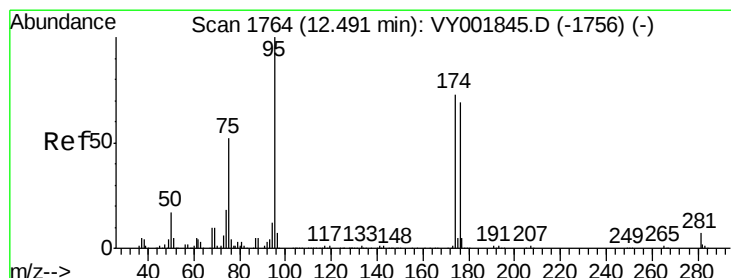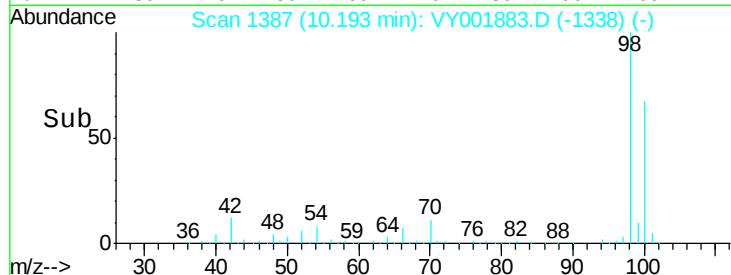

#62

4-Bromofluorobenzene

Concen: 18.630 ug/l

RT: 12.49 min Scan# 1764

Delta R.T. 0.00 min

Lab File: VY001883.D

Acq: 05 Mar 2020 15:43


Tgt Ion: 95 Resp: 31195

Ion Ratio Lower Upper

95 100

174 75.2 0.0 145.0

176 69.3 0.0 137.4

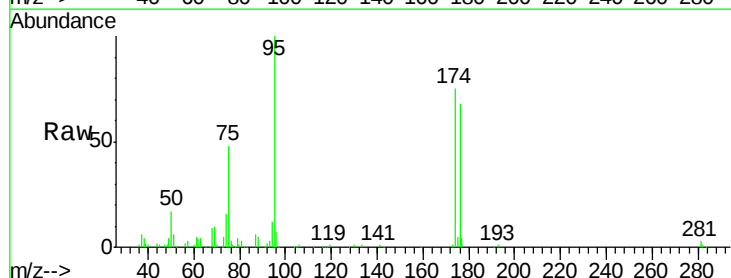

Abundance Ion 94.90 (94.60 to 95.60): VY001845.D (-1756) (-)

Ion 173.80 (173.50 to 174.50): VY001883.D (-1715) (-)

Ion 175.80 (175.50 to 176.50): VY001883.D (-1715) (-)

12.49

25000

20000


15000


10000

5000

0

Time-->




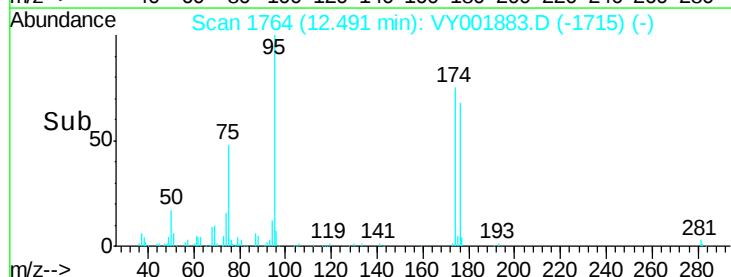


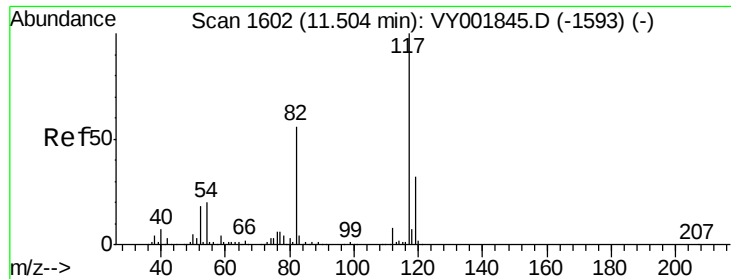

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.50 min Scan# 1601
Delta R.T. -0.01 min
Lab File: VY001883.D
Acq: 05 Mar 2020 15:43

Instrument :
MSVOA_Y
ClientSampleId :
GP-10-030220RE

Tot Ion	Ratio	Lower	Upper
117	100		
82	58.3	44.5	66.7
119	32.5	25.7	38.5

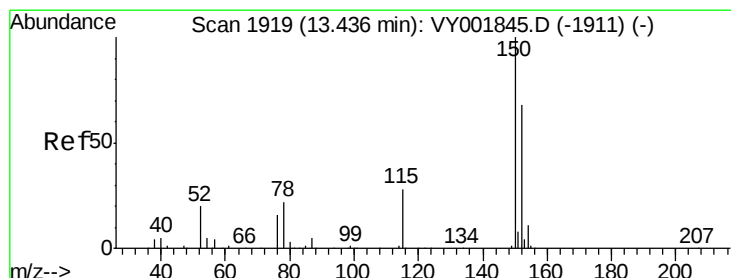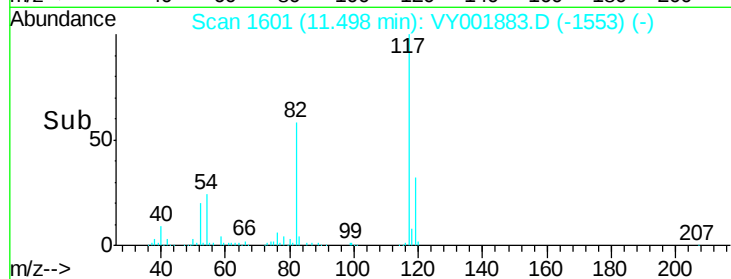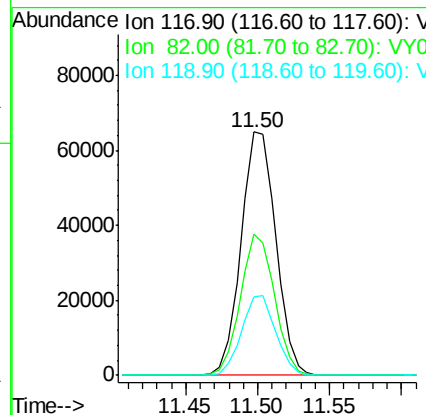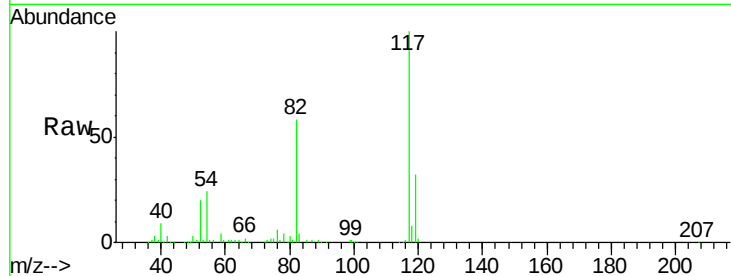

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.44 min Scan# 1919
Delta R.T. 0.00 min
Lab File: VY001883.D
Acq: 05 Mar 2020 15:43

Tgt Ion	Ratio	Lower	Upper
152	100		
115	60.5	29.9	89.7
150	160.1	0.0	340.6

