


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv030520\  
 Data File : VY001867.D  
 Acq On : 05 Mar 2020 09:12  
 Operator : SY/MD  
 Sample : BFB  
 Misc : 5.00G/5ML/MSVOA Y/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_Y\METHODS\82Y030420S.M  
 Title : SW846 8260  
 Last Update : Thu Mar 05 04:05:33 2020

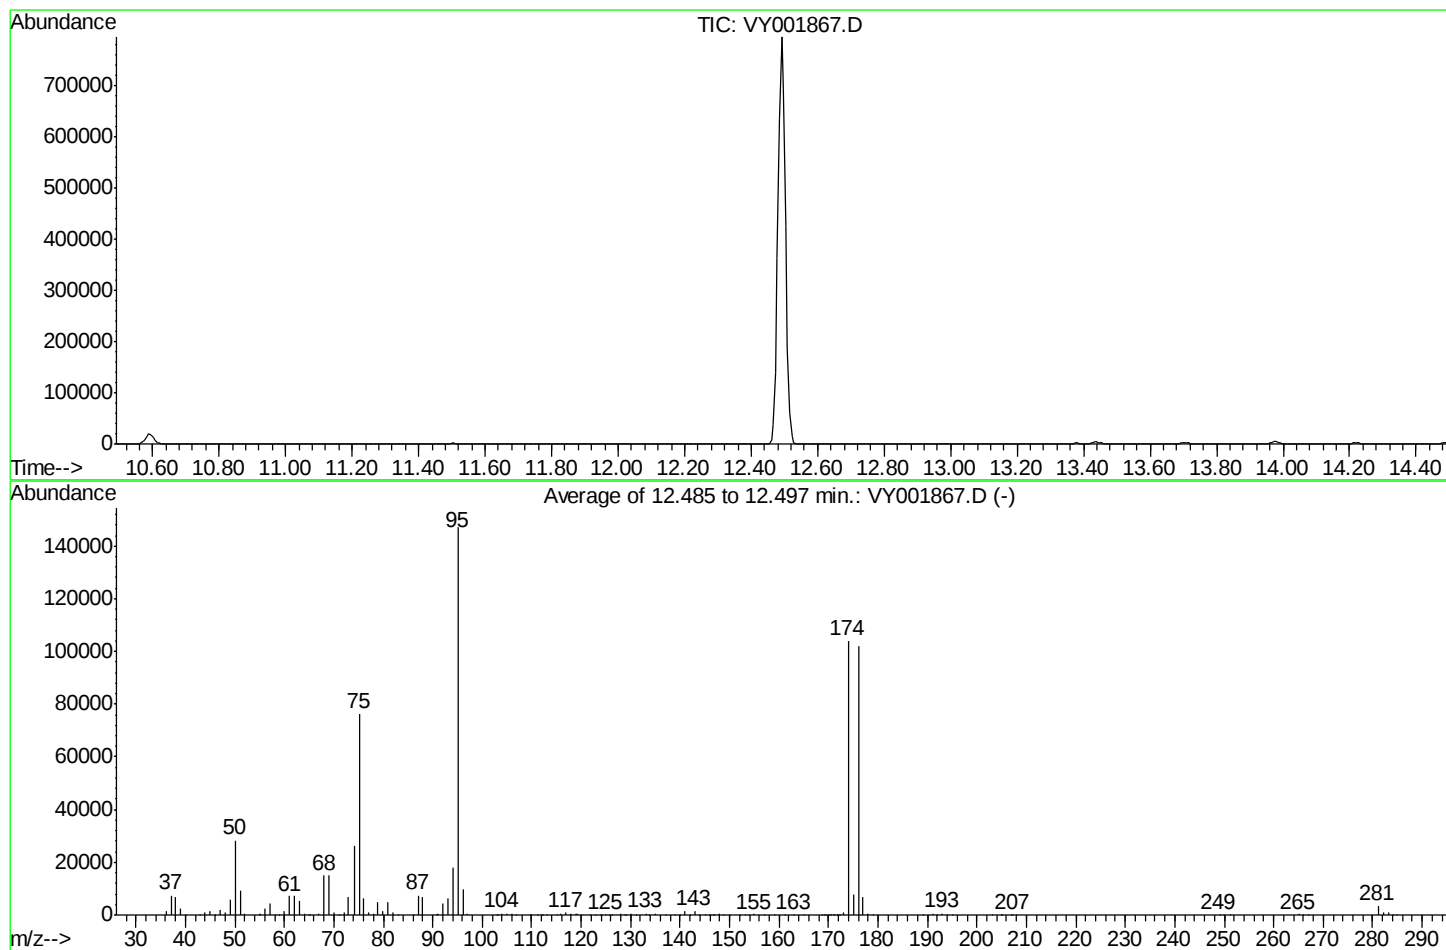

AutoFind: Scans 1763, 1764, 1765; Background Corrected with Scan 1755

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 19.3      | 28416   | PASS             |
| 75          | 95           | 30           | 60           | 51.9      | 76296   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 147093  | PASS             |
| 96          | 95           | 5            | 9            | 6.8       | 9973    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.9       | 981     | PASS             |
| 174         | 95           | 50           | 100          | 70.8      | 104098  | PASS             |
| 175         | 174          | 5            | 9            | 7.4       | 7715    | PASS             |
| 176         | 174          | 95           | 101          | 98.0      | 102010  | PASS             |
| 177         | 176          | 5            | 9            | 6.8       | 6940    | PASS             |