
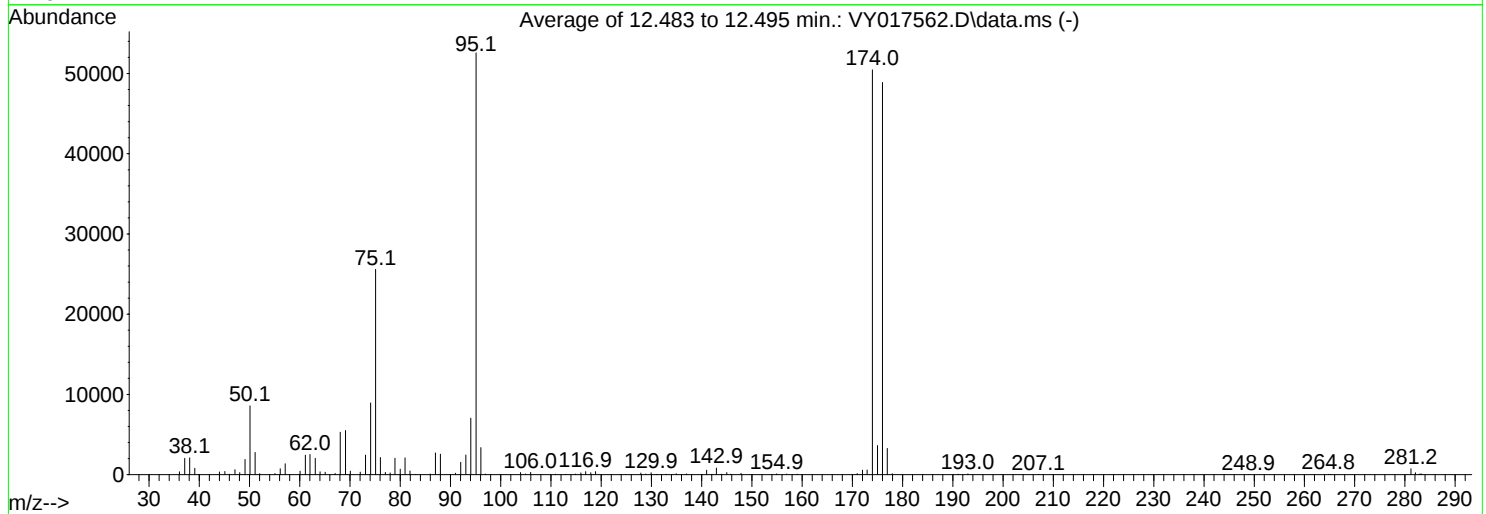


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030524\
Data File : VY017562.D
Acq On : 05 Mar 2024 09:11
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022324S.M
Title : SW846 8260
Last Update : Sat Feb 24 04:41:20 2024

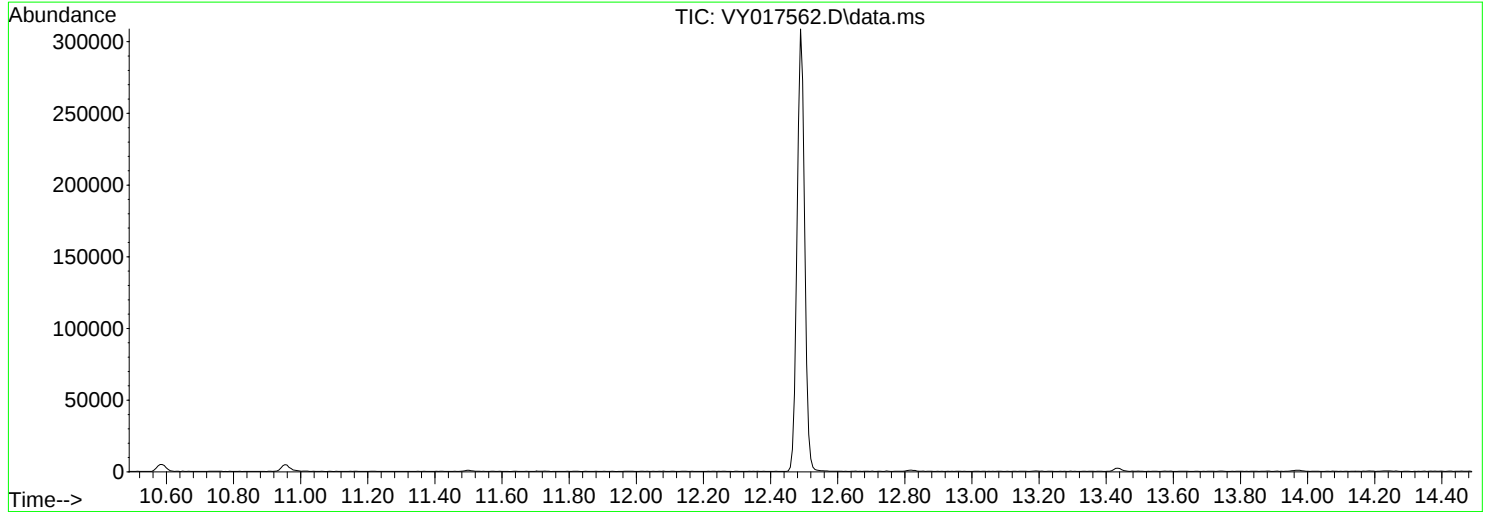

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	8571	PASS
75	95	30	60	48.7	25584	PASS
95	95	100	100	100.0	52571	PASS
96	95	5	9	6.4	3374	PASS
173	174	0.00	2	1.1	580	PASS
174	95	50	100	96.0	50451	PASS
175	174	5	9	7.2	3635	PASS
176	174	95	101	96.9	48872	PASS
177	176	5	9	6.7	3280	PASS