
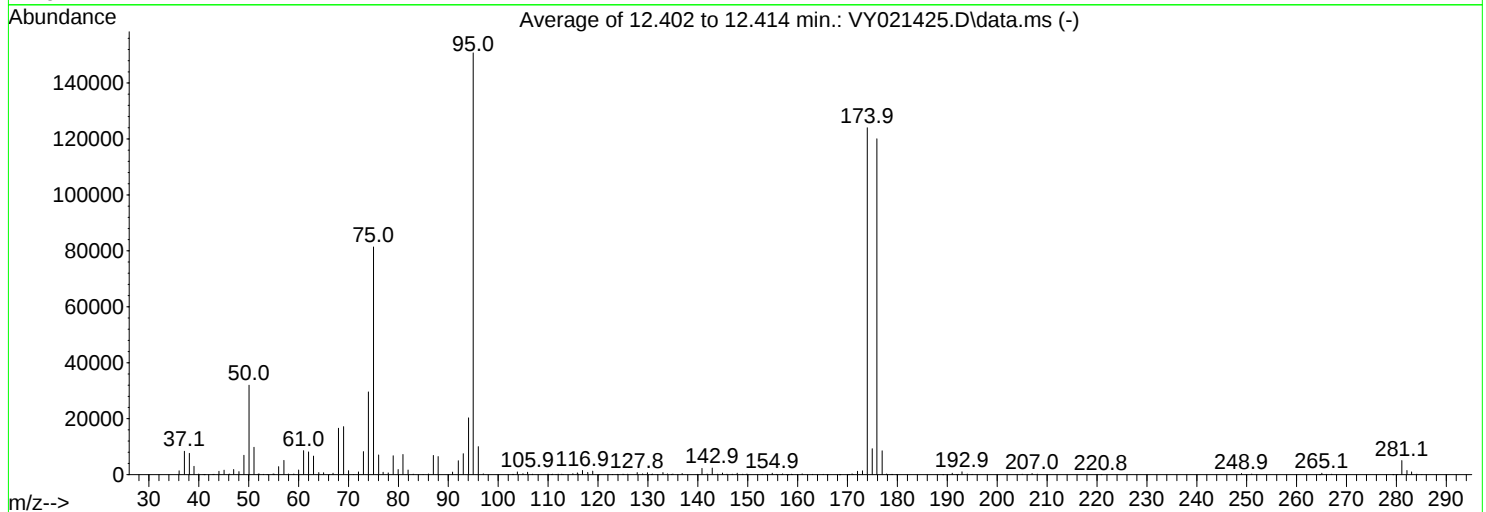


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030625\
Data File : VY021425.D
Acq On : 06 Mar 2025 09:39
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030425S.M
Title : SW846 8260
Last Update : Wed Mar 05 12:42:45 2025

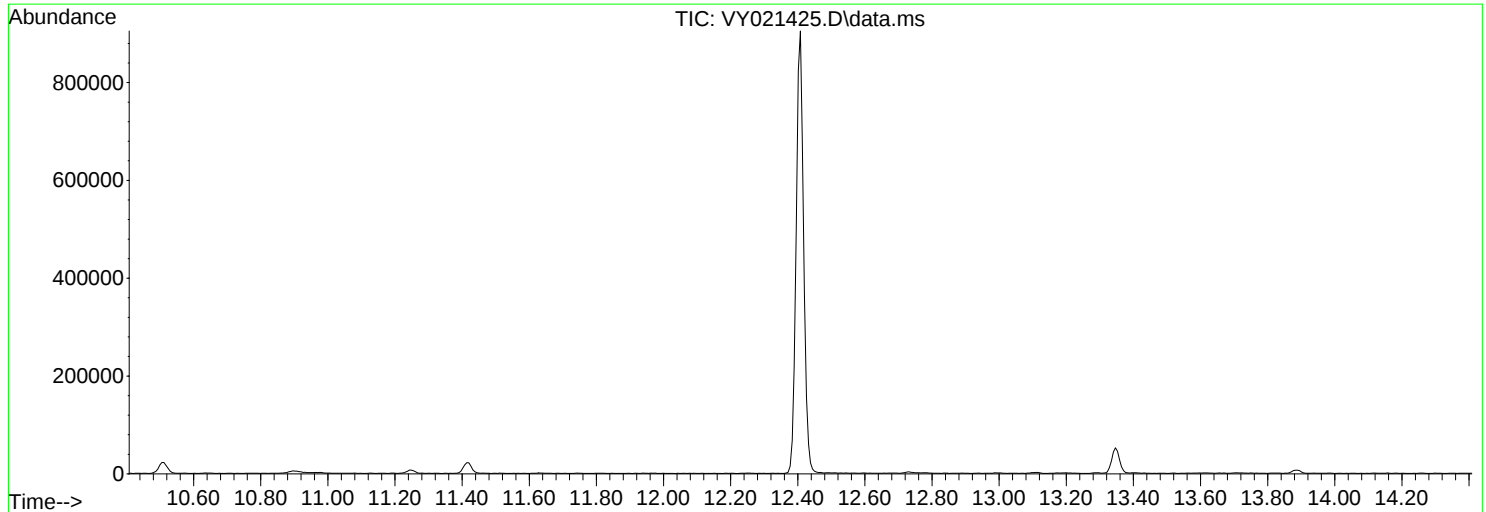

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1743

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.2	31960	PASS
75	95	30	60	54.0	81405	PASS
95	95	100	100	100.0	150795	PASS
96	95	5	9	6.6	10000	PASS
173	174	0.00	2	1.1	1384	PASS
174	95	50	100	82.3	124032	PASS
175	174	5	9	7.5	9302	PASS
176	174	95	101	96.8	120088	PASS
177	176	5	9	7.1	8525	PASS