

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030724\
 Data File : VY017600.D
 Acq On : 07 Mar 2024 11:43
 Operator : SY/MD
 Sample : VY0307SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0307SBL01

Quant Time: Mar 08 03:24:02 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022324S.M
 Quant Title : SW846 8260
 QLast Update : Sat Feb 24 04:41:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.795	168	123903	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	221569	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.496	117	195231	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	74937	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	60550	51.564	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	103.120%
35) Dibromofluoromethane	7.722	113	70836	45.879	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	91.760%
50) Toluene-d8	10.185	98	255299	47.293	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	94.580%
62) 4-Bromofluorobenzene	12.489	95	67506	39.791	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	79.580%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030724\
Data File : VY017600.D
Acq On : 07 Mar 2024 11:43
Operator : SY/MD
Sample : VY0307SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0307SBL01

Quant Time: Mar 08 03:24:02 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022324S.M
Quant Title : SW846 8260
QLast Update : Sat Feb 24 04:41:20 2024
Response via : Initial Calibration




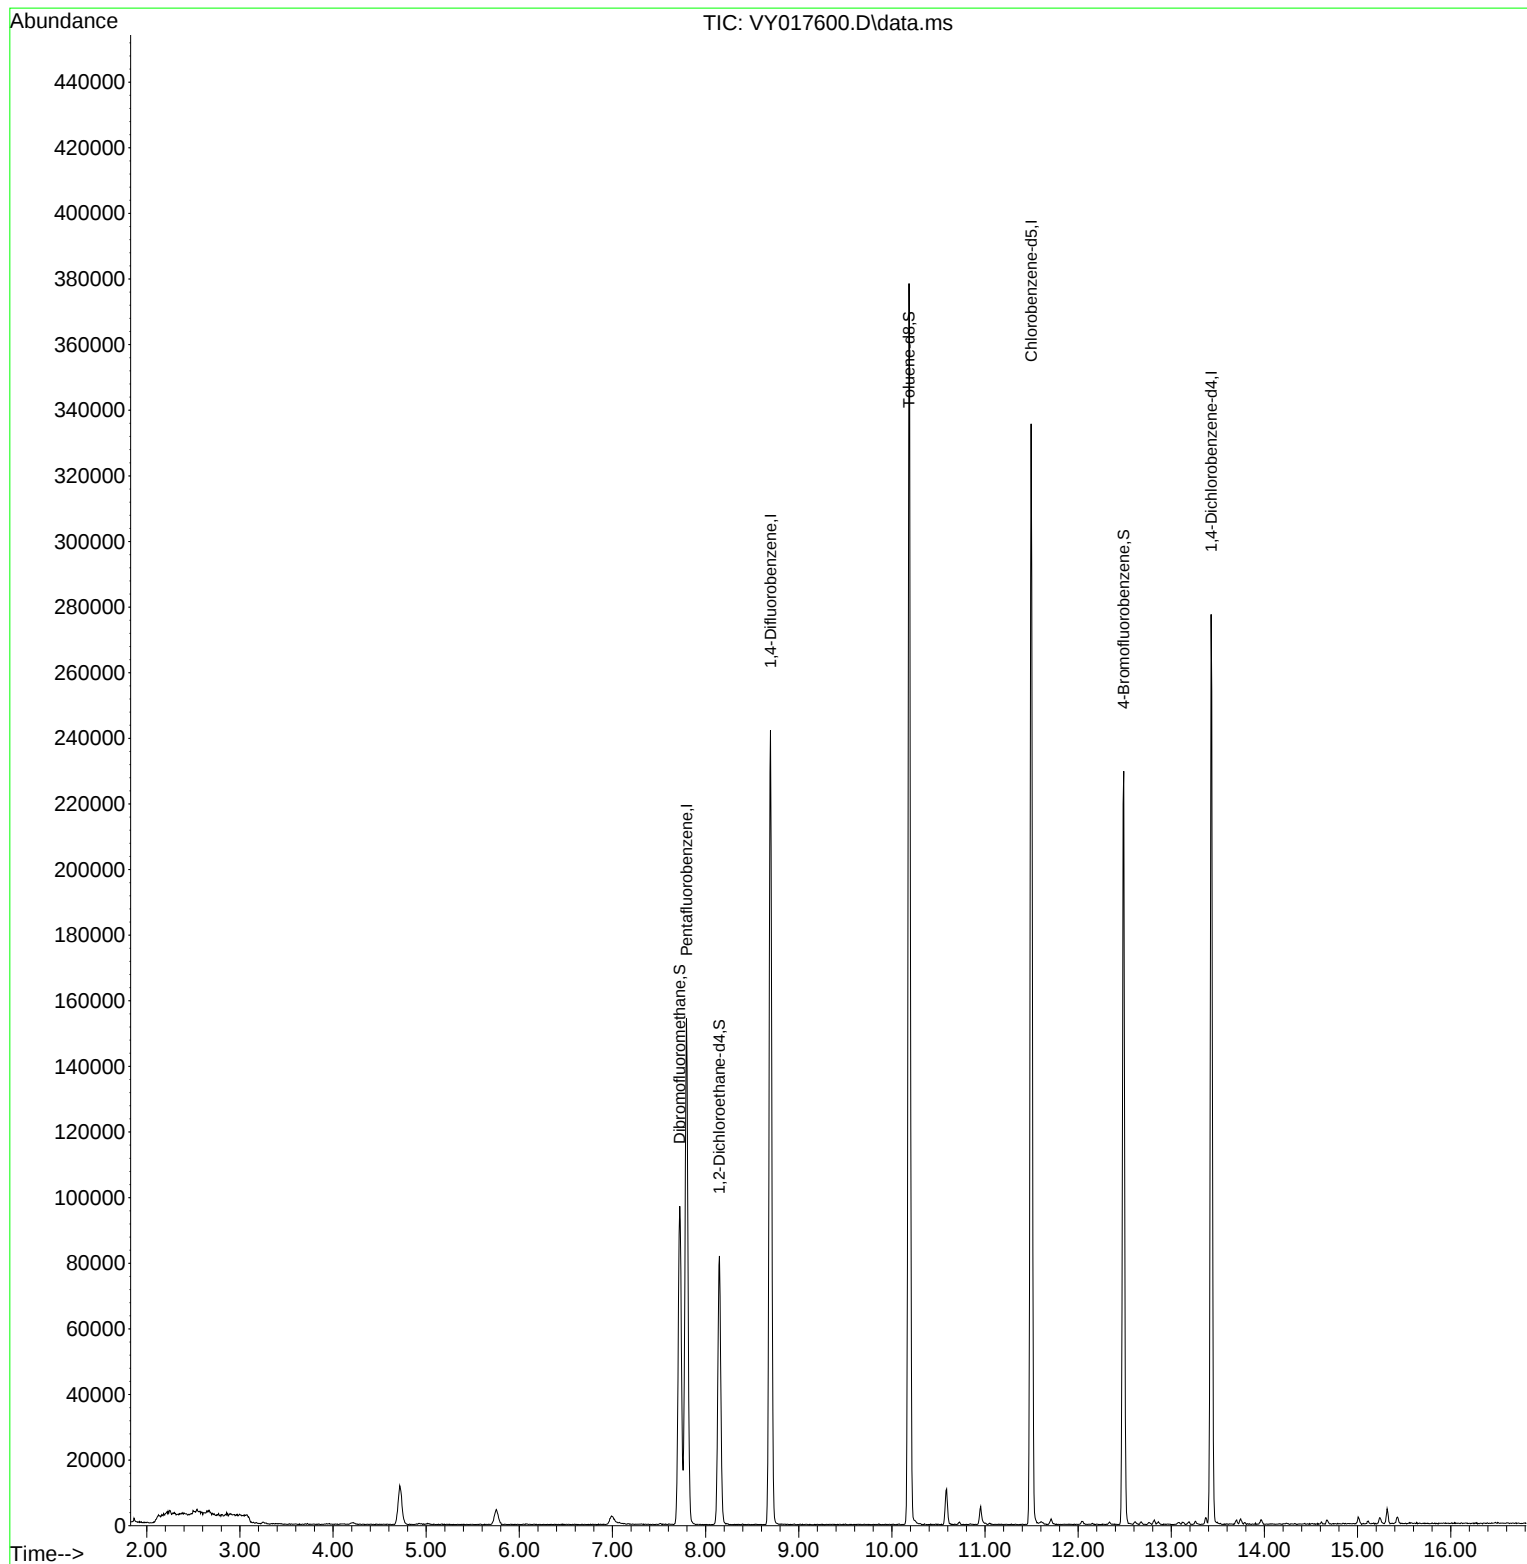


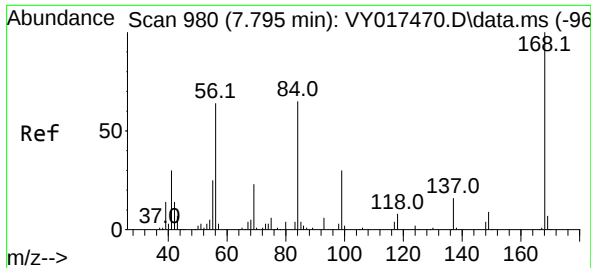

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.795 min Scan# 980
Delta R.T. 0.000 min
Lab File: VY017600.D
Acq: 07 Mar 2024 11:43




Instrument :
MSVOA_Y
ClientSampleId :
VY0307SBL01


Tgt Ion:168 Resp: 123903
Ion Ratio Lower Upper
168 100
99 49.6 39.1 58.7

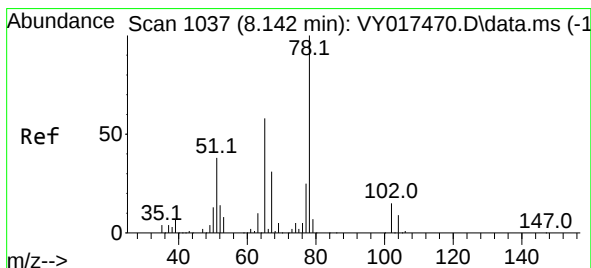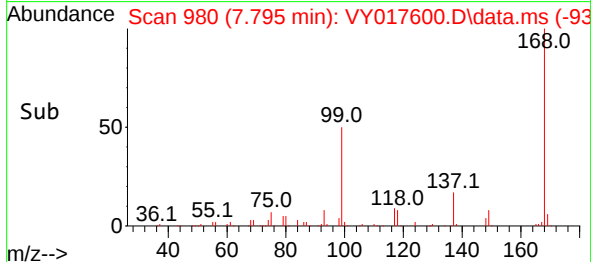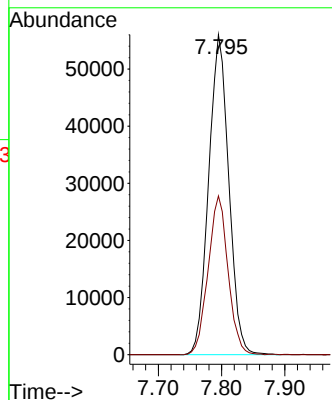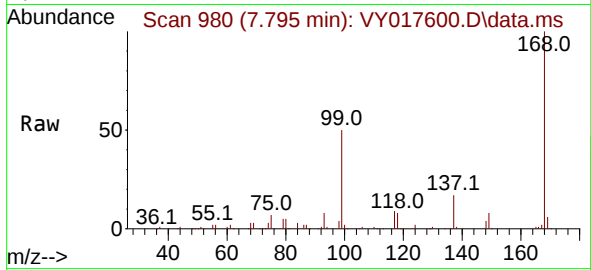

#33
1,2-Dichloroethane-d4
Concen: 51.564 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. 0.006 min
Lab File: VY017600.D
Acq: 07 Mar 2024 11:43

Tgt Ion: 65 Resp: 60550
Ion Ratio Lower Upper
65 100
67 55.0 0.0 109.6

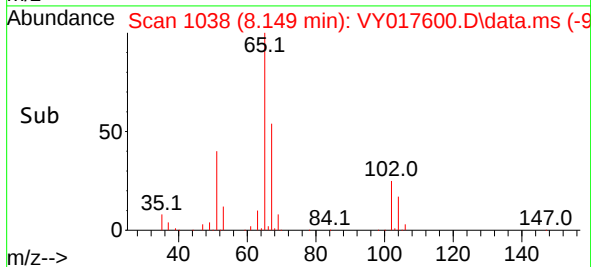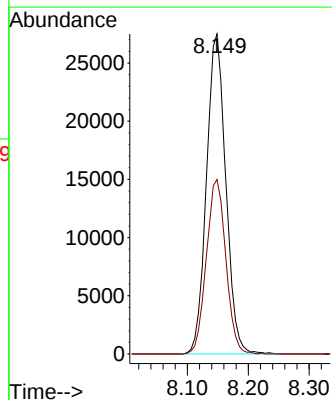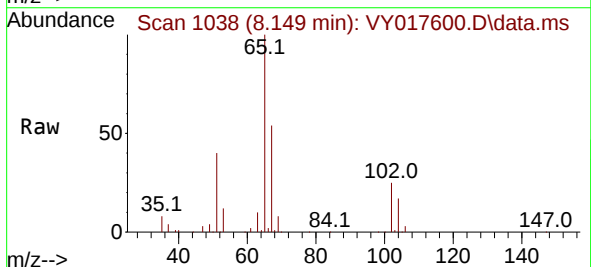

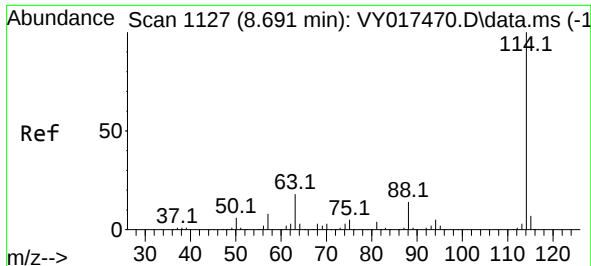

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.697 min Scan# 1127

Delta R.T. 0.006 min

Lab File: VY017600.D

Acq: 07 Mar 2024 11:43

Instrument :

MSVOA_Y

ClientSampleId :

VY0307SBL01





Tgt Ion:114 Resp: 221569

Ion Ratio Lower Upper

114 100

63 17.7 0.0 35.0

88 13.9 0.0 27.2

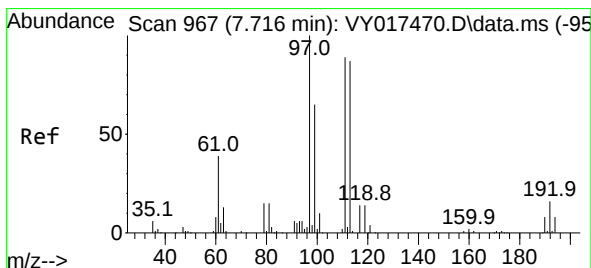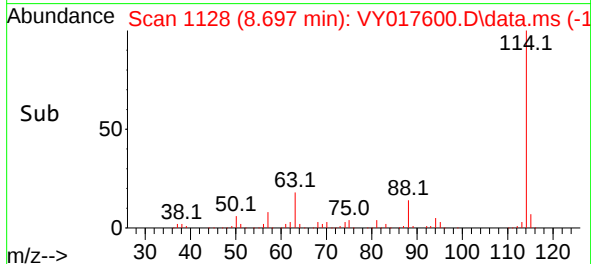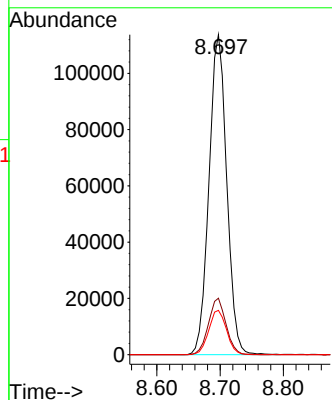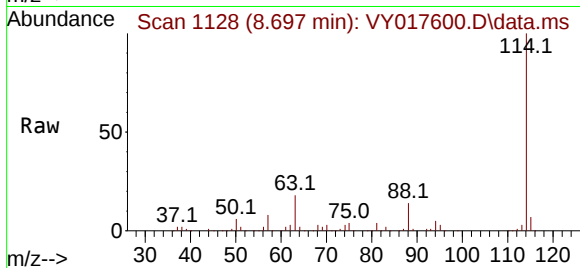

#35

Dibromofluoromethane

Concen: 45.879 ug/l

RT: 7.722 min Scan# 968

Delta R.T. 0.006 min

Lab File: VY017600.D

Acq: 07 Mar 2024 11:43




Tgt Ion:113 Resp: 70836


Ion Ratio Lower Upper

113 100

111 103.7 82.2 123.4

192 21.0 15.9 23.9


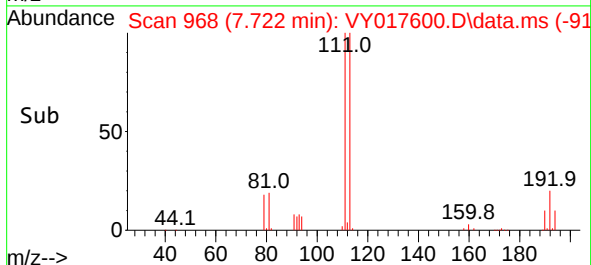
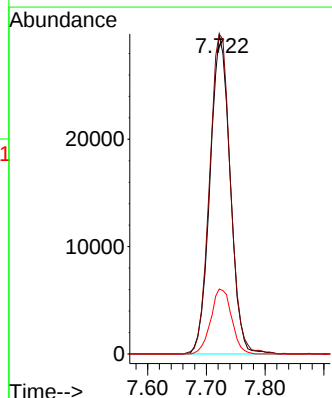
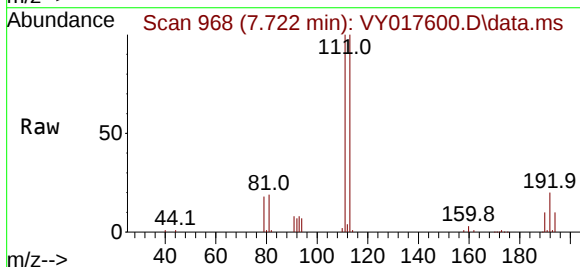


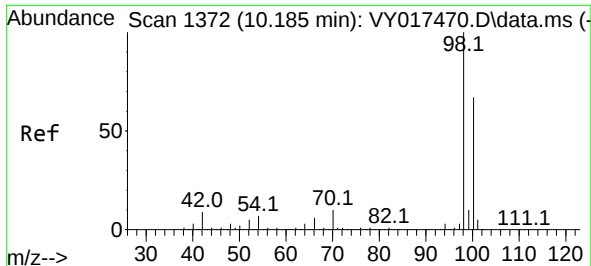

#50
Toluene-d8
Concen: 47.293 ug/l
RT: 10.185 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY017600.D
Acq: 07 Mar 2024 11:43




Instrument :
MSVOA_Y
ClientSampleId :
VY0307SBL01


Tgt Ion: 98 Resp: 255299
Ion Ratio Lower Upper
98 100
100 64.2 52.0 78.0

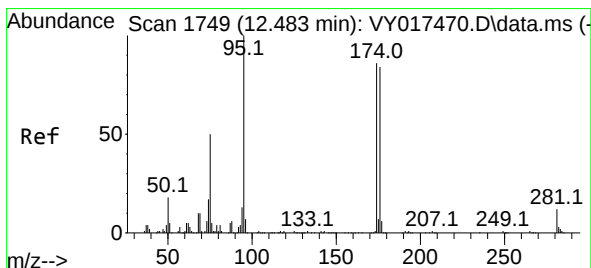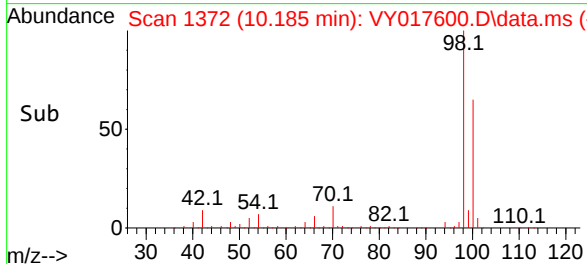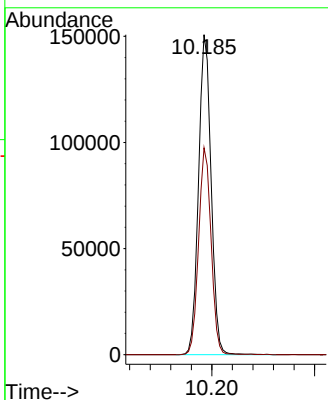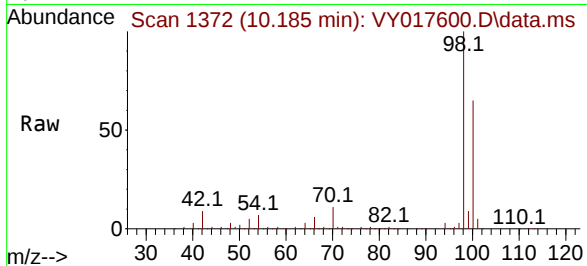

#62
4-Bromofluorobenzene
Concen: 39.791 ug/l
RT: 12.489 min Scan# 1750
Delta R.T. 0.006 min
Lab File: VY017600.D
Acq: 07 Mar 2024 11:43

Tgt Ion: 95 Resp: 67506
Ion Ratio Lower Upper
95 100
174 96.2 0.0 175.6
176 91.0 0.0 171.4


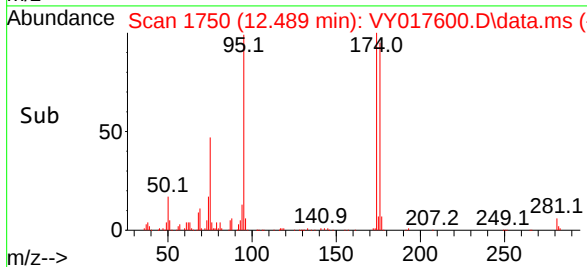
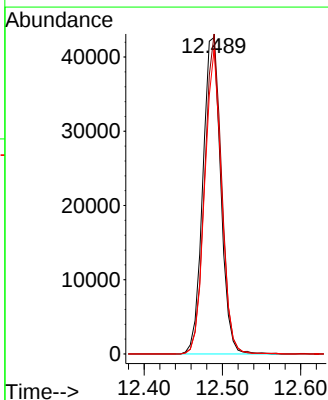
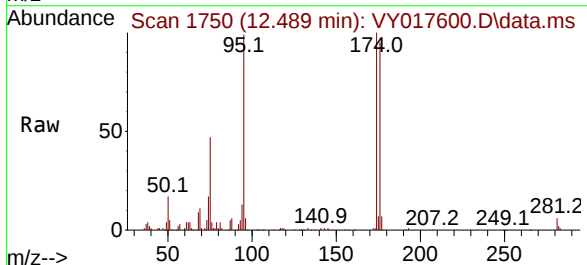


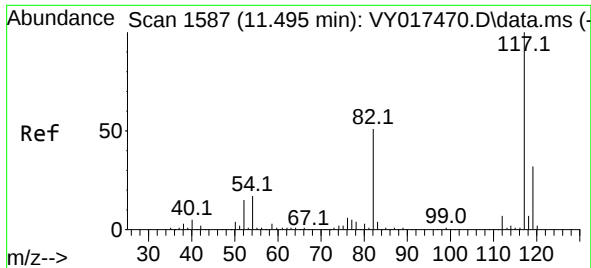

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.496 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY017600.D
Acq: 07 Mar 2024 11:43

Instrument :
MSVOA_Y
ClientSampleId :
VY0307SBL01

Tgt Ion:117 Resp: 195231
Ion Ratio Lower Upper
117 100
82 51.6 42.4 63.6
119 32.2 25.9 38.9

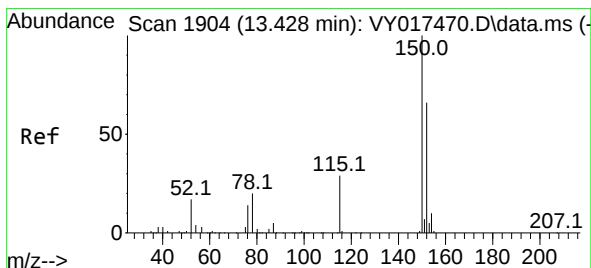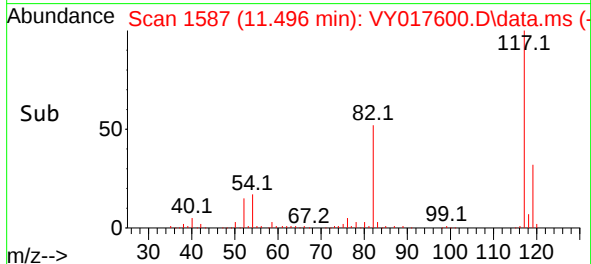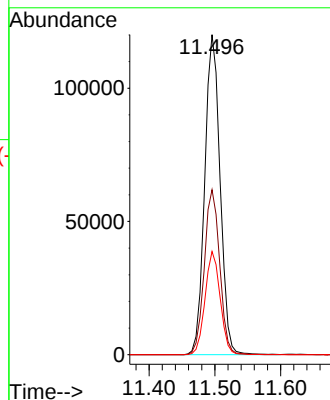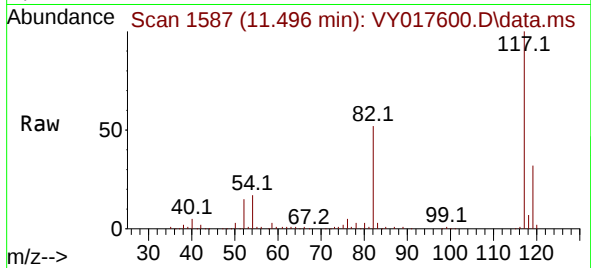

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY017600.D
Acq: 07 Mar 2024 11:43

Tgt Ion:152 Resp: 74937
Ion Ratio Lower Upper
152 100
115 54.3 28.2 84.7
150 157.4 0.0 345.6

