

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030724\
 Data File : VY017607.D
 Acq On : 07 Mar 2024 17:08
 Operator : SY/MD
 Sample : P1701-08
 Misc : 6.91g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VOC-5-GRAB

Quant Time: Mar 08 03:27:36 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022324S.M
 Quant Title : SW846 8260
 QLast Update : Sat Feb 24 04:41:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.795	168	109553	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	198237	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.495	117	183195	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	74314	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	60558	58.326	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	116.660%
35) Dibromofluoromethane	7.722	113	65323	47.288	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	94.580%
50) Toluene-d8	10.185	98	233335	48.311	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	96.620%
62) 4-Bromofluorobenzene	12.489	95	65933	43.438	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	86.880%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030724\
Data File : VY017607.D
Acq On : 07 Mar 2024 17:08
Operator : SY/MD
Sample : P1701-08
Misc : 6.91g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VOC-5-GRAB

Quant Time: Mar 08 03:27:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022324S.M
Quant Title : SW846 8260
QLast Update : Sat Feb 24 04:41:20 2024
Response via : Initial Calibration




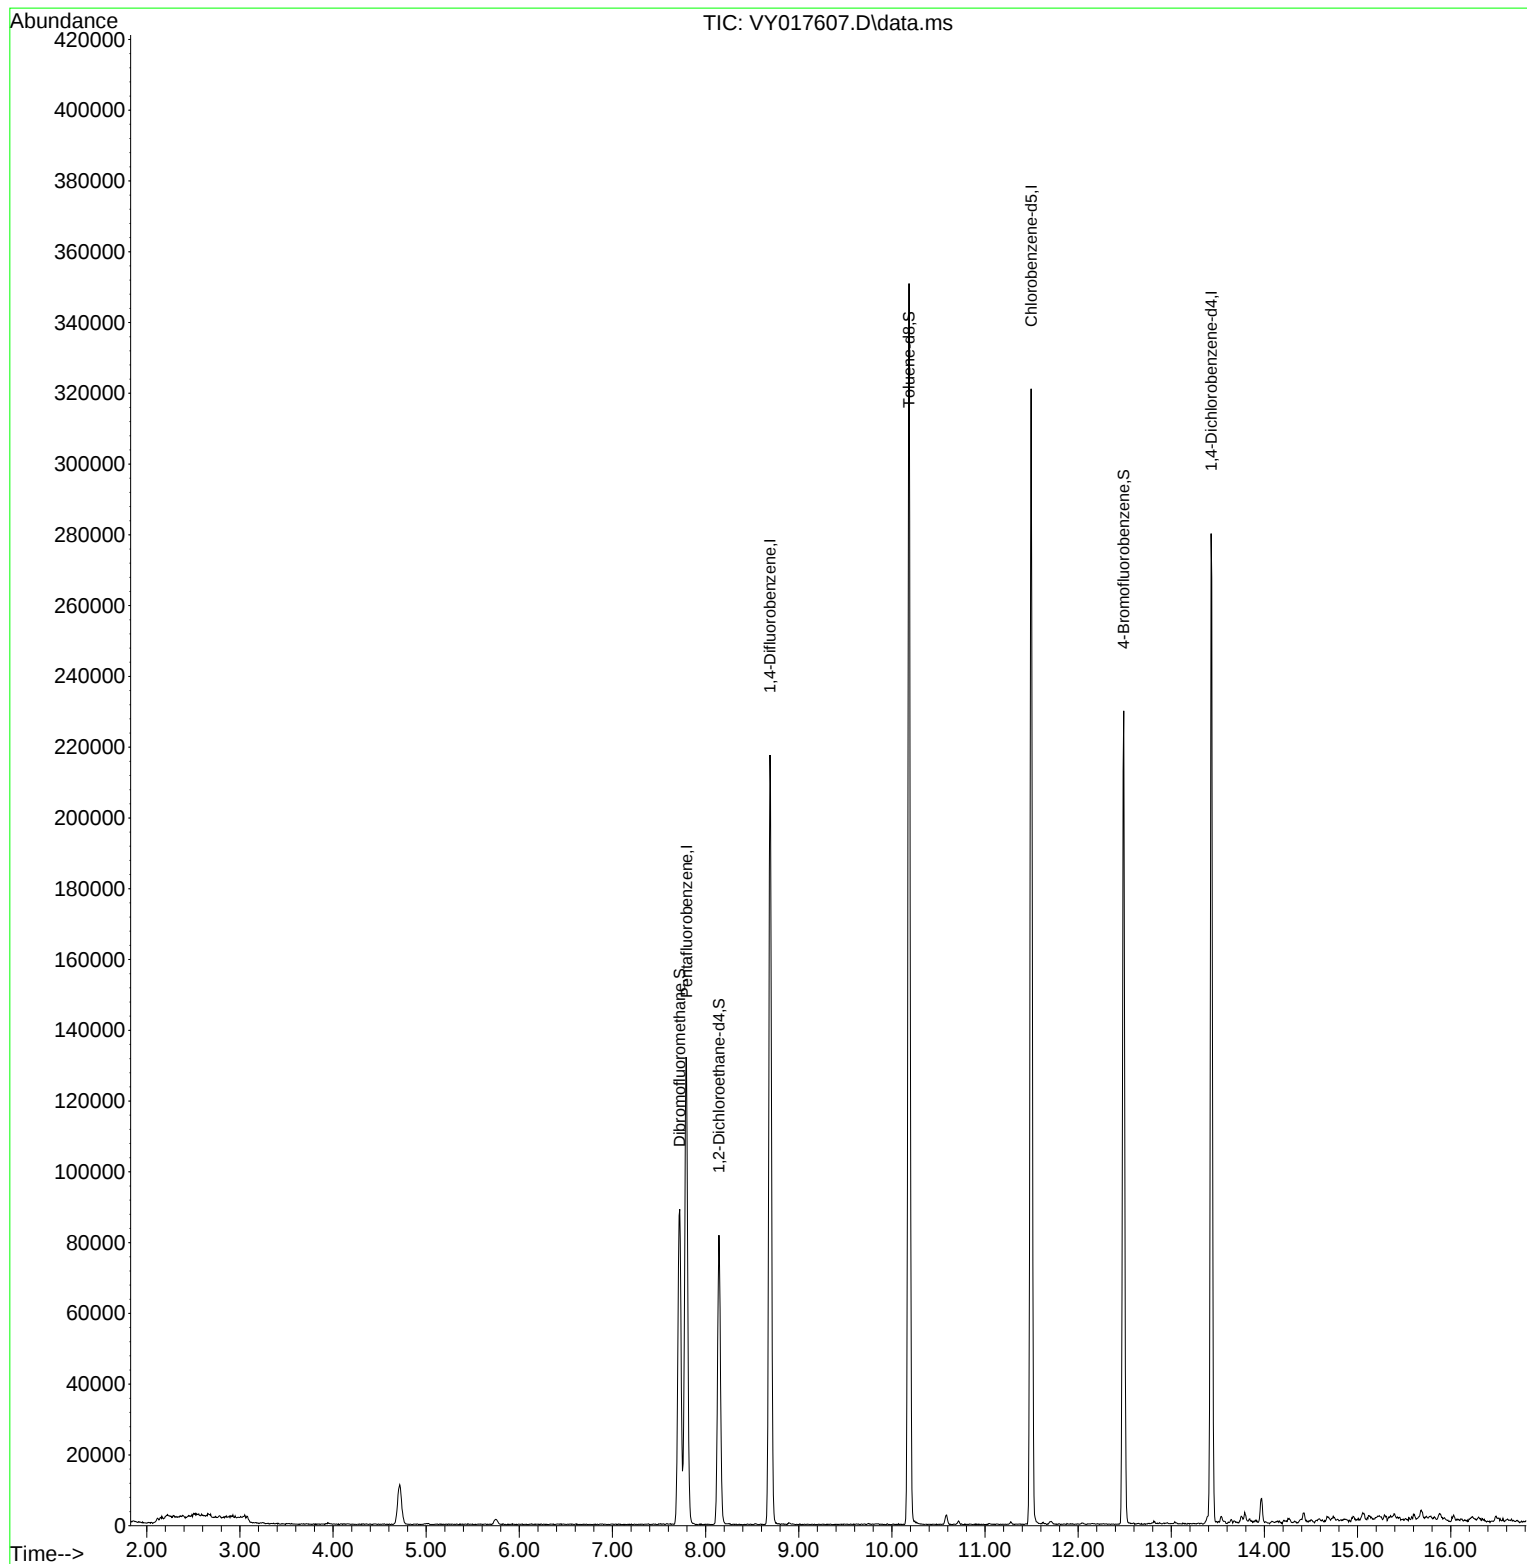


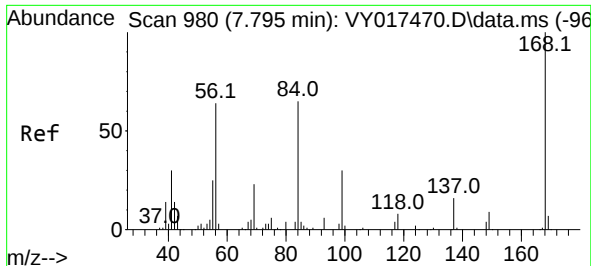

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.795 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY017607.D
Acq: 07 Mar 2024 17:08




Instrument :
MSVOA_Y
ClientSampleId :
VOC-5-GRAB


Tgt Ion:168 Resp: 109553
Ion Ratio Lower Upper
168 100
99 45.6 39.1 58.7

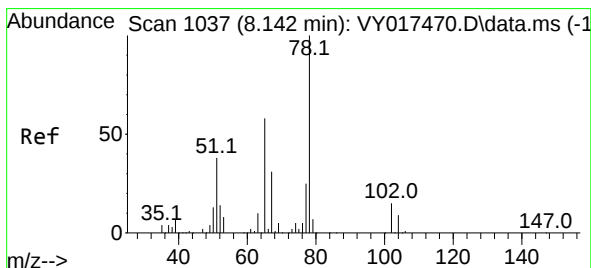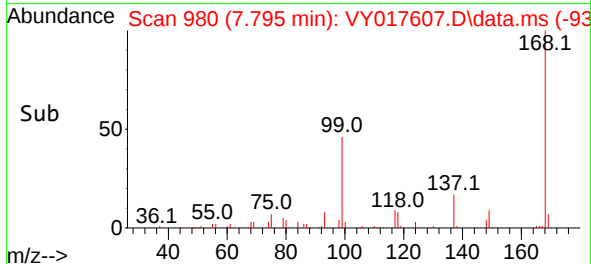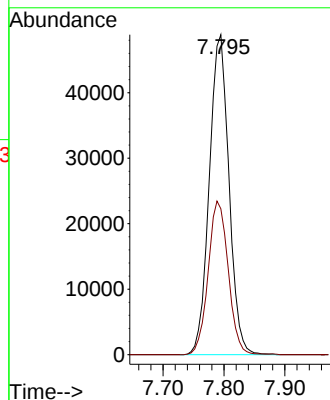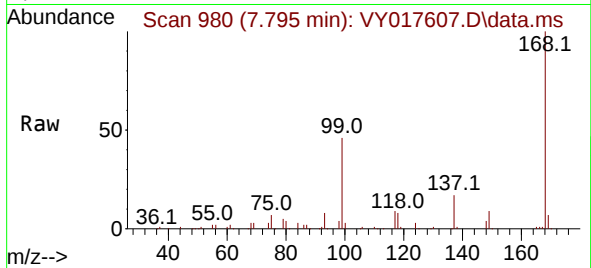

#33
1,2-Dichloroethane-d4
Concen: 58.326 ug/l
RT: 8.142 min Scan# 1037
Delta R.T. -0.000 min
Lab File: VY017607.D
Acq: 07 Mar 2024 17:08

Tgt Ion: 65 Resp: 60558
Ion Ratio Lower Upper
65 100
67 54.5 0.0 109.6

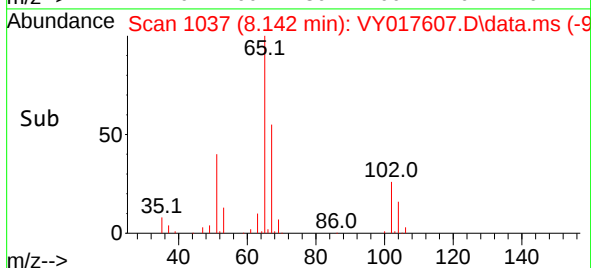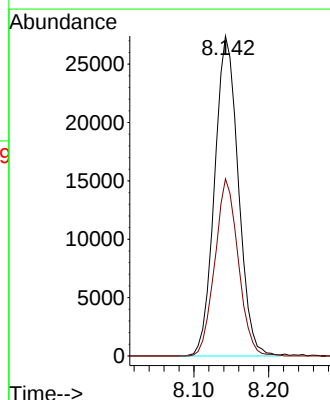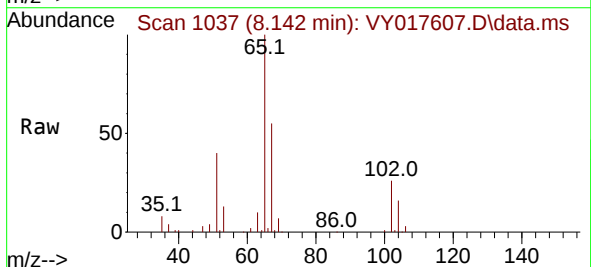

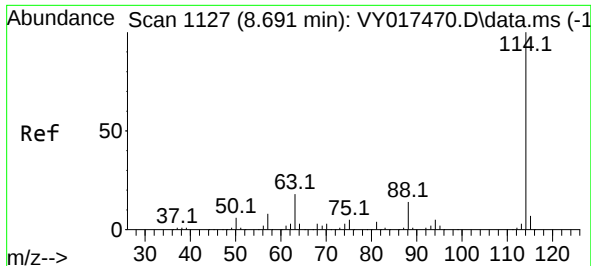

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. -0.000 min

Lab File: VY017607.D

Acq: 07 Mar 2024 17:08

Instrument :

MSVOA_Y

ClientSampleId :

VOC-5-GRAB




Tgt Ion:114 Resp: 198237

Ion Ratio Lower Upper

114 100

63 18.1 0.0 35.0

88 13.7 0.0 27.2

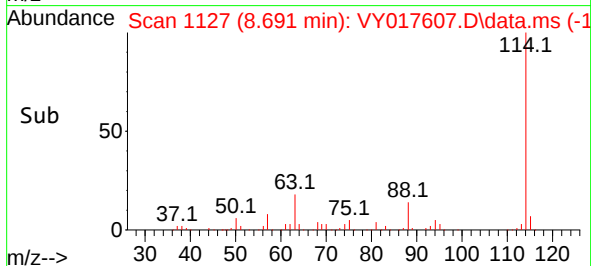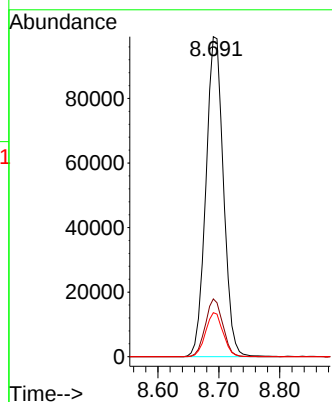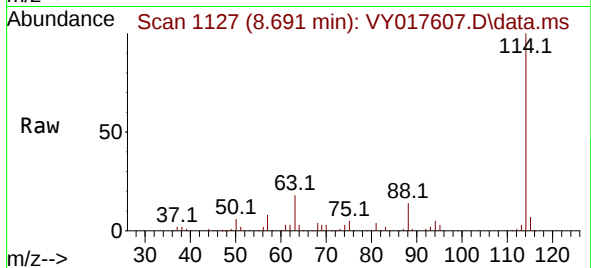

#35

Dibromofluoromethane

Concen: 47.288 ug/l

RT: 7.722 min Scan# 968

Delta R.T. 0.006 min

Lab File: VY017607.D

Acq: 07 Mar 2024 17:08




Tgt Ion:113 Resp: 65323


Ion Ratio Lower Upper

113 100

111 104.0 82.2 123.4

192 20.5 15.9 23.9


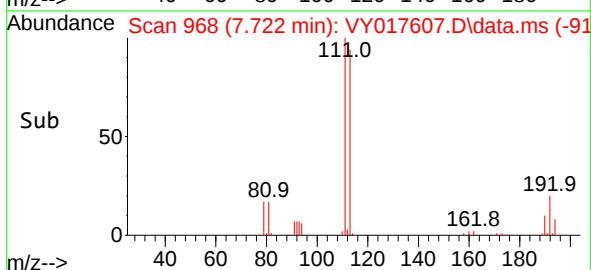
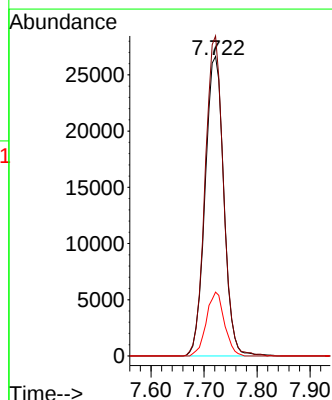
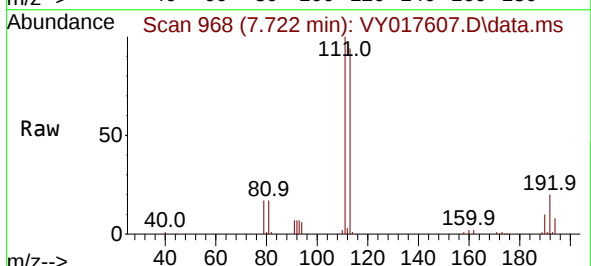


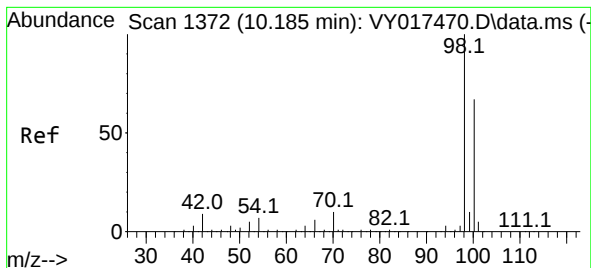

#50
Toluene-d8
Concen: 48.311 ug/l
RT: 10.185 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY017607.D
Acq: 07 Mar 2024 17:08




Instrument :
MSVOA_Y
ClientSampleId :
VOC-5-GRAB


Tgt Ion: 98 Resp: 233335
Ion Ratio Lower Upper
98 100
100 63.4 52.0 78.0

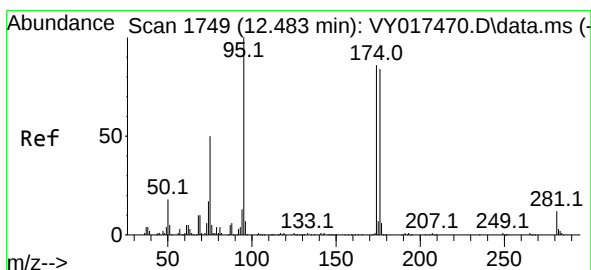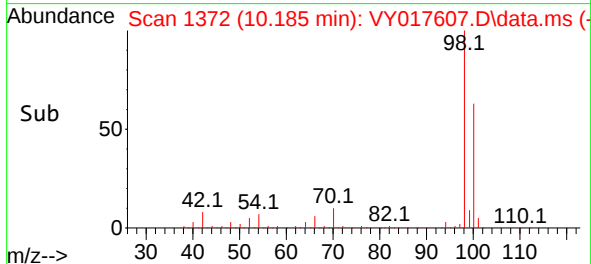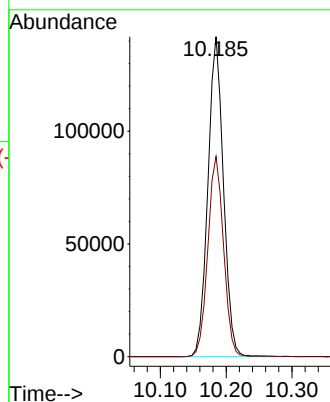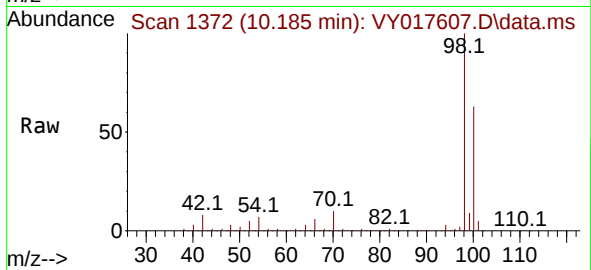

#62
4-Bromofluorobenzene
Concen: 43.438 ug/l
RT: 12.489 min Scan# 1750
Delta R.T. 0.006 min
Lab File: VY017607.D
Acq: 07 Mar 2024 17:08

Tgt Ion: 95 Resp: 65933
Ion Ratio Lower Upper
95 100
174 92.7 0.0 175.6
176 91.1 0.0 171.4

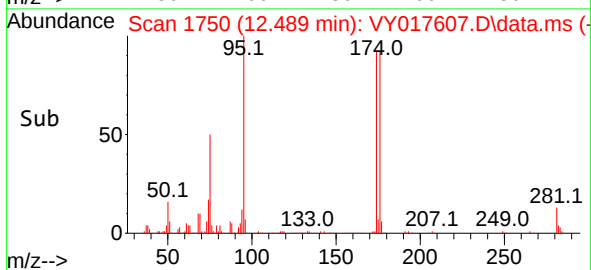
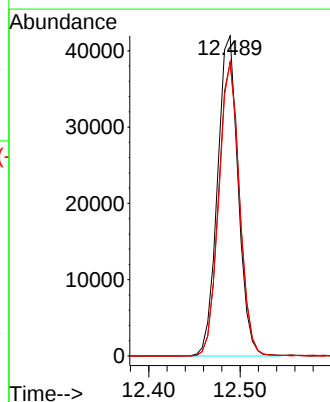
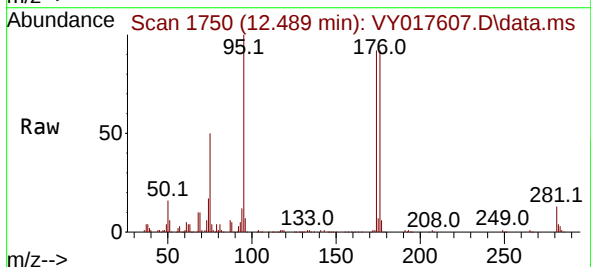


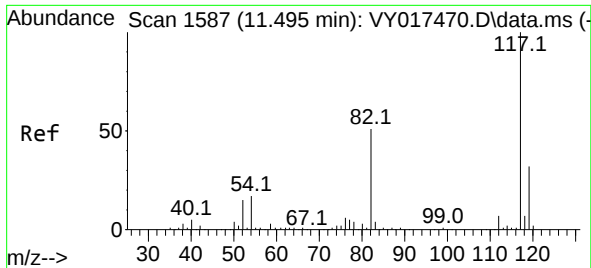

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.495 min Scan# 117
Delta R.T. -0.000 min
Lab File: VY017607.D
Acq: 07 Mar 2024 17:08

Instrument :
MSVOA_Y
ClientSampleId :
VOC-5-GRAB

Tgt Ion:117 Resp: 183195
Ion Ratio Lower Upper
117 100
82 51.6 42.4 63.6
119 32.6 25.9 38.9

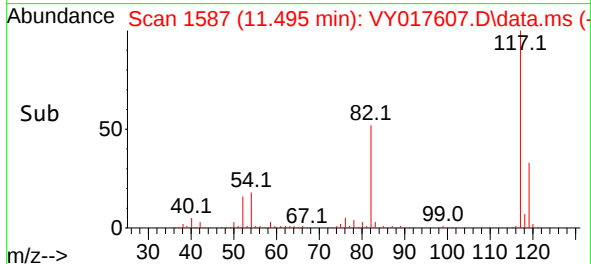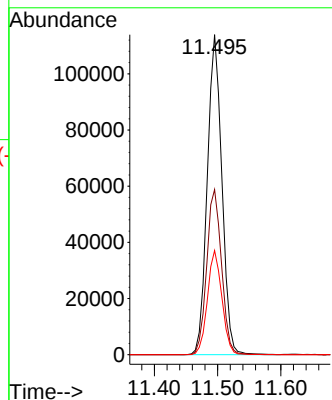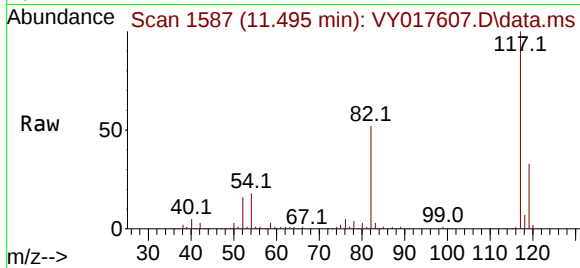

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY017607.D
Acq: 07 Mar 2024 17:08

Tgt Ion:152 Resp: 74314
Ion Ratio Lower Upper
152 100
115 54.6 28.2 84.7
150 155.8 0.0 345.6

