


Dichlorodifluoromethane

Response Ratio

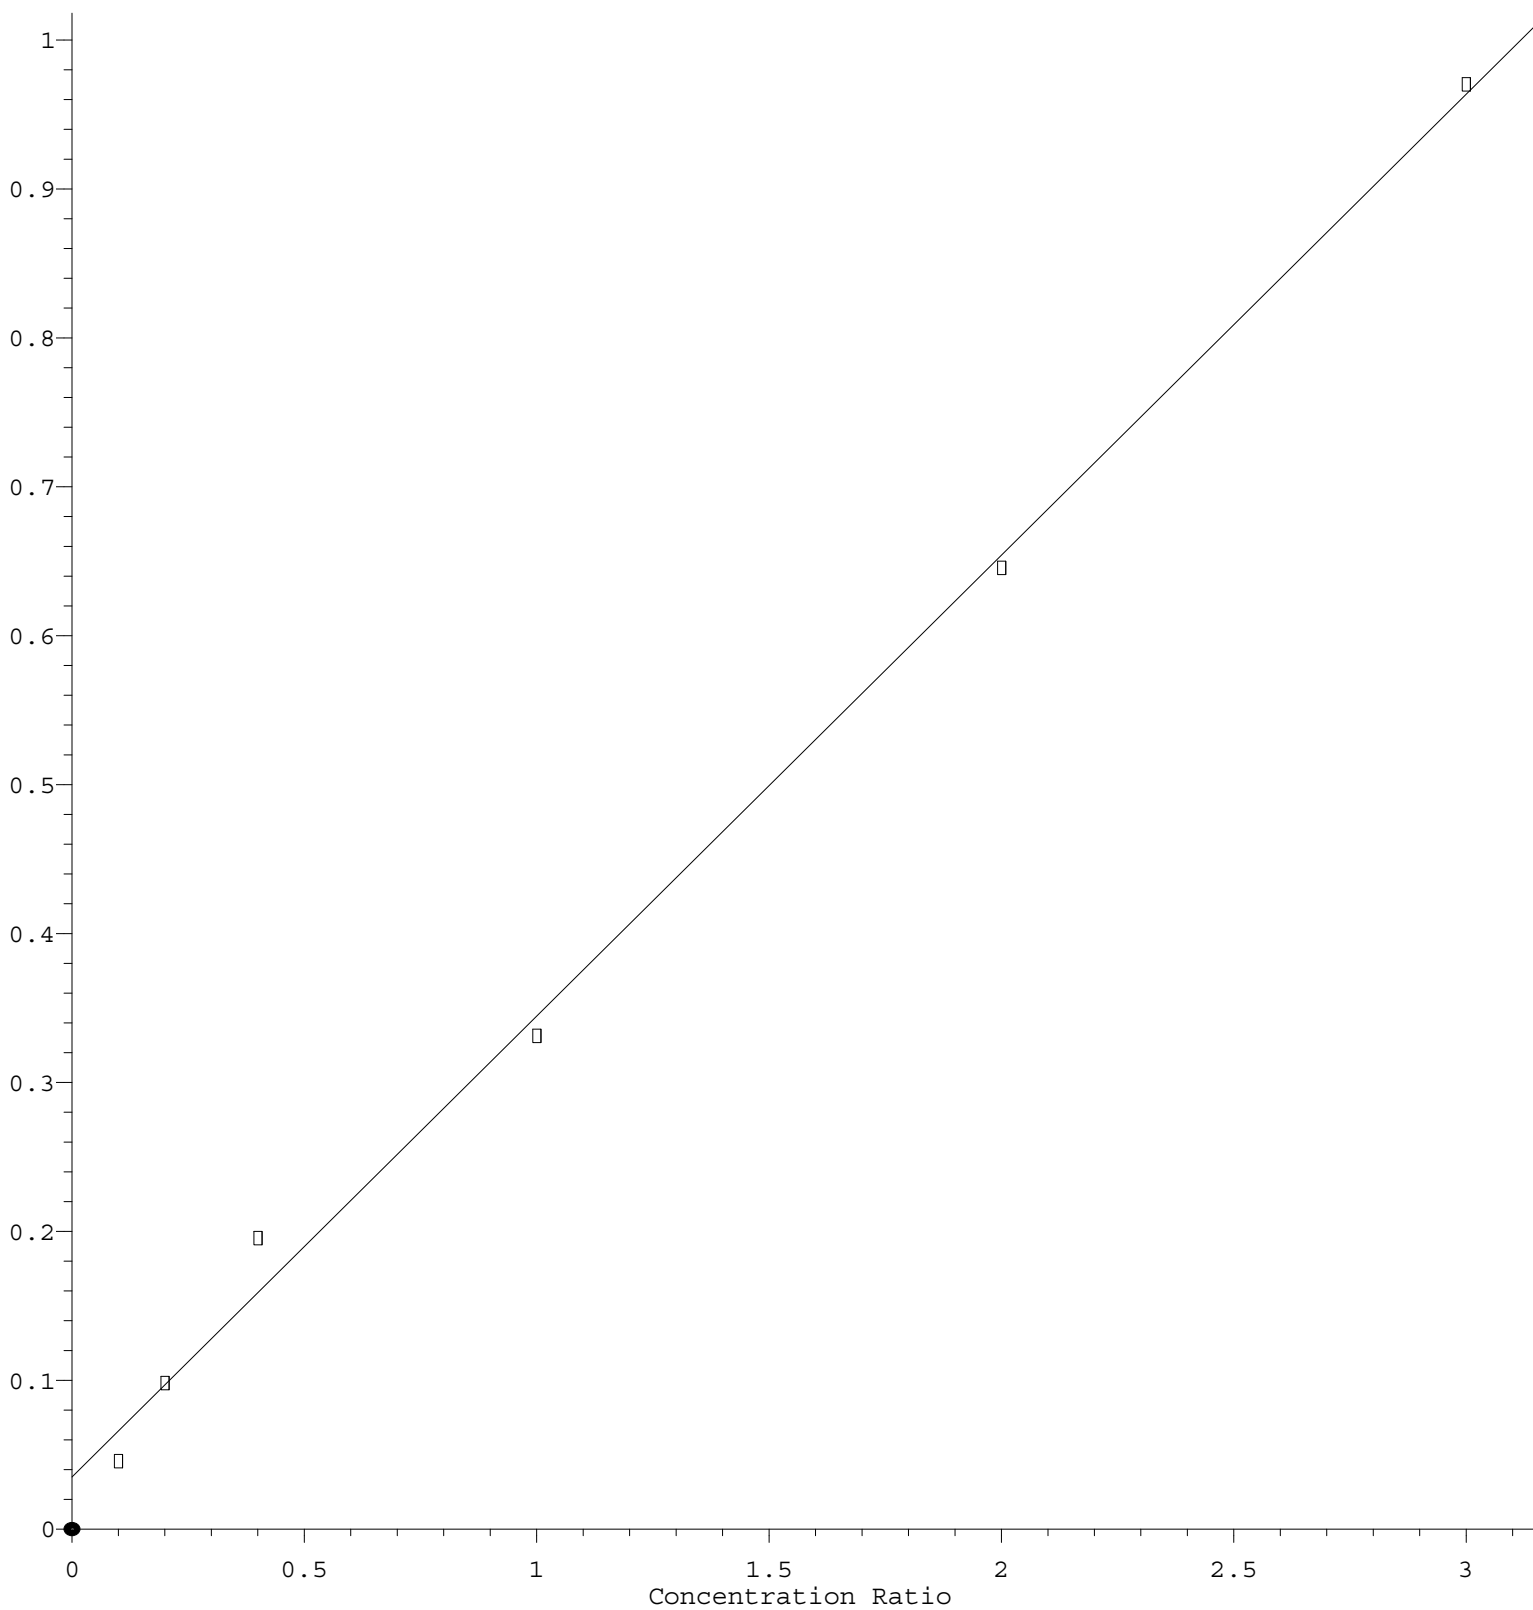

$$\text{Response} = 3.095\text{e-}001 * \text{Amt} + 3.542\text{e-}002$$


Coef of Det (r^2) = 0.996826 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y030821S.M

Calibration Table Last Updated: Mon Mar 08 12:28:55 2021

Chloromethane

Response Ratio

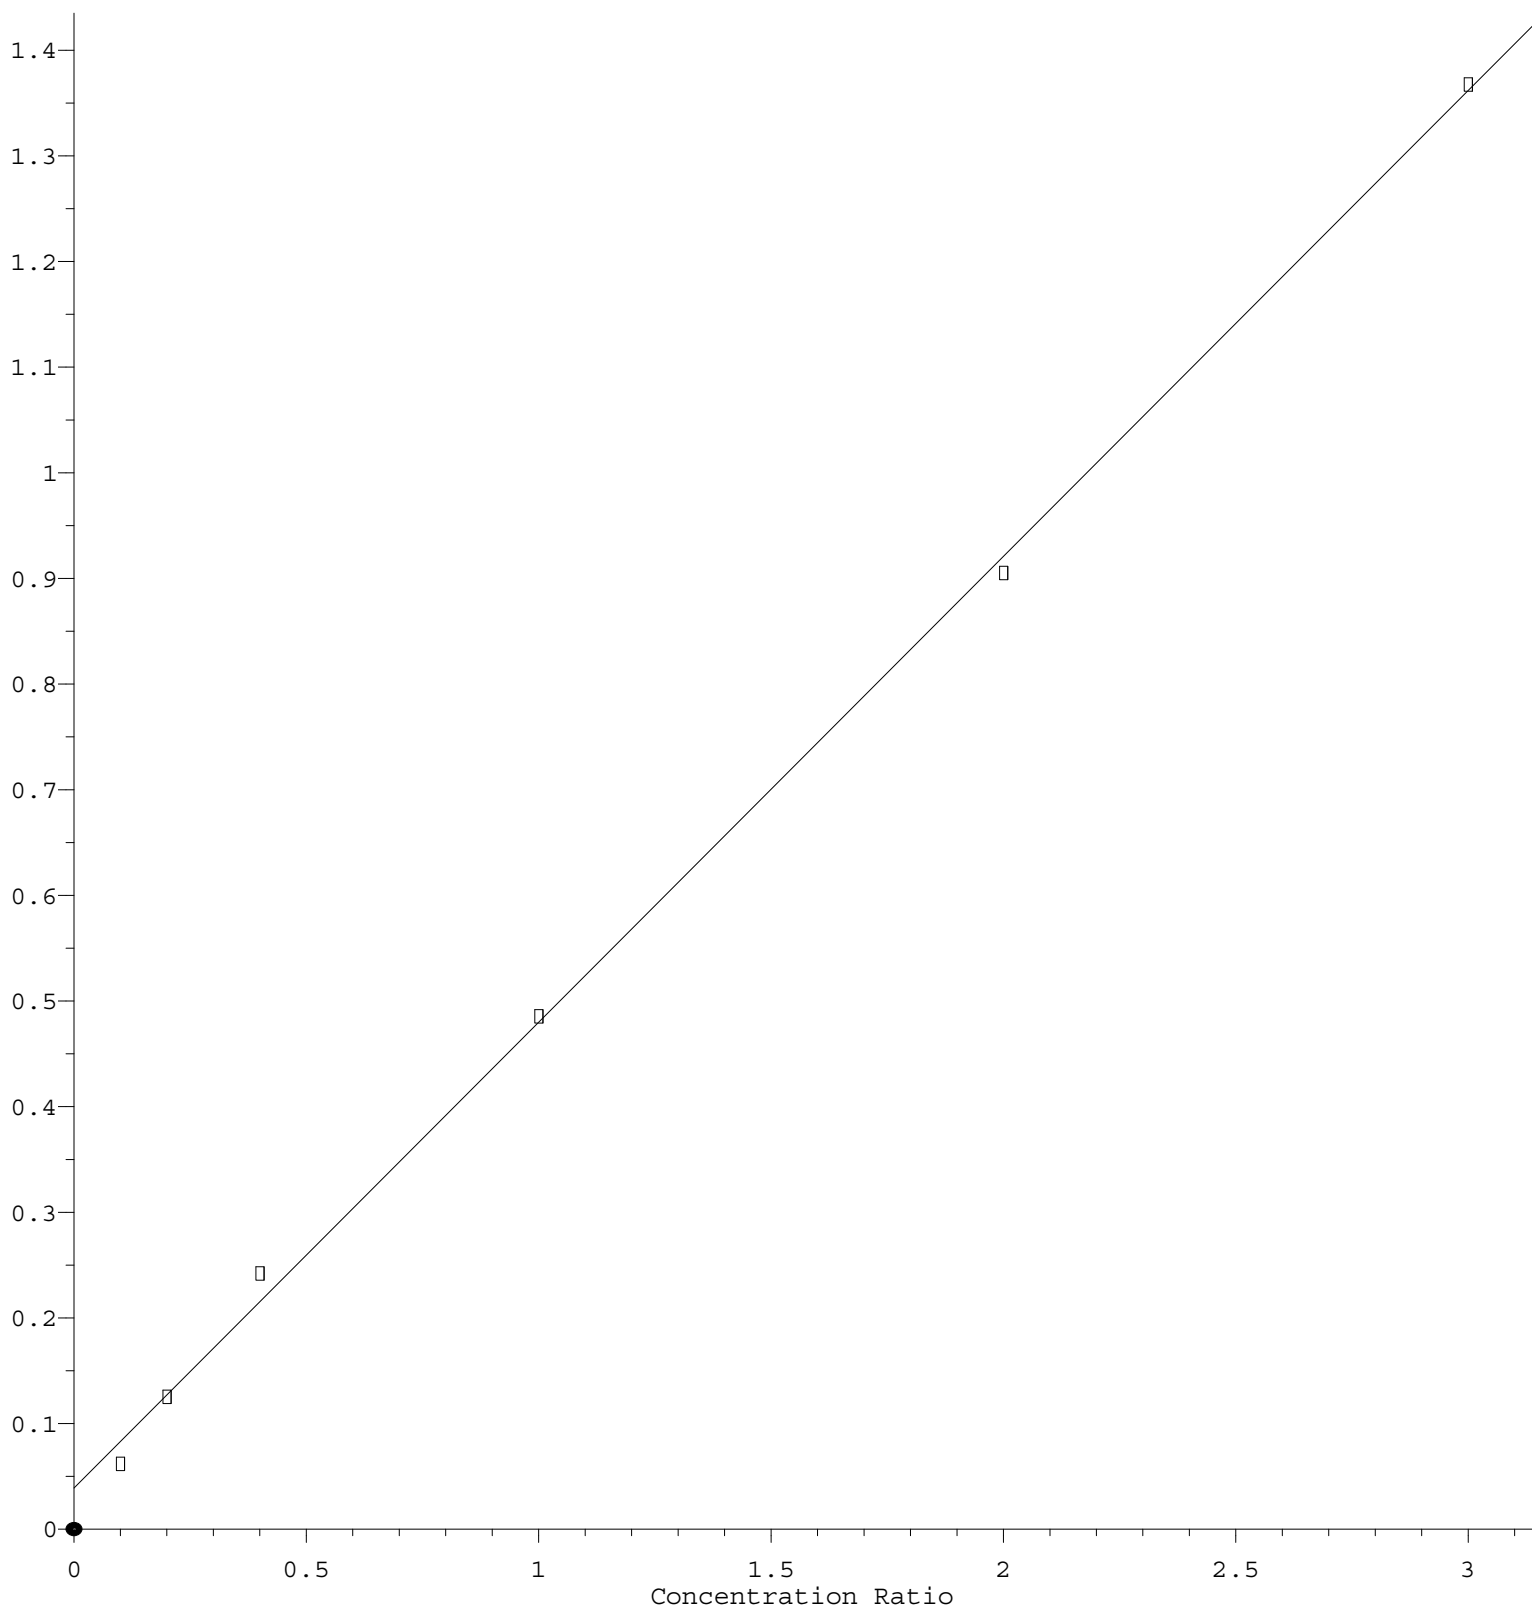

$$\text{Response} = 4.410\text{e-}001 * \text{Amt} + 3.877\text{e-}002$$


Coef of Det (r^2) = 0.998872 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y030821S.M

Calibration Table Last Updated: Mon Mar 08 12:28:55 2021

Methylene Chloride

Response Ratio

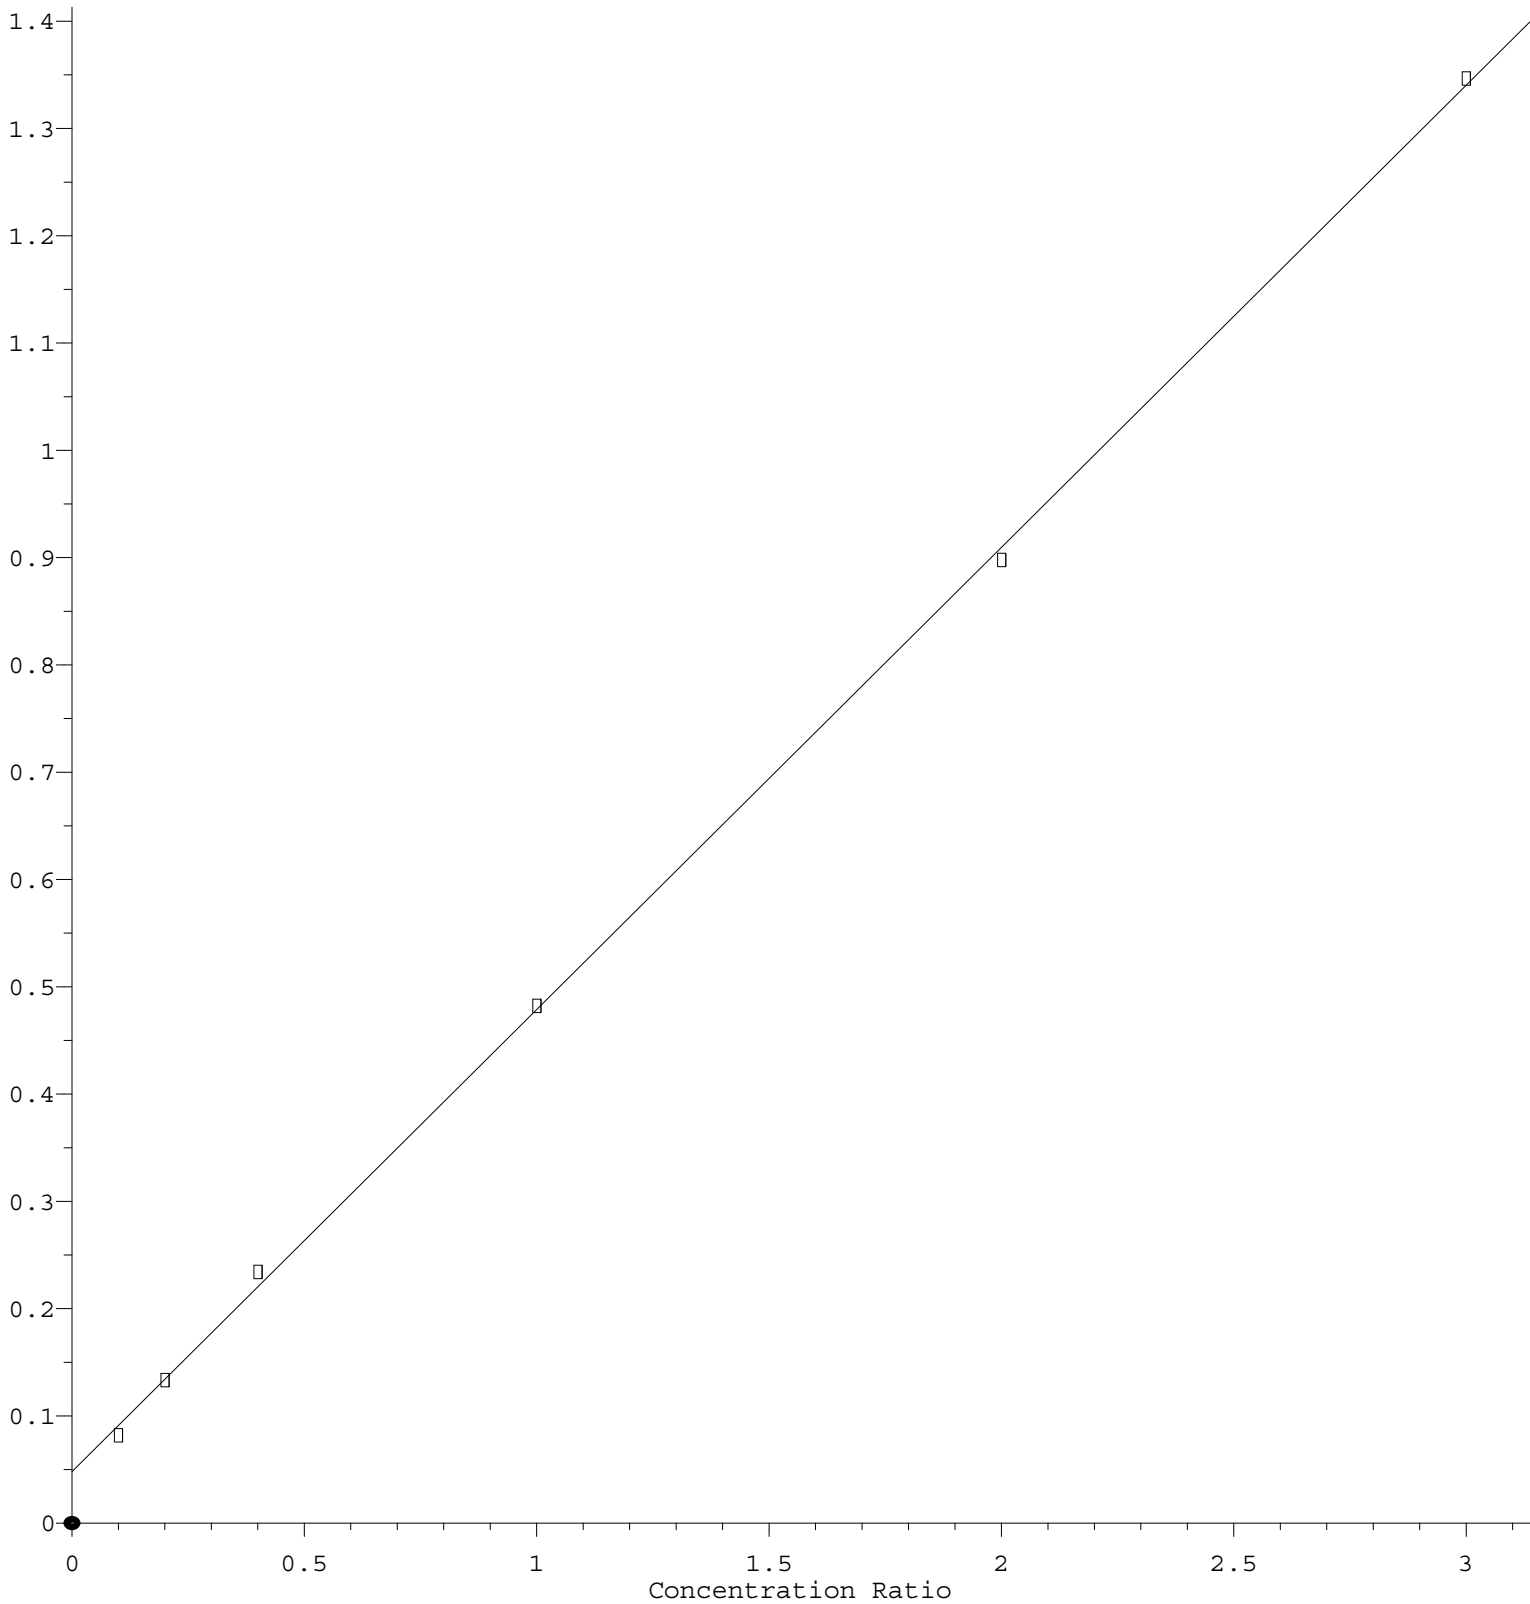

$$\text{Response} = 4.309\text{e-}001 * \text{Amt} + 4.811\text{e-}002$$


Coef of Det (r^2) = 0.999627 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y030821S.M

Calibration Table Last Updated: Mon Mar 08 12:28:55 2021

2-Chloroethyl Vinyl ether

Response Ratio

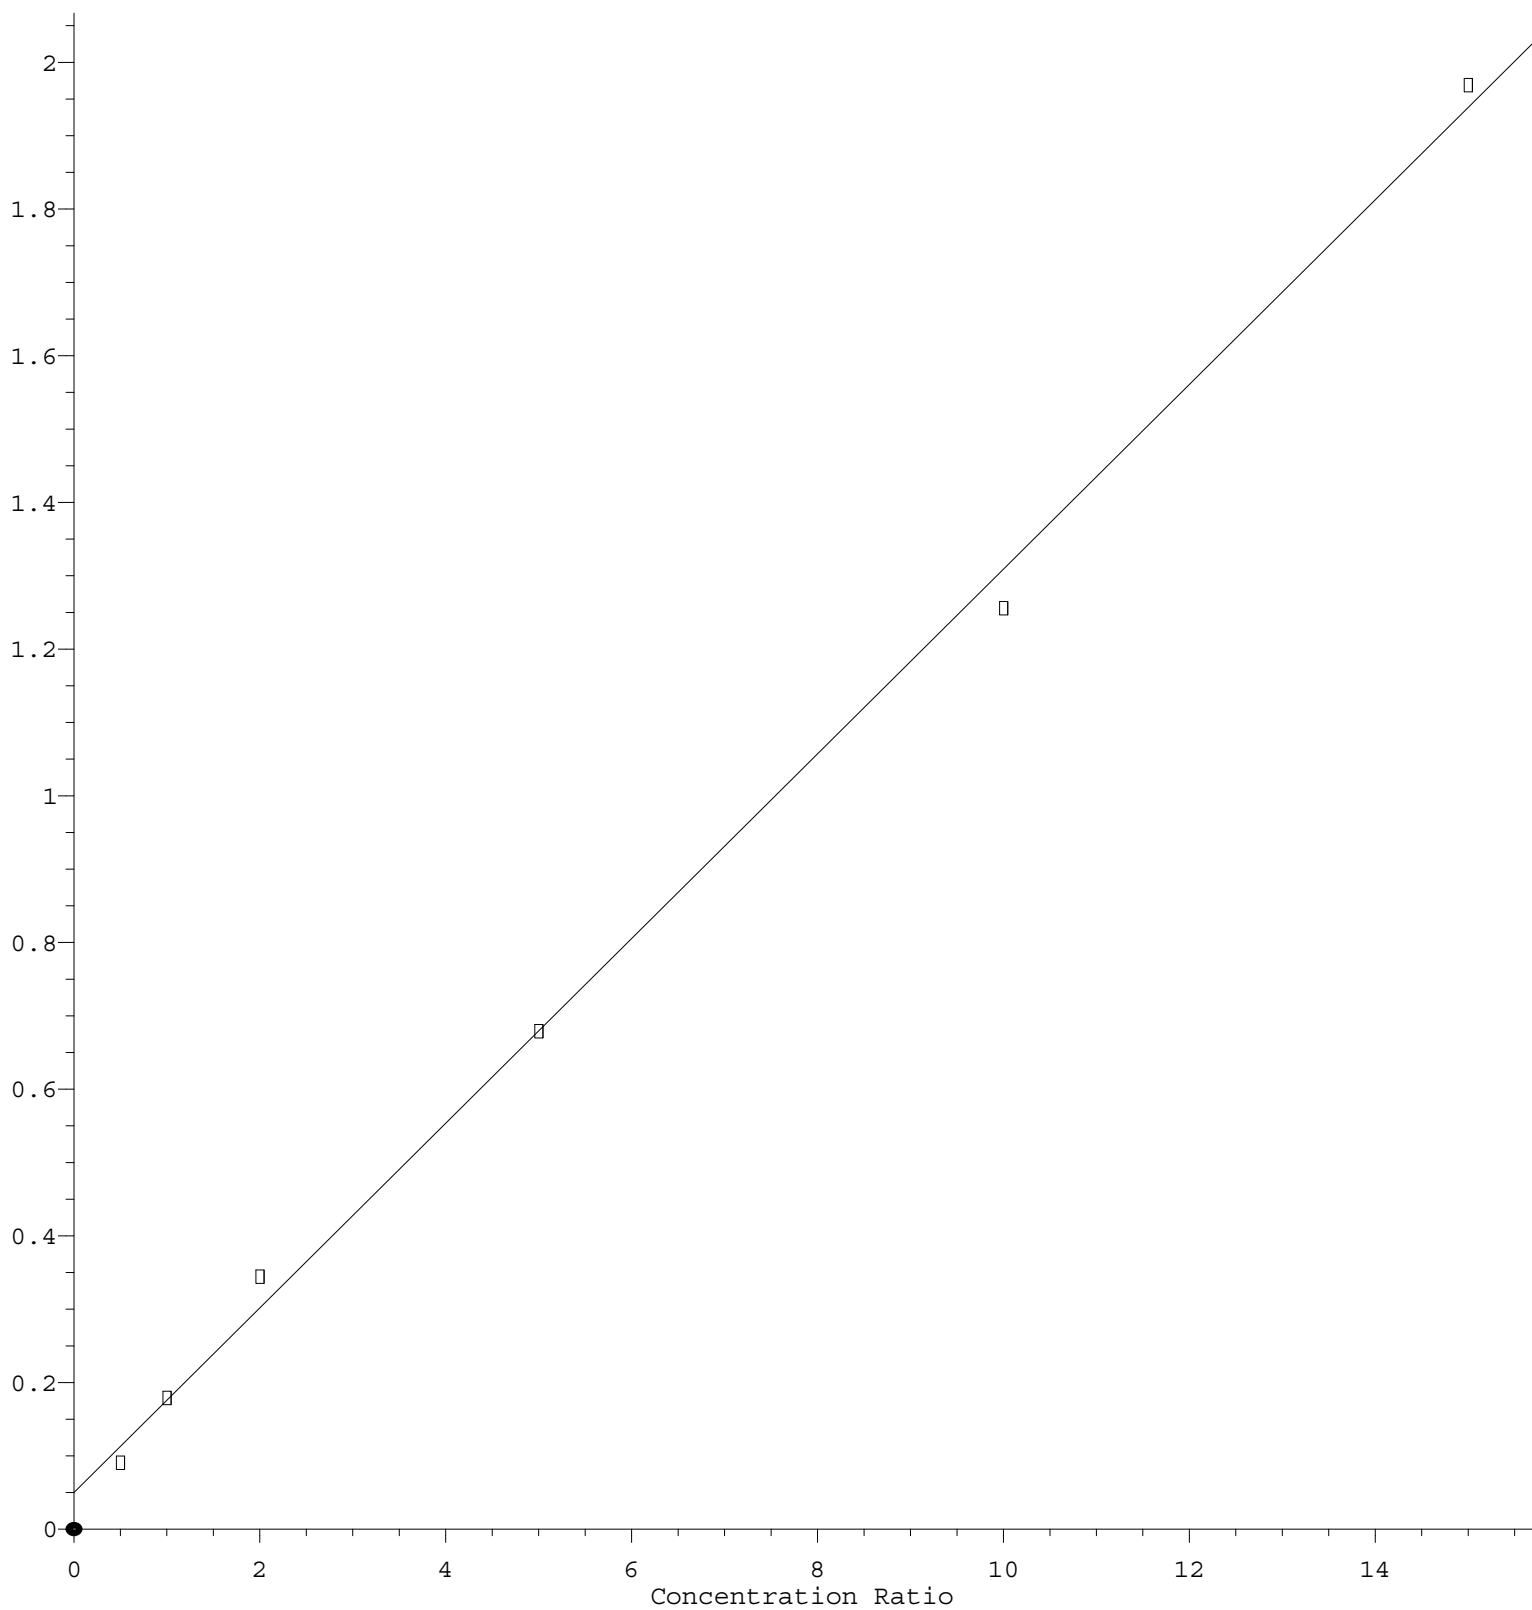

$$\text{Response} = 1.259\text{e-}001 * \text{Amt} + 4.992\text{e-}002$$

Coef of Det (r^2) = 0.997721 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y030821S.M

Calibration Table Last Updated: Mon Mar 08 12:28:55 2021