
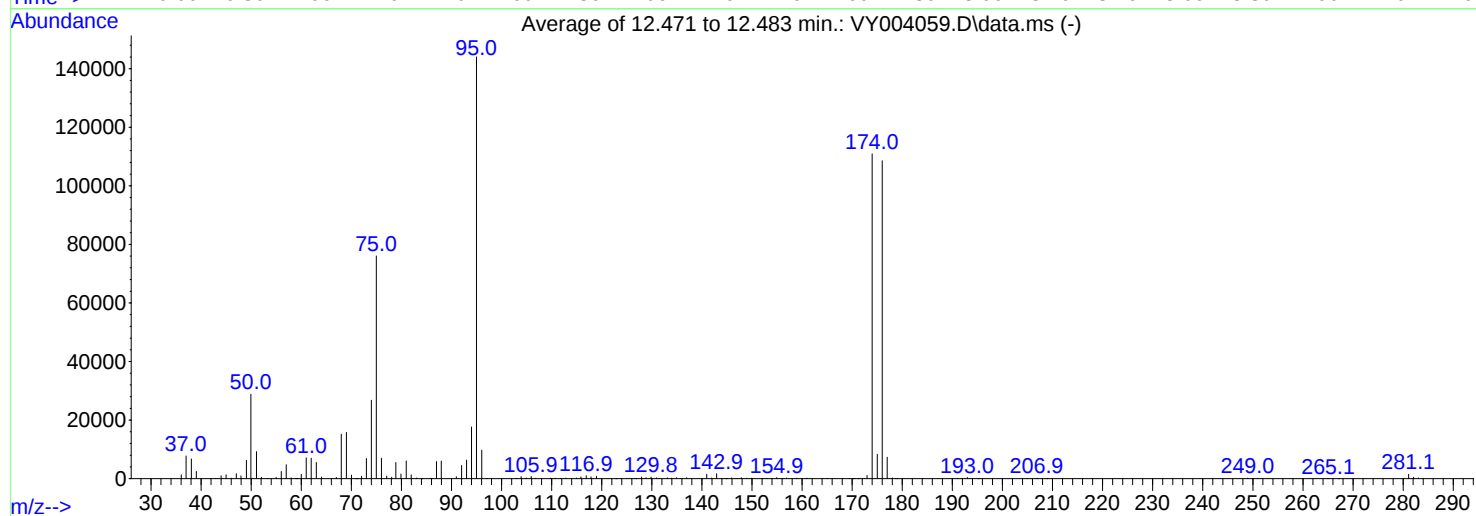


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030821\
 Data File : VY004059.D
 Acq On : 08 Mar 2021 09:12
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030821S.M
 Title : SW846 8260
 Last Update : Mon Mar 08 12:28:55 2021

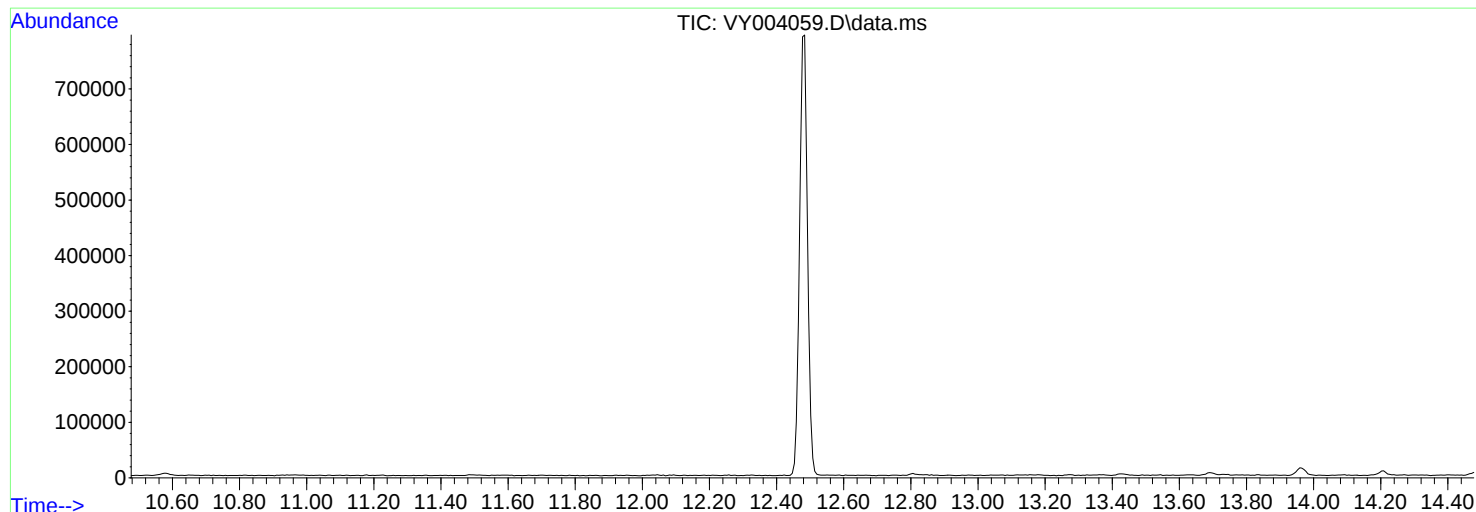

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	28868	PASS
75	95	30	60	52.8	76088	PASS
95	95	100	100	100.0	144051	PASS
96	95	5	9	6.7	9723	PASS
173	174	0.00	2	1.0	1075	PASS
174	95	50	100	77.0	110933	PASS
175	174	5	9	7.5	8313	PASS
176	174	95	101	97.9	108592	PASS
177	176	5	9	6.7	7315	PASS