
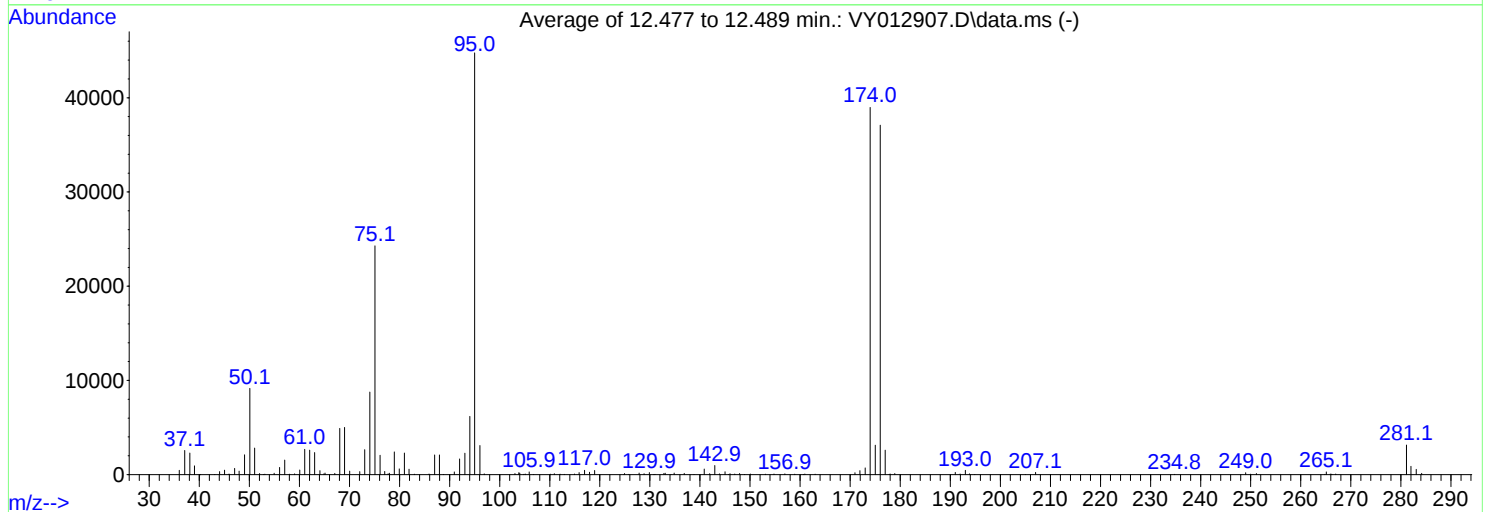


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY031023\
Data File : VY012907.D
Acq On : 10 Mar 2023 09:13
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030223S.M
Title : SW846 8260
Last Update : Fri Mar 03 01:13:13 2023

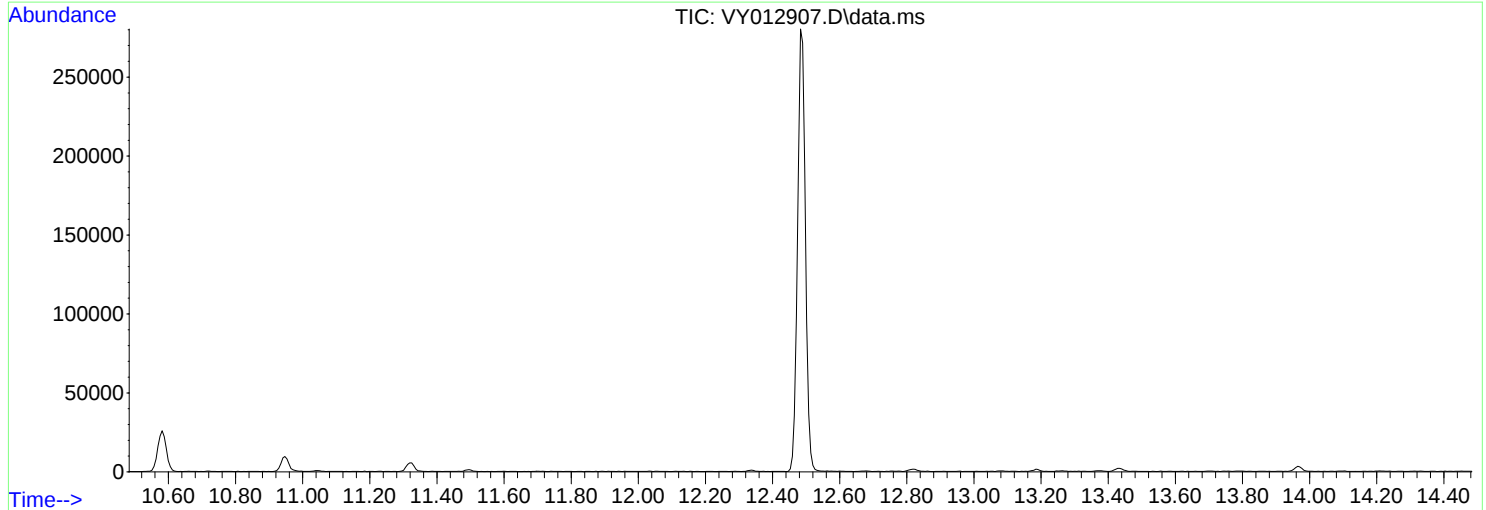

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	9150	PASS
75	95	30	60	54.2	24285	PASS
95	95	100	100	100.0	44768	PASS
96	95	5	9	6.9	3098	PASS
173	174	0.00	2	1.8	709	PASS
174	95	50	100	87.1	38976	PASS
175	174	5	9	8.0	3132	PASS
176	174	95	101	95.2	37096	PASS
177	176	5	9	7.0	2602	PASS