

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY031121\
 Data File : VY004069.D
 Acq On : 11 Mar 2021 11:43
 Operator : SY/MD
 Sample : VY0311SBL03
 Misc : 5.00g/5mL/MSVOA_Y/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0311SBL03

Quant Time: Mar 12 01:16:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030821S.M
 Quant Title : SW846 8260
 QLast Update : Mon Mar 08 12:28:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.801	168	229307	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	399667	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.495	117	372803	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	184789	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.148	65	131122	57.94	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	115.88%
35) Dibromofluoromethane	7.728	113	123854	54.95	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	109.90%
50) Toluene-d8	10.185	98	476788	53.96	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	107.92%
62) 4-Bromofluorobenzene	12.483	95	176463	54.08	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	108.16%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY031121\
Data File : VY004069.D
Acq On : 11 Mar 2021 11:43
Operator : SY/MD
Sample : VY0311SBL03
Misc : 5.00g/5mL/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0311SBL03

Quant Time: Mar 12 01:16:53 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030821S.M
Quant Title : SW846 8260
QLast Update : Mon Mar 08 12:28:55 2021
Response via : Initial Calibration




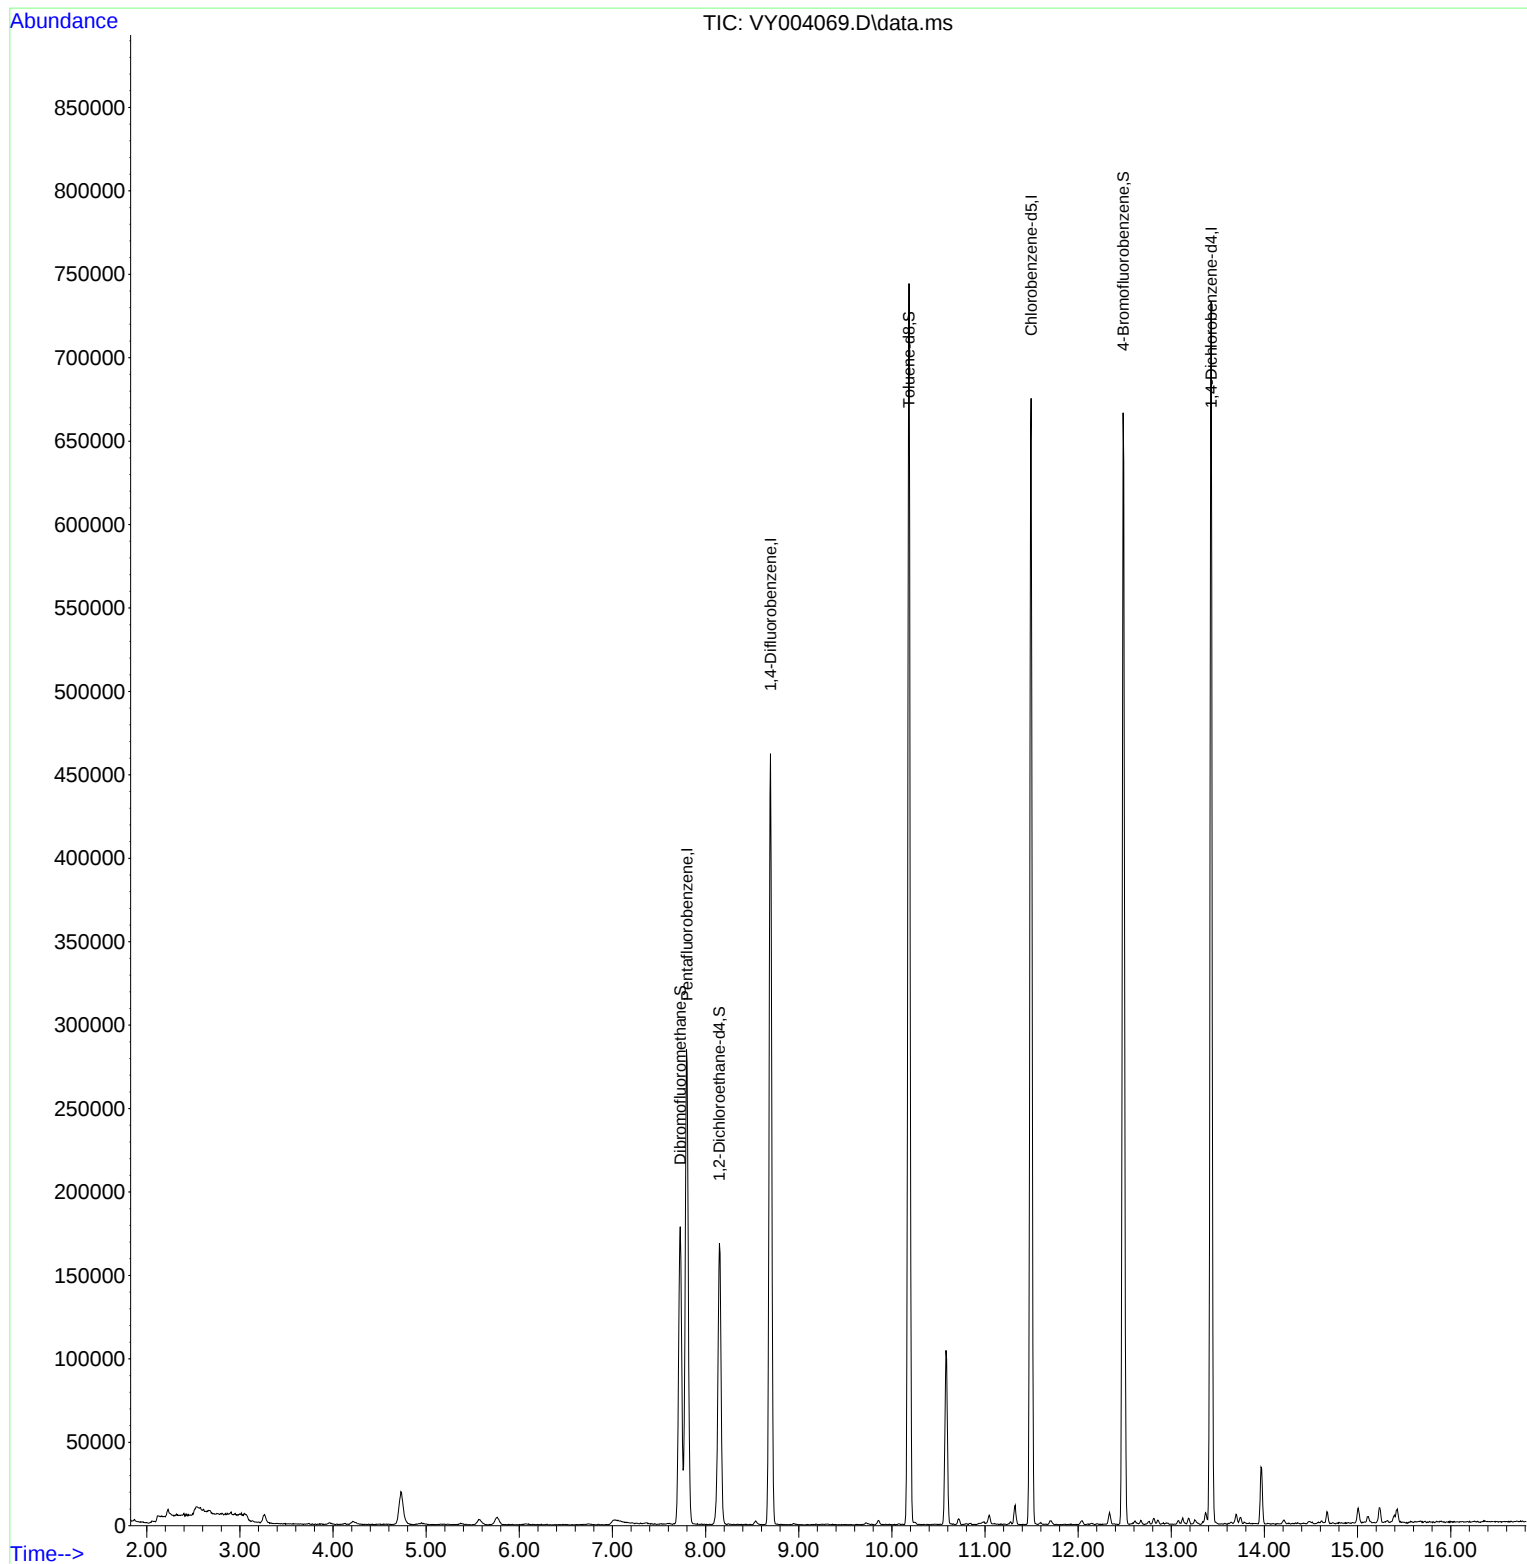


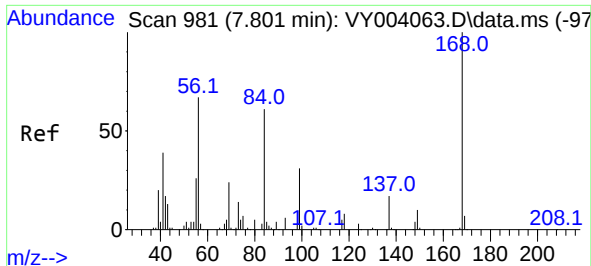

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.801 min Scan# 981
Delta R.T. -0.000 min
Lab File: VY004069.D
Acq: 11 Mar 2021 11:43




Instrument :
MSVOA_Y
ClientSampleId :
VY0311SBL03


Tgt Ion:168 Resp: 229307
Ion Ratio Lower Upper
168 100
99 51.4 41.2 61.8

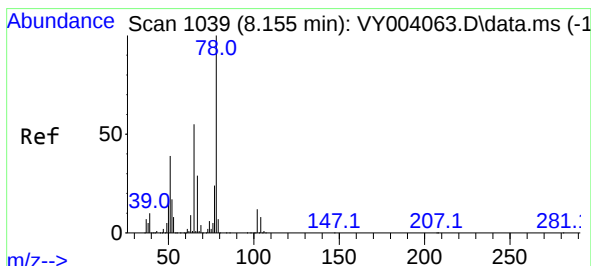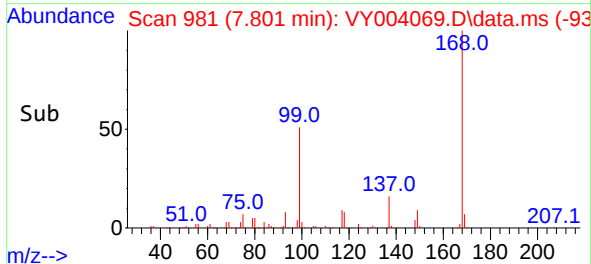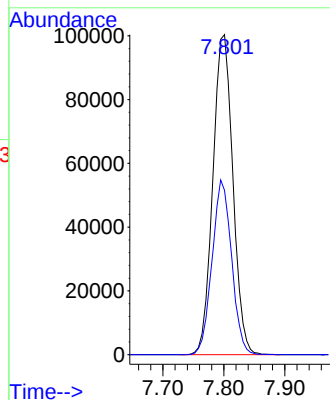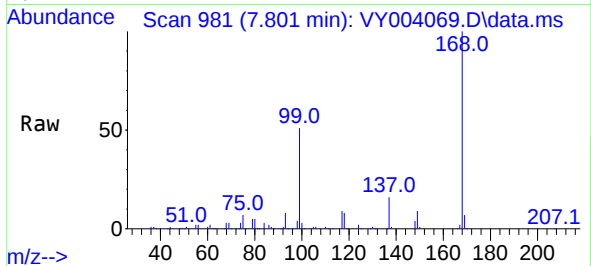

#33
1,2-Dichloroethane-d4
Concen: 57.94 ug/l
RT: 8.148 min Scan# 1038
Delta R.T. -0.007 min
Lab File: VY004069.D
Acq: 11 Mar 2021 11:43

Tgt Ion: 65 Resp: 131122
Ion Ratio Lower Upper
65 100
67 52.1 0.0 101.4


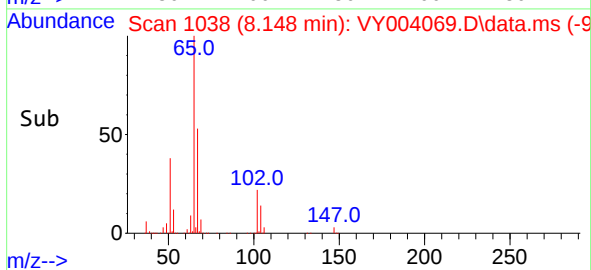
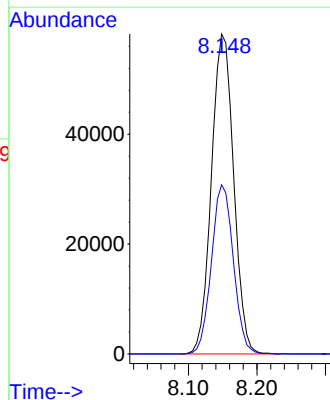
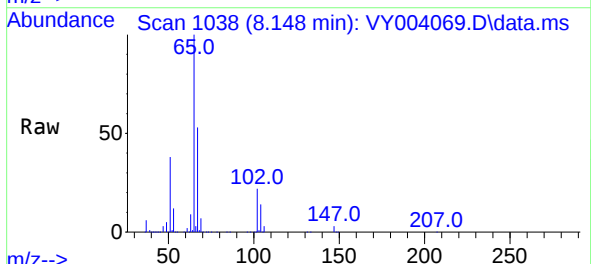


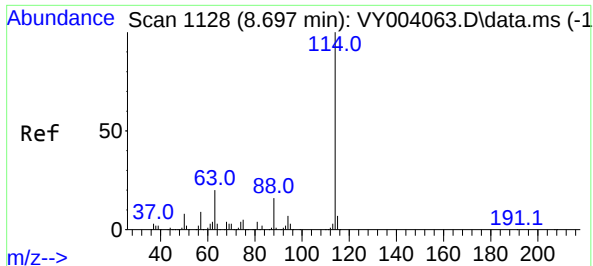

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. 0.000 min
Lab File: VY004069.D
Acq: 11 Mar 2021 11:43




Instrument :
MSVOA_Y
ClientSampleId :
VY0311SBL03


Tgt Ion:	114	Resp:	399667
Ion	Ratio	Lower	Upper
114	100		
63	18.9	0.0	41.6
88	16.0	0.0	31.4

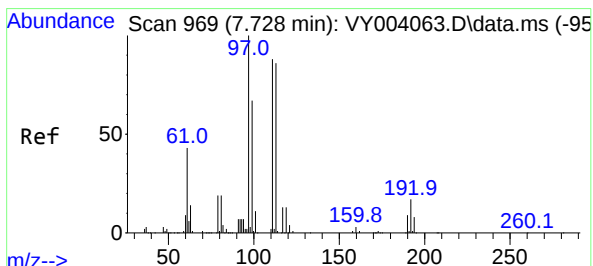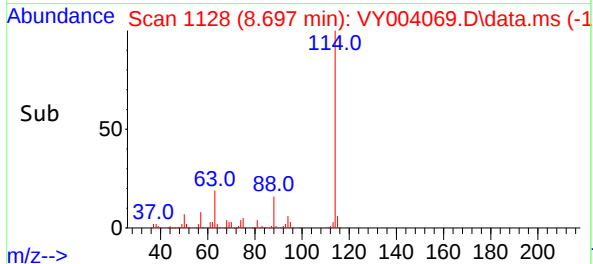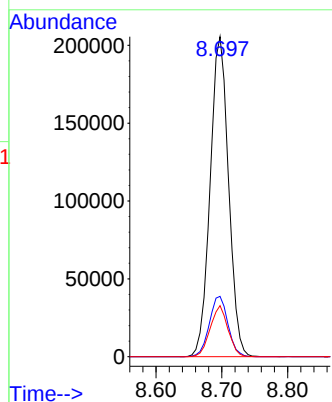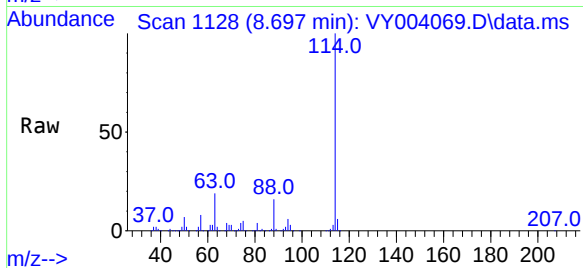

#35
Dibromofluoromethane
Concen: 54.95 ug/l
RT: 7.728 min Scan# 969
Delta R.T. -0.000 min
Lab File: VY004069.D
Acq: 11 Mar 2021 11:43

Tgt Ion:	113	Resp:	123854
Ion	Ratio	Lower	Upper
113	100		
111	102.6	83.2	124.8
192	20.4	18.5	27.7


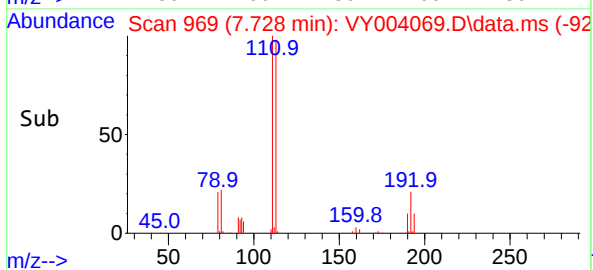
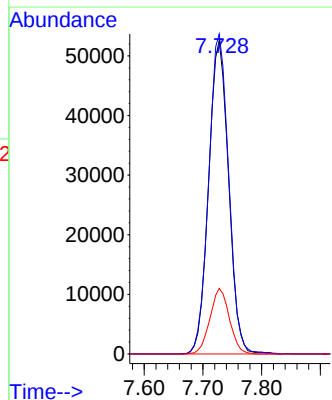
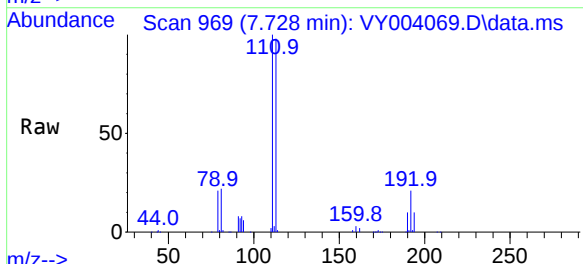


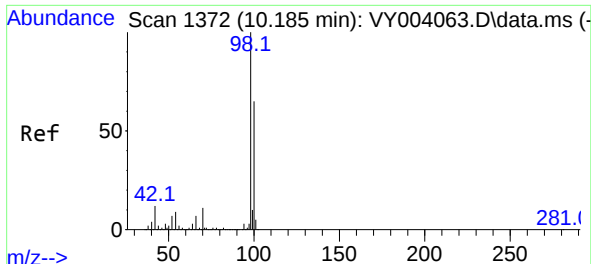

#50
Toluene-d8
Concen: 53.96 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. -0.000 min
Lab File: VY004069.D
Acq: 11 Mar 2021 11:43




Instrument :
MSVOA_Y
ClientSampleId :
VY0311SBL03


Tgt Ion: 98 Resp: 476788
Ion Ratio Lower Upper
98 100
100 65.2 51.8 77.6

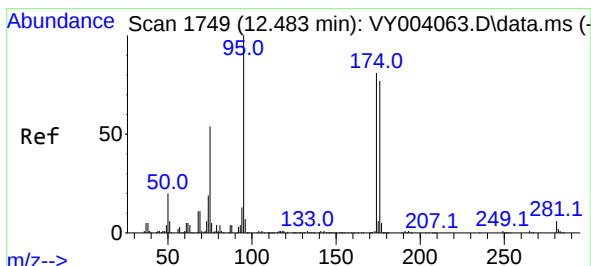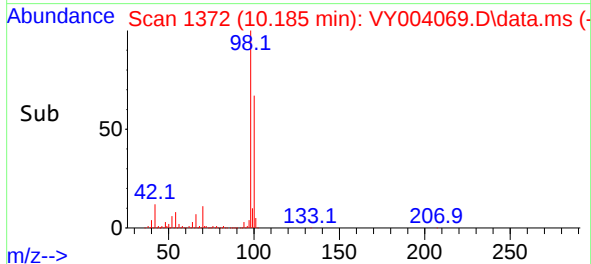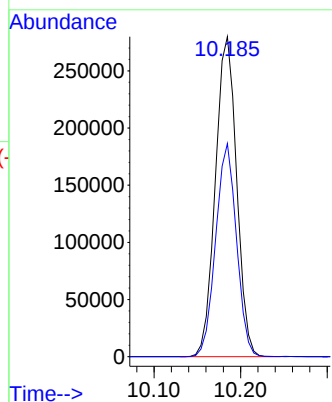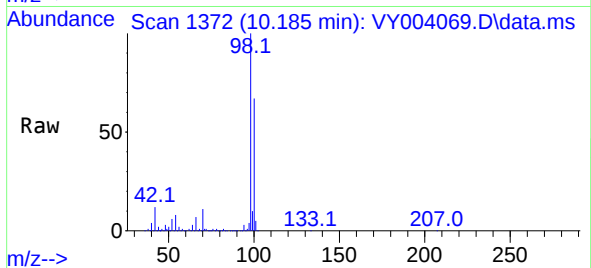

#62
4-Bromofluorobenzene
Concen: 54.08 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY004069.D
Acq: 11 Mar 2021 11:43

Tgt Ion: 95 Resp: 176463
Ion Ratio Lower Upper
95 100
174 84.3 0.0 179.0
176 81.6 0.0 174.4


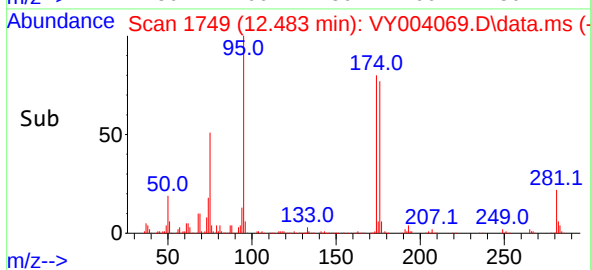
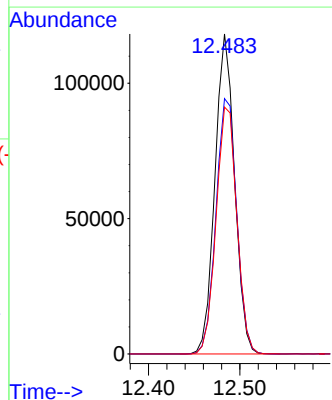
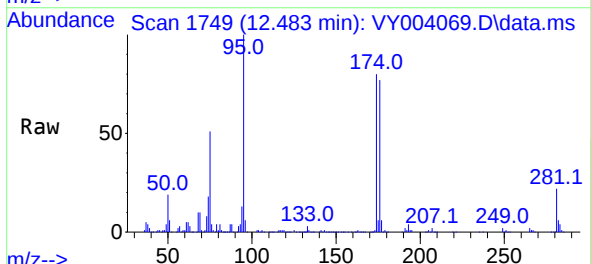


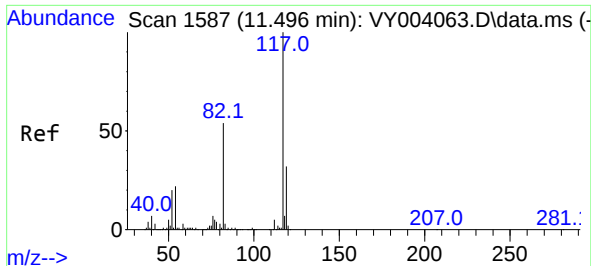

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.495 min Scan# 1587
Delta R.T. -0.001 min
Lab File: VY004069.D
Acq: 11 Mar 2021 11:43

Instrument :
MSVOA_Y
ClientSampleId :
VY0311SBL03

Tgt Ion:117 Resp: 372803
Ion Ratio Lower Upper
117 100
82 53.4 43.8 65.6
119 32.6 26.2 39.2

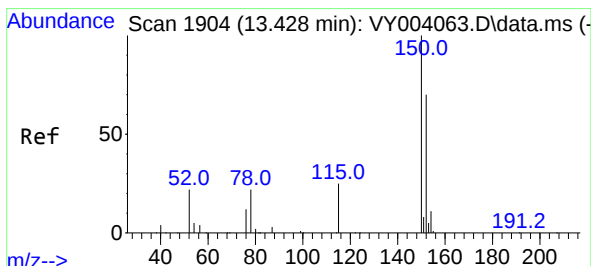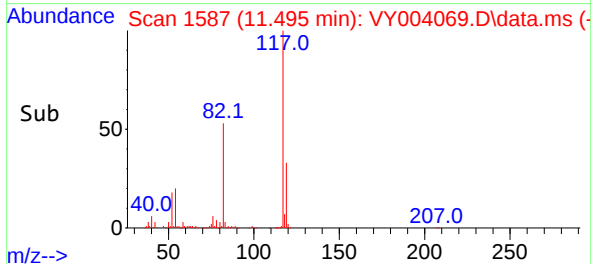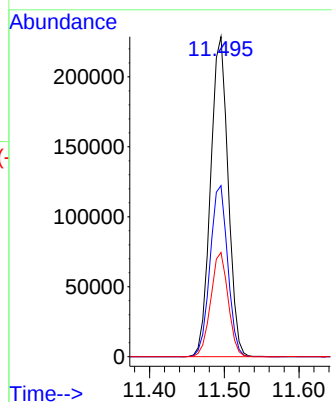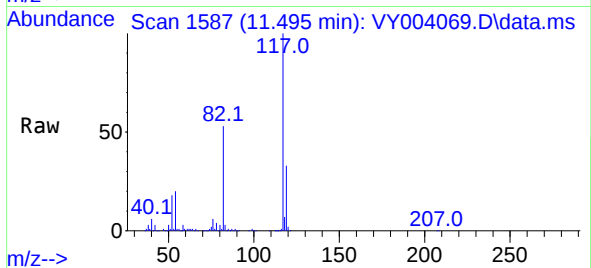

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY004069.D
Acq: 11 Mar 2021 11:43

Tgt Ion:152 Resp: 184789
Ion Ratio Lower Upper
152 100
115 58.0 28.2 84.6
150 157.6 0.0 347.2

