

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY031121\
 Data File : VY004077.D
 Acq On : 11 Mar 2021 15:17
 Operator : SY/MD
 Sample : M1607-01
 Misc : 4.86g/5mL/MSVOA_Y/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 NB-07-030921

Quant Time: Mar 12 01:18:41 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030821S.M
 Quant Title : SW846 8260
 QLast Update : Mon Mar 08 12:28:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.801	168	210556	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	370751	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.496	117	349833	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	173088	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.155	65	126285	60.78	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	121.56%
35) Dibromofluoromethane	7.728	113	116078	55.52	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	111.04%
50) Toluene-d8	10.185	98	445359	54.34	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	108.68%
62) 4-Bromofluorobenzene	12.483	95	163826	54.12	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	108.24%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY031121\
Data File : VY004077.D
Acq On : 11 Mar 2021 15:17
Operator : SY/MD
Sample : M1607-01
Misc : 4.86g/5mL/MSVOA_Y/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
NB-07-030921


Quant Time: Mar 12 01:18:41 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030821S.M
Quant Title : SW846 8260
QLast Update : Mon Mar 08 12:28:55 2021
Response via : Initial Calibration

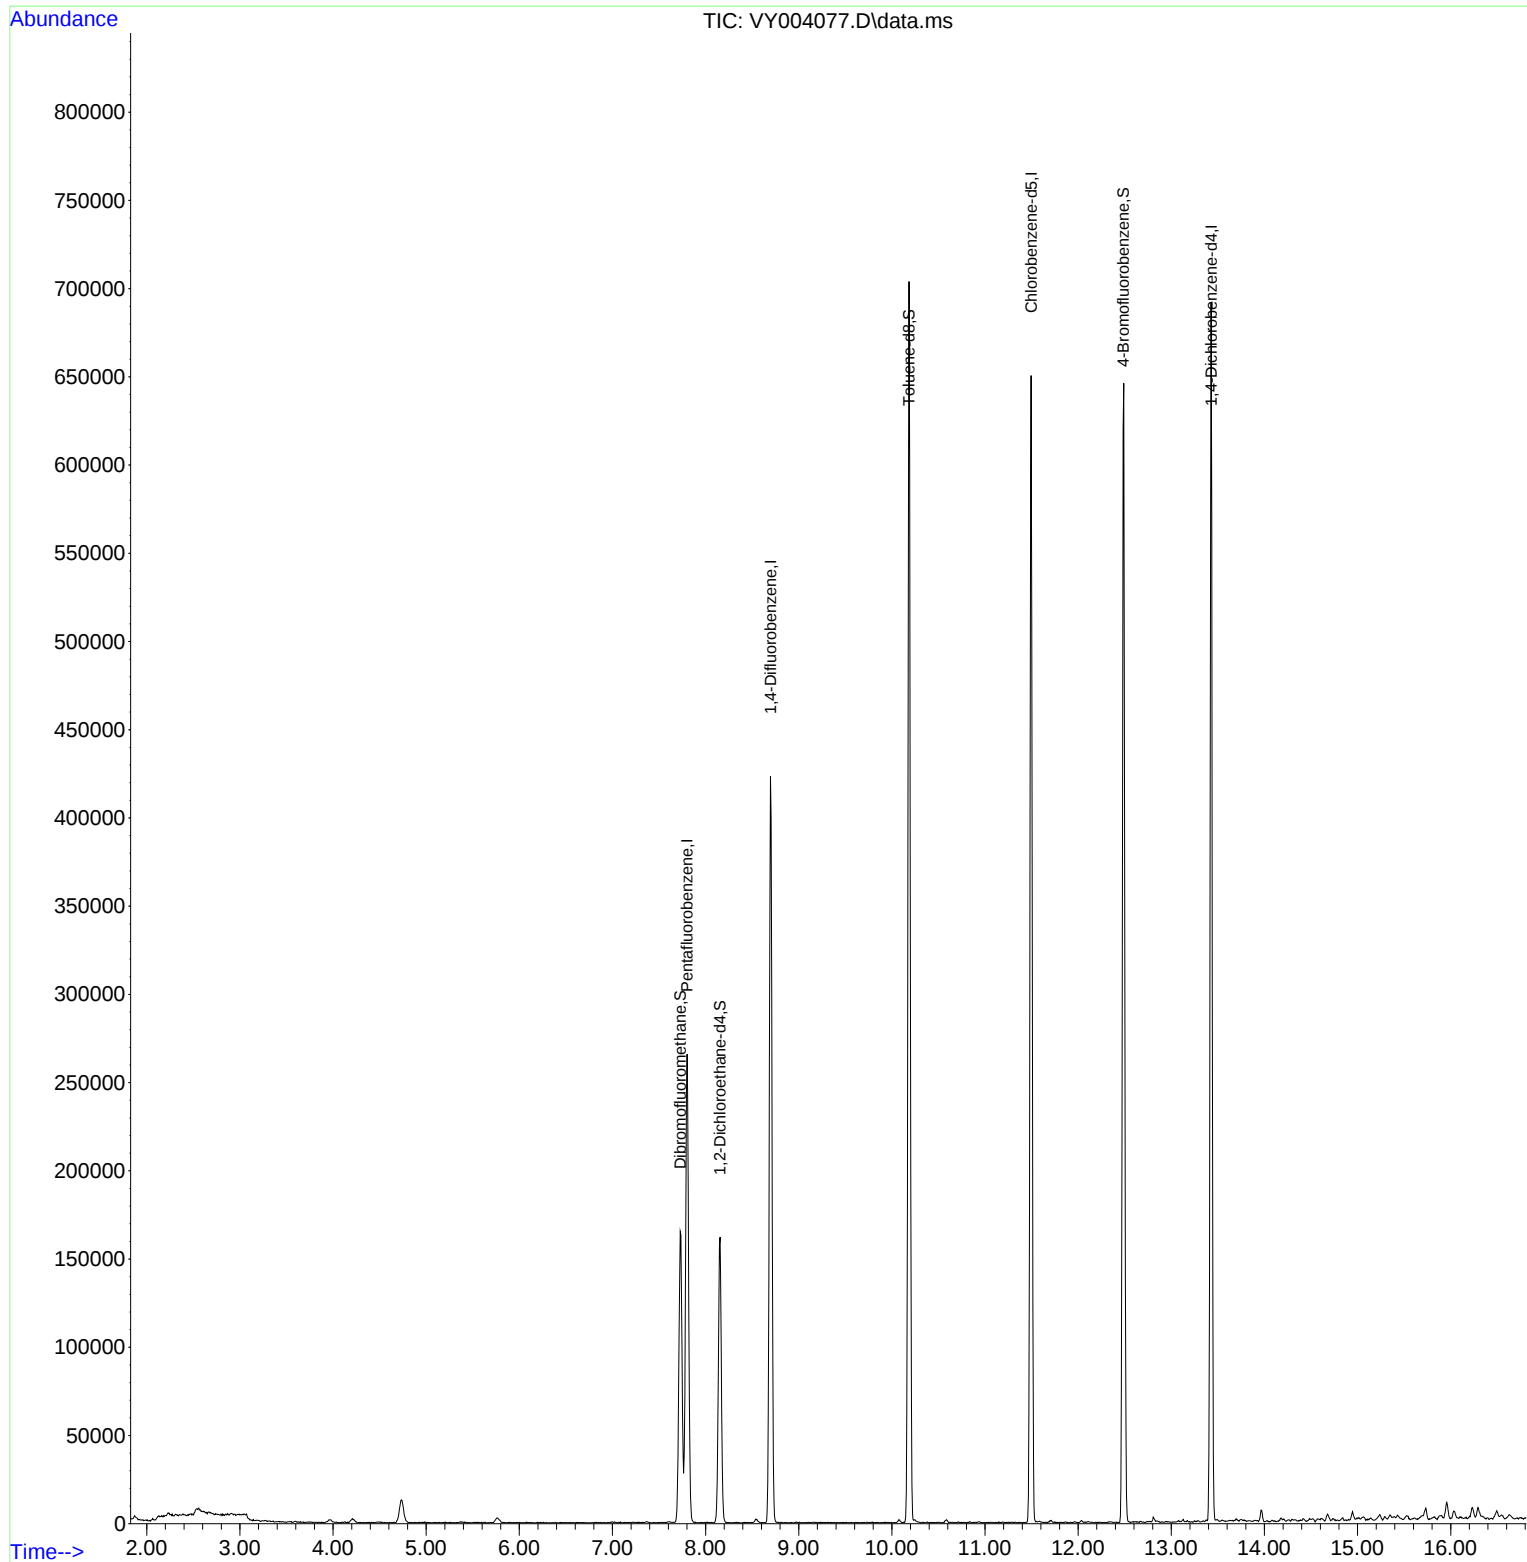



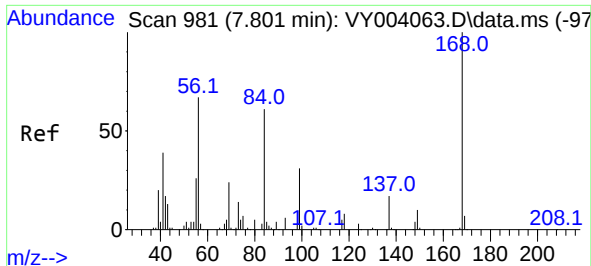


#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.801 min Scan# 981
Delta R.T. 0.000 min
Lab File: VY004077.D
Acq: 11 Mar 2021 15:17

Instrument :
MSVOA_Y
ClientSampleId :
NB-07-030921



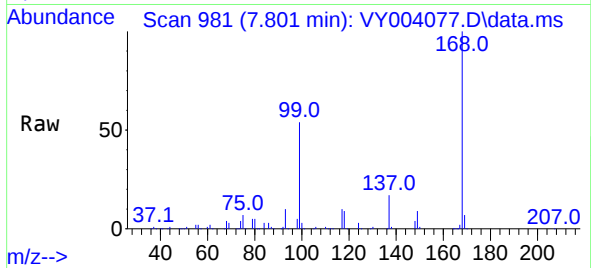



Tgt Ion:168 Resp: 210556
Ion Ratio Lower Upper
168 100
99 53.8 41.2 61.8

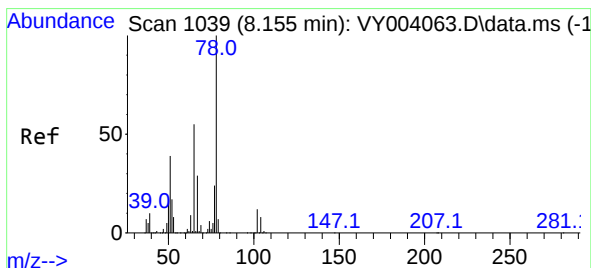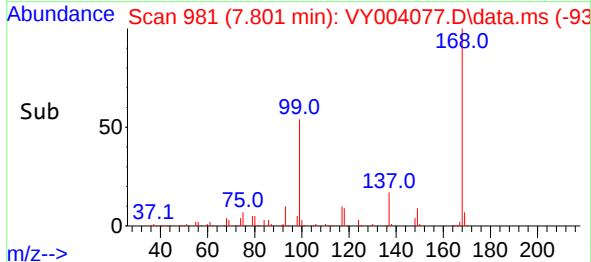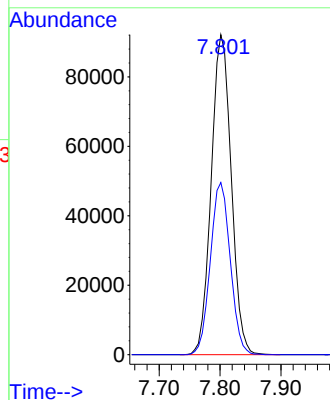

#33
1,2-Dichloroethane-d4
Concen: 60.78 ug/l
RT: 8.155 min Scan# 1039
Delta R.T. -0.000 min
Lab File: VY004077.D
Acq: 11 Mar 2021 15:17

Tgt Ion: 65 Resp: 126285
Ion Ratio Lower Upper
65 100
67 51.8 0.0 101.4


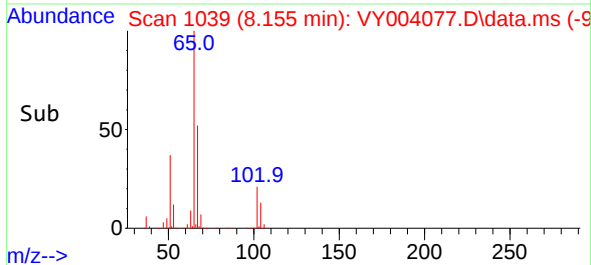
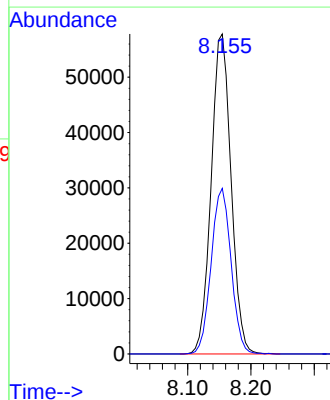
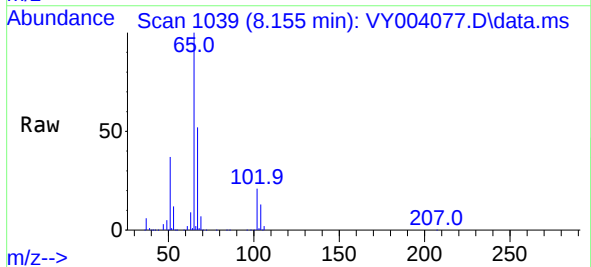


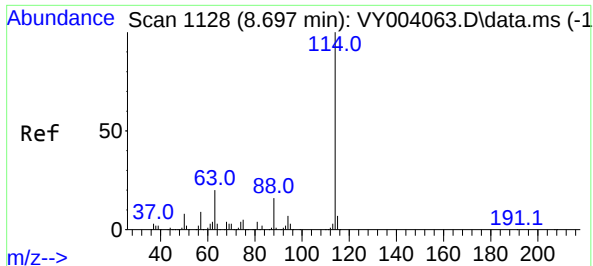

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. 0.000 min
Lab File: VY004077.D
Acq: 11 Mar 2021 15:17




Instrument :
MSVOA_Y
ClientSampleId :
NB-07-030921


Tgt Ion:	114	Resp:	370751
Ion	Ratio	Lower	Upper
114	100		
63	18.8	0.0	41.6
88	15.7	0.0	31.4

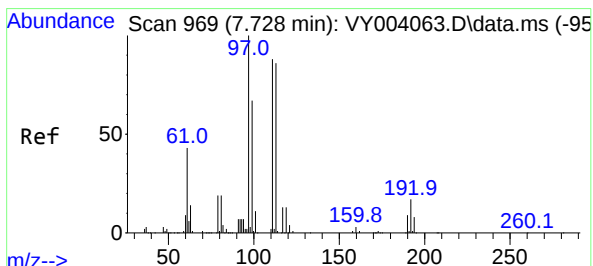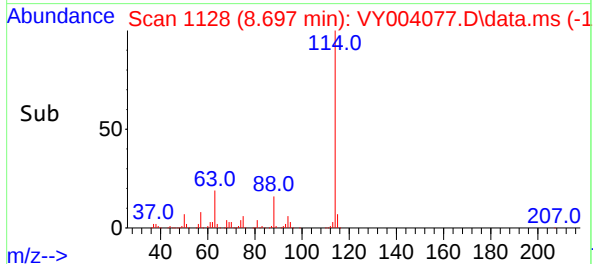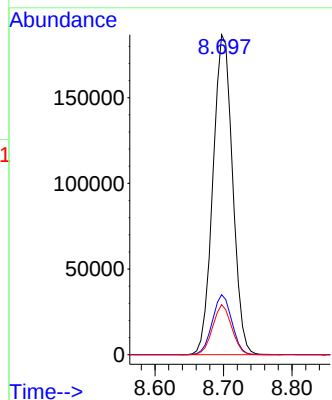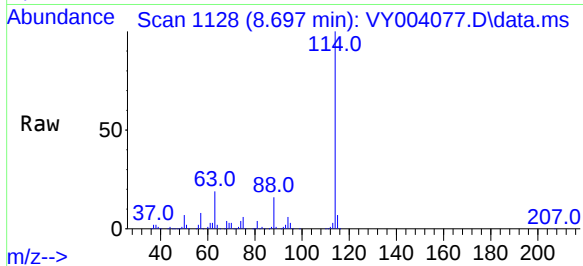

#35
Dibromofluoromethane
Concen: 55.52 ug/l
RT: 7.728 min Scan# 969
Delta R.T. -0.000 min
Lab File: VY004077.D
Acq: 11 Mar 2021 15:17

Tgt Ion:	113	Resp:	116078
Ion	Ratio	Lower	Upper
113	100		
111	102.9	83.2	124.8
192	20.2	18.5	27.7


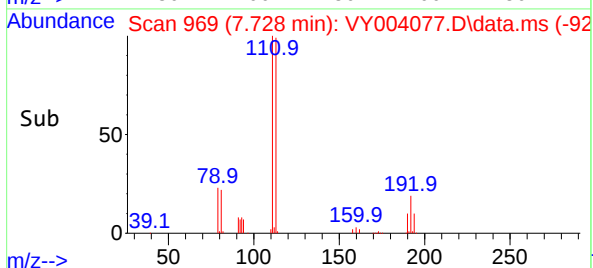
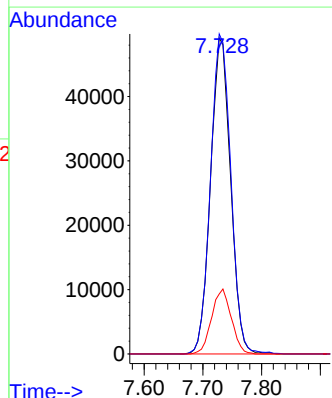
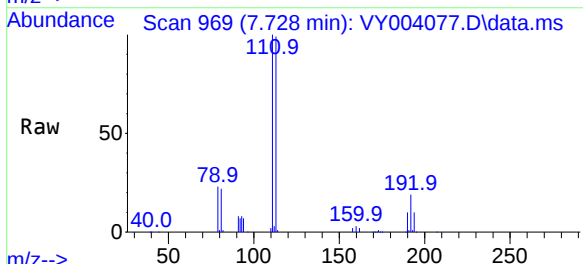


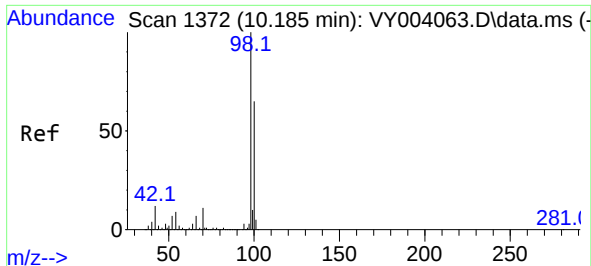

#50
Toluene-d8
Concen: 54.34 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. -0.000 min
Lab File: VY004077.D
Acq: 11 Mar 2021 15:17




Instrument :
MSVOA_Y
ClientSampleId :
NB-07-030921


Tgt Ion: 98 Resp: 445359
Ion Ratio Lower Upper
98 100
100 65.2 51.8 77.6

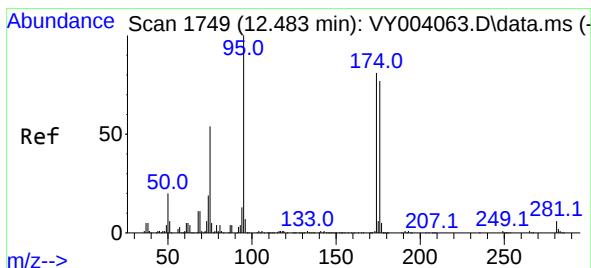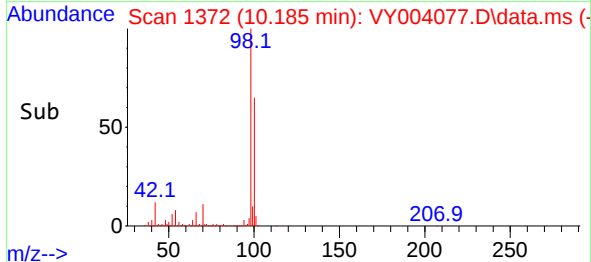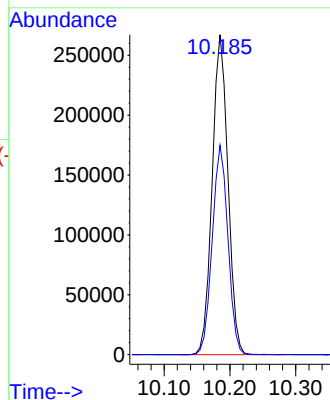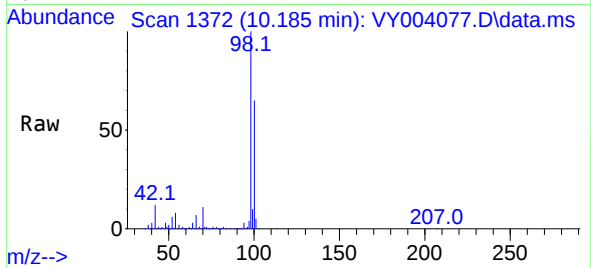

#62
4-Bromofluorobenzene
Concen: 54.12 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY004077.D
Acq: 11 Mar 2021 15:17

Tgt Ion: 95 Resp: 163826
Ion Ratio Lower Upper
95 100
174 85.5 0.0 179.0
176 83.3 0.0 174.4

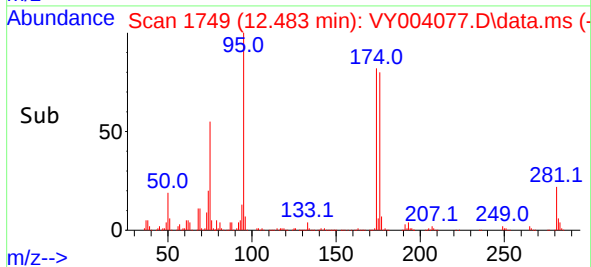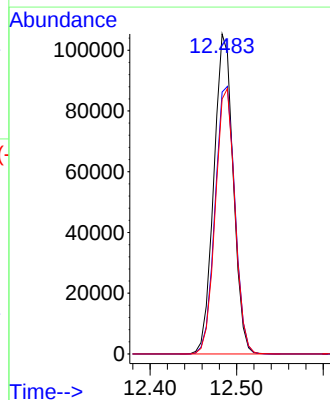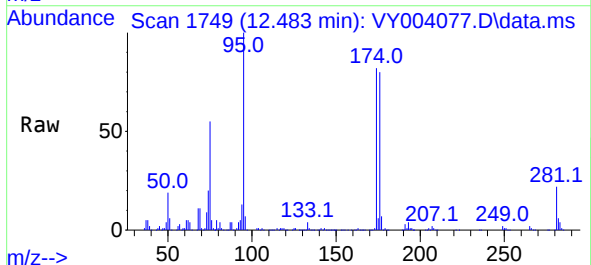




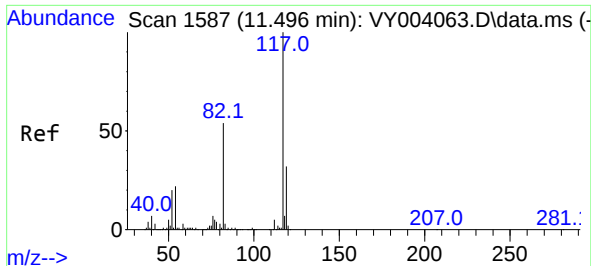


#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.496 min Scan# 1587
Delta R.T. -0.000 min
Lab File: VY004077.D
Acq: 11 Mar 2021 15:17

Instrument :
MSVOA_Y
ClientSampleId :
NB-07-030921

Tgt Ion:117 Resp: 349833

Ion	Ratio	Lower	Upper
117	100		
82	52.8	43.8	65.6
119	32.5	26.2	39.2

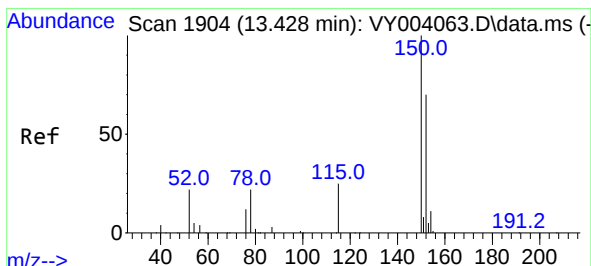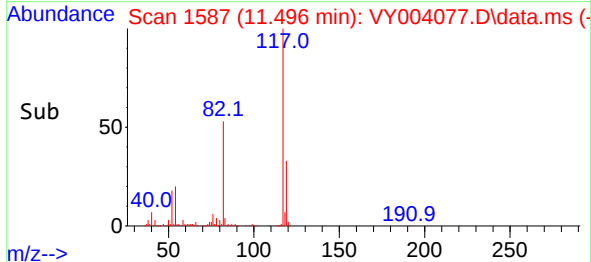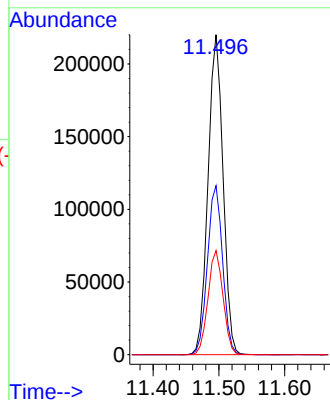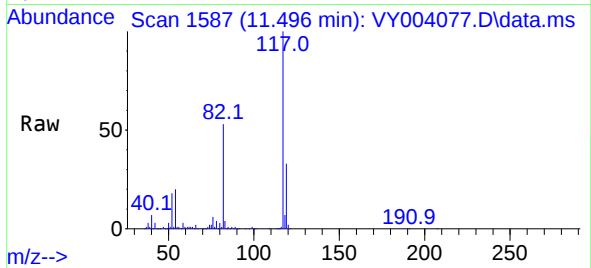

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY004077.D
Acq: 11 Mar 2021 15:17

Tgt Ion:152 Resp: 173088

Ion	Ratio	Lower	Upper
152	100		
115	58.2	28.2	84.6
150	156.2	0.0	347.2

