
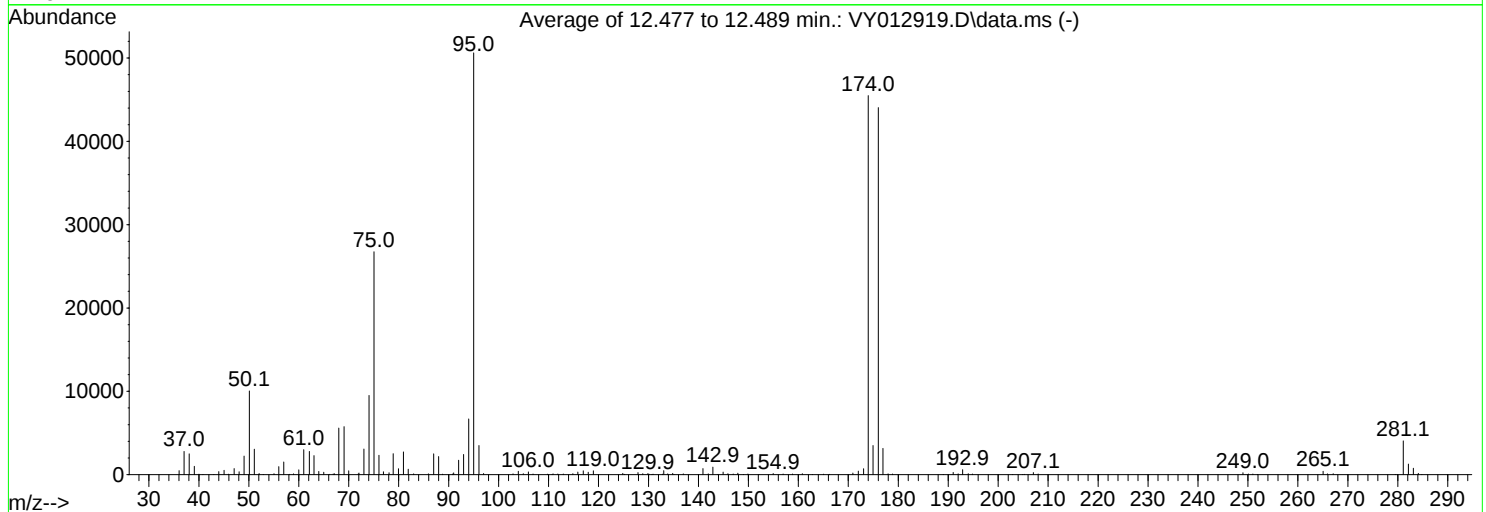


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY031323\
 Data File : VY012919.D
 Acq On : 13 Mar 2023 10:00
 Operator : KP/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030223S.M
 Title : SW846 8260
 Last Update : Fri Mar 03 01:13:13 2023

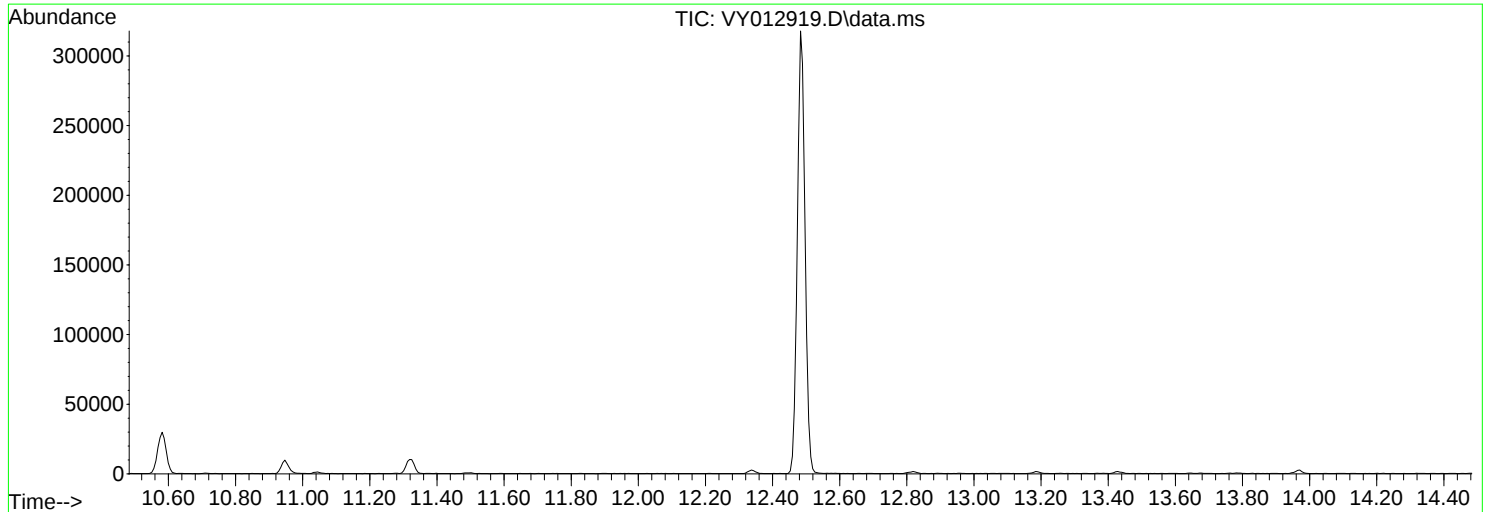

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	10037	PASS
75	95	30	60	52.9	26755	PASS
95	95	100	100	100.0	50624	PASS
96	95	5	9	6.9	3503	PASS
173	174	0.00	2	1.6	708	PASS
174	95	50	100	89.9	45488	PASS
175	174	5	9	7.7	3500	PASS
176	174	95	101	96.9	44059	PASS
177	176	5	9	7.2	3159	PASS