

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY031423\
 Data File : VY012941.D
 Acq On : 14 Mar 2023 14:36
 Operator : KP/MD
 Sample : 01905-10
 Misc : 5.35g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 MAPLE-3

Quant Time: Mar 15 01:43:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030223S.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 03 01:13:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	3006	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	4268	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.495	117	3775	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	1144	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	2023	67.782	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	135.560%
35) Dibromofluoromethane	7.716	113	1574	61.109	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	122.220%
50) Toluene-d8	10.185	98	5065	53.789	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	107.580%
62) 4-Bromofluorobenzene	12.483	95	1302	40.966	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	81.940%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY031423\
Data File : VY012941.D
Acq On : 14 Mar 2023 14:36
Operator : KP/MD
Sample : 01905-10
Misc : 5.35g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
MAPLE-3

Quant Time: Mar 15 01:43:04 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030223S.M
Quant Title : SW846 8260
QLast Update : Fri Mar 03 01:13:13 2023
Response via : Initial Calibration




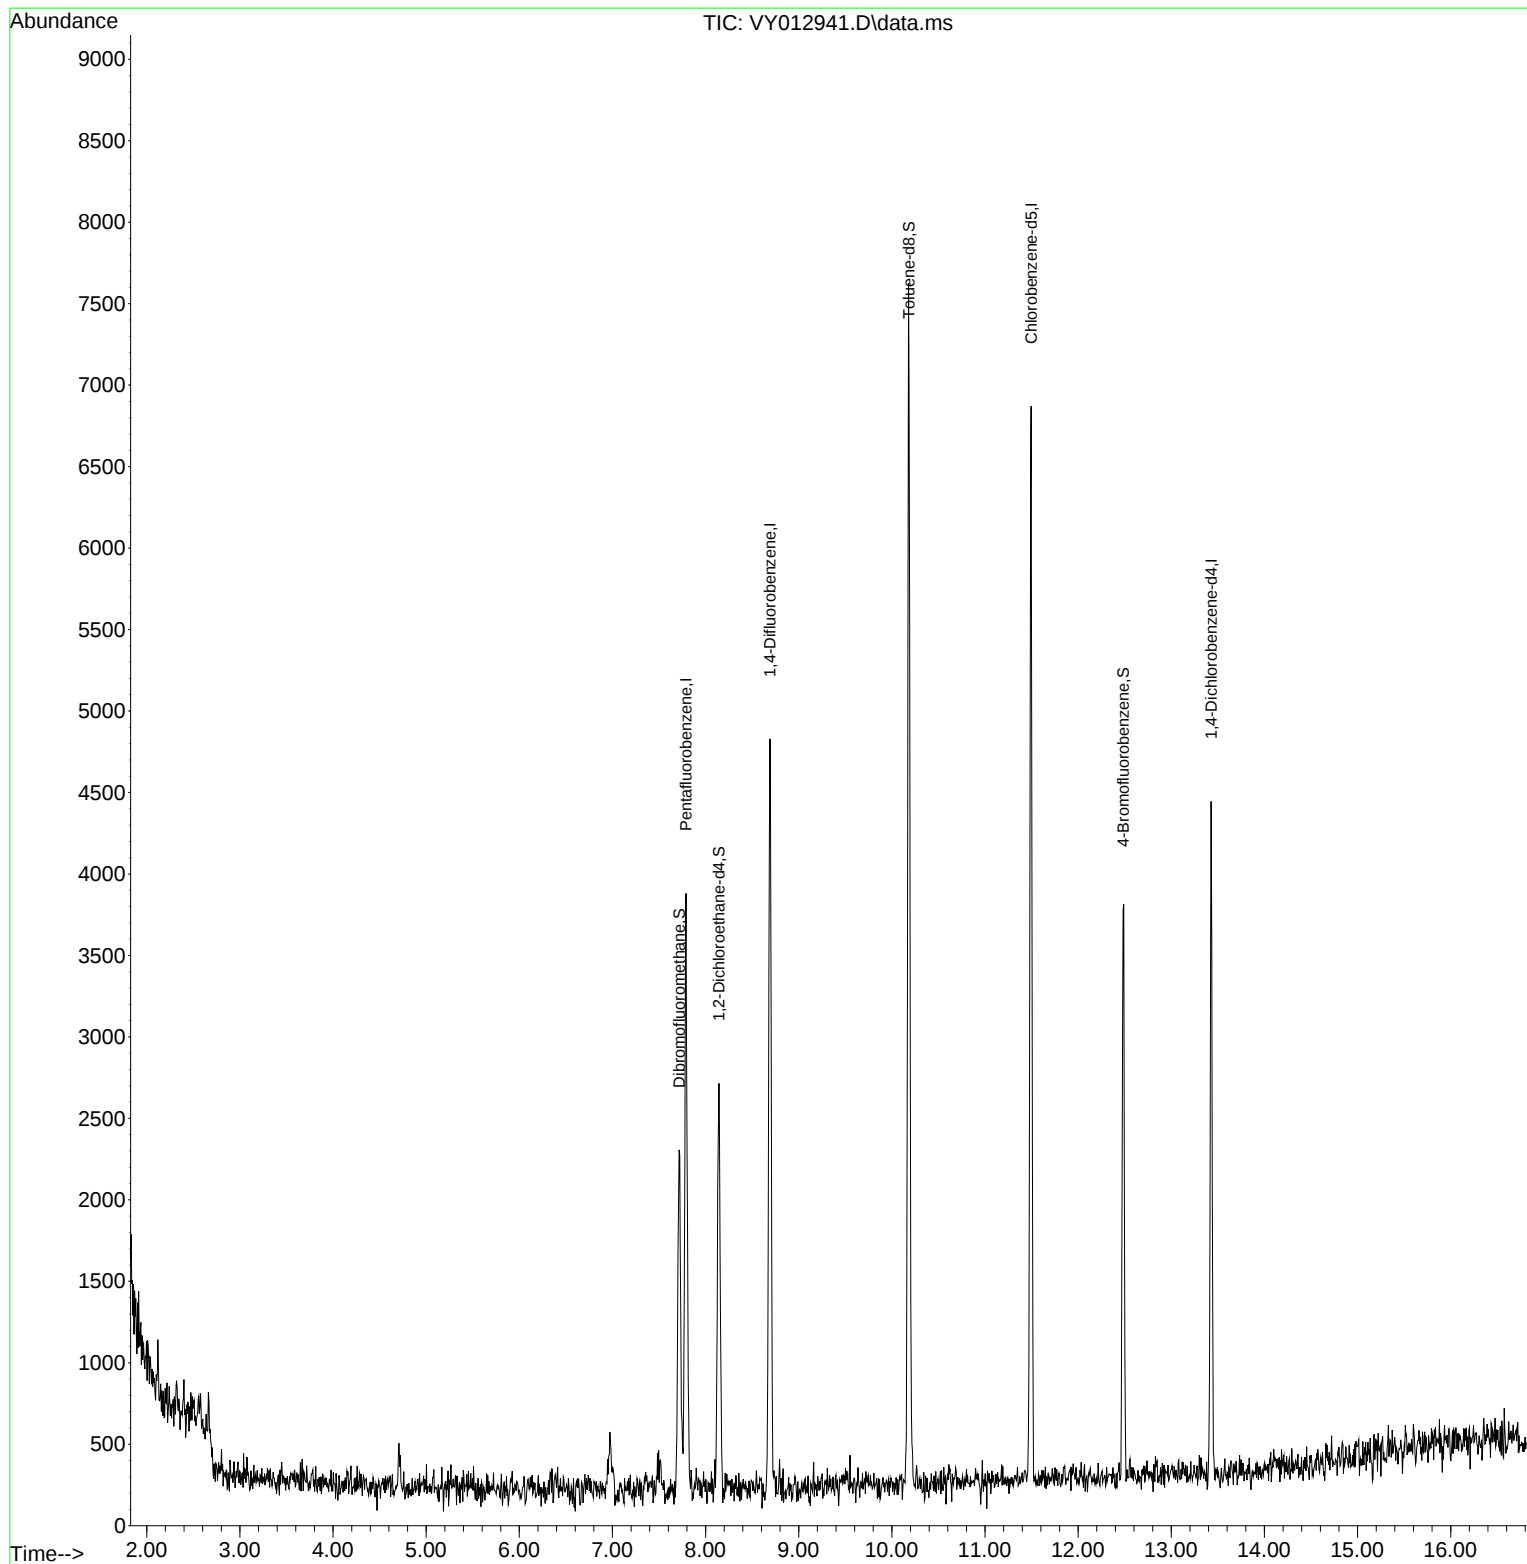


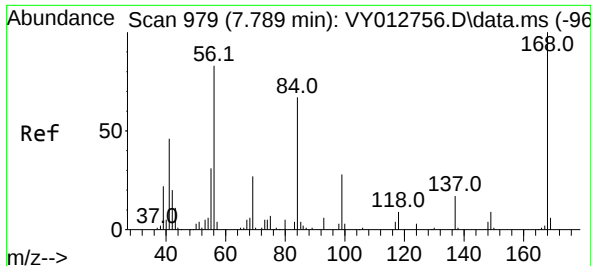

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY012941.D
Acq: 14 Mar 2023 14:36




Instrument :
MSVOA_Y
ClientSampleId :
MAPLE-3

Tgt Ion:168 Resp: 3006
Ion Ratio Lower Upper
168 100
99 57.3 41.7 62.5

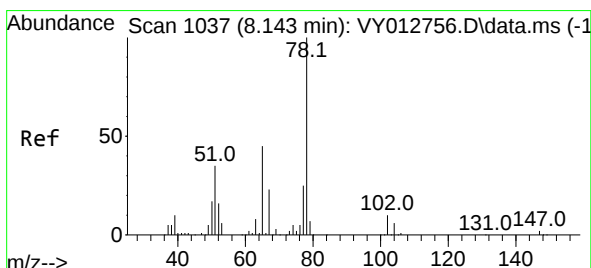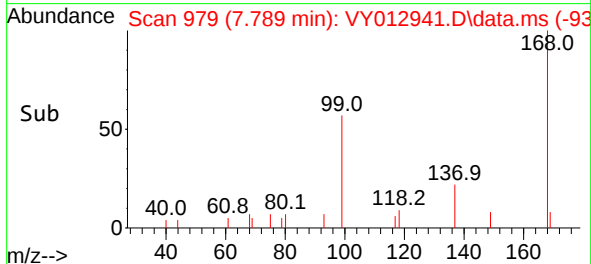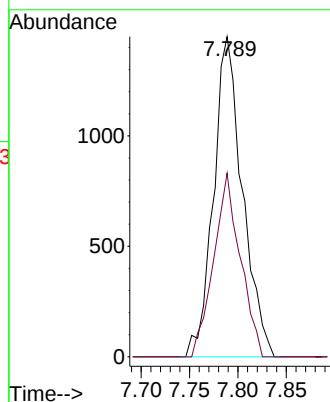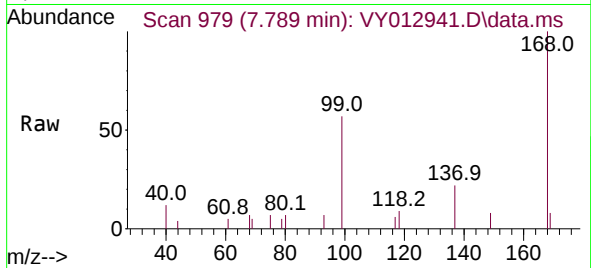

#33
1,2-Dichloroethane-d4
Concen: 67.782 ug/l
RT: 8.142 min Scan# 1037
Delta R.T. -0.001 min
Lab File: VY012941.D
Acq: 14 Mar 2023 14:36

Tgt Ion: 65 Resp: 2023
Ion Ratio Lower Upper
65 100
67 51.2 0.0 104.0

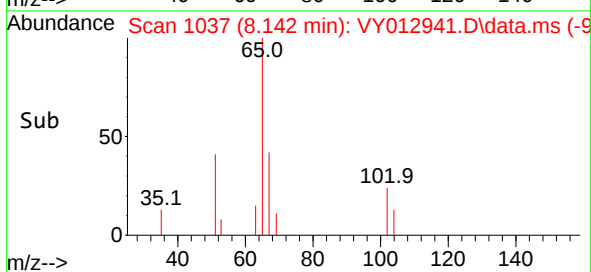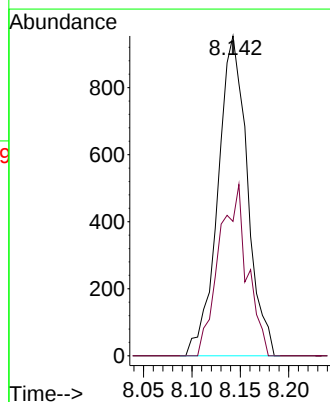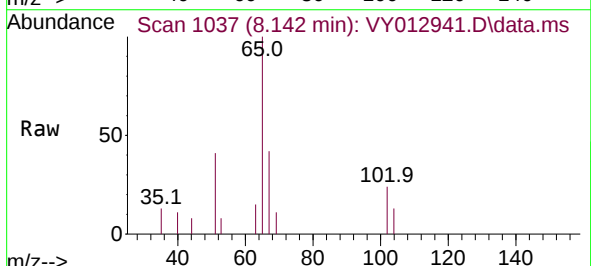



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. -0.000 min

Lab File: VY012941.D

Acq: 14 Mar 2023 14:36

Instrument :

MSVOA_Y

ClientSampleId :

MAPLE-3





Tgt Ion:114 Resp: 4268

Ion Ratio Lower Upper

114 100

63 18.1 0.0 37.4

88 15.6 0.0 28.6

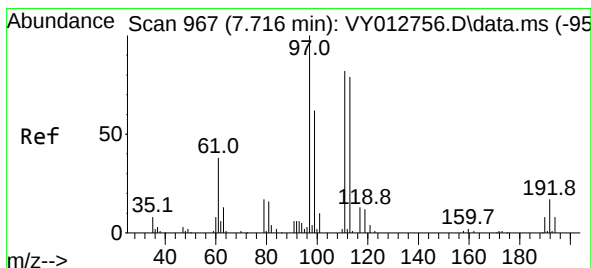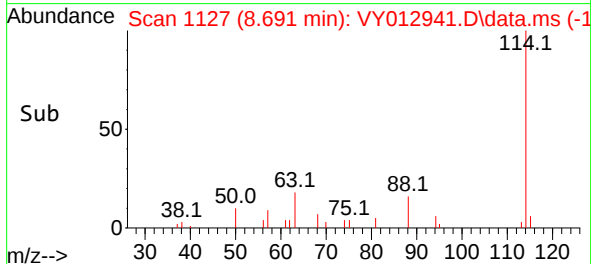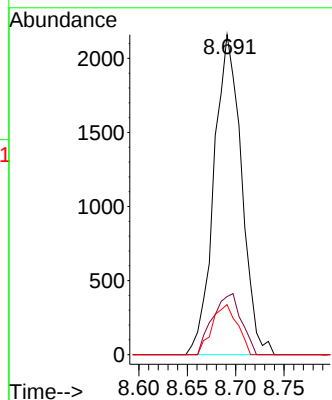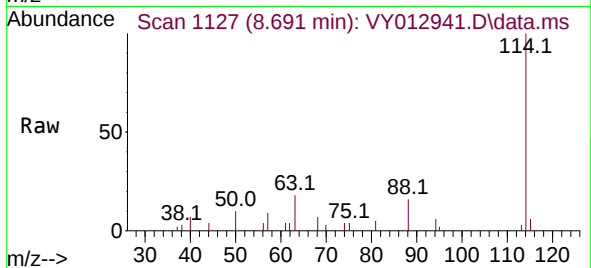

#35

Dibromofluoromethane

Concen: 61.109 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY012941.D

Acq: 14 Mar 2023 14:36




Tgt Ion:113 Resp: 1574


Ion Ratio Lower Upper

113 100

111 109.4 82.2 123.2

192 15.4 16.8 25.2#

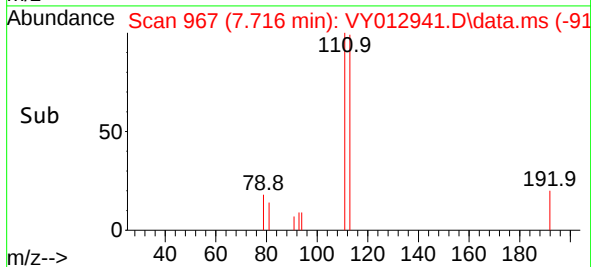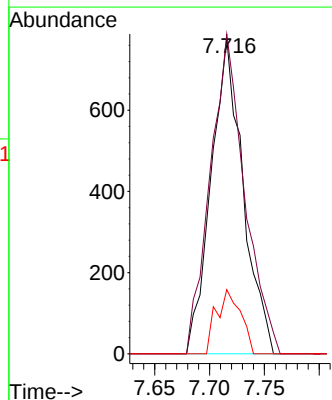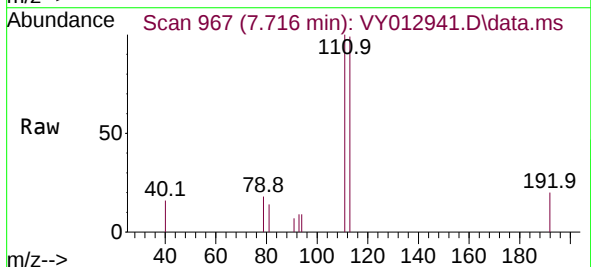

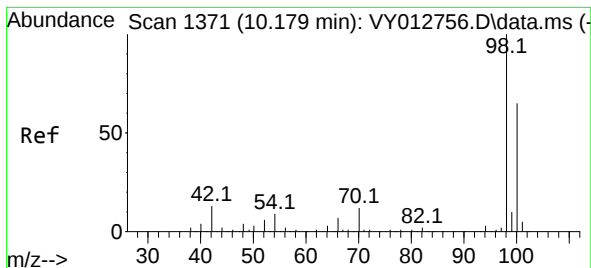

#50

Toluene-d8

Concen: 53.789 ug/l

RT: 10.185 min Scan# 11

Delta R.T. 0.006 min

Lab File: VY012941.D

Acq: 14 Mar 2023 14:36

Instrument :

MSVOA_Y

ClientSampleId :





MAPLE-3

Tgt Ion: 98 Resp: 5065

Ion Ratio Lower Upper

98 100

100 65.8 50.9 76.3

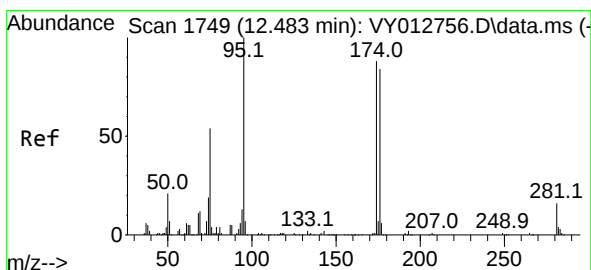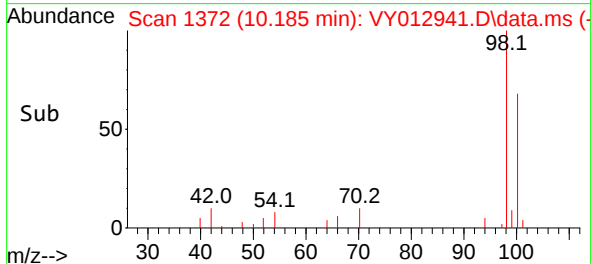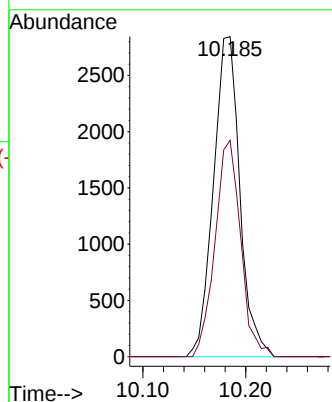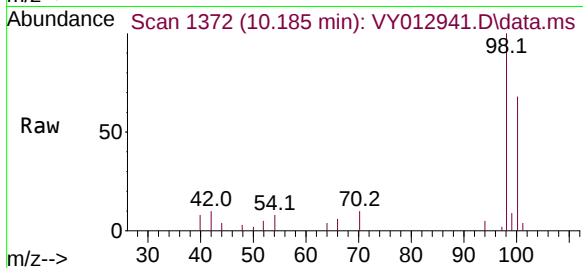

#62

4-Bromofluorobenzene

Concen: 40.966 ug/l

RT: 12.483 min Scan# 1749

Delta R.T. -0.000 min

Lab File: VY012941.D

Acq: 14 Mar 2023 14:36




Tgt Ion: 95 Resp: 1302


Ion Ratio Lower Upper

95 100

174 92.9 0.0 176.6

176 85.3 0.0 170.2


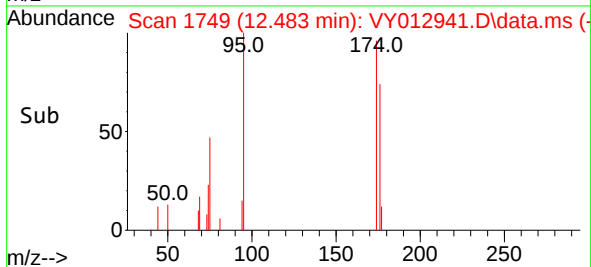
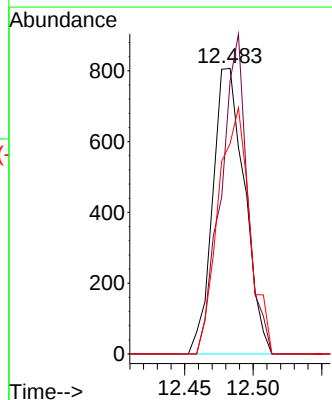
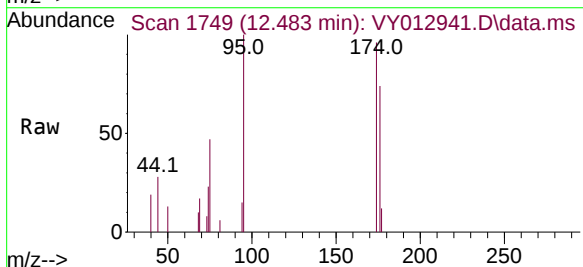


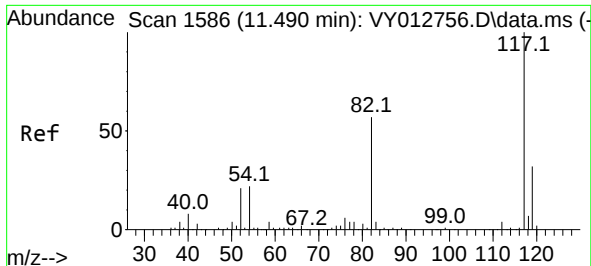

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.495 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY012941.D
Acq: 14 Mar 2023 14:36

Instrument :
MSVOA_Y
ClientSampleId :
MAPLE-3

Tgt Ion:117 Resp: 3775
Ion Ratio Lower Upper
117 100
82 51.8 45.4 68.0
119 31.9 25.6 38.4

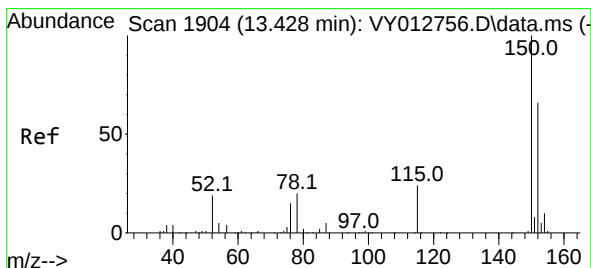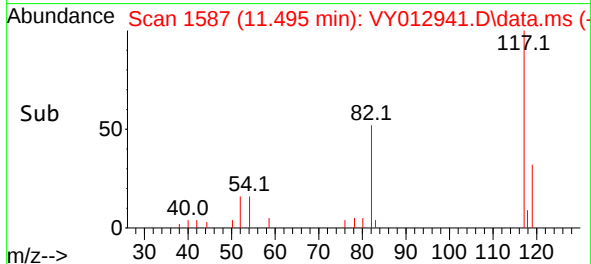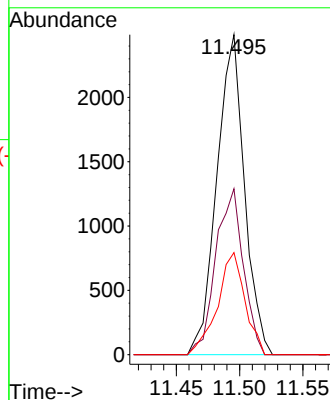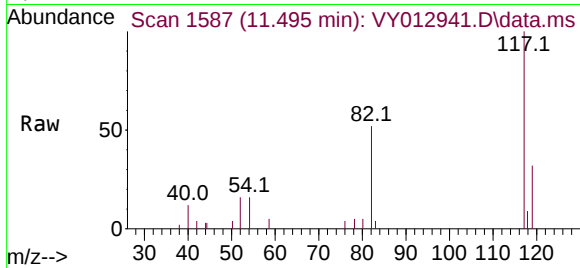

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY012941.D
Acq: 14 Mar 2023 14:36

Tgt Ion:152 Resp: 1144
Ion Ratio Lower Upper
152 100
115 60.8 27.1 81.3
150 162.0 0.0 347.8

