
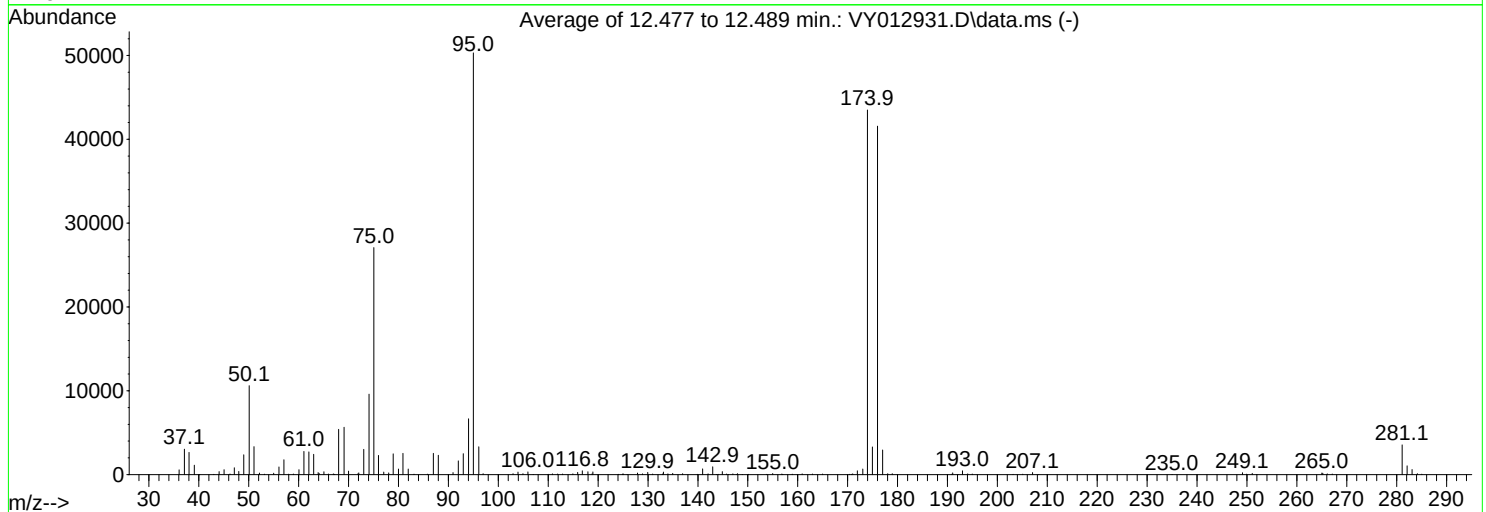


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY031423\
Data File : VY012931.D
Acq On : 14 Mar 2023 09:54
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030223S.M
Title : SW846 8260
Last Update : Fri Mar 03 01:13:13 2023

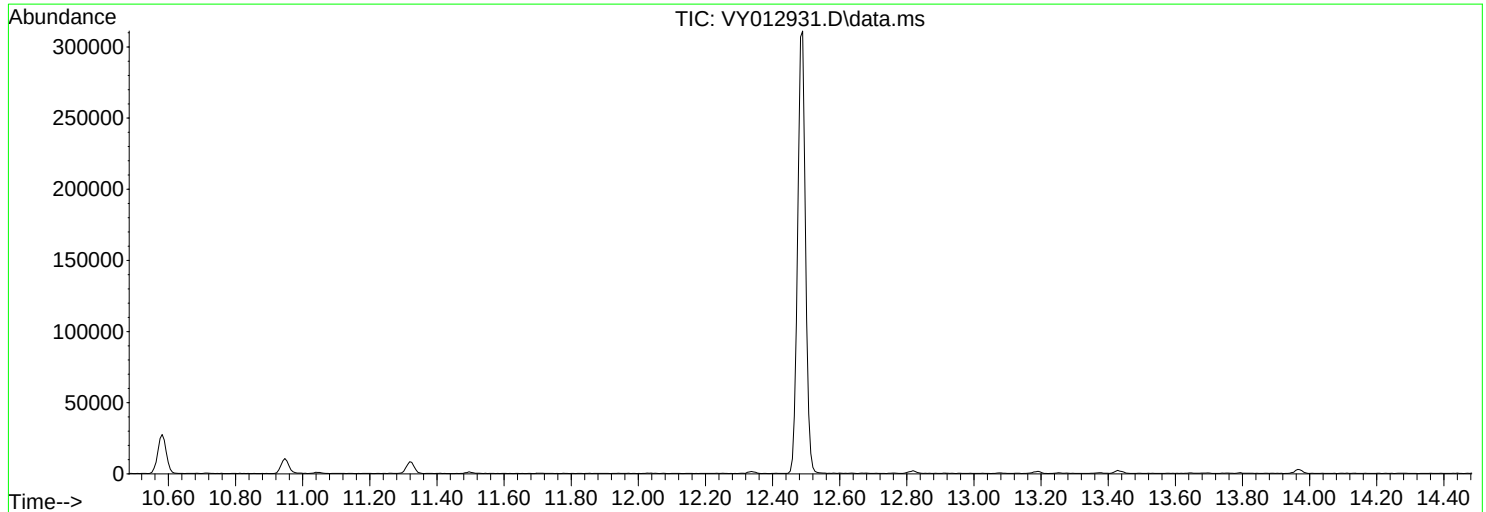

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.1	10608	PASS
75	95	30	60	53.8	27077	PASS
95	95	100	100	100.0	50315	PASS
96	95	5	9	6.6	3316	PASS
173	174	0.00	2	1.6	675	PASS
174	95	50	100	86.5	43501	PASS
175	174	5	9	7.6	3312	PASS
176	174	95	101	95.5	41563	PASS
177	176	5	9	7.1	2932	PASS