
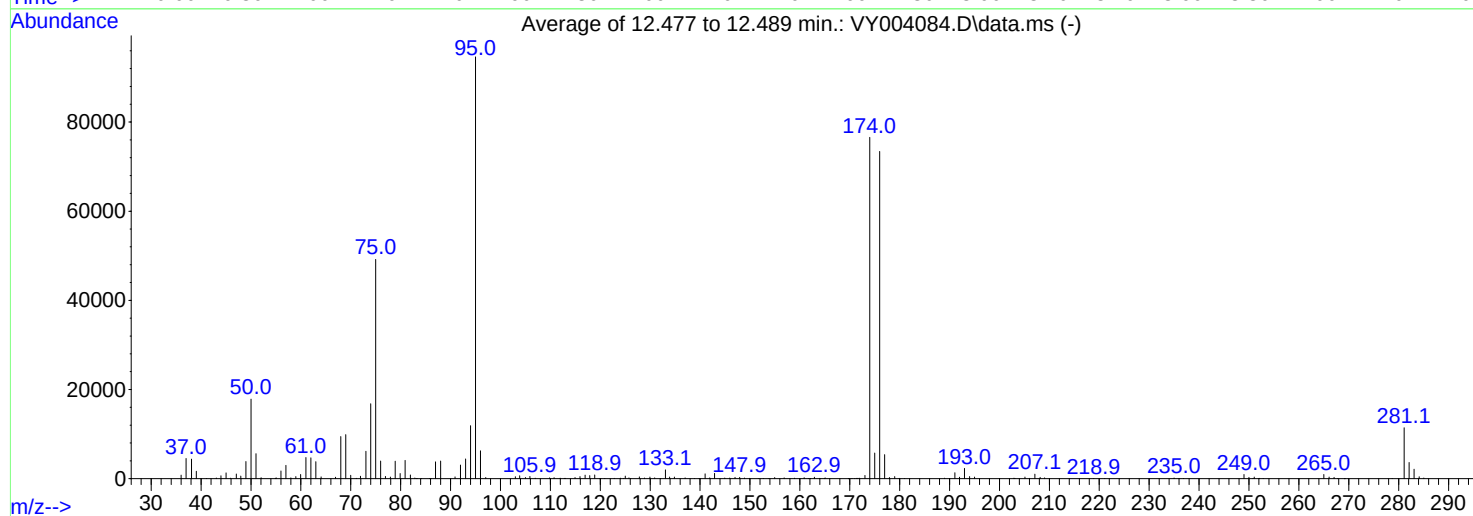


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY031621\
Data File : VY004084.D
Acq On : 16 Mar 2021 08:49
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030821S.M
Title : SW846 8260
Last Update : Mon Mar 08 12:28:55 2021

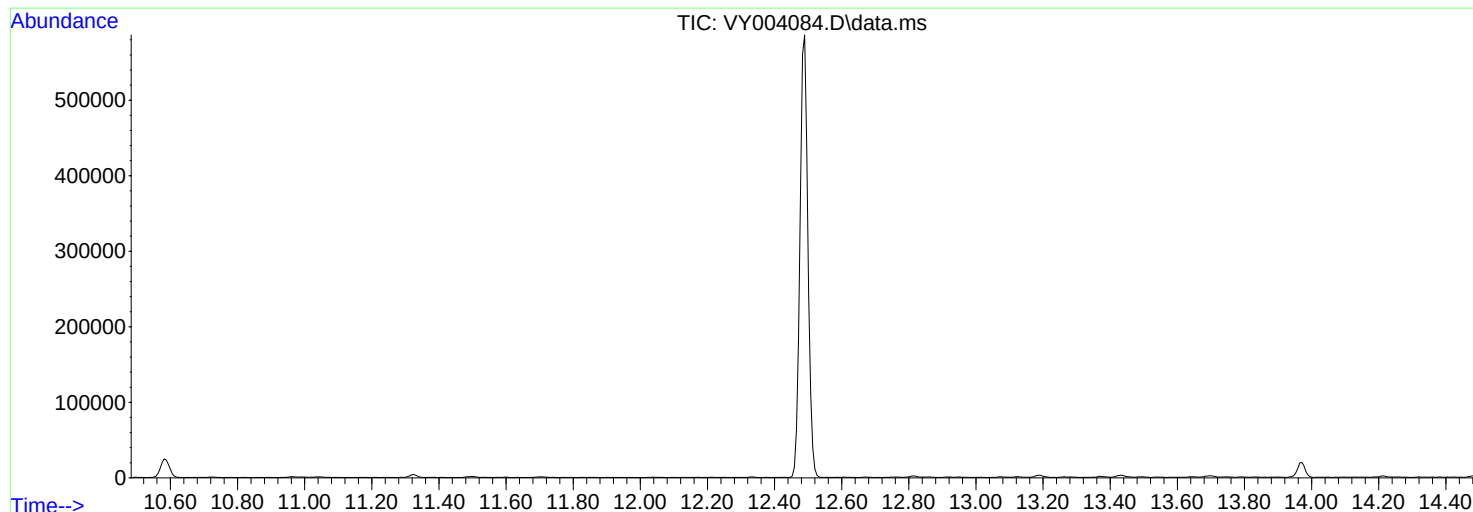

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	17838	PASS
75	95	30	60	52.0	49189	PASS
95	95	100	100	100.0	94629	PASS
96	95	5	9	6.6	6255	PASS
173	174	0.00	2	1.0	735	PASS
174	95	50	100	80.9	76552	PASS
175	174	5	9	7.5	5738	PASS
176	174	95	101	95.9	73405	PASS
177	176	5	9	7.3	5380	PASS