
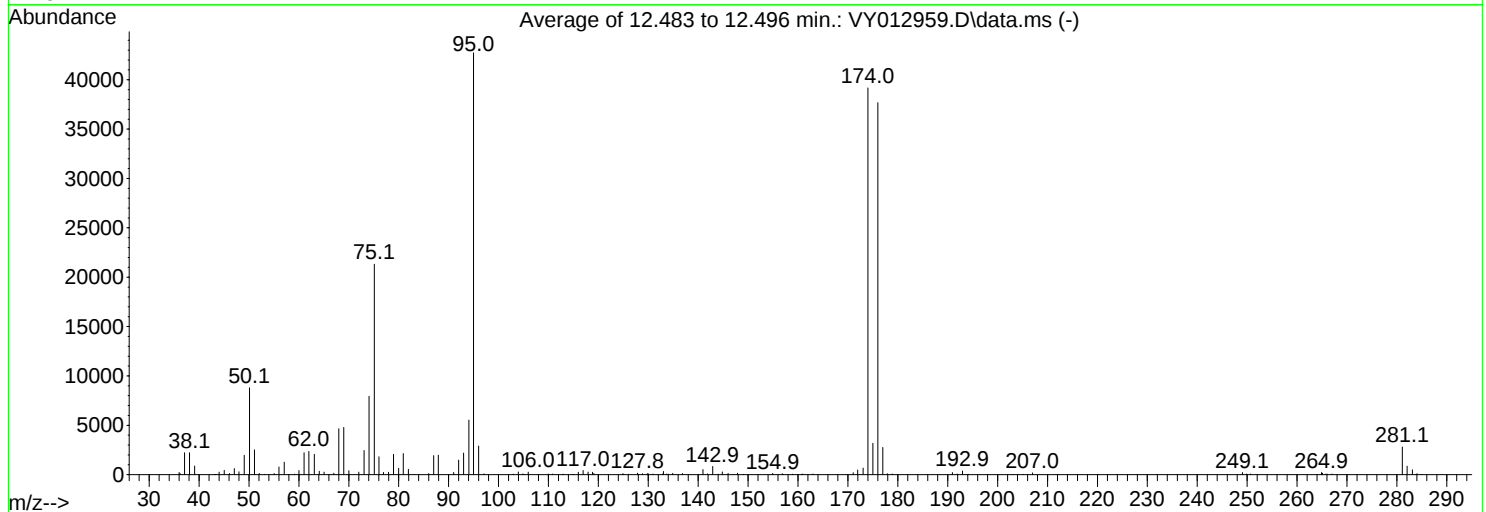


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY031623\
Data File : VY012959.D
Acq On : 16 Mar 2023 09:18
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030223S.M
Title : SW846 8260
Last Update : Fri Mar 03 01:13:13 2023

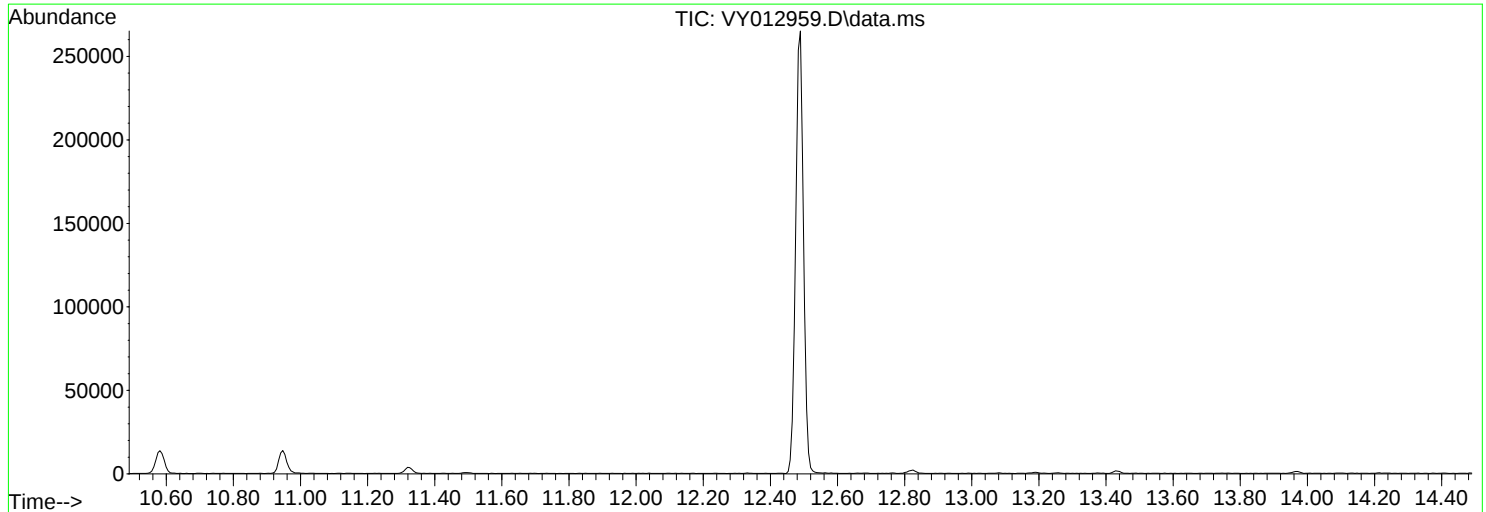

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	8797	PASS
75	95	30	60	49.9	21312	PASS
95	95	100	100	100.0	42725	PASS
96	95	5	9	6.8	2902	PASS
173	174	0.00	2	1.7	663	PASS
174	95	50	100	91.7	39181	PASS
175	174	5	9	8.1	3180	PASS
176	174	95	101	96.2	37680	PASS
177	176	5	9	7.3	2754	PASS