
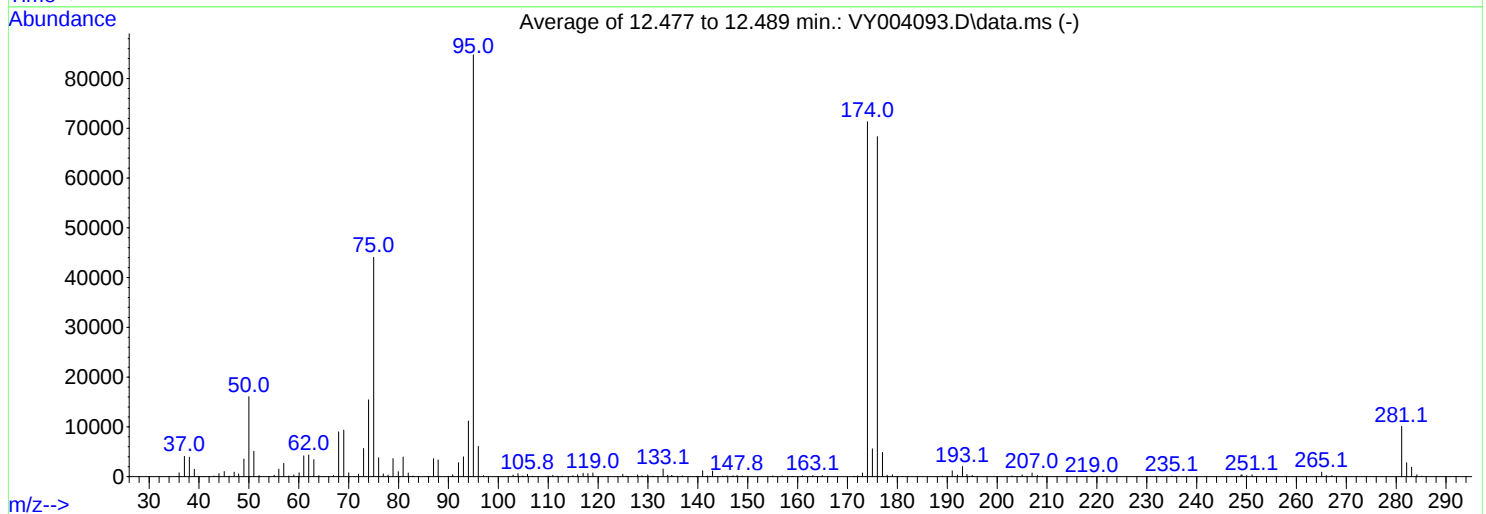


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY031721\
Data File : VY004093.D
Acq On : 17 Mar 2021 09:33
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030821S.M
Title : SW846 8260
Last Update : Mon Mar 08 12:28:55 2021

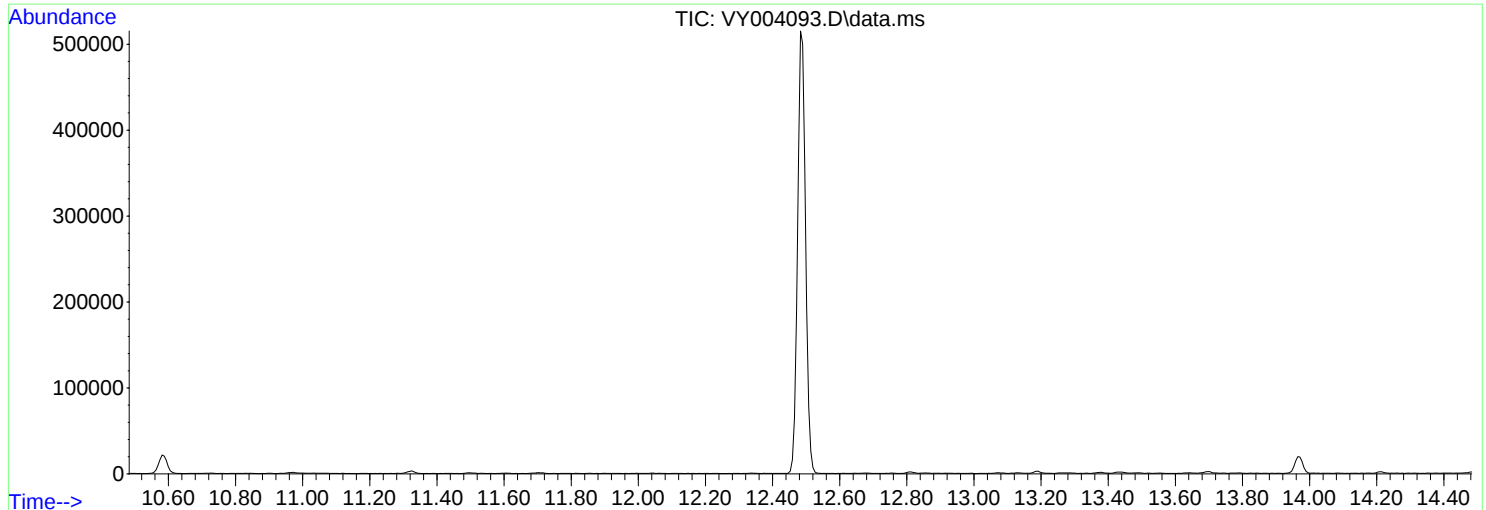

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.0	16086	PASS
75	95	30	60	52.0	44069	PASS
95	95	100	100	100.0	84755	PASS
96	95	5	9	7.2	6075	PASS
173	174	0.00	2	1.0	731	PASS
174	95	50	100	84.1	71296	PASS
175	174	5	9	7.8	5585	PASS
176	174	95	101	95.8	68315	PASS
177	176	5	9	7.1	4844	PASS