

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY031723\
 Data File : VY013000.D
 Acq On : 17 Mar 2023 20:29
 Operator : KP/MD
 Sample : 01974-06
 Misc : 6.64g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :

Quant Time: Mar 18 05:50:28 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030223S.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 03 01:13:13 2023
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.783	168	73772	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	124733	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	112353	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	45420	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	52099	71.129	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 142.260%	
35) Dibromofluoromethane	7.710	113	44336	58.898	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 117.800%	
50) Toluene-d8	10.179	98	151490	55.048	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 110.100%	
62) 4-Bromofluorobenzene	12.477	95	43308	46.625	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 93.260%	
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	4.930	59	23	Below Cal	#	74
16) Acetone	3.948	43	364	1.266	ug/l #	44
20) Methylene Chloride	4.704	84	8459	4.783	ug/l	95
31) Cyclohexane	7.789	56	1735	1.237	ug/l #	2
36) 1,1-Dichloropropene	7.783	75	5820	4.614	ug/l #	48
38) Carbon Tetrachloride	7.783	117	7100	5.450	ug/l #	15
76) 1,2,3-Trichloropropane	12.477	75	22630	41.723	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.477	75	22630	86.451	ug/l #	13


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY031723\
Data File : VY013000.D
Acq On : 17 Mar 2023 20:29
Operator : KP/MD
Sample : 01974-06
Misc : 6.64g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :


Quant Time: Mar 18 05:50:28 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030223S.M
Quant Title : SW846 8260
QLast Update : Fri Mar 03 01:13:13 2023
Response via : Initial Calibration

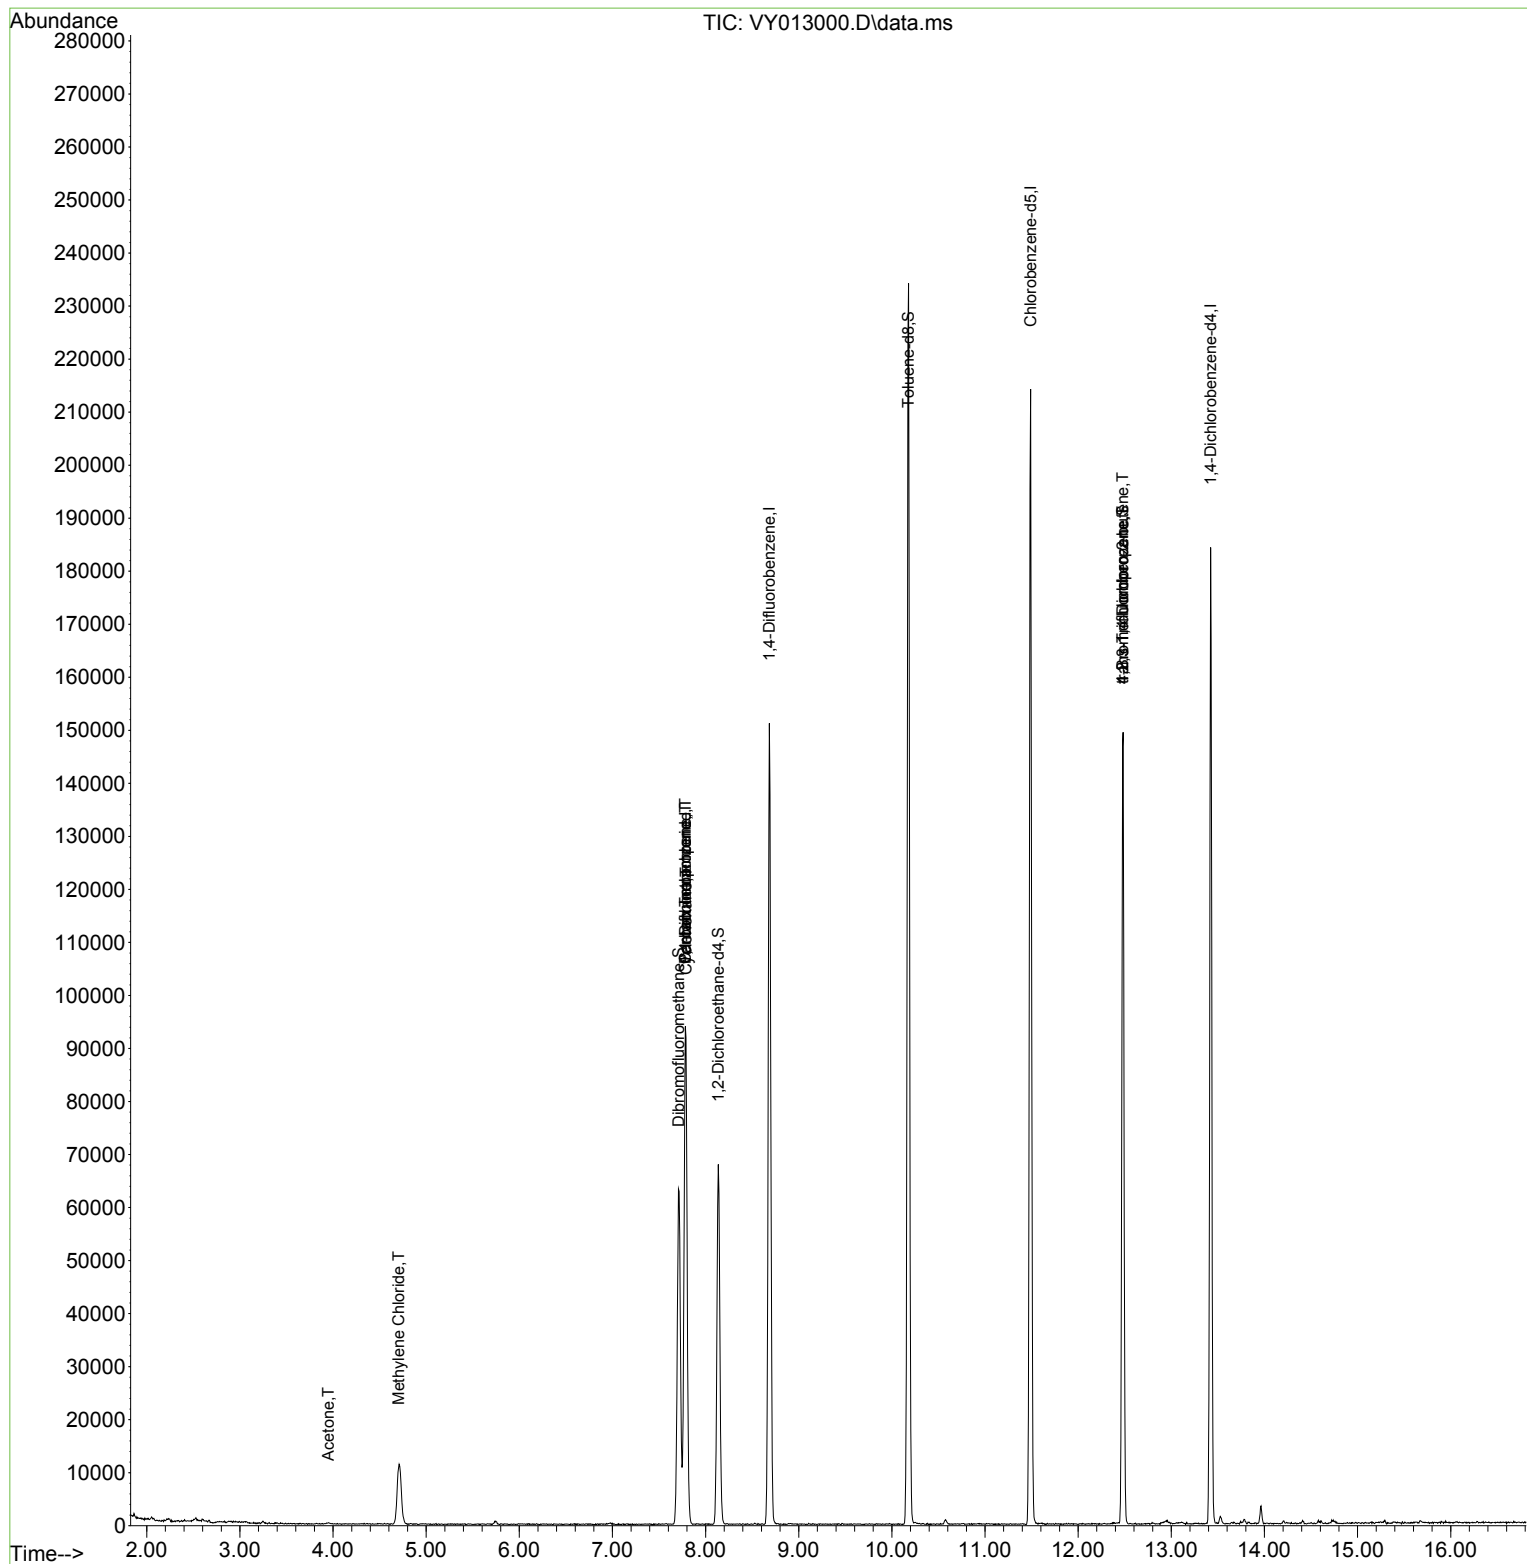



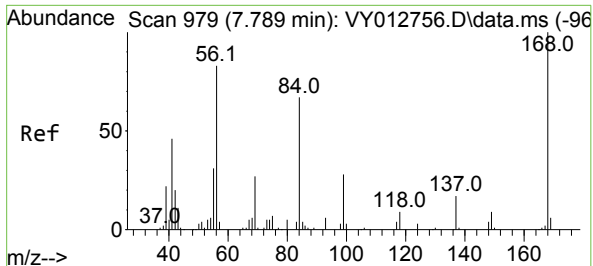


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY013000.D
Acq: 17 Mar 2023 20:29

Instrument :
MSVOA_Y
ClientSampleId :



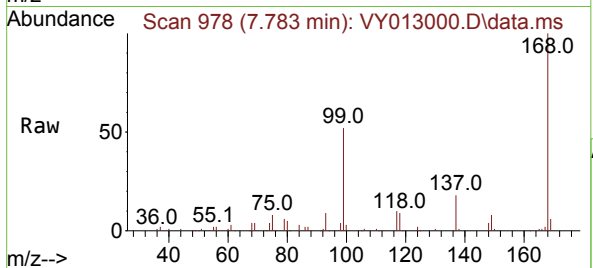



Tgt Ion:168 Resp: 73772
Ion Ratio Lower Upper
168 100
99 51.9 41.7 62.5

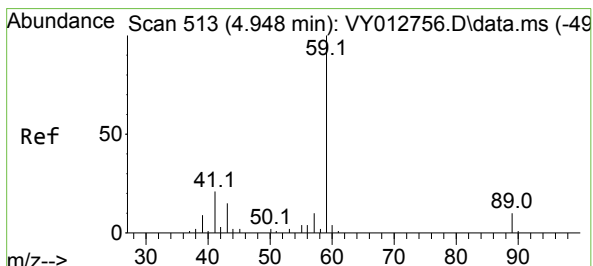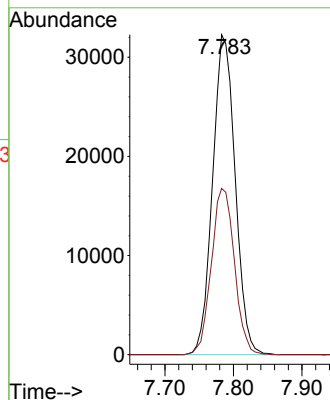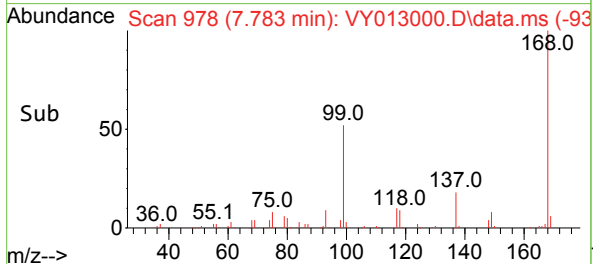

#11
Tert butyl alcohol
Concen: Below Cal
RT: 4.930 min Scan# 510
Delta R.T. -0.018 min
Lab File: VY013000.D
Acq: 17 Mar 2023 20:29

Tgt Ion: 59 Resp: 23
Ion Ratio Lower Upper
59 100
57 0.0 7.7 11.5#

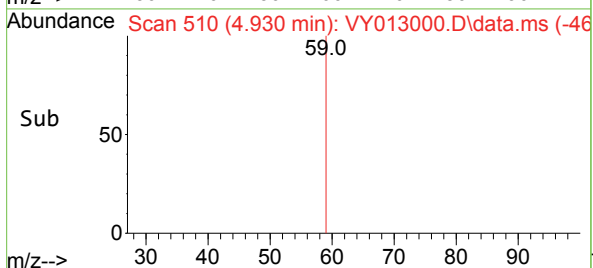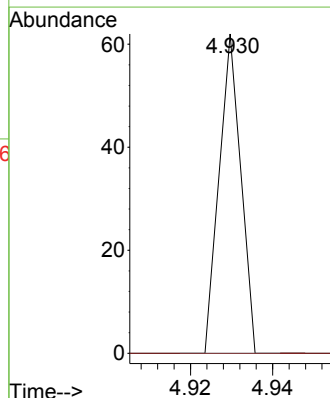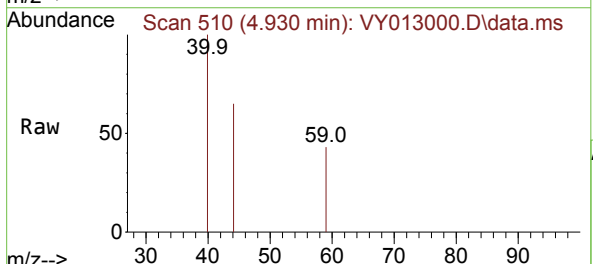

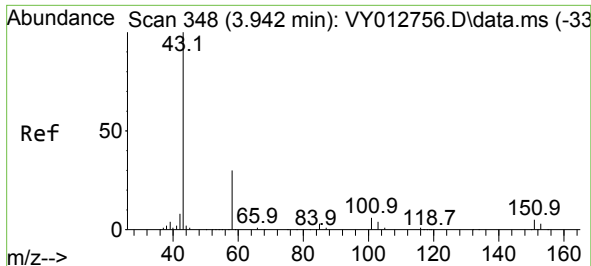

#16

Acetone

Concen: 1.266 ug/l

RT: 3.948 min Scan# 34

Delta R.T. 0.006 min

Lab File: VY013000.D

Acq: 17 Mar 2023 20:29

Instrument :

MSVOA_Y





ClientSampleId :

Tgt Ion: 43 Resp: 364

Ion Ratio Lower Upper

43 100

58 0.0 24.2 36.2#

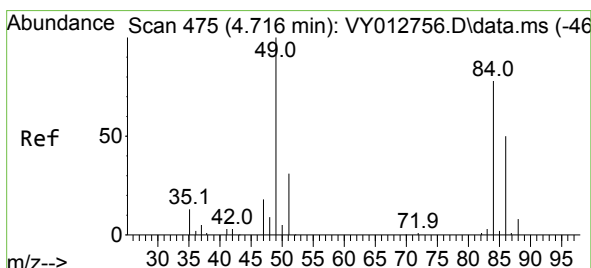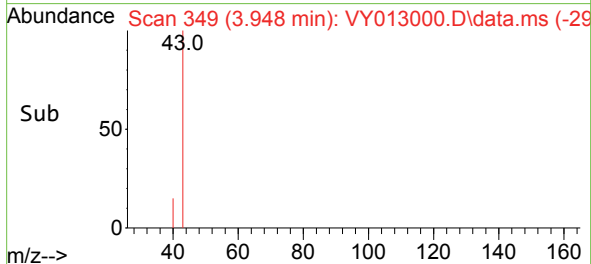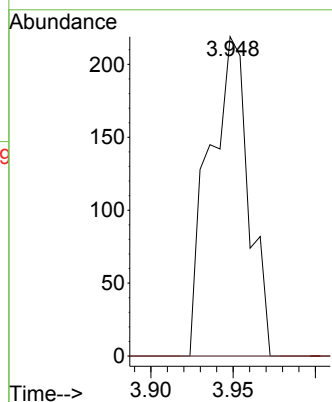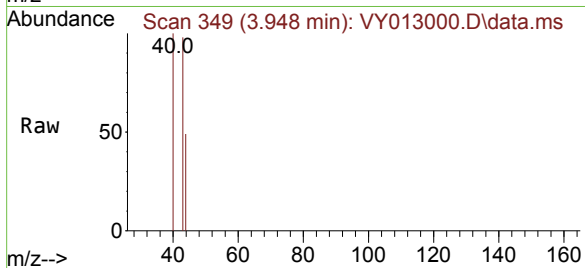

#20

Methylene Chloride

Concen: 4.783 ug/l

RT: 4.704 min Scan# 473

Delta R.T. -0.012 min

Lab File: VY013000.D

Acq: 17 Mar 2023 20:29

Tgt Ion: 84 Resp: 8459




Ion Ratio Lower Upper


84 100

49 132.8 102.6 154.0

51 38.6 31.9 47.9


86 55.9 51.0 76.6

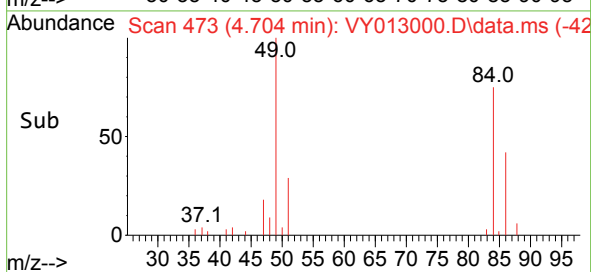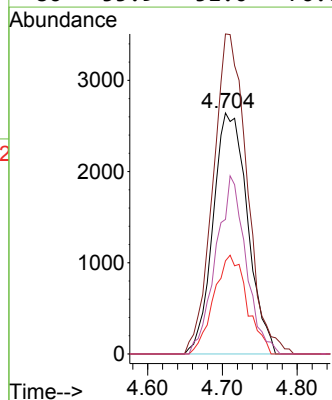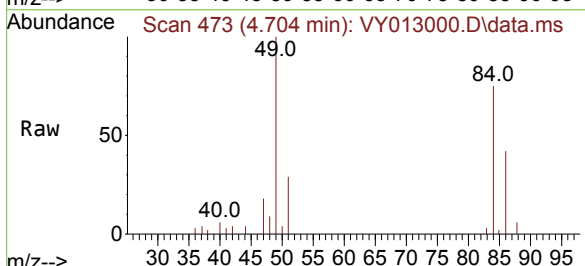



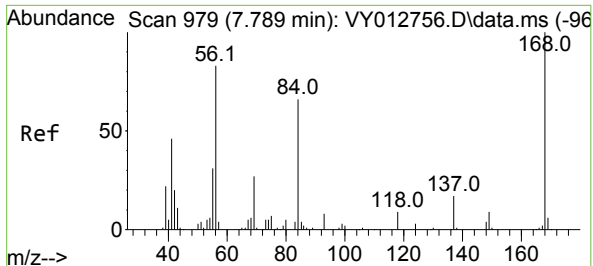


#31
Cyclohexane
Concen: 1.237 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY013000.D
Acq: 17 Mar 2023 20:29

Instrument :
MSVOA_Y
ClientSampleId :



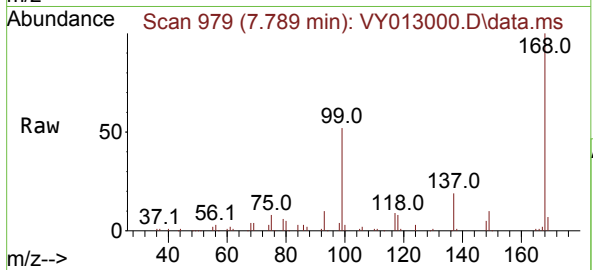



Tgt Ion: 56 Resp: 1735
Ion Ratio Lower Upper
56 100
69 161.8 25.7 38.5#
84 119.2 64.3 96.5#

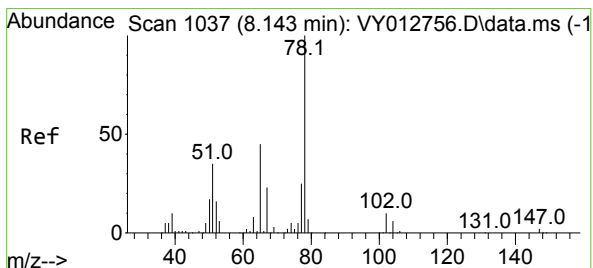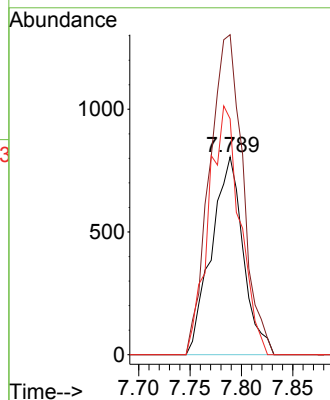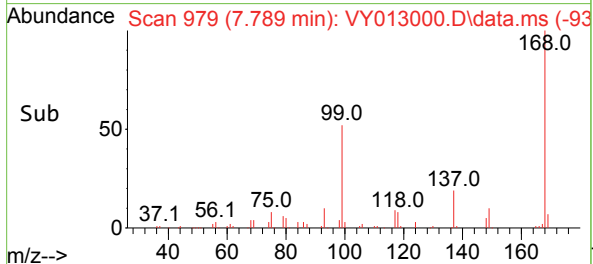

#33
1,2-Dichloroethane-d4
Concen: 71.129 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. -0.007 min
Lab File: VY013000.D
Acq: 17 Mar 2023 20:29

Tgt Ion: 65 Resp: 52099
Ion Ratio Lower Upper
65 100
67 51.4 0.0 104.0

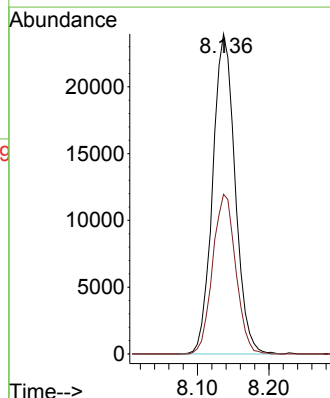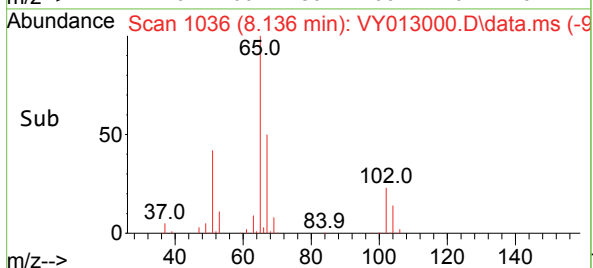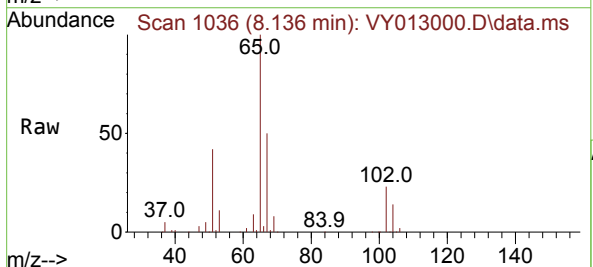

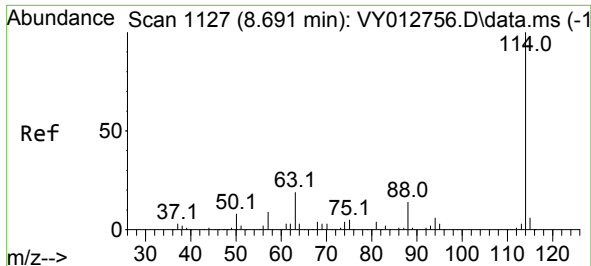

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. -0.006 min

Lab File: VY013000.D

Acq: 17 Mar 2023 20:29

Instrument :

MSVOA_Y

ClientSampleId :





Tgt Ion:114 Resp: 124733

Ion Ratio Lower Upper

114 100

63 19.5 0.0 37.4

88 14.3 0.0 28.6

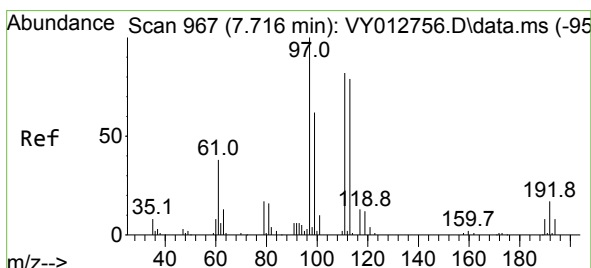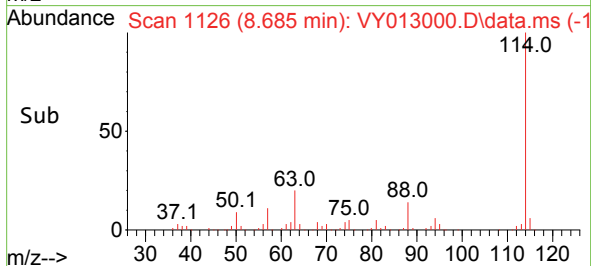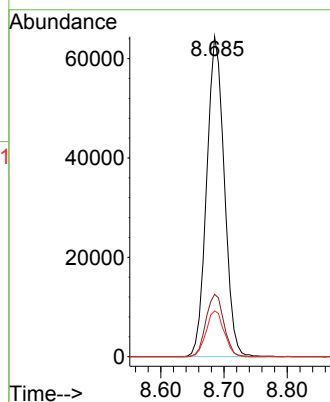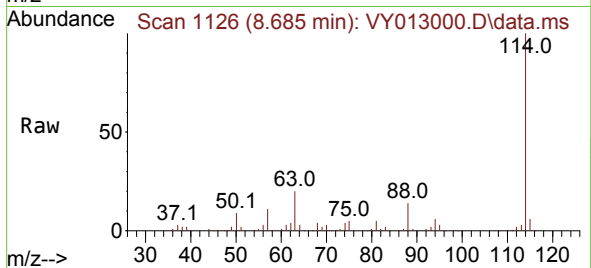

#35

Dibromofluoromethane

Concen: 58.898 ug/l

RT: 7.710 min Scan# 966

Delta R.T. -0.006 min

Lab File: VY013000.D

Acq: 17 Mar 2023 20:29




Tgt Ion:113 Resp: 44336


Ion Ratio Lower Upper

113 100

111 103.9 82.2 123.2

192 20.9 16.8 25.2

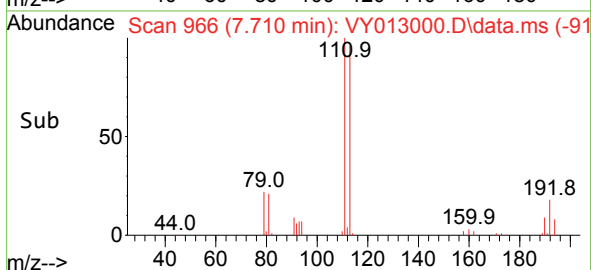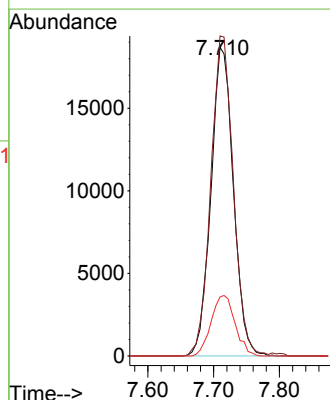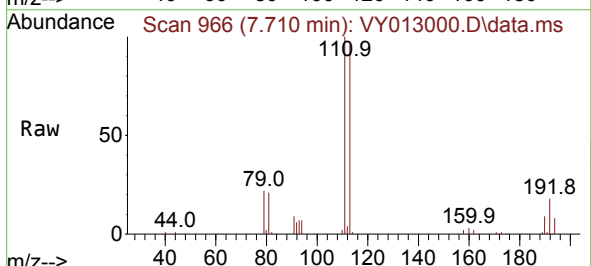

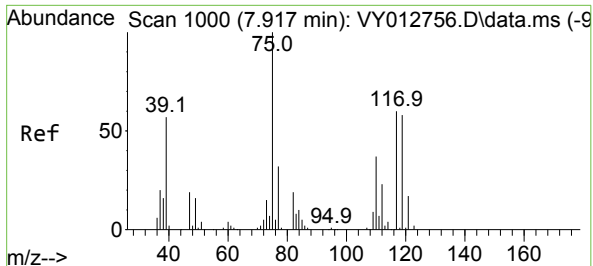

#36

1,1-Dichloropropene

Concen: 4.614 ug/l

RT: 7.783 min Scan# 91

Delta R.T. -0.134 min


Lab File: VY013000.D

Acq: 17 Mar 2023 20:29




Instrument :

MSVOA_Y

ClientSampleId :

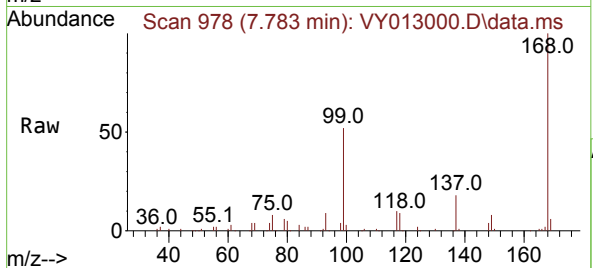

Tgt Ion: 75	Resp: 5820
Ion Ratio	Lower Upper
75	100
110	7.7 17.8 53.3#
77	0.0 25.0 37.4#

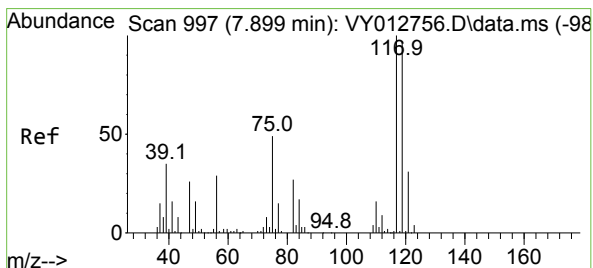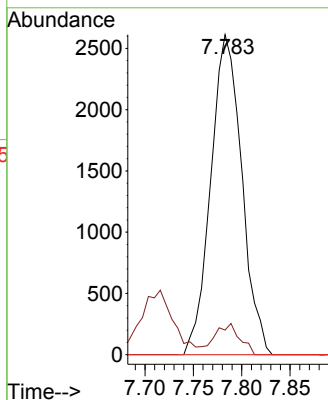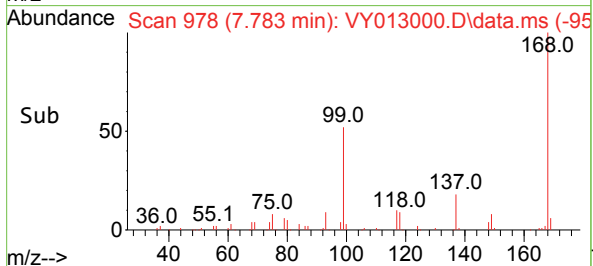

#38

Carbon Tetrachloride

Concen: 5.450 ug/l




RT: 7.783 min Scan# 978


Delta R.T. -0.116 min

Lab File: VY013000.D

Acq: 17 Mar 2023 20:29

Tgt Ion: 117	Resp: 7100
Ion Ratio	Lower Upper
117	100
119	4.5 77.2 115.8#
121	0.0 24.7 37.1#


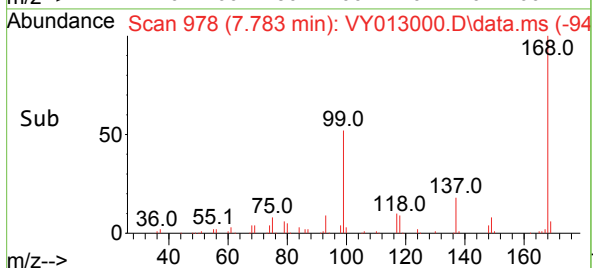
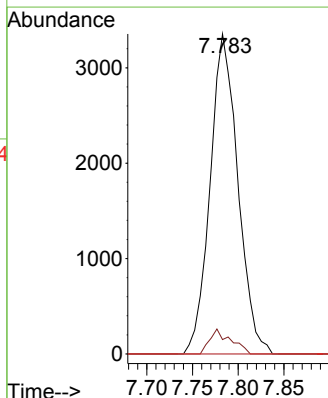
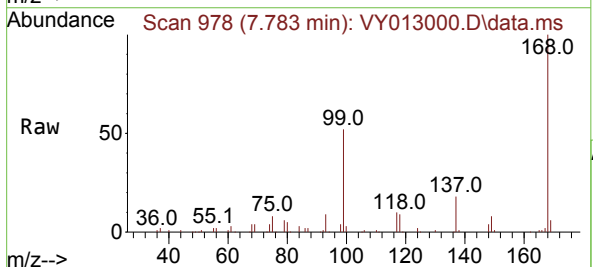


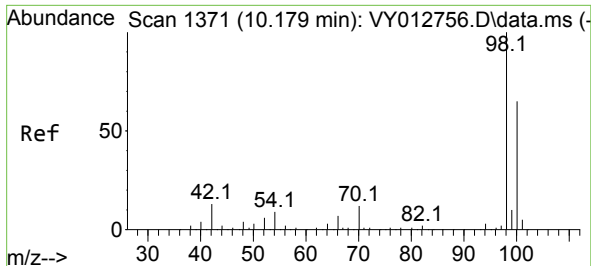

#50
Toluene-d8
Concen: 55.048 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY013000.D
Acq: 17 Mar 2023 20:29




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 98 Resp: 151490
Ion Ratio Lower Upper
98 100
100 63.7 50.9 76.3

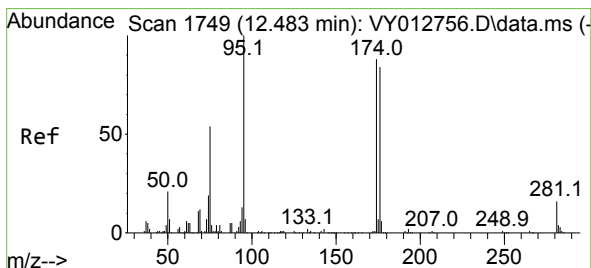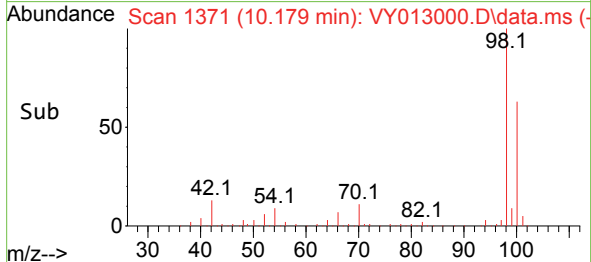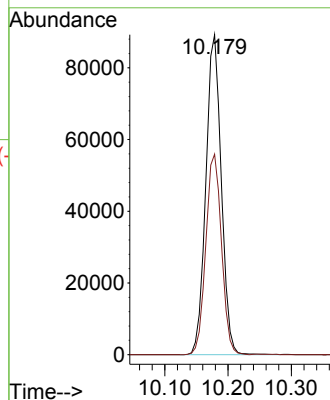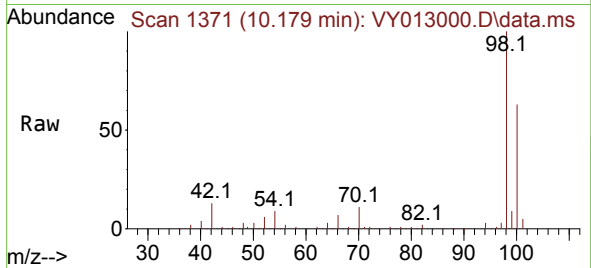

#62
4-Bromofluorobenzene
Concen: 46.625 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.006 min
Lab File: VY013000.D
Acq: 17 Mar 2023 20:29

Tgt Ion: 95 Resp: 43308
Ion Ratio Lower Upper
95 100
174 88.7 0.0 176.6
176 86.1 0.0 170.2


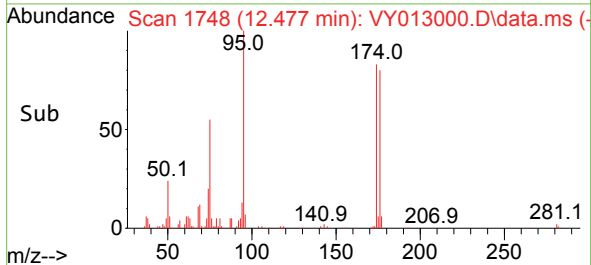
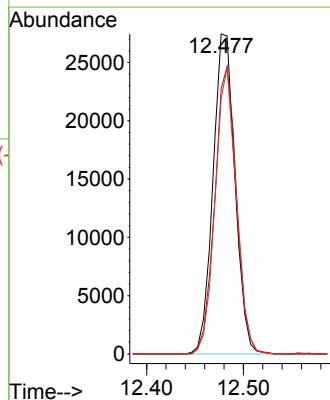
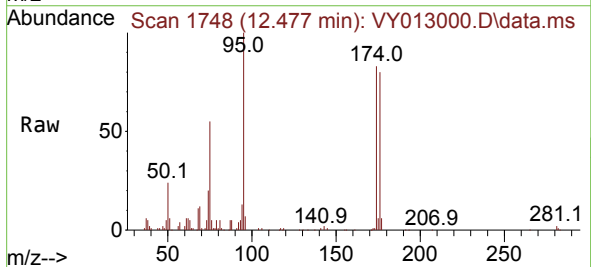


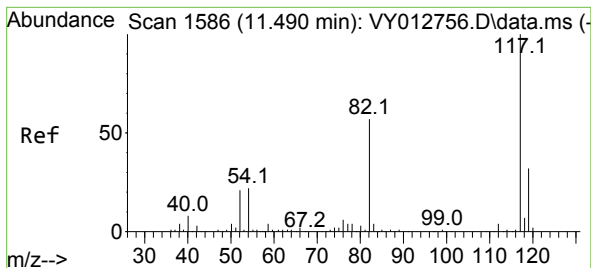

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY013000.D
Acq: 17 Mar 2023 20:29




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:117 Resp: 112353
Ion Ratio Lower Upper
117 100
82 53.4 45.4 68.0
119 32.0 25.6 38.4

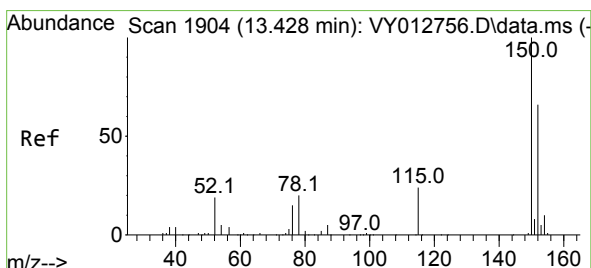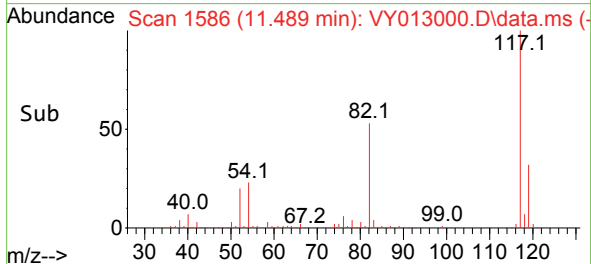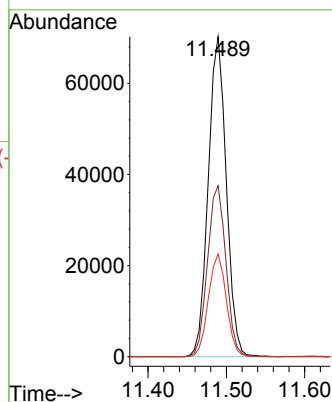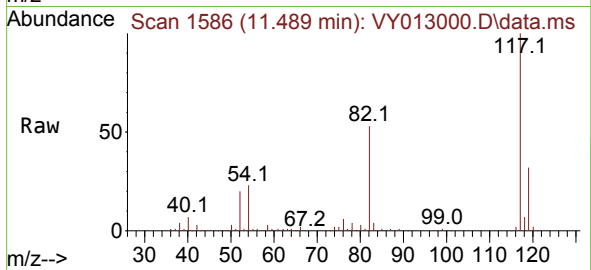

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. -0.006 min
Lab File: VY013000.D
Acq: 17 Mar 2023 20:29

Tgt Ion:152 Resp: 45420
Ion Ratio Lower Upper
152 100
115 56.8 27.1 81.3
150 158.8 0.0 347.8


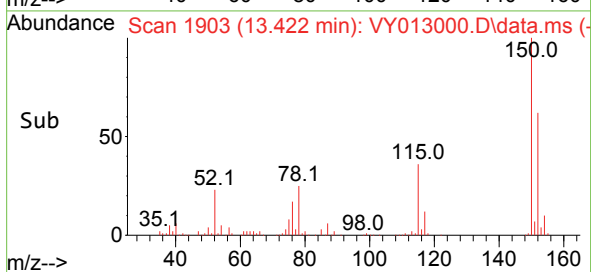
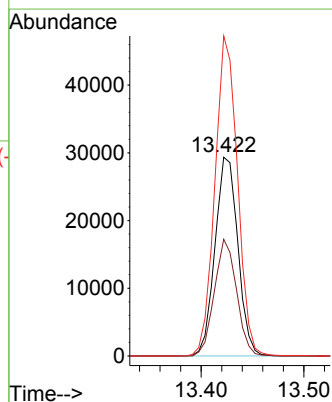
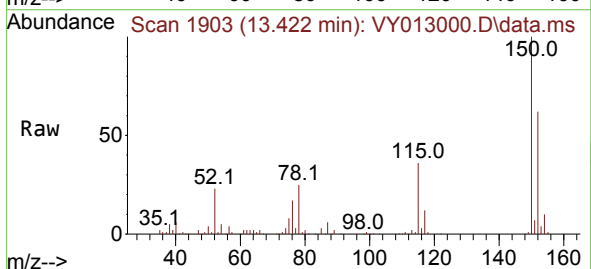


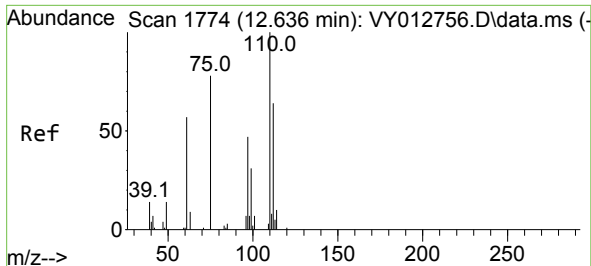

#76
1,2,3-Trichloropropane
Concen: 41.723 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.159 min
Lab File: VY013000.D
Acq: 17 Mar 2023 20:29

Instrument :
MSVOA_Y
ClientSampleId :

Tgt Ion: 75 Resp: 22630
Ion Ratio Lower Upper
75 100
77 1.2 0.0 0.0#

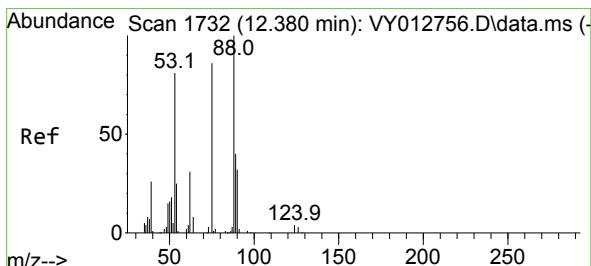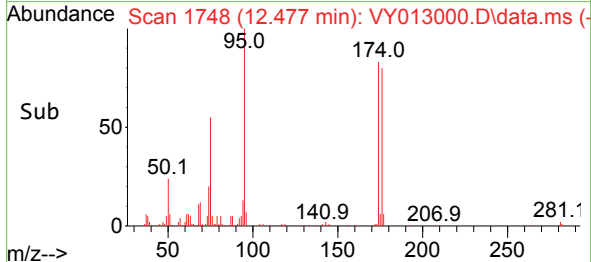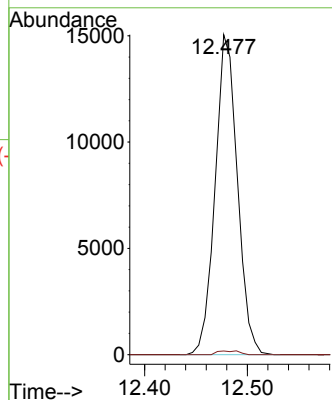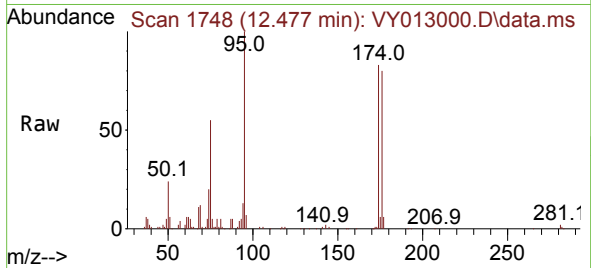

#81
trans-1,4-Dichloro-2-butene
Concen: 86.451 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.097 min
Lab File: VY013000.D
Acq: 17 Mar 2023 20:29

Tgt Ion: 75 Resp: 22630
Ion Ratio Lower Upper
75 100
53 0.0 73.4 110.0#
89 0.0 36.6 55.0#

