
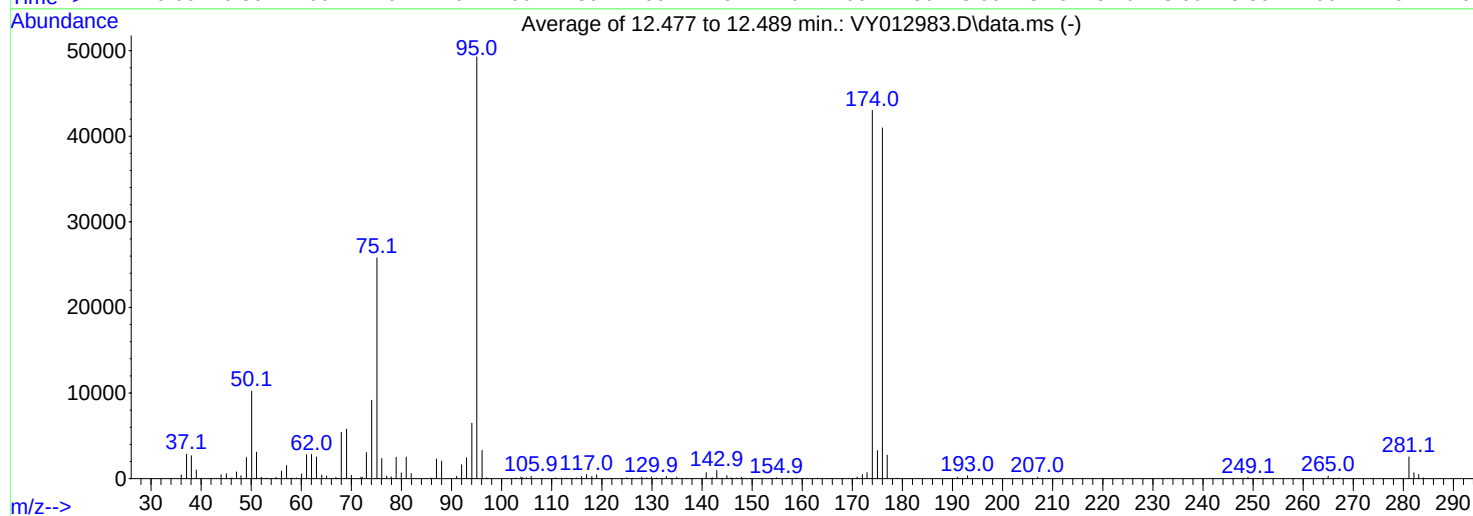


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY031723\
 Data File : VY012983.D
 Acq On : 17 Mar 2023 09:18
 Operator : KP/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030223S.M
 Title : SW846 8260
 Last Update : Fri Mar 03 01:13:13 2023

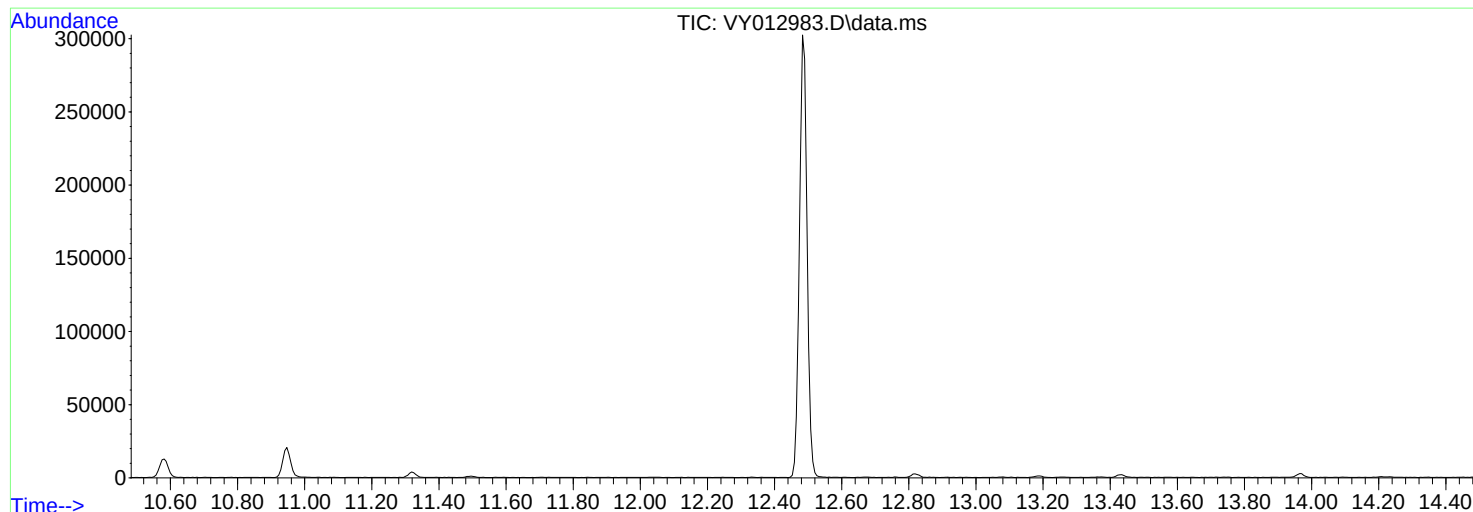

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	10234	PASS
75	95	30	60	52.4	25800	PASS
95	95	100	100	100.0	49275	PASS
96	95	5	9	6.7	3308	PASS
173	174	0.00	2	1.7	716	PASS
174	95	50	100	87.3	43021	PASS
175	174	5	9	7.6	3280	PASS
176	174	95	101	95.2	40973	PASS
177	176	5	9	6.7	2756	PASS