
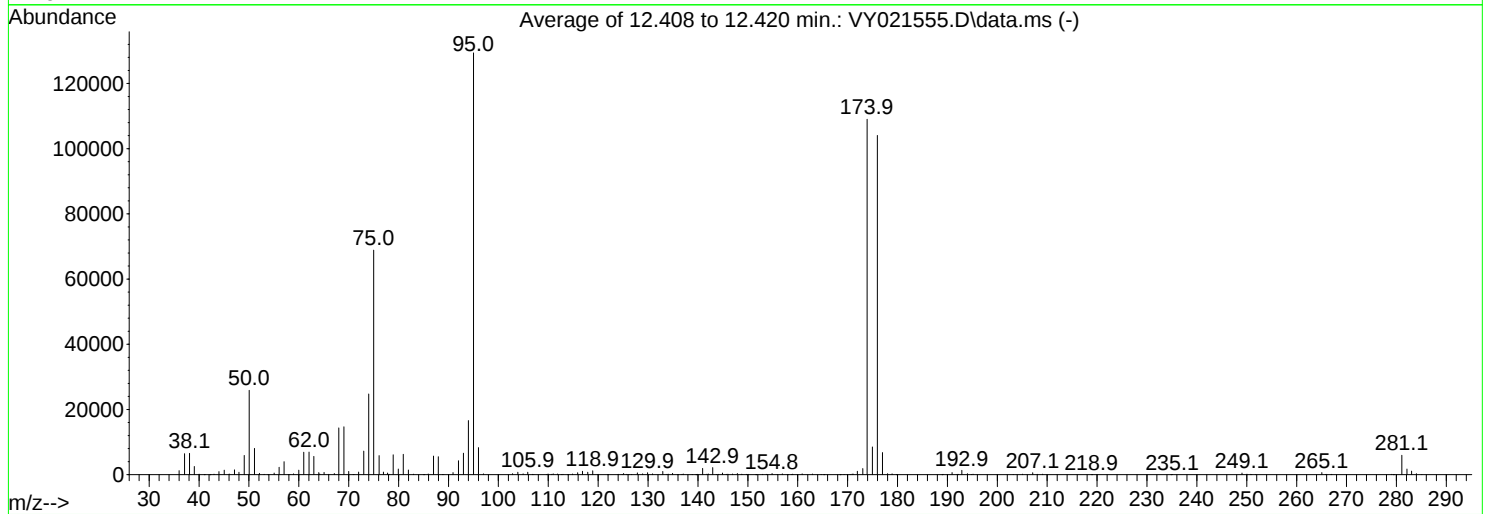


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY031825\
Data File : VY021555.D
Acq On : 18 Mar 2025 09:14
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030425S.M
Title : SW846 8260
Last Update : Wed Mar 05 12:42:45 2025

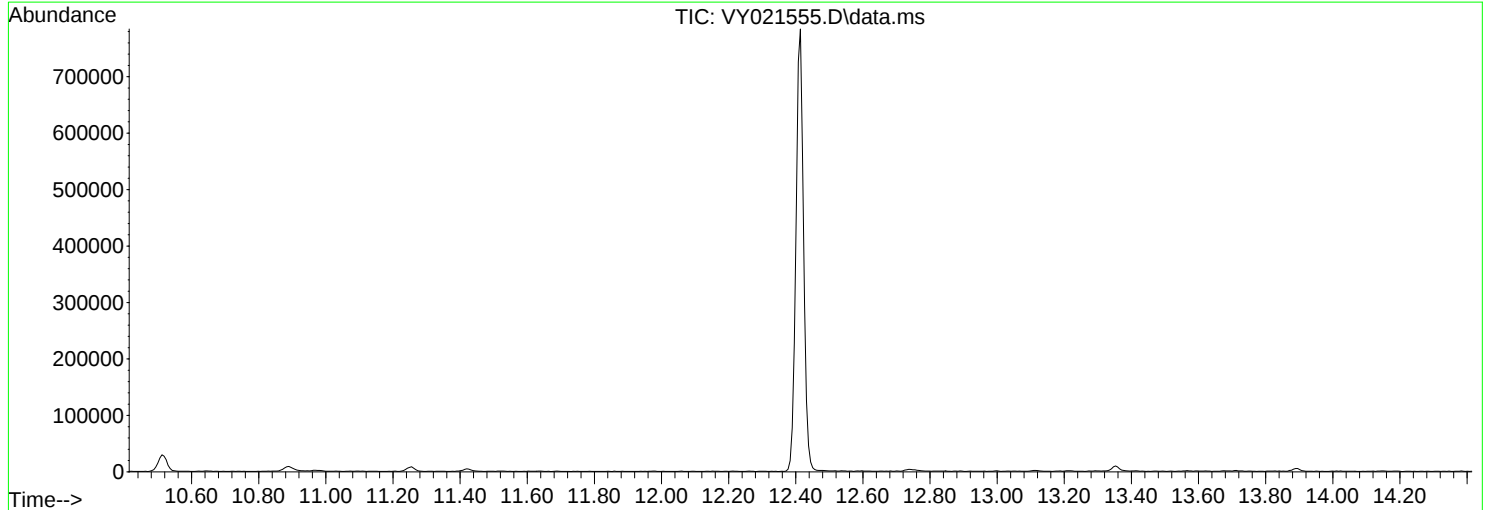

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	25885	PASS
75	95	30	60	53.2	68872	PASS
95	95	100	100	100.0	129395	PASS
96	95	5	9	6.4	8294	PASS
173	174	0.00	2	1.7	1860	PASS
174	95	50	100	84.3	109043	PASS
175	174	5	9	7.8	8502	PASS
176	174	95	101	95.4	104080	PASS
177	176	5	9	6.5	6776	PASS