
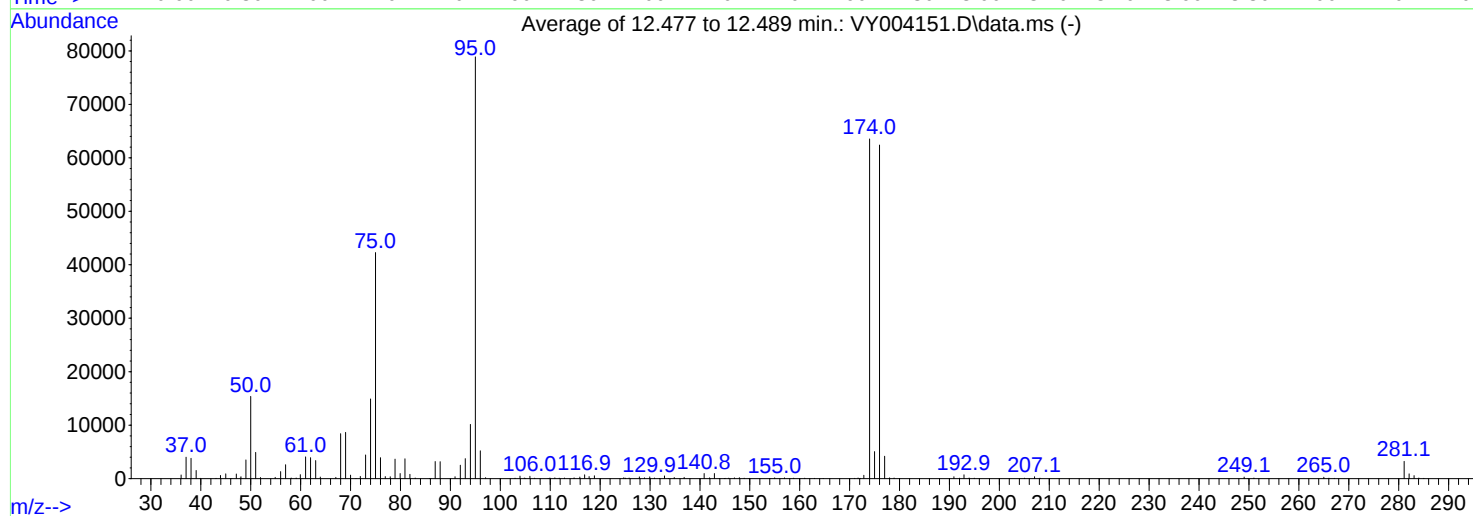


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY032221\  
 Data File : VY004151.D  
 Acq On : 22 Mar 2021 09:29  
 Operator : SY/MD  
 Sample : BFB  
 Misc : 5.00g/5mL/MSVOA\_Y/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y0308215.M  
 Title : SW846 8260  
 Last Update : Mon Mar 08 12:28:55 2021

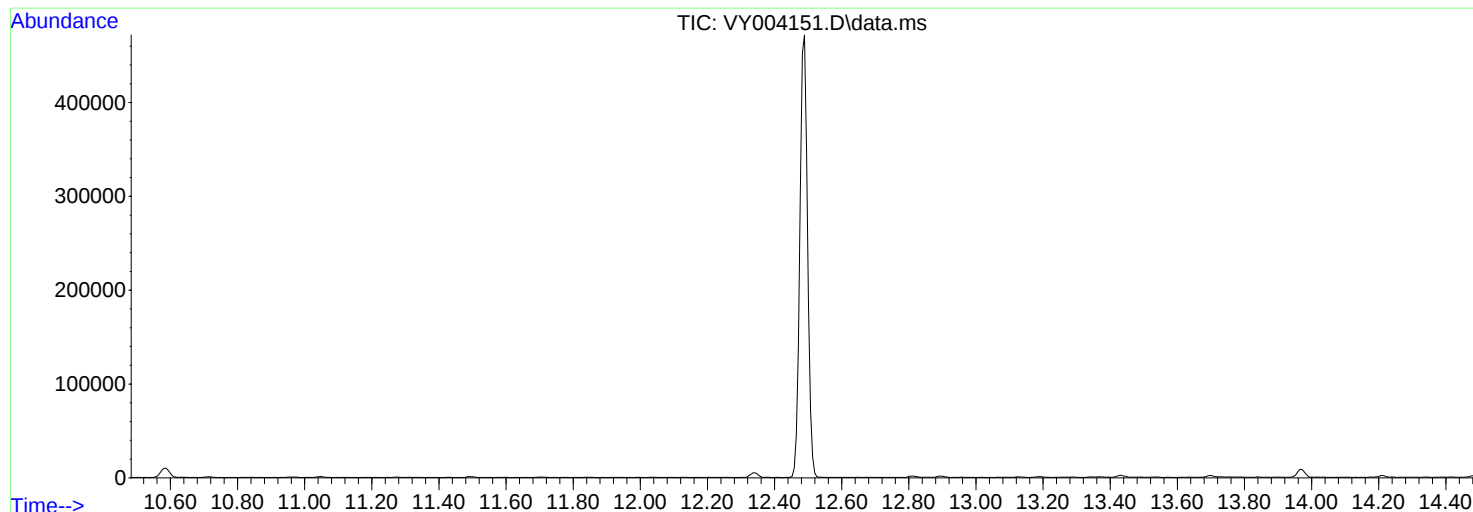

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1741

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 19.5         | 15380      | PASS                |
| 75             | 95              | 30              | 60              | 53.6         | 42296      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 78885      | PASS                |
| 96             | 95              | 5               | 9               | 6.6          | 5205       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.0          | 643        | PASS                |
| 174            | 95              | 50              | 100             | 80.5         | 63536      | PASS                |
| 175            | 174             | 5               | 9               | 8.0          | 5068       | PASS                |
| 176            | 174             | 95              | 101             | 98.2         | 62392      | PASS                |
| 177            | 176             | 5               | 9               | 6.7          | 4201       | PASS                |