

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY032321\
 Data File : VY004166.D
 Acq On : 23 Mar 2021 10:05
 Operator : SY/MD
 Sample : VY0323SBL01
 Misc : 5.00g/5mL/MSVOA_Y/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0323SBL01

Quant Time: Mar 24 01:16:40 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030821S.M
 Quant Title : SW846 8260
 QLast Update : Mon Mar 08 12:28:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.801	168	208968	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	354188	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.496	117	339576	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	169971	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	116298	56.39	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	112.78%
35) Dibromofluoromethane	7.728	113	108951	54.55	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	109.10%
50) Toluene-d8	10.185	98	422422	53.95	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	107.90%
62) 4-Bromofluorobenzene	12.483	95	157412	54.43	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	108.86%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY032321\
Data File : VY004166.D
Acq On : 23 Mar 2021 10:05
Operator : SY/MD
Sample : VY0323SBL01
Misc : 5.00g/5mL/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0323SBL01

Quant Time: Mar 24 01:16:40 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030821S.M
Quant Title : SW846 8260
QLast Update : Mon Mar 08 12:28:55 2021
Response via : Initial Calibration




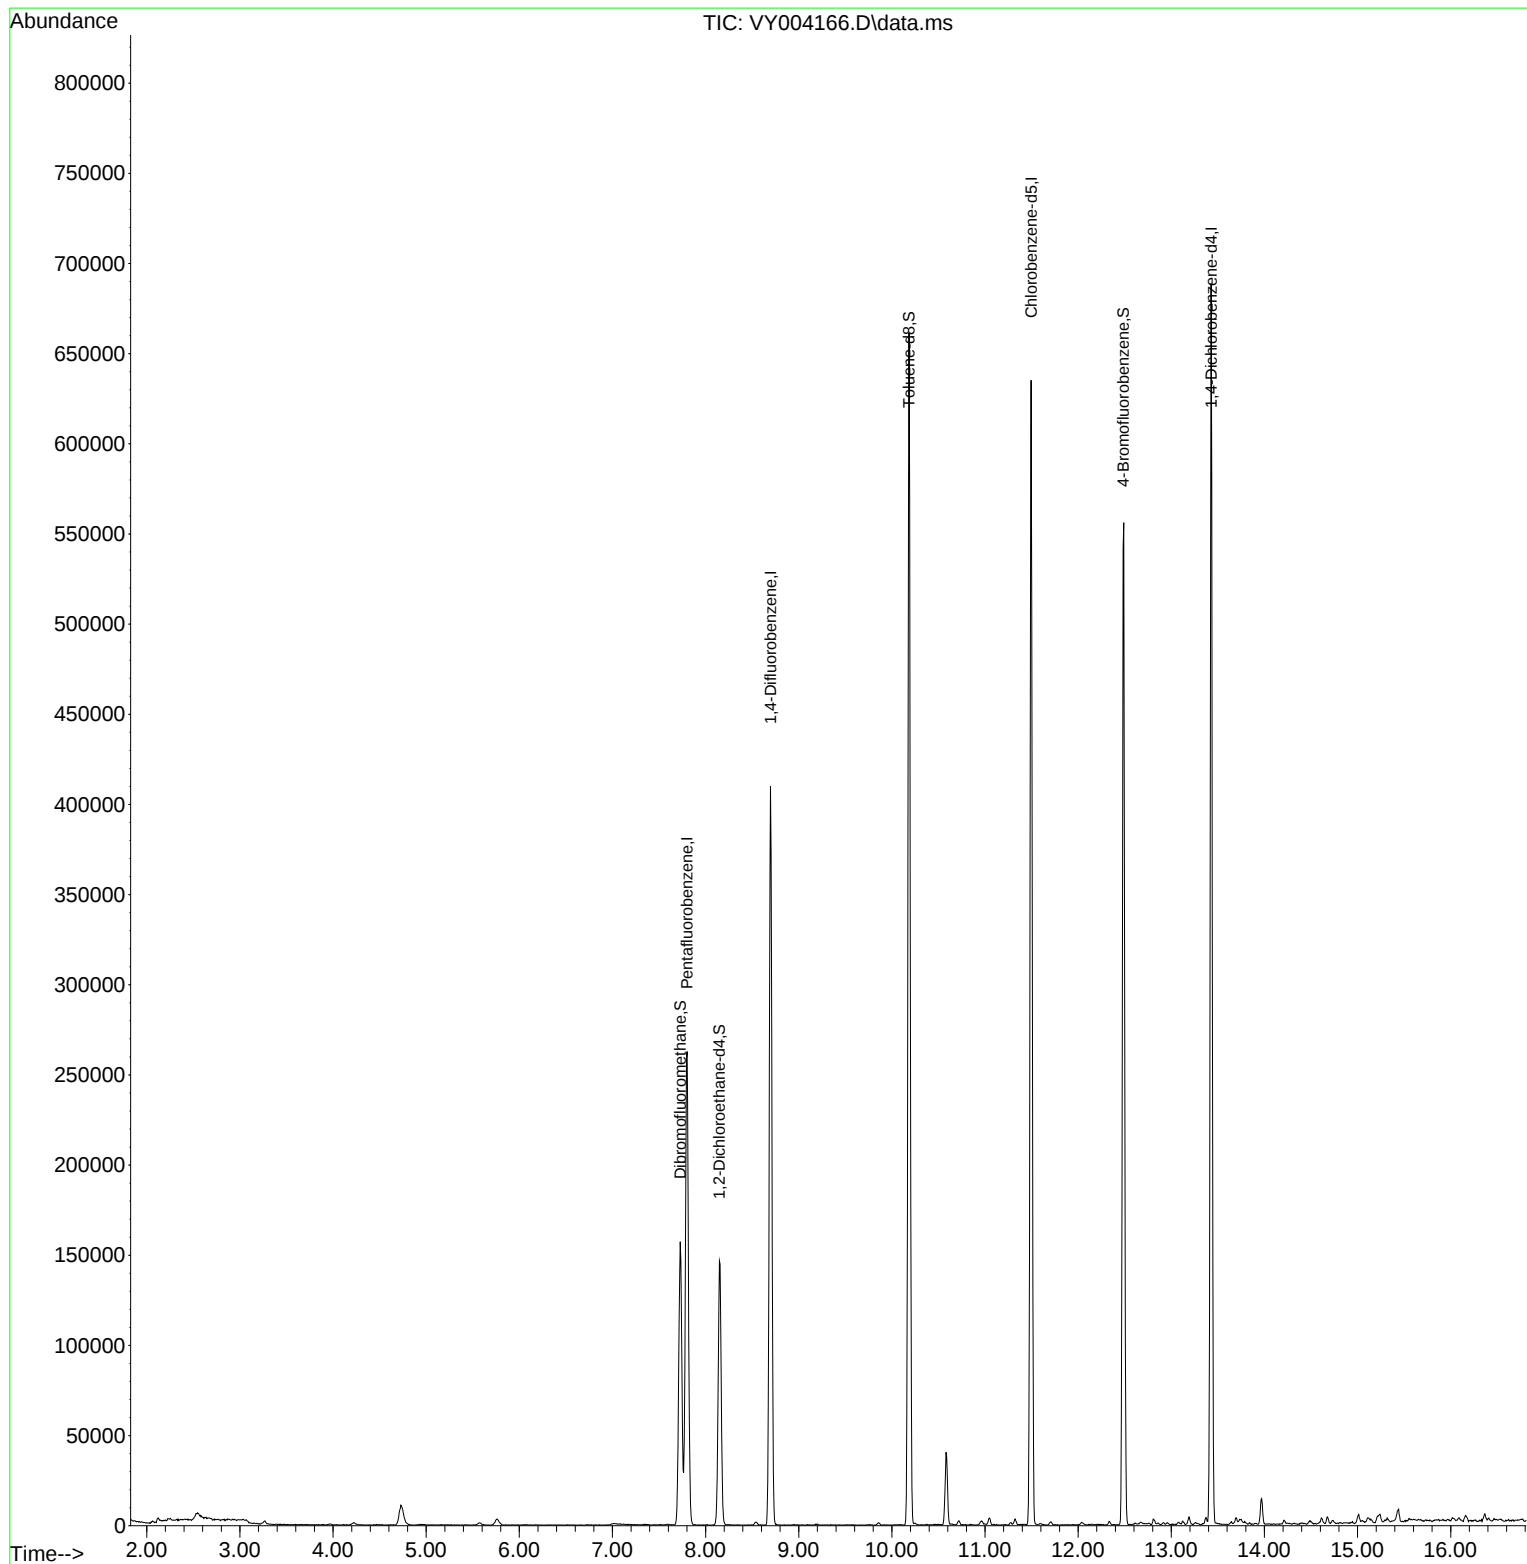




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.801 min Scan# 981
Delta R.T. 0.000 min
Lab File: VY004166.D
Acq: 23 Mar 2021 10:05




Instrument :
MSVOA_Y
ClientSampleId :
VY0323SBL01


Tgt Ion:168 Resp: 208968
Ion Ratio Lower Upper
168 100
99 53.3 41.2 61.8

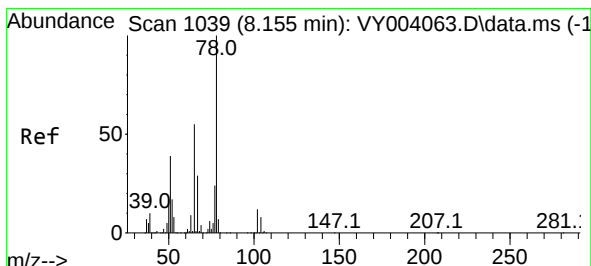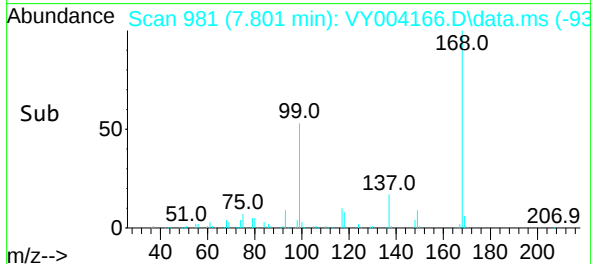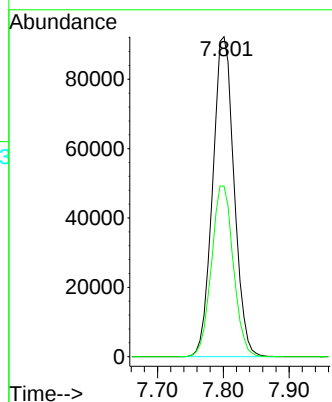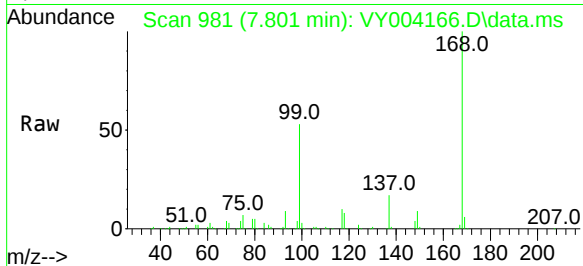

#33
1,2-Dichloroethane-d4
Concen: 56.39 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. -0.006 min
Lab File: VY004166.D
Acq: 23 Mar 2021 10:05

Tgt Ion: 65 Resp: 116298
Ion Ratio Lower Upper
65 100
67 51.8 0.0 101.4

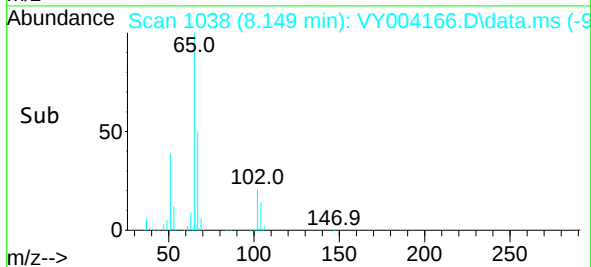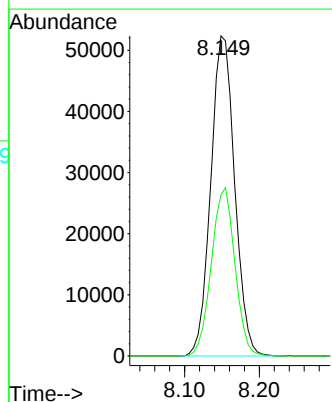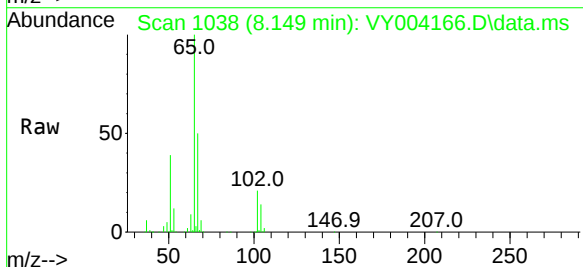

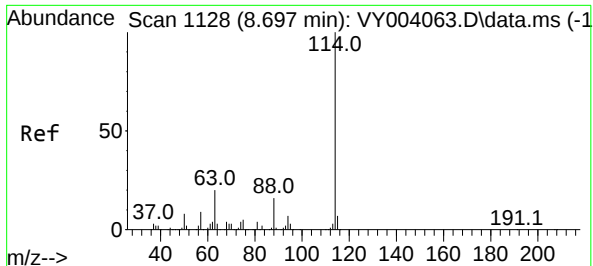

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 8.697 min Scan# 1128

Delta R.T. 0.000 min

Lab File: VY004166.D

Acq: 23 Mar 2021 10:05





Tgt Ion:114 Resp: 354188

Ion Ratio Lower Upper

114 100

63 19.1 0.0 41.6

88 15.8 0.0 31.4

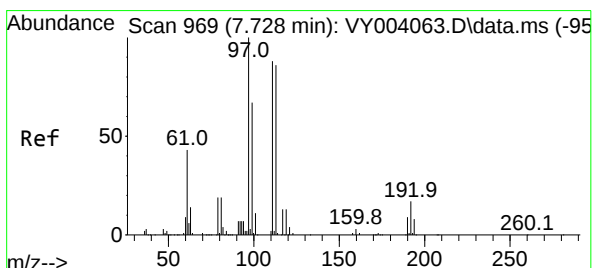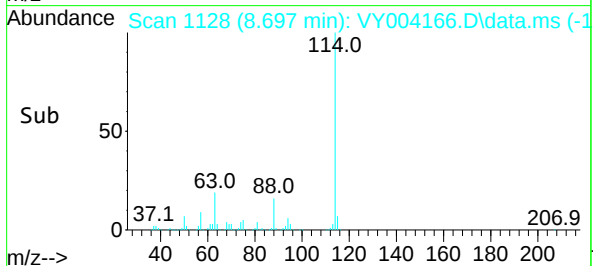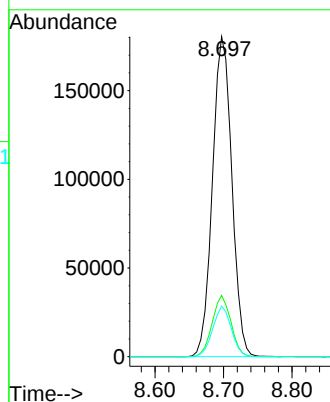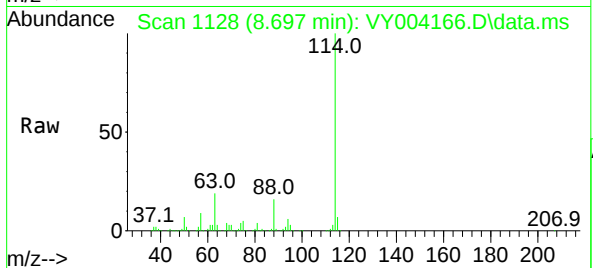

#35

Dibromofluoromethane

Concen: 54.55 ug/l

RT: 7.728 min Scan# 969

Delta R.T. -0.000 min

Lab File: VY004166.D

Acq: 23 Mar 2021 10:05




Tgt Ion:113 Resp: 108951


Ion Ratio Lower Upper

113 100

111 102.6 83.2 124.8

192 20.4 18.5 27.7


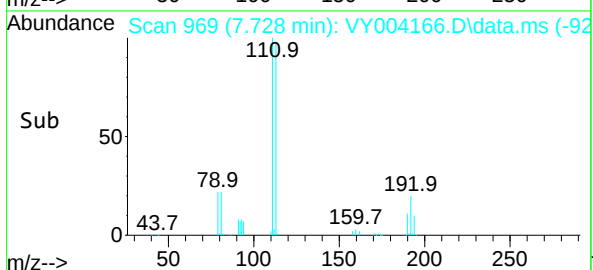
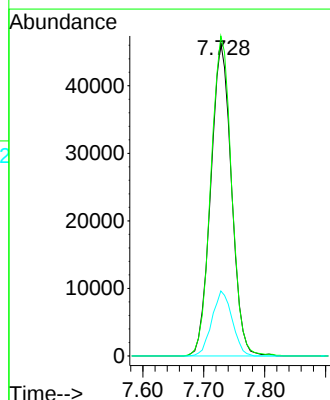
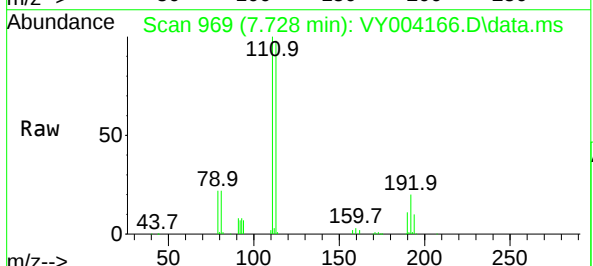


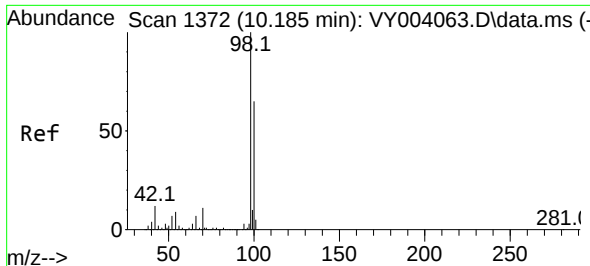

#50
Toluene-d8
Concen: 53.95 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. -0.000 min
Lab File: VY004166.D
Acq: 23 Mar 2021 10:05




Instrument :
MSVOA_Y
ClientSampleId :
VY0323SBL01


Tgt Ion: 98 Resp: 422422
Ion Ratio Lower Upper
98 100
100 65.3 51.8 77.6

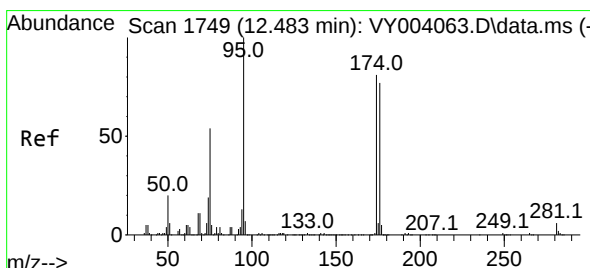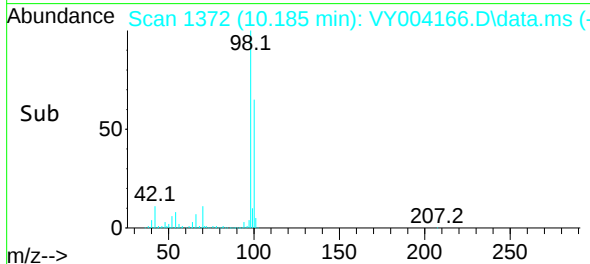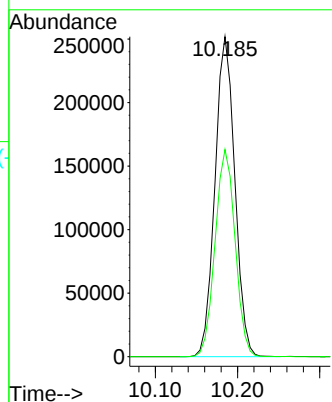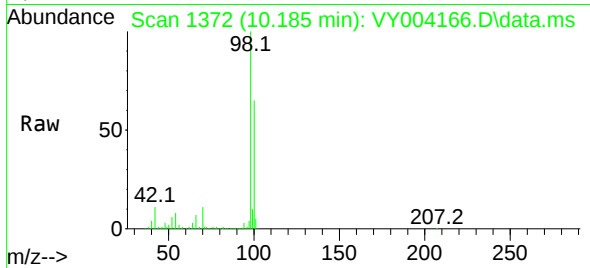

#62
4-Bromofluorobenzene
Concen: 54.43 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY004166.D
Acq: 23 Mar 2021 10:05

Tgt Ion: 95 Resp: 157412
Ion Ratio Lower Upper
95 100
174 86.0 0.0 179.0
176 83.4 0.0 174.4


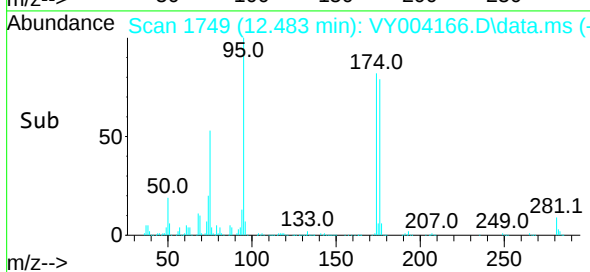
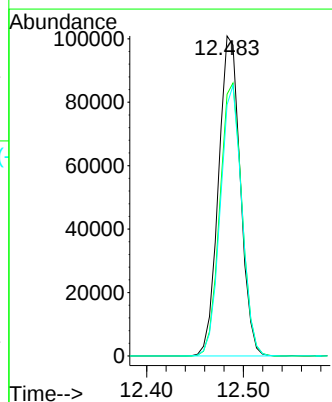
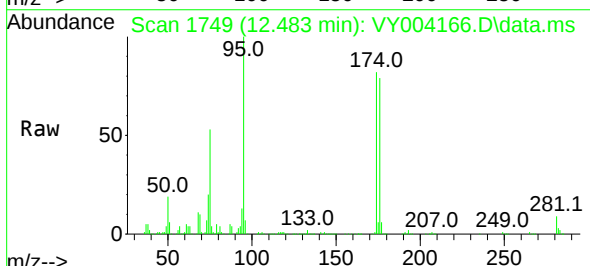


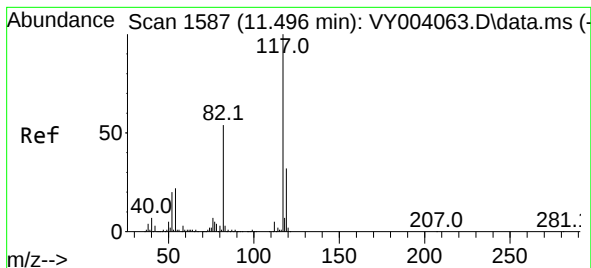

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.496 min Scan# 1587
Delta R.T. -0.001 min
Lab File: VY004166.D
Acq: 23 Mar 2021 10:05

Instrument :
MSVOA_Y
ClientSampleId :
VY0323SBL01

Tgt Ion:117 Resp: 339576
Ion Ratio Lower Upper
117 100
82 51.9 43.8 65.6
119 33.1 26.2 39.2

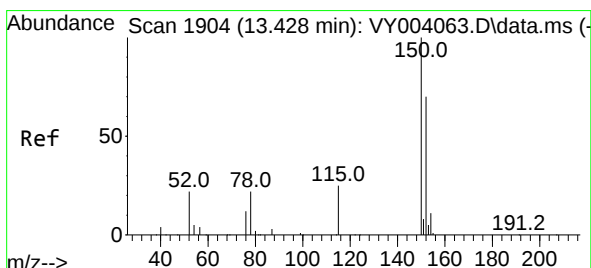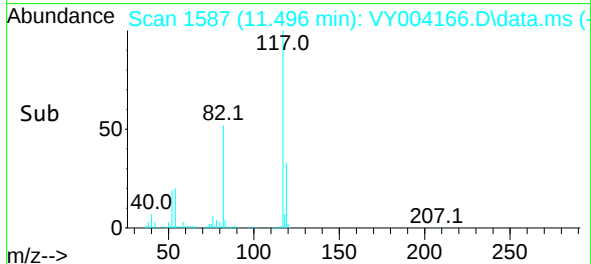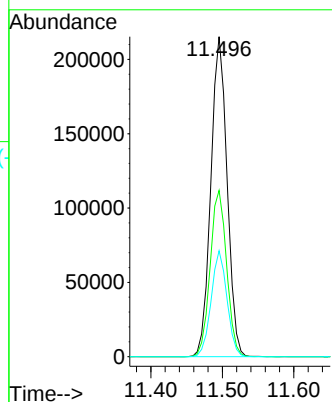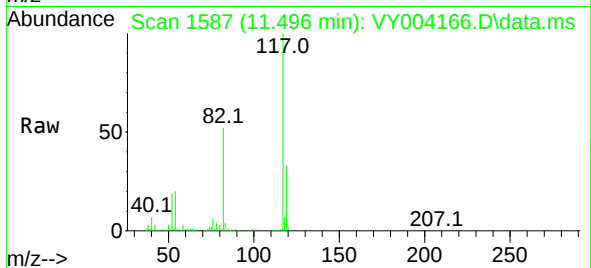

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY004166.D
Acq: 23 Mar 2021 10:05

Tgt Ion:152 Resp: 169971
Ion Ratio Lower Upper
152 100
115 57.4 28.2 84.6
150 155.7 0.0 347.2

