


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv032420\
 Data File : VY002040.D
 Acq On : 24 Mar 2020 09:27
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y030420S.M
 Title : SW846 8260
 Last Update : Thu Mar 05 04:05:33 2020

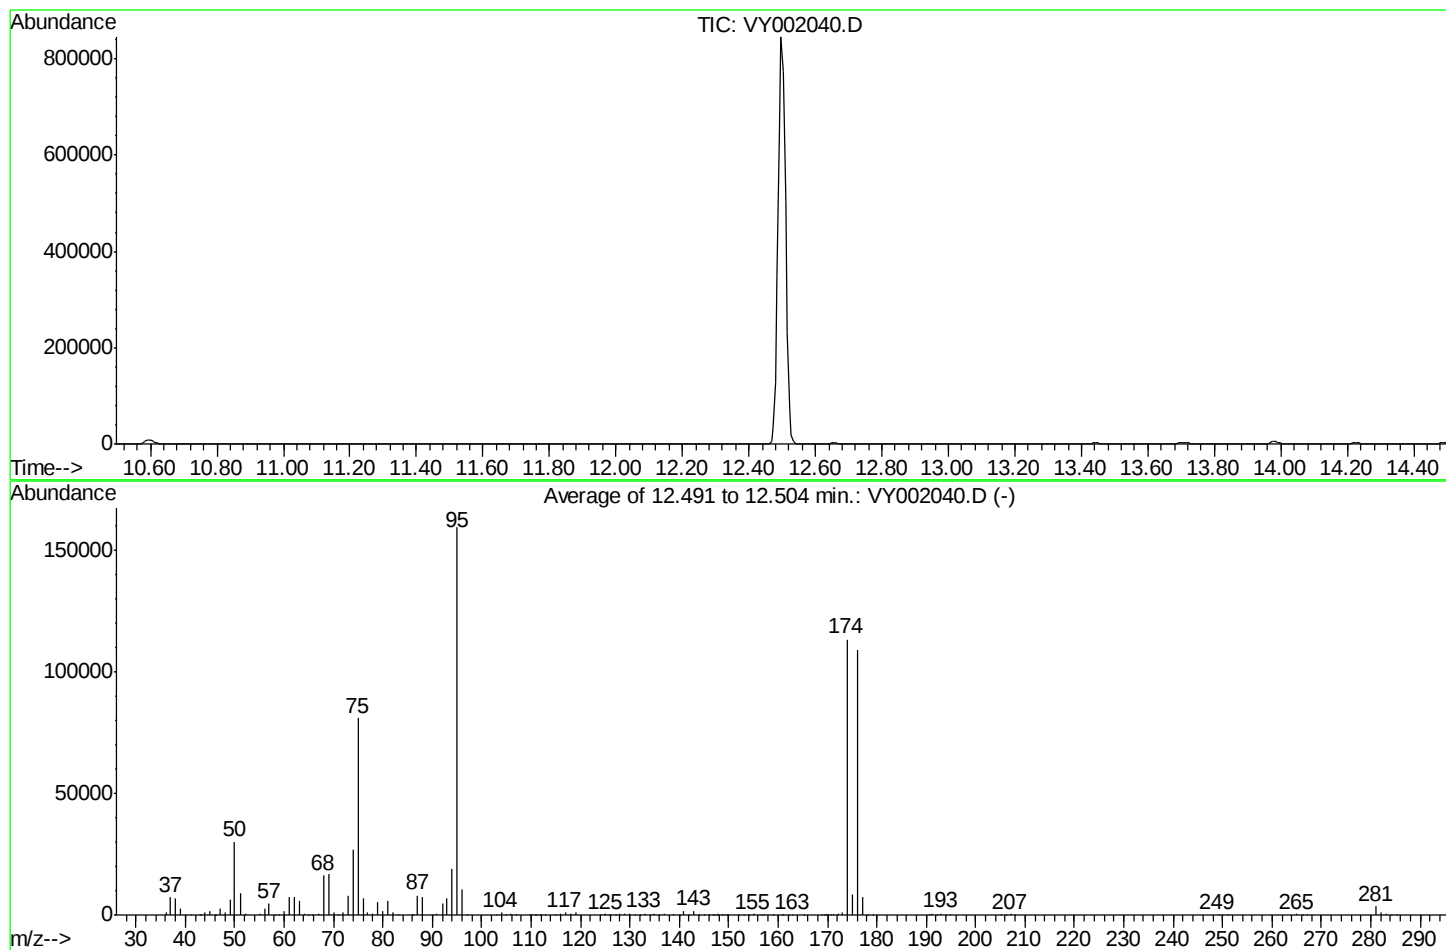

AutoFind: Scans 1764, 1765, 1766; Background Corrected with Scan 1756

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	30133	PASS
75	95	30	60	50.7	80853	PASS
95	95	100	100	100.0	159402	PASS
96	95	5	9	6.7	10728	PASS
173	174	0.00	2	0.8	960	PASS
174	95	50	100	71.1	113360	PASS
175	174	5	9	7.5	8507	PASS
176	174	95	101	96.3	109189	PASS
177	176	5	9	6.9	7535	PASS