

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY032425\
 Data File : VY021617.D
 Acq On : 24 Mar 2025 14:51
 Operator : SY/MD
 Sample : Q1614-01
 Misc : 5.10g/5.0mL/MSVOA_Y/SOIL/B
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 TR-04-032025RE

Quant Time: Mar 25 01:30:48 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030425S.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 05 12:42:45 2025
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.713	168	2755	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.615	114	4424	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.420	117	2655	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	504	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.054	65	2126	73.012	ug/l	-0.01
Spiked Amount	50.000	Range 50 - 163	Recovery	= 146.020%		
35) Dibromofluoromethane	7.628	113	1622	55.778	ug/l	-0.01
Spiked Amount	50.000	Range 54 - 147	Recovery	= 111.560%		
50) Toluene-d8	10.109	98	4755	43.186	ug/l	0.00
Spiked Amount	50.000	Range 58 - 134	Recovery	= 86.380%		
62) 4-Bromofluorobenzene	12.407	95	581	15.513	ug/l	0.00
Spiked Amount	50.000	Range 30 - 143	Recovery	= 31.020%		
Target Compounds						
						Qvalue
3) Chloromethane	2.074	50	389	10.914	ug/l	# 79
5) Bromomethane	2.616	94	343	12.184	ug/l	# 71
8) Diethyl Ether	3.256	74	48	3.186	ug/l	86
10) Methyl Iodide	4.006	142	336	10.649	ug/l	# 68
13) Acrolein	3.586	56	50	33.759	ug/l	# 10
15) Acrylonitrile	5.110	53	20	3.118	ug/l	# 1
16) Acetone	3.866	43	173	27.240	ug/l	# 47
18) Methyl Acetate	4.409	43	20	1.419	ug/l	# 51
25) 2-Butanone	6.957	43	28	3.187	ug/l	# 48
29) Tetrahydrofuran	7.237	42	19	3.503	ug/l	# 33
36) 1,1-Dichloropropene	7.713	75	227	4.987	ug/l	# 41
37) Ethyl Acetate	6.957	43	28	1.392	ug/l	# 68
38) Carbon Tetrachloride	7.713	117	291	5.559	ug/l	# 12
41) Methacrylonitrile	7.231	41	19	1.734	ug/l	# 24
42) 1,2-Dichloroethane	8.146	62	72	1.919	ug/l	# 75
46) Dibromomethane	9.463	93	23	1.295	ug/l	# 4
48) Methyl methacrylate	9.194	41	48	2.676	ug/l	# 13
51) 4-Methyl-2-Pentanone	9.999	43	51	2.531	ug/l	# 36
52) Toluene	10.170	92	474	5.607	ug/l	99
55) 1,1,2-Trichloroethane	10.822	97	26	1.119	ug/l	# 14
59) 2-Hexanone	10.822	43	93	6.980	ug/l	# 24
74) N-amyl acetate	12.084	43	25	2.900	ug/l	# 42
76) 1,2,3-Trichloropropane	12.407	75	353	69.506	ug/l	# 100
79) 2-Chlorotoluene	12.712	91	41	1.487	ug/l	# 40
81) trans-1,4-Dichloro-2-b...	12.407	75	353	158.008	ug/l	# 9
82) 4-Chlorotoluene	12.712	91	41	1.436	ug/l	# 41
90) Hexachloroethane	13.742	117	23	3.056	ug/l	# 12
92) 1,2-Dibromo-3-Chloropr...	14.230	75	20	19.057	ug/l	# 1
95) Naphthalene	15.145	128	237	18.222	ug/l	# 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY032425\
Data File : VY021617.D
Acq On : 24 Mar 2025 14:51
Operator : SY/MD
Sample : Q1614-01
Misc : 5.10g/5.0mL/MSVOA_Y/SOIL/B
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
TR-04-032025RE

Quant Time: Mar 25 01:30:48 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030425S.M
Quant Title : SW846 8260
QLast Update : Wed Mar 05 12:42:45 2025
Response via : Initial Calibration




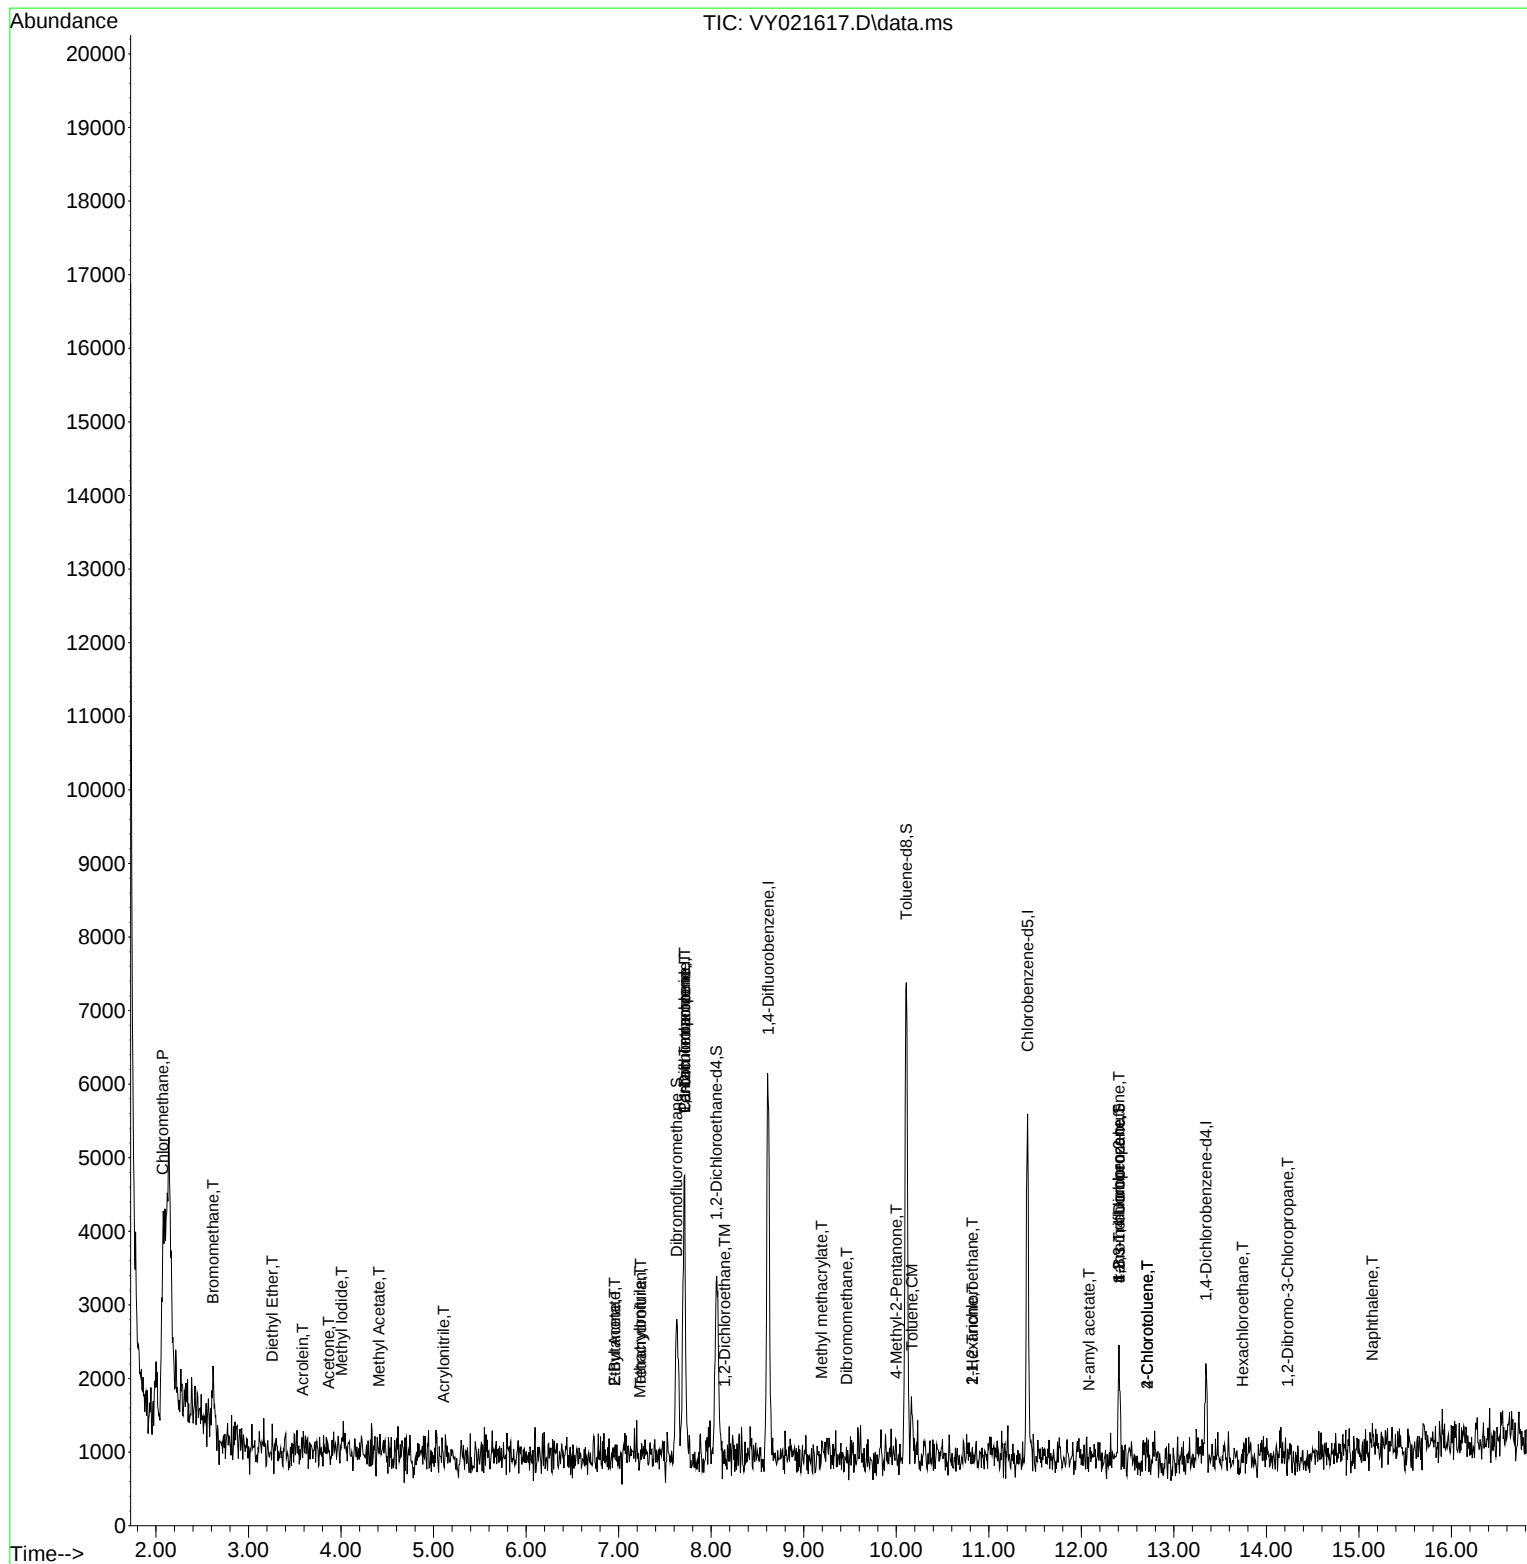




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.713 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY021617.D
Acq: 24 Mar 2025 14:51




Instrument :
MSVOA_Y
ClientSampleId :
TR-04-032025RE


Tgt Ion:168 Resp: 2755
Ion Ratio Lower Upper
168 100
99 35.9 46.0 69.0#

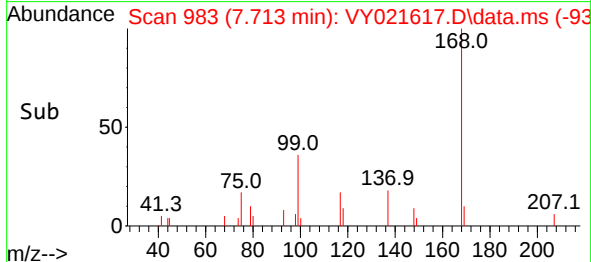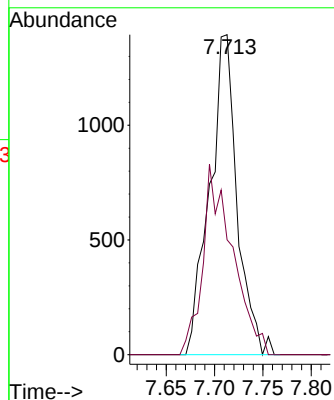

#3
Chloromethane
Concen: 10.914 ug/l
RT: 2.074 min Scan# 58
Delta R.T. -0.000 min
Lab File: VY021617.D
Acq: 24 Mar 2025 14:51

Tgt Ion: 50 Resp: 389
Ion Ratio Lower Upper
50 100
52 44.5 26.2 39.2#


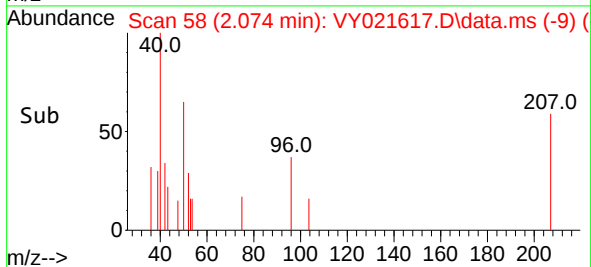
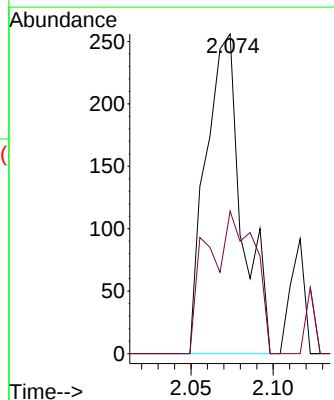
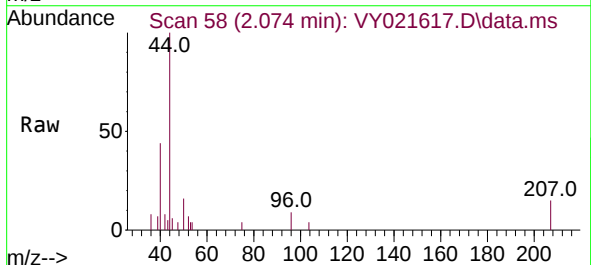


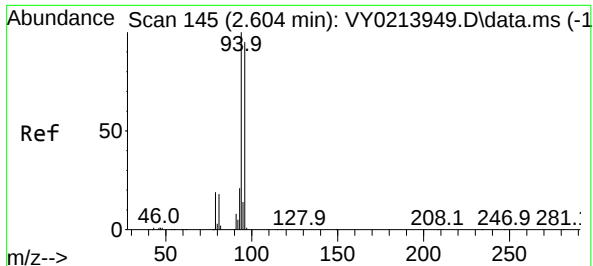

#5
Bromomethane
Concen: 12.184 ug/l
RT: 2.616 min Scan# 145
Delta R.T. 0.012 min
Lab File: VY021617.D
Acq: 24 Mar 2025 14:51




Instrument :
MSVOA_Y
ClientSampleId :
TR-04-032025RE


Tgt Ion: 94 Resp: 343
Ion Ratio Lower Upper
94 100
96 67.1 76.3 114.5#

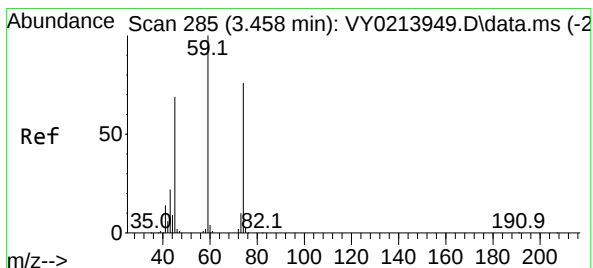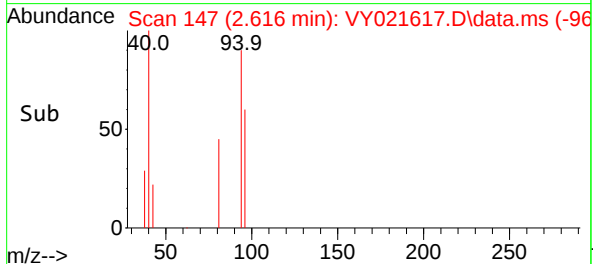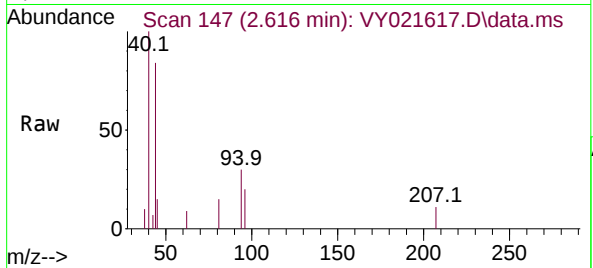

#8
Diethyl Ether
Concen: 3.186 ug/l
RT: 3.256 min Scan# 252
Delta R.T. -0.201 min
Lab File: VY021617.D
Acq: 24 Mar 2025 14:51

Tgt Ion: 74 Resp: 48
Ion Ratio Lower Upper
74 100
45 85.4 49.7 149.1


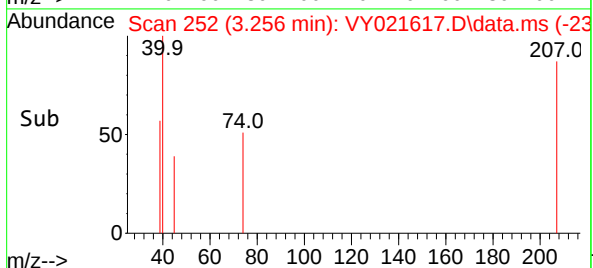

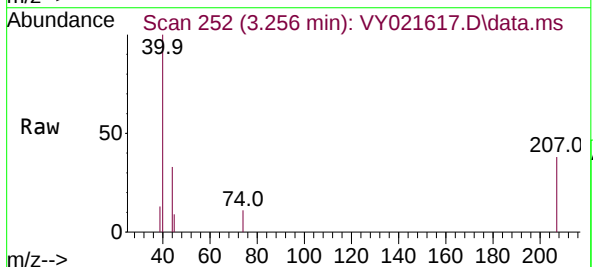




#10
Methyl Iodide
Concen: 10.649 ug/l
RT: 4.006 min Scan# 31
Delta R.T. -0.006 min
Lab File: VY021617.D
Acq: 24 Mar 2025 14:51




Instrument :
MSVOA_Y
ClientSampleId :
TR-04-032025RE


Tgt Ion:142 Resp: 336
Ion Ratio Lower Upper
142 100
127 28.0 39.1 58.7#
141 0.0 11.8 17.6#

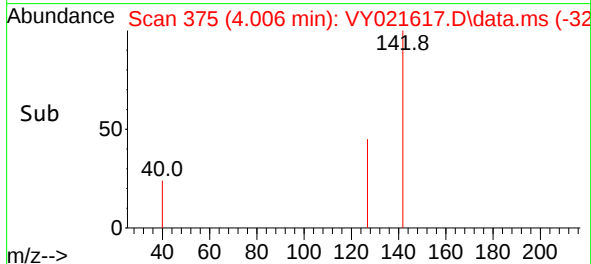

#13
Acrolein
Concen: 33.759 ug/l
RT: 3.586 min Scan# 306
Delta R.T. -0.079 min
Lab File: VY021617.D
Acq: 24 Mar 2025 14:51

Tgt Ion: 56 Resp: 50
Ion Ratio Lower Upper
56 100
55 0.0 63.4 95.2#


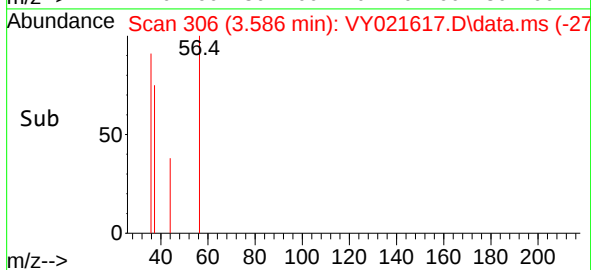

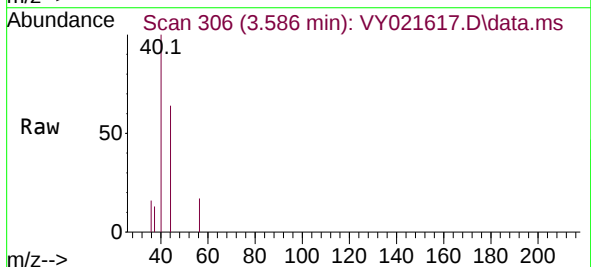




#15
Acrylonitrile
Concen: 3.118 ug/l
RT: 5.110 min Scan# 51
Delta R.T. 0.043 min
Lab File: VY021617.D
Acq: 24 Mar 2025 14:51




Instrument :
MSVOA_Y
ClientSampleId :
TR-04-032025RE


Tgt Ion: 53 Resp: 20
Ion Ratio Lower Upper
53 100
52 305.0 66.3 99.5#
51 0.0 30.3 45.5#

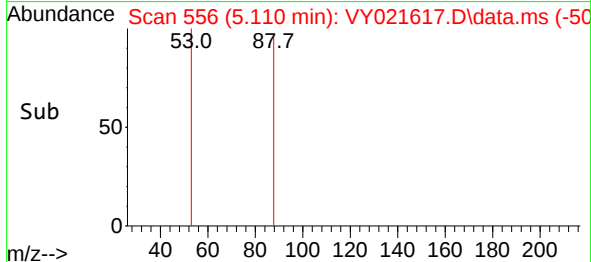

#16
Acetone
Concen: 27.240 ug/l
RT: 3.866 min Scan# 352
Delta R.T. -0.006 min
Lab File: VY021617.D
Acq: 24 Mar 2025 14:51

Tgt Ion: 43 Resp: 173
Ion Ratio Lower Upper
43 100
58 0.0 22.1 33.1#

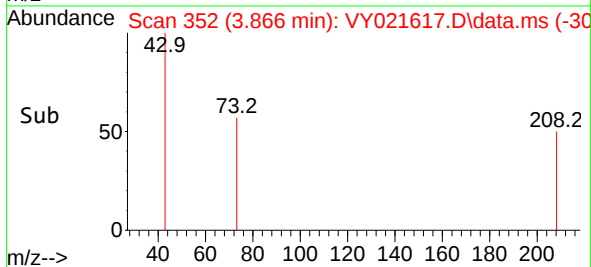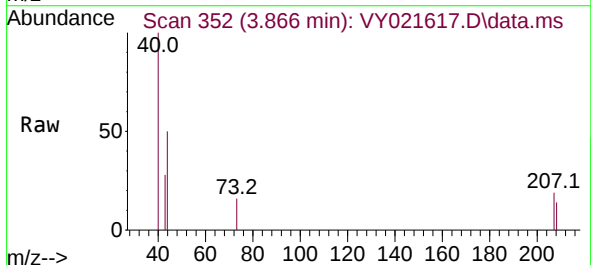



#18

Methyl Acetate

Concen: 1.419 ug/l

RT: 4.409 min Scan# 441

Delta R.T. 0.018 min

Lab File: VY021617.D

Acq: 24 Mar 2025 14:51

Instrument :

MSVOA_Y

ClientSampleId :





TR-04-032025RE

Tgt Ion: 43 Resp: 20

Ion Ratio Lower Upper

43 100

74 0.0 19.4 29.0#

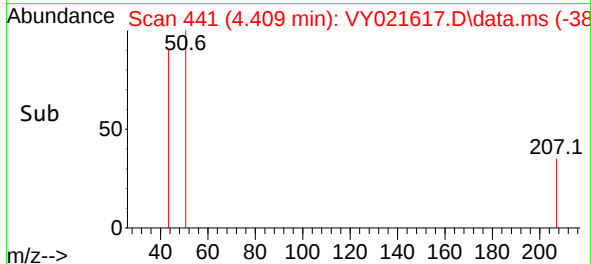

#25

2-Butanone

Concen: 3.187 ug/l

RT: 6.957 min Scan# 859

Delta R.T. 0.061 min

Lab File: VY021617.D




Acq: 24 Mar 2025 14:51


Tgt Ion: 43 Resp: 28

Ion Ratio Lower Upper

43 100

72 0.0 21.4 32.0#

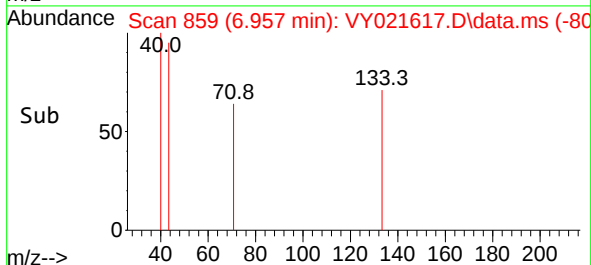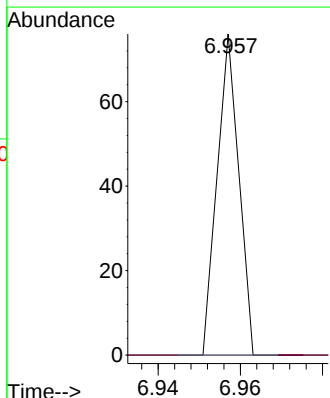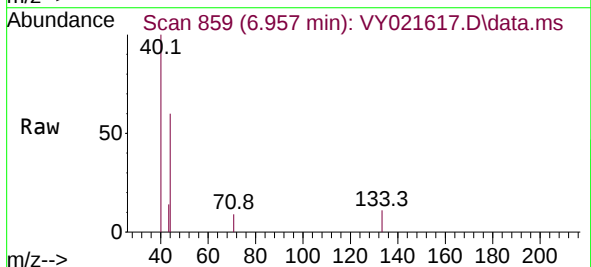



#29

Tetrahydrofuran

Concen: 3.503 ug/l

RT: 7.237 min Scan# 90

Delta R.T. -0.031 min

Lab File: VY021617.D


Acq: 24 Mar 2025 14:51

Instrument :

MSVOA_Y

ClientSampleId :

TR-04-032025RE






Tgt Ion: 42 Resp: 19

Ion Ratio Lower Upper

42 100

72 0.0 34.8 52.2#

71 0.0 32.6 48.8#

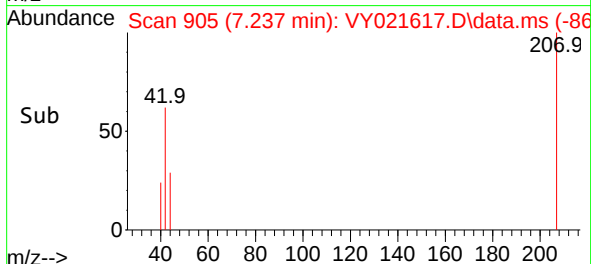

#33

1,2-Dichloroethane-d4

Concen: 73.012 ug/l

RT: 8.054 min Scan# 1039

Delta R.T. -0.012 min

Lab File: VY021617.D




Acq: 24 Mar 2025 14:51


Tgt Ion: 65 Resp: 2126

Ion Ratio Lower Upper

65 100

67 57.7 0.0 102.8


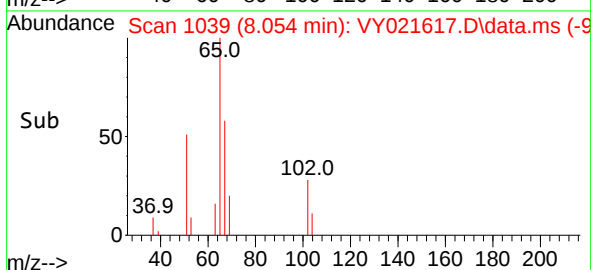




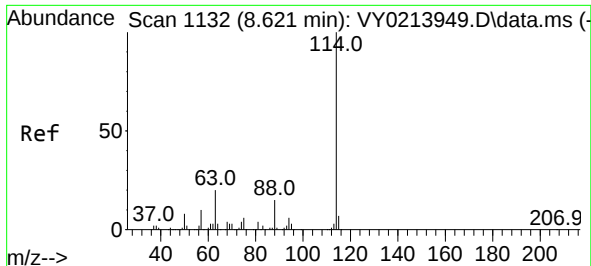

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.615 min Scan# 1132
Delta R.T. -0.006 min
Lab File: VY021617.D
Acq: 24 Mar 2025 14:51




Instrument :
MSVOA_Y
ClientSampleId :
TR-04-032025RE


Tgt Ion:114	Resp:	4424
Ion	Ratio	Lower Upper
114	100	
63	26.5	0.0 40.8
88	9.8	0.0 30.8

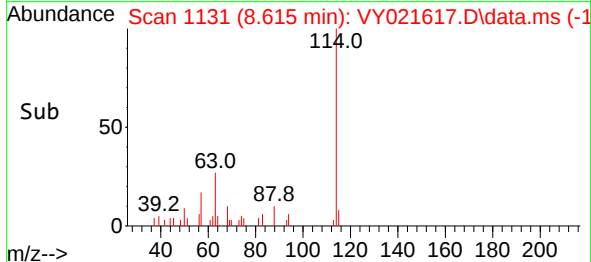

#35
Dibromofluoromethane
Concen: 55.778 ug/l
RT: 7.628 min Scan# 969
Delta R.T. -0.012 min
Lab File: VY021617.D
Acq: 24 Mar 2025 14:51

Tgt Ion:113	Resp:	1622
Ion	Ratio	Lower Upper
113	100	
111	88.0	82.0 123.0
192	22.7	15.9 23.9


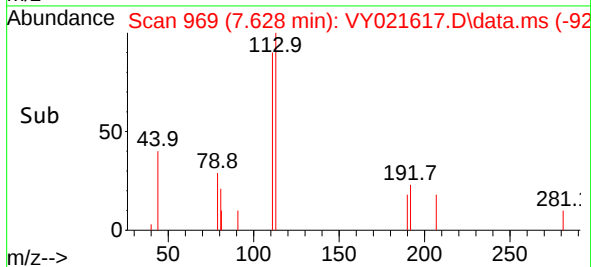

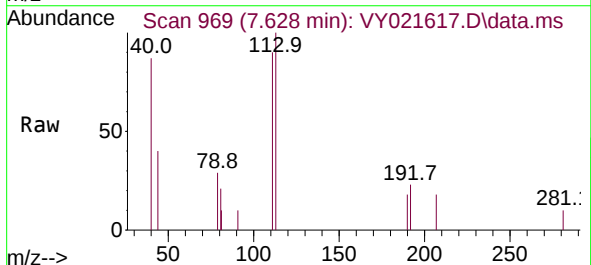




#36
1,1-Dichloropropene
Concen: 4.987 ug/l
RT: 7.713 min Scan# 911
Delta R.T. -0.128 min
Lab File: VY021617.D
Acq: 24 Mar 2025 14:51




Instrument :
MSVOA_Y
ClientSampleId :
TR-04-032025RE


Tgt Ion: 75 Resp: 227
Ion Ratio Lower Upper
75 100
110 0.0 17.3 51.7#
77 0.0 25.4 38.2#

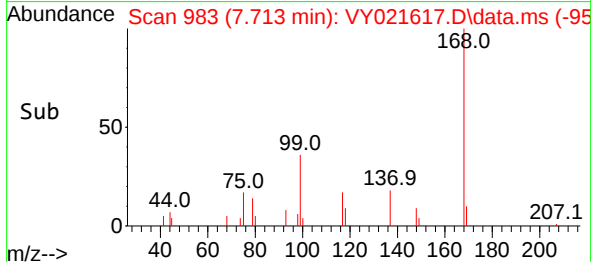

#37
Ethyl Acetate
Concen: 1.392 ug/l
RT: 6.957 min Scan# 859
Delta R.T. -0.031 min
Lab File: VY021617.D
Acq: 24 Mar 2025 14:51

Tgt Ion: 43 Resp: 28
Ion Ratio Lower Upper
43 100
61 0.0 11.4 17.0#
70 0.0 8.2 12.2#

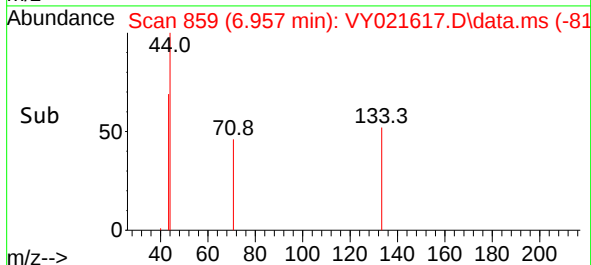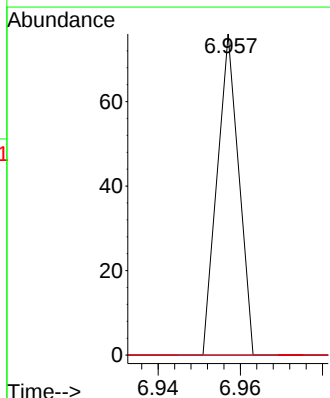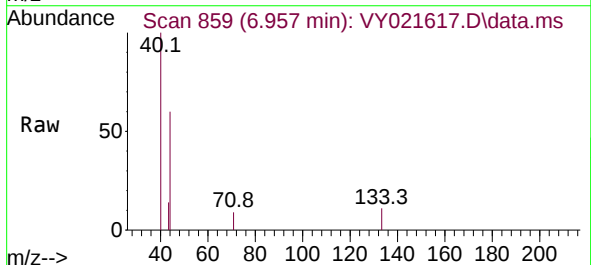



#38

Carbon Tetrachloride

Concen: 5.559 ug/l

RT: 7.713 min Scan# 901

Delta R.T. -0.110 min

Lab File: VY021617.D

Acq: 24 Mar 2025 14:51

Instrument :

MSVOA_Y

ClientSampleId :

TR-04-032025RE





Tgt Ion:117 Resp: 291

Ion Ratio Lower Upper

117 100

119 0.0 75.8 113.8#

121 0.0 23.9 35.9#

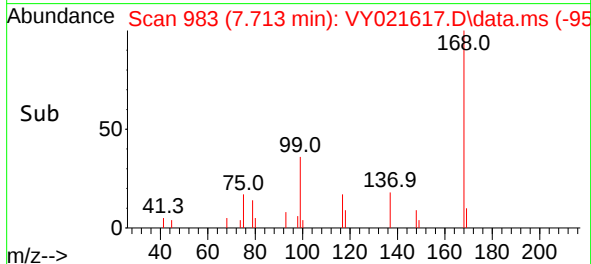

#41

Methacrylonitrile

Concen: 1.734 ug/l

RT: 7.231 min Scan# 904

Delta R.T. 0.012 min

Lab File: VY021617.D

Acq: 24 Mar 2025 14:51

Tgt Ion: 41 Resp: 19




Ion Ratio Lower Upper


41 100

39 0.0 35.0 52.6#

67 0.0 61.2 91.8#

52 0.0 26.8 40.2#

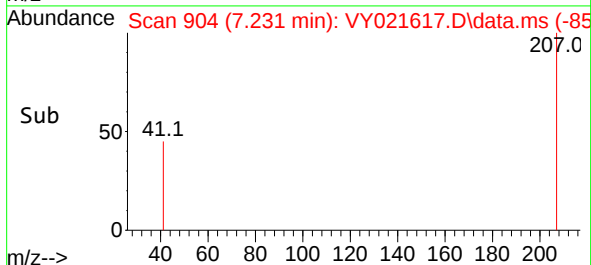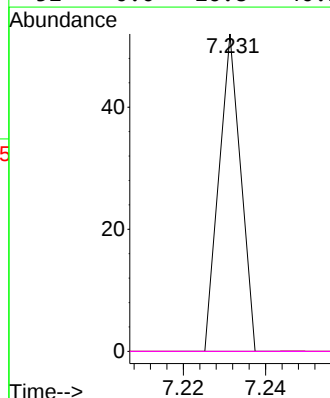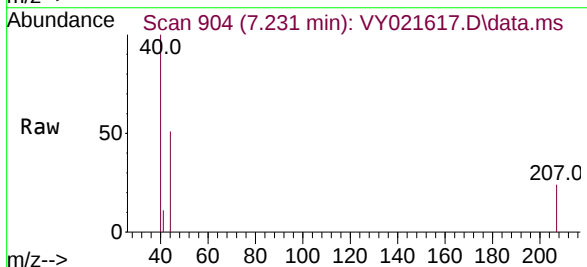



#42

1,2-Dichloroethane

Concen: 1.919 ug/l

RT: 8.146 min Scan# 110

Delta R.T. -0.018 min

Lab File: VY021617.D

Acq: 24 Mar 2025 14:51

Instrument :

MSVOA_Y

ClientSampleId :





TR-04-032025RE

Tgt Ion: 62 Resp: 72

Ion Ratio Lower Upper

62 100

98 0.0 0.0 18.2

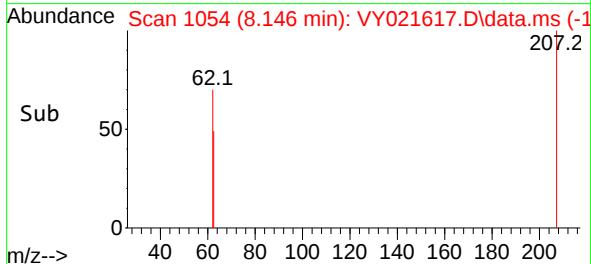

#46

Dibromomethane

Concen: 1.295 ug/l

RT: 9.463 min Scan# 1270

Delta R.T. 0.226 min

Lab File: VY021617.D

Acq: 24 Mar 2025 14:51




Tgt Ion: 93 Resp: 23


Ion Ratio Lower Upper

93 100

95 0.0 65.8 98.8#

174 0.0 77.9 116.9#

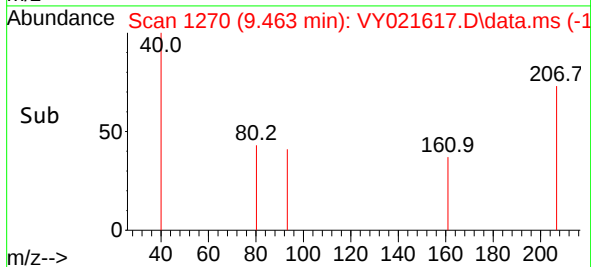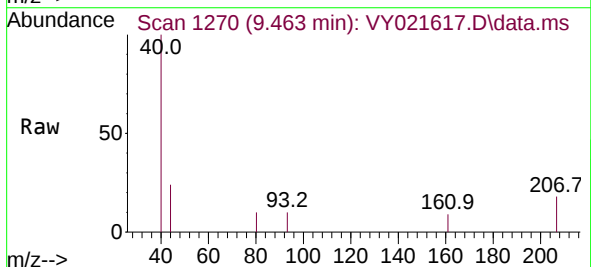



#48

Methyl methacrylate

Concen: 2.676 ug/l

RT: 9.194 min Scan# 11

Delta R.T. -0.031 min

Lab File: VY021617.D

Acq: 24 Mar 2025 14:51





Instrument :

MSVOA_Y

ClientSampleId :

TR-04-032025RE

Tgt Ion:	41	Resp:	48
Ion	Ratio	Lower	Upper
41	100		
69	0.0	67.8	101.8#
39	0.0	46.4	69.6#

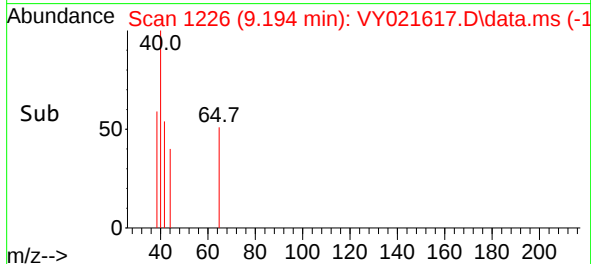

#50

Toluene-d8

Concen: 43.186 ug/l




RT: 10.109 min Scan# 1376


Delta R.T. -0.000 min

Lab File: VY021617.D

Acq: 24 Mar 2025 14:51

Tgt Ion:	98	Resp:	4755
Ion	Ratio	Lower	Upper
98	100		
100	68.6	52.1	78.1


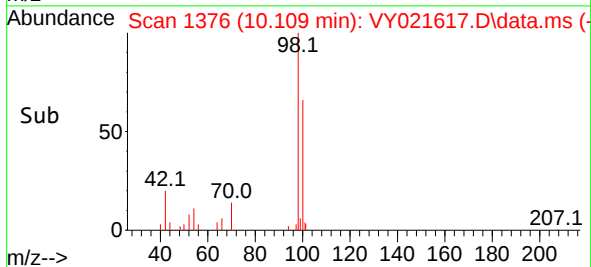

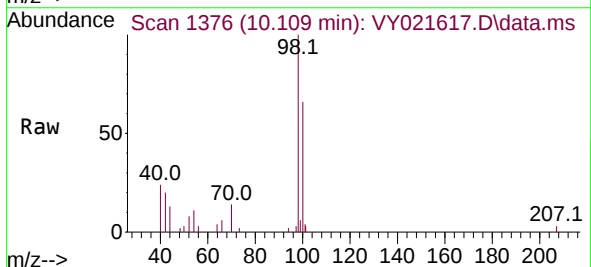




#51
4-Methyl-2-Pentanone
Concen: 2.531 ug/l
RT: 9.999 min Scan# 1358
Delta R.T. -0.000 min
Lab File: VY021617.D
Acq: 24 Mar 2025 14:51




Instrument :
MSVOA_Y
ClientSampleId :
TR-04-032025RE


Tgt Ion: 43 Resp: 51
Ion Ratio Lower Upper
43 100
58 0.0 31.4 47.2#

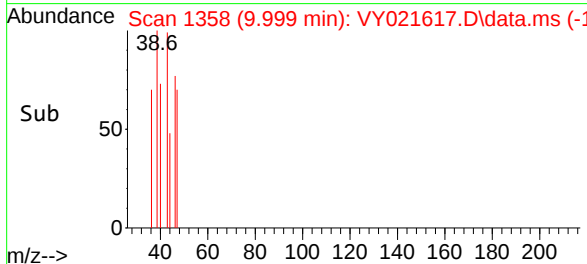

#52
Toluene
Concen: 5.607 ug/l
RT: 10.170 min Scan# 1386
Delta R.T. -0.006 min
Lab File: VY021617.D
Acq: 24 Mar 2025 14:51

Tgt Ion: 92 Resp: 474
Ion Ratio Lower Upper
92 100
91 171.1 138.2 207.2

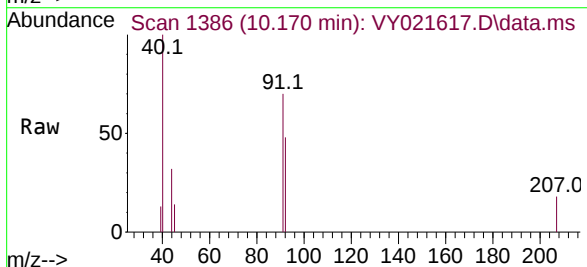

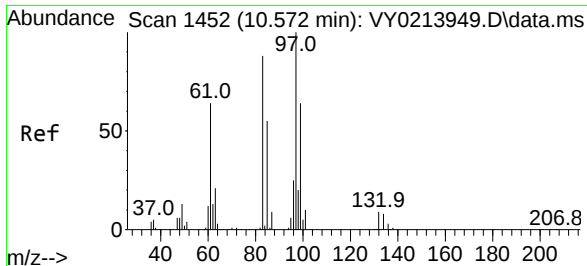

#55

1,1,2-Trichloroethane

Concen: 1.119 ug/l

RT: 10.822 min Scan# 14

Delta R.T. 0.250 min

Lab File: VY021617.D


Acq: 24 Mar 2025 14:51

Instrument :

MSVOA_Y

ClientSampleId :

TR-04-032025RE



Tgt Ion: 97 Resp: 26




Ion Ratio Lower Upper

97 100

83 0.0 70.0 105.0#

85 0.0 44.3 66.5#

99 0.0 51.4 77.0#

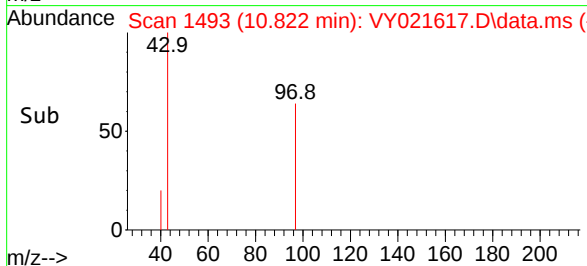

#59

2-Hexanone

Concen: 6.980 ug/l

RT: 10.822 min Scan# 1493

Delta R.T. 0.061 min

Lab File: VY021617.D




Acq: 24 Mar 2025 14:51


Tgt Ion: 43 Resp: 93

Ion Ratio Lower Upper

43 100

58 0.0 27.3 81.8#


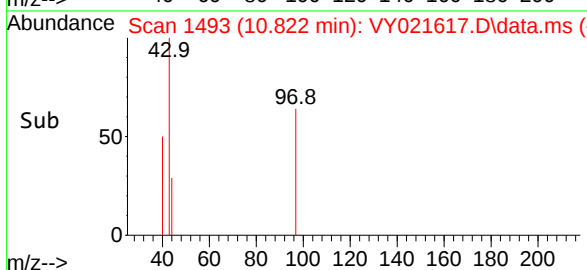

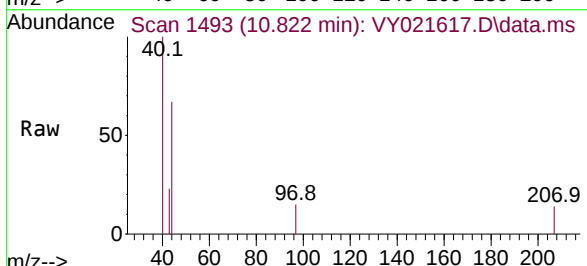


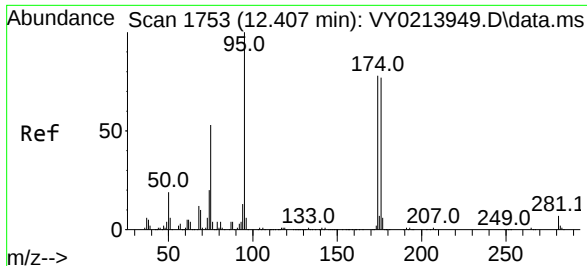

#62
4-Bromofluorobenzene
Concen: 15.513 ug/l
RT: 12.407 min Scan# 1753
Delta R.T. -0.000 min
Lab File: VY021617.D
Acq: 24 Mar 2025 14:51




Instrument :
MSVOA_Y
ClientSampleId :
TR-04-032025RE


Tgt Ion:	95	Resp:	581
Ion Ratio	Lower	Upper	
95	100		
174	88.5	0.0	165.0
176	75.0	0.0	160.0

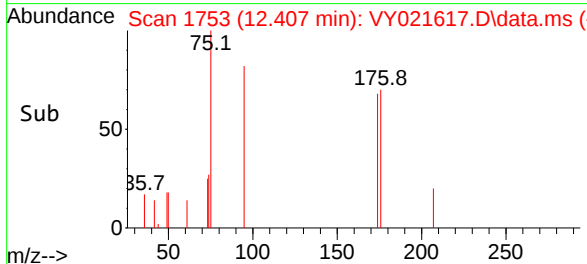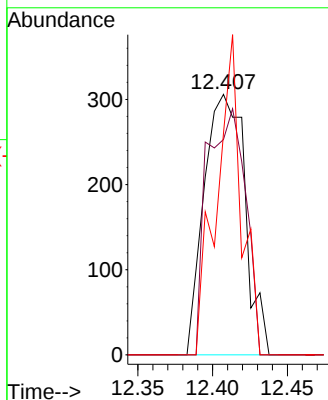

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.420 min Scan# 1591
Delta R.T. -0.000 min
Lab File: VY021617.D
Acq: 24 Mar 2025 14:51

Tgt Ion:	117	Resp:	2655
Ion Ratio	Lower	Upper	
117	100		
82	57.9	44.6	67.0
119	34.2	25.4	38.0


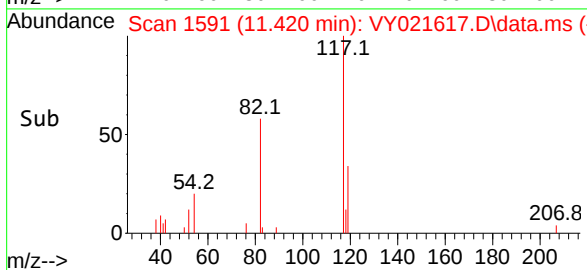
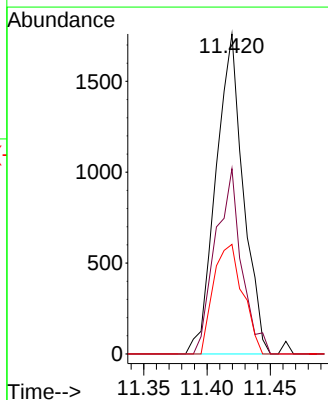
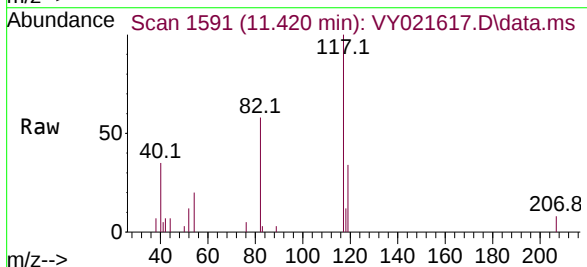


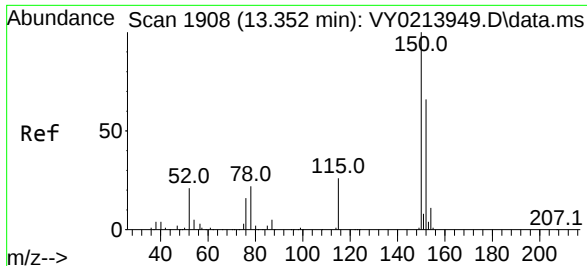

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.346 min Scan# 1908
 Delta R.T. -0.006 min
 Lab File: VY021617.D
 Acq: 24 Mar 2025 14:51




Instrument :
 MSVOA_Y
 ClientSampleId :
 TR-04-032025RE


Tgt Ion:152 Resp: 504
 Ion Ratio Lower Upper
 152 100
 115 43.3 29.0 87.0
 150 137.9 0.0 347.2

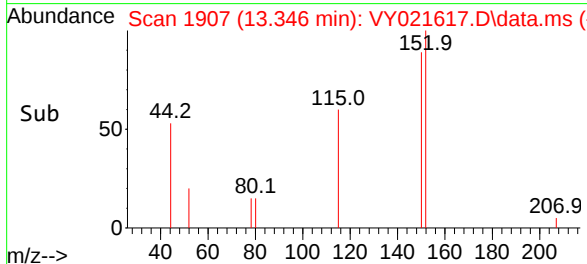

#74
 N-ethyl acetate
 Concen: 2.900 ug/l
 RT: 12.084 min Scan# 1700
 Delta R.T. 0.012 min
 Lab File: VY021617.D
 Acq: 24 Mar 2025 14:51

Tgt Ion: 43 Resp: 25
 Ion Ratio Lower Upper
 43 100
 70 0.0 34.6 51.8#
 55 0.0 21.1 31.7#
 61 0.0 19.4 29.0#


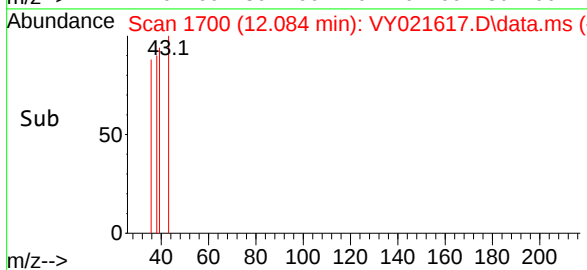

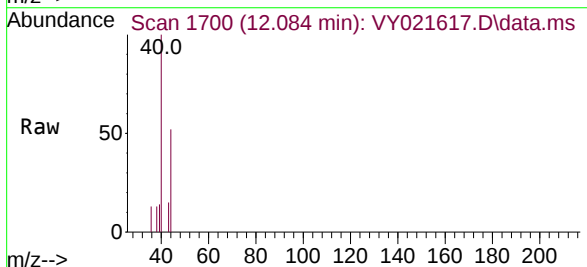


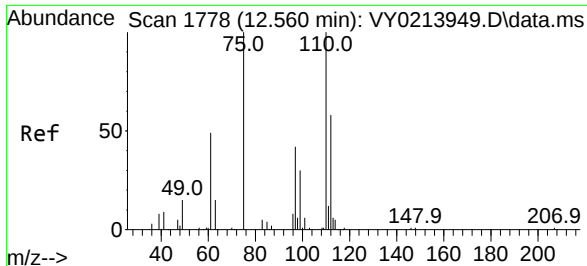

#76
1,2,3-Trichloropropane
Concen: 69.506 ug/l
RT: 12.407 min Scan# 11
Delta R.T. -0.152 min
Lab File: VY021617.D
Acq: 24 Mar 2025 14:51




Instrument :
MSVOA_Y
ClientSampleId :
TR-04-032025RE


Tgt Ion: 75 Resp: 353
Ion Ratio Lower Upper
75 100
77 0.0 0.0 0.0

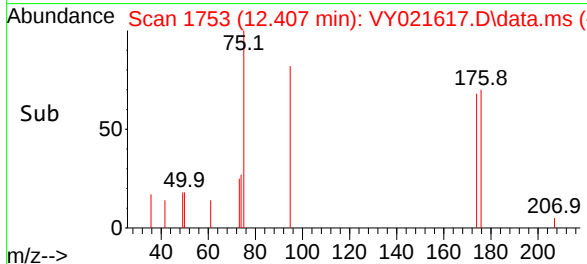

#79
2-Chlorotoluene
Concen: 1.487 ug/l
RT: 12.712 min Scan# 1803
Delta R.T. 0.030 min
Lab File: VY021617.D
Acq: 24 Mar 2025 14:51

Tgt Ion: 91 Resp: 41
Ion Ratio Lower Upper
91 100
126 0.0 17.2 51.6#


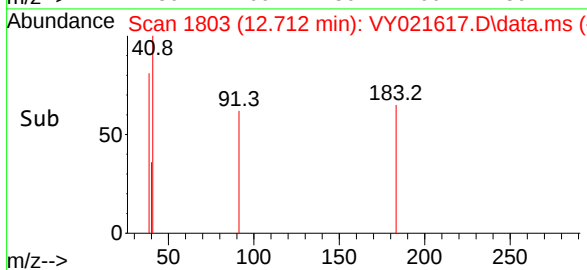

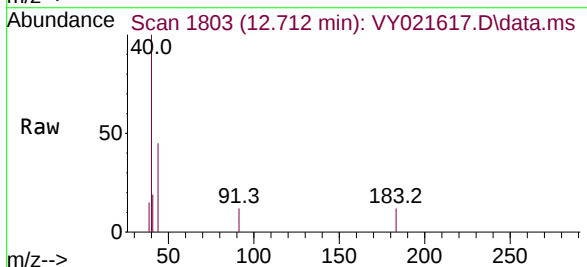


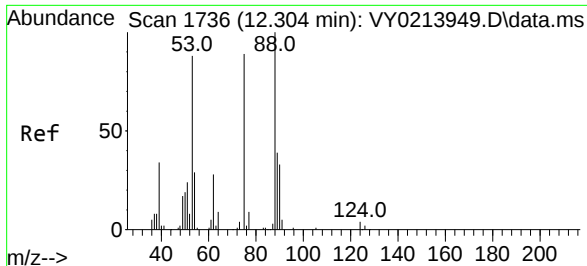

#81
trans-1,4-Dichloro-2-butene
Concen: 158.008 ug/l
RT: 12.407 min Scan# 11
Delta R.T. 0.104 min
Lab File: VY021617.D
Acq: 24 Mar 2025 14:51




Instrument :
MSVOA_Y
ClientSampleId :
TR-04-032025RE


Tgt Ion: 75 Resp: 353
Ion Ratio Lower Upper
75 100
53 0.0 81.0 121.4#
89 0.0 36.9 55.3#

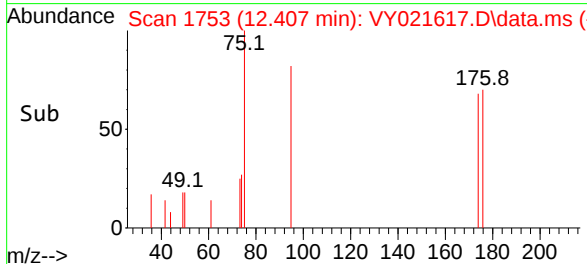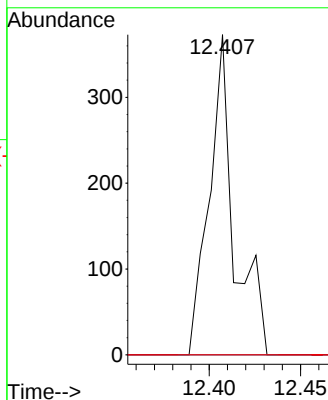

#82
4-Chlorotoluene
Concen: 1.436 ug/l
RT: 12.712 min Scan# 1803
Delta R.T. -0.067 min
Lab File: VY021617.D
Acq: 24 Mar 2025 14:51

Tgt Ion: 91 Resp: 41
Ion Ratio Lower Upper
91 100
126 0.0 17.0 51.0#


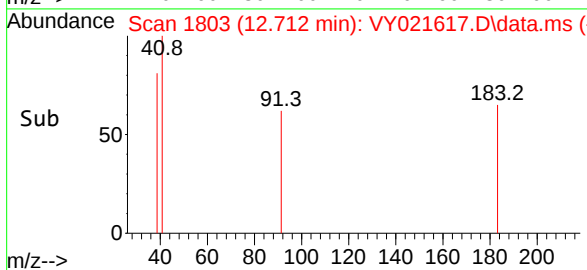
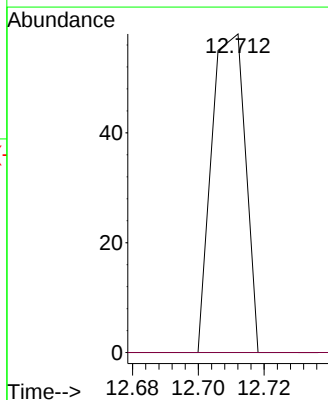
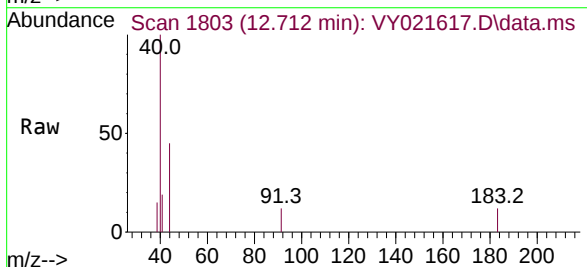


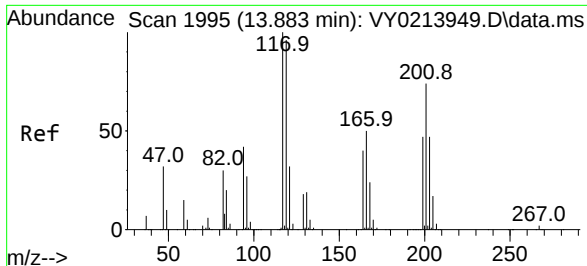

#90
Hexachloroethane
Concen: 3.056 ug/l
RT: 13.742 min Scan# 1995
Delta R.T. -0.140 min
Lab File: VY021617.D
Acq: 24 Mar 2025 14:51




Instrument :
MSVOA_Y
ClientSampleId :
TR-04-032025RE


Tgt Ion:117 Resp: 23
Ion Ratio Lower Upper
117 100
201 0.0 37.4 112.2#

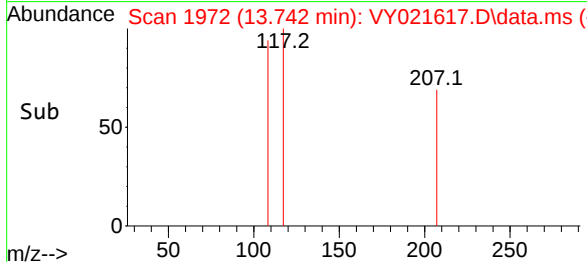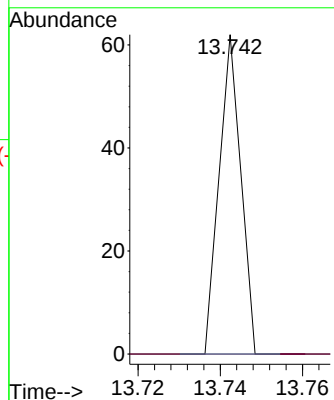

#92
1,2-Dibromo-3-Chloropropane
Concen: 19.057 ug/l
RT: 14.230 min Scan# 2052
Delta R.T. -0.049 min
Lab File: VY021617.D
Acq: 24 Mar 2025 14:51

Tgt Ion: 75 Resp: 20
Ion Ratio Lower Upper
75 100
155 0.0 43.5 130.5#
157 0.0 54.4 163.2#

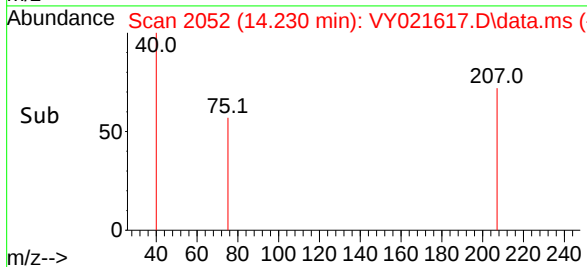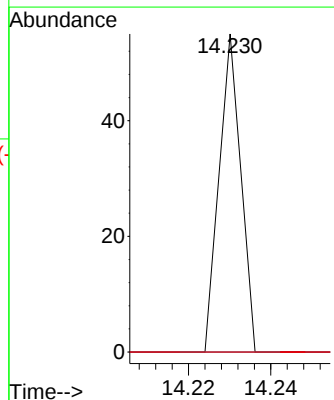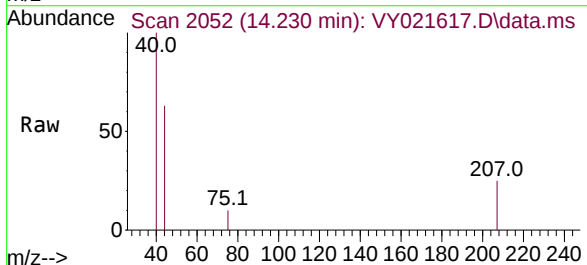



#95

Naphthalene

Concen: 18.222 ug/l

RT: 15.145 min Scan# 21

Delta R.T. -0.006 min

Lab File: VY021617.D


Acq: 24 Mar 2025 14:51

Instrument :

MSVOA_Y

ClientSampleId :

TR-04-032025RE

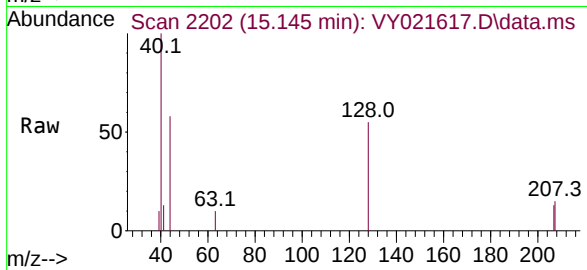

Tgt Ion:128 Resp: 237

Ion Ratio Lower Upper

128 100

127 0.0 10.6 15.8#

129 0.0 8.6 13.0#

