

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY032520\
 Data File : VY002074.D
 Acq On : 25 Mar 2020 17:59
 Operator : SY/MD
 Sample : L2037-02
 Misc : 6.28G/5ML/MSVOA Y/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 FK-BPM-01-C4-D4-C4A-D4A

Quant Time: Mar 26 08:04:59 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y030420S.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 05 04:05:33 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.82	168	131883	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.71	114	261958	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.50	117	239577	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.44	152	106671	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.16	65	85966	61.06	ug/l	0.00
Spiked Amount	50.000		Recovery	=	122.12%	
35) Dibromofluoromethane	7.74	113	77937	54.49	ug/l	0.00
Spiked Amount	50.000		Recovery	=	108.98%	
50) Toluene-d8	10.19	98	318083	52.73	ug/l	0.00
Spiked Amount	50.000		Recovery	=	105.46%	
62) 4-Bromofluorobenzene	12.49	95	109298	52.11	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.22%	


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY032520\
Data File : VY002074.D
Acq On : 25 Mar 2020 17:59
Operator : SY/MD
Sample : L2037-02
Misc : 6.28G/5ML/MSVOA Y/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
FK-BPM-01-C4-D4-C4A-D4A

Quant Time: Mar 26 08:04:59 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y030420S.M
Quant Title : SW846 8260
QLast Update : Thu Mar 05 04:05:33 2020
Response via : Initial Calibration

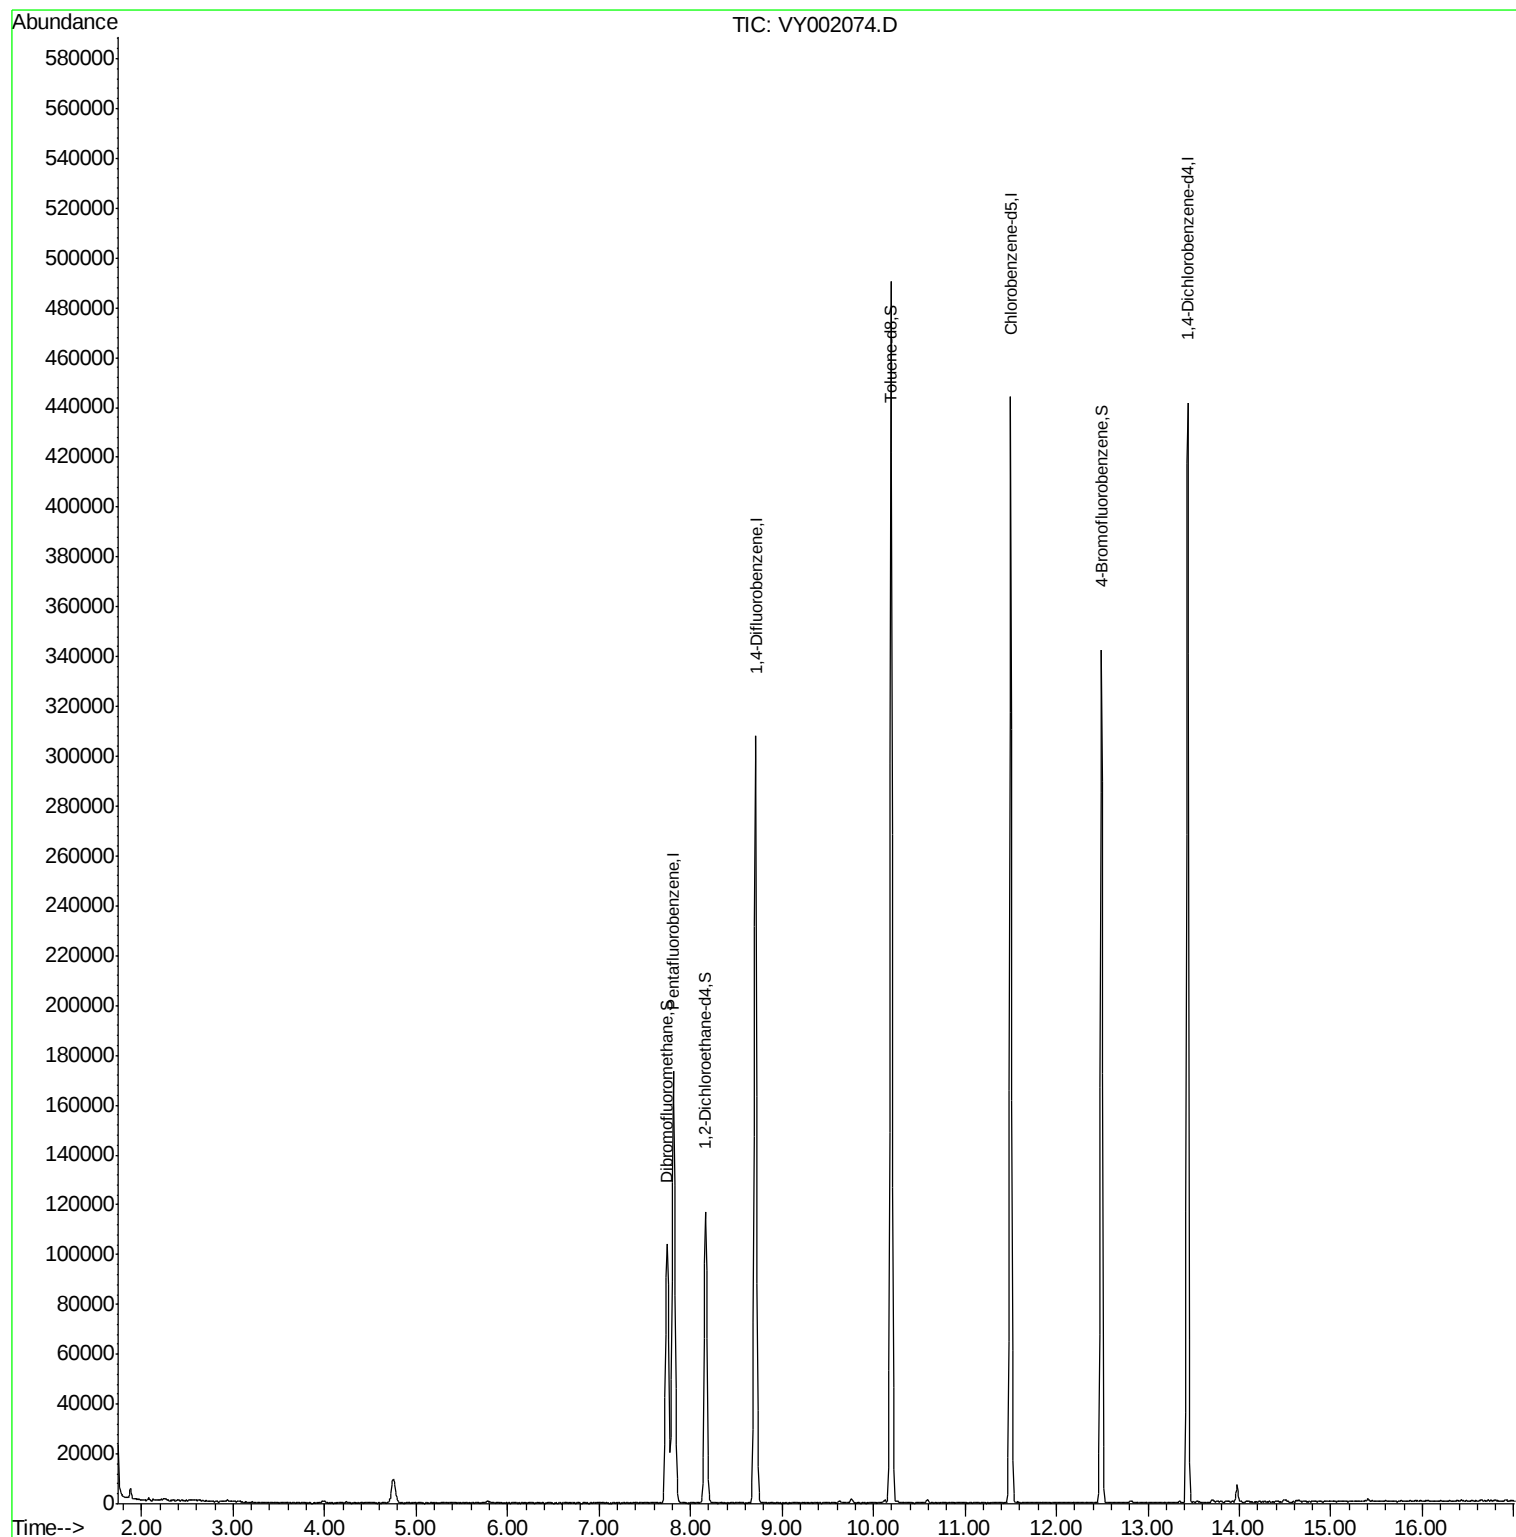



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.82 min Scan# 997

Delta R.T. 0.00 min

Lab File: VY002074.D

Acq: 25 Mar 2020 17:59

Instrument :

MSVOA_Y

ClientSampleId :


FK-BPM-01-C4-D4-C4A-D4A

Tot Ion:168 Resp: 131883

Ion Ratio Lower Upper




168 100

99 59.0 46.7 70.1

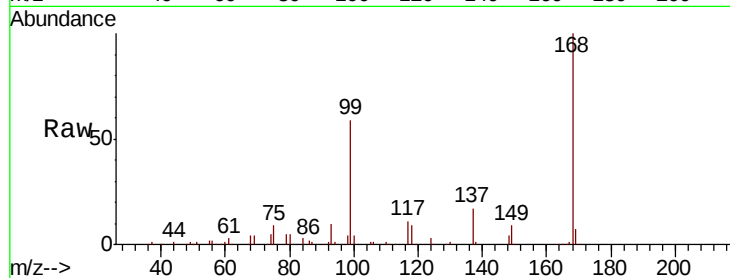

Abundance Ion 167.90 (167.60 to 168.60): VY001845.D (-986) (-)

Ion 98.90 (98.60 to 99.60): VY001845.D (-986) (-)

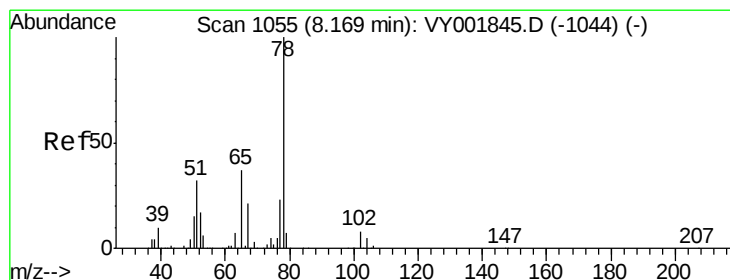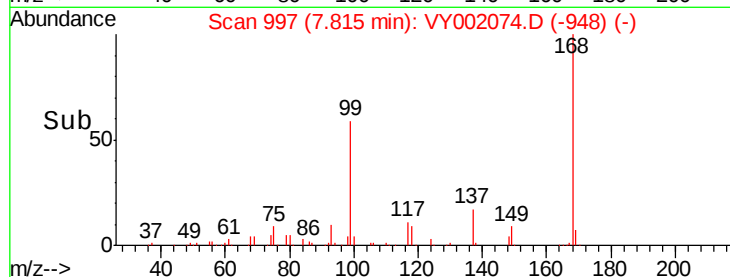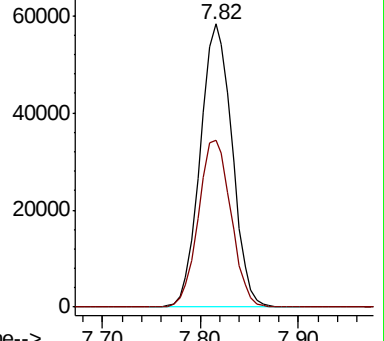

#33

1,2-Dichloroethane-d4

Concen: 61.058 ug/l

RT: 8.16 min Scan# 1054

Delta R.T. -0.01 min

Lab File: VY002074.D


Acq: 25 Mar 2020 17:59

Tgt Ion: 65 Resp: 85966

Ion Ratio Lower Upper



65 100

67 55.4 0.0 110.8

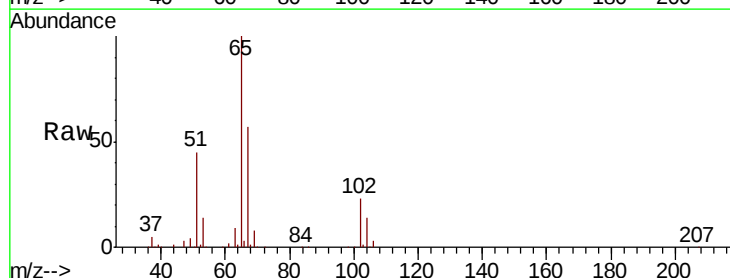

Abundance Ion 64.90 (64.60 to 65.60): VY001845.D (-1044) (-)

Ion 66.90 (66.60 to 67.60): VY001845.D (-1044) (-)

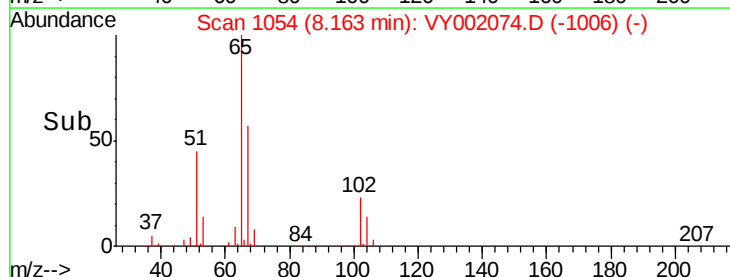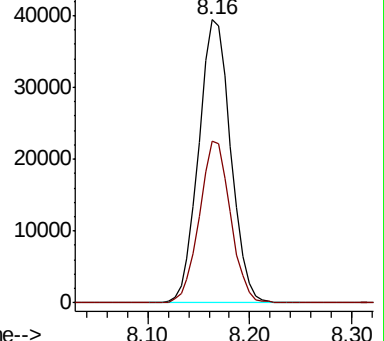



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.71 min Scan# 1144

Delta R.T. 0.00 min

Lab File: VY002074.D

Acq: 25 Mar 2020 17:59

Instrument :

MSVOA_Y

ClientSampleId :

FK-BPM-01-C4-D4-C4A-D4A


Tot Ion:114 Resp: 261958

Ion Ratio Lower Upper

114 100

63 20.2 0.0 39.4




88 16.4 0.0 30.4

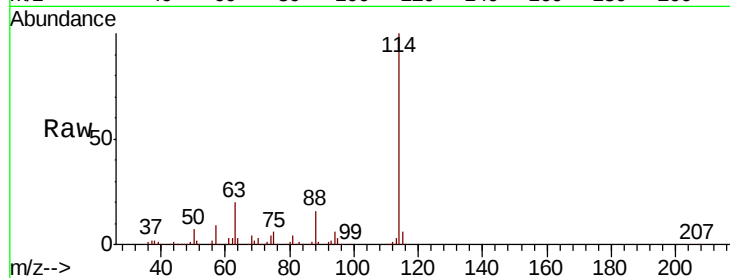

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VY0

Ion 87.90 (87.60 to 88.60): VY0

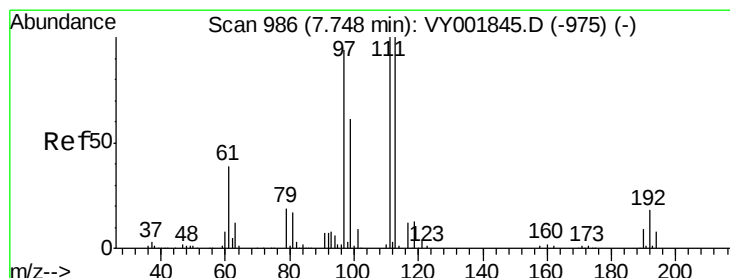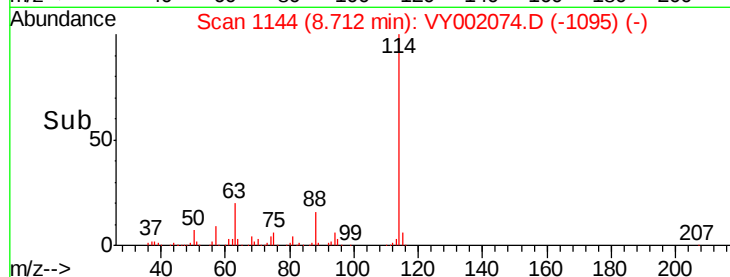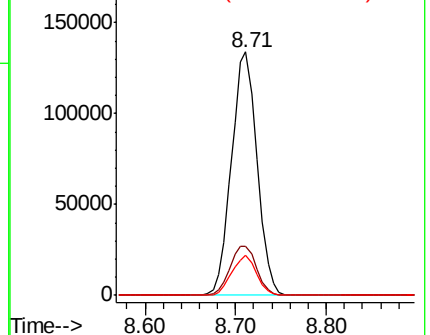

#35

Dibromofluoromethane

Concen: 54.486 ug/l

RT: 7.74 min Scan# 985

Delta R.T. -0.01 min

Lab File: VY002074.D

Acq: 25 Mar 2020 17:59


Tgt Ion:113 Resp: 77937

Ion Ratio Lower Upper

113 100

111 100.7 81.8 122.8



192 17.4 14.2 21.2

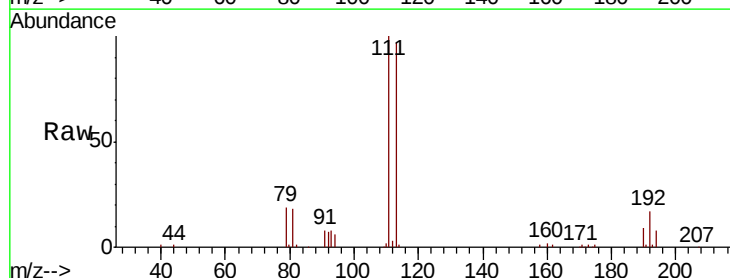


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

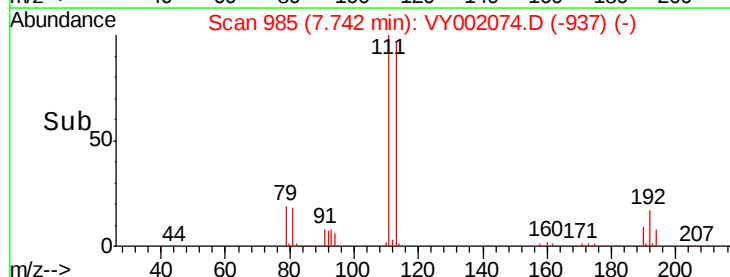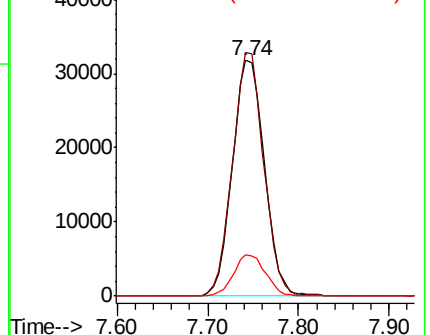

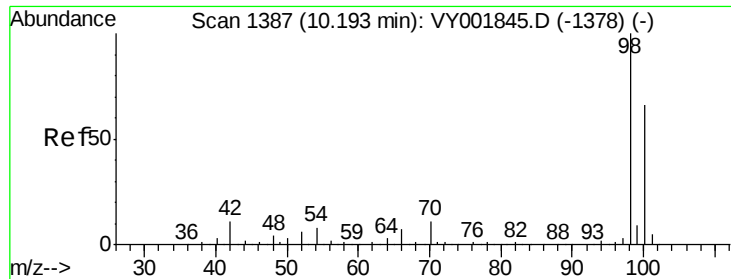

#50

Toluene-d8

Concen: 52.734 ug/l

RT: 10.19 min Scan# 1387

Delta R.T. 0.00 min

Lab File: VY002074.D

Acq: 25 Mar 2020 17:59

Instrument :

MSVOA_Y

ClientSampleId :


FK-BPM-01-C4-D4-C4A-D4A

Tot Ion: 98 Resp: 318083




Ion Ratio Lower Upper

98 100

100 65.6 53.0 79.4

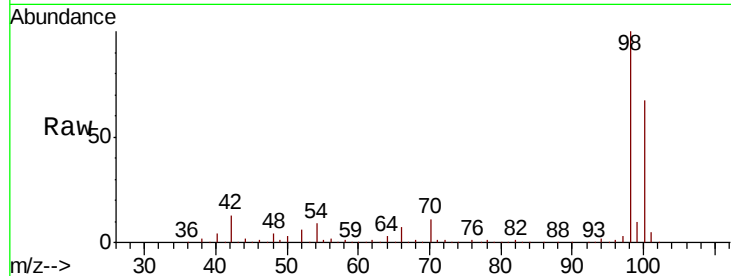

Abundance Ion 98.00 (97.70 to 98.70): VY001845.D (-1378) (-)

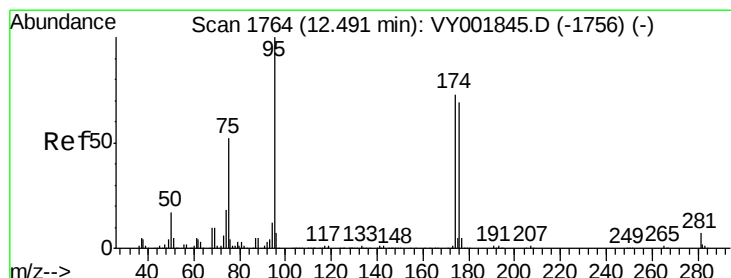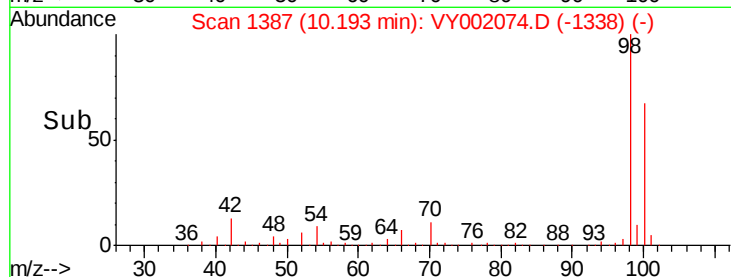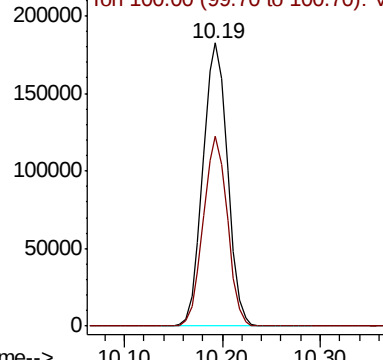

#62

4-Bromofluorobenzene

Concen: 52.113 ug/l

RT: 12.49 min Scan# 1764

Delta R.T. 0.00 min

Lab File: VY002074.D

Acq: 25 Mar 2020 17:59


Tgt Ion: 95 Resp: 109298

Ion Ratio Lower Upper



95 100


174 73.0 0.0 145.0

176 70.6 0.0 137.4

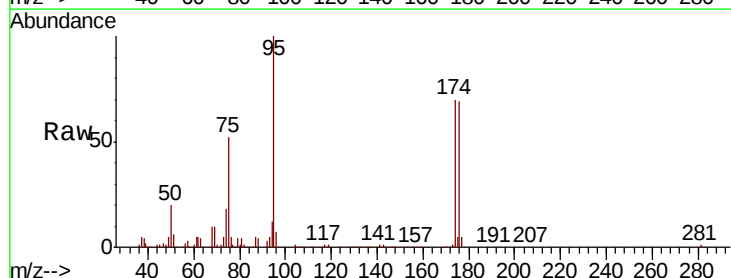

Abundance Ion 94.90 (94.60 to 95.60): VY001845.D (-1756) (-)



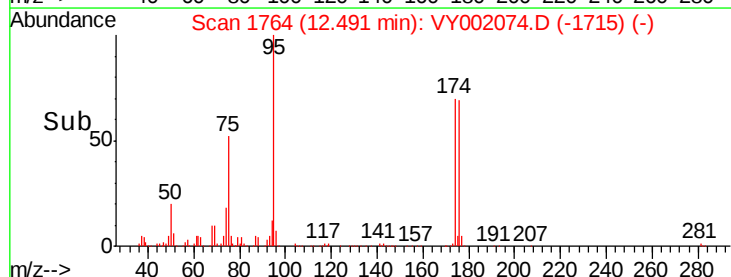
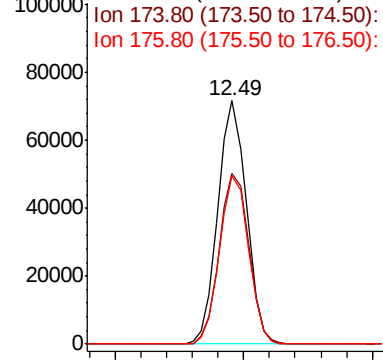


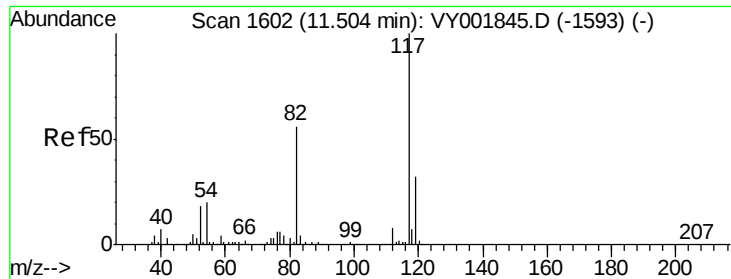

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.50 min Scan# 1601
Delta R.T. -0.01 min
Lab File: VY002074.D
Acq: 25 Mar 2020 17:59

Instrument :
MSVOA_Y
ClientSampleId :
FK-BPM-01-C4-D4-C4A-D4A

Tot Ion	Ratio	Lower	Upper
117	100		
82	57.0	44.5	66.7
119	30.2	25.7	38.5

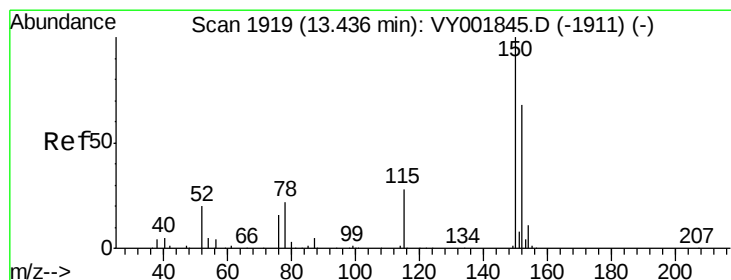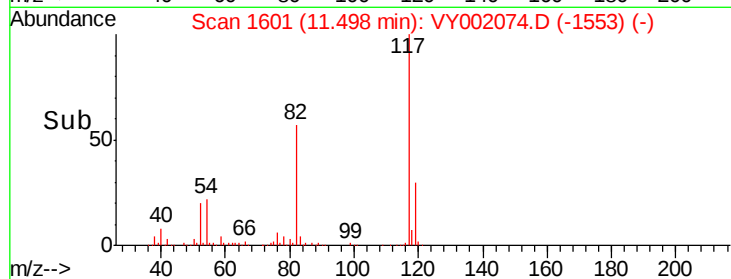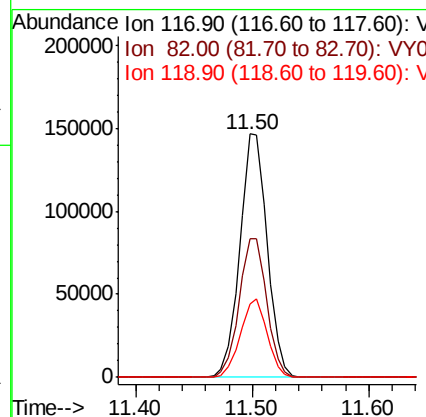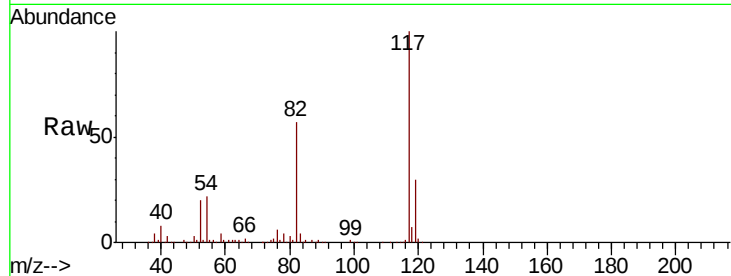

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.44 min Scan# 1919
Delta R.T. 0.00 min
Lab File: VY002074.D
Acq: 25 Mar 2020 17:59

Tgt Ion	Ratio	Lower	Upper
152	100		
115	61.5	29.9	89.7
150	159.4	0.0	340.6

