


Methyl Iodide

Response Ratio

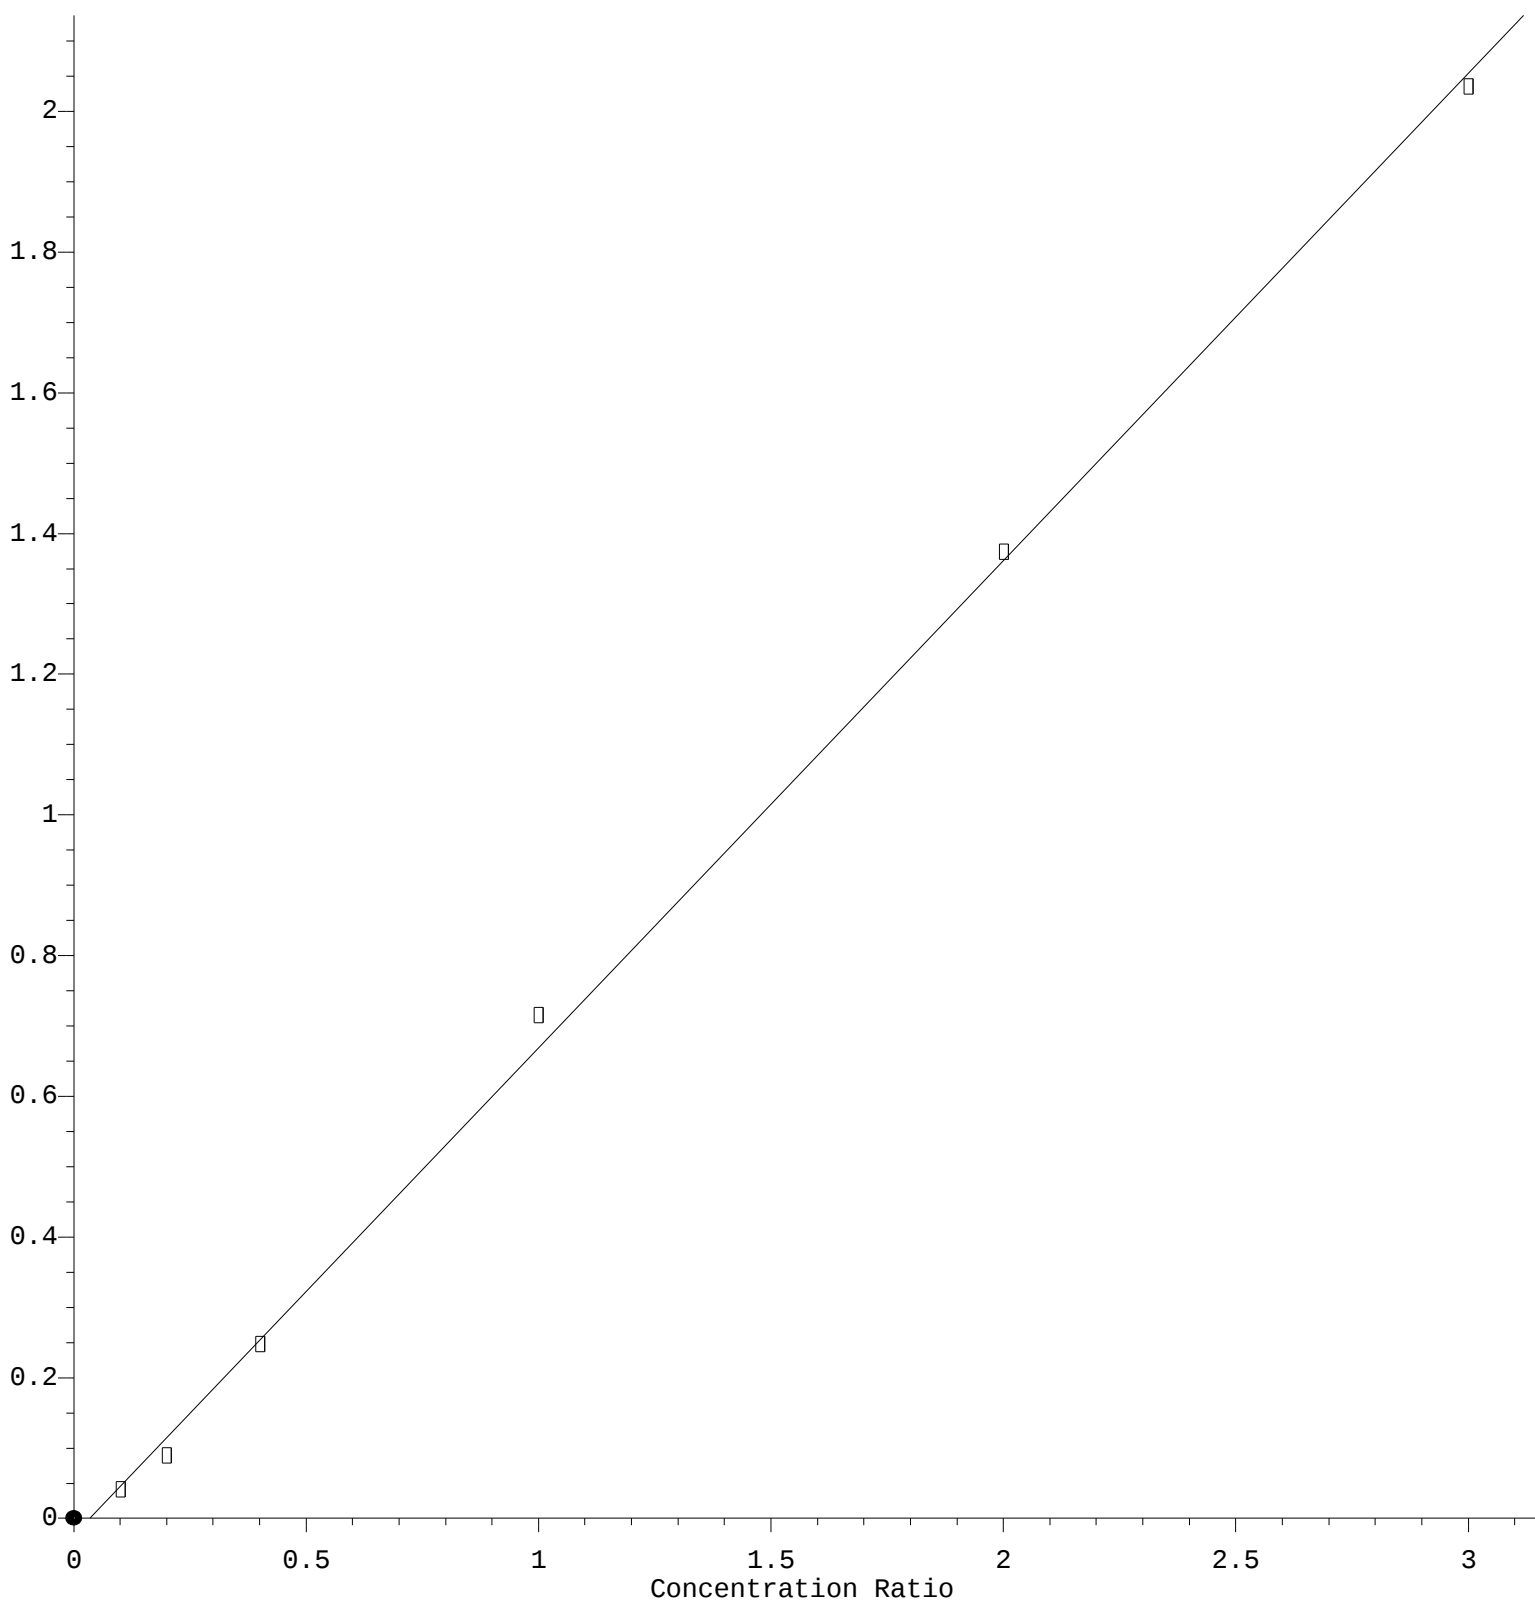


$$\text{Response} = 6.928\text{e-}001 * \text{Amt} - 2.352\text{e-}002$$

Coef of Det (r^2) = 0.998957 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032522S.M

Calibration Table Last Updated: Sat Mar 26 03:24:51 2022


Methyl Acetate

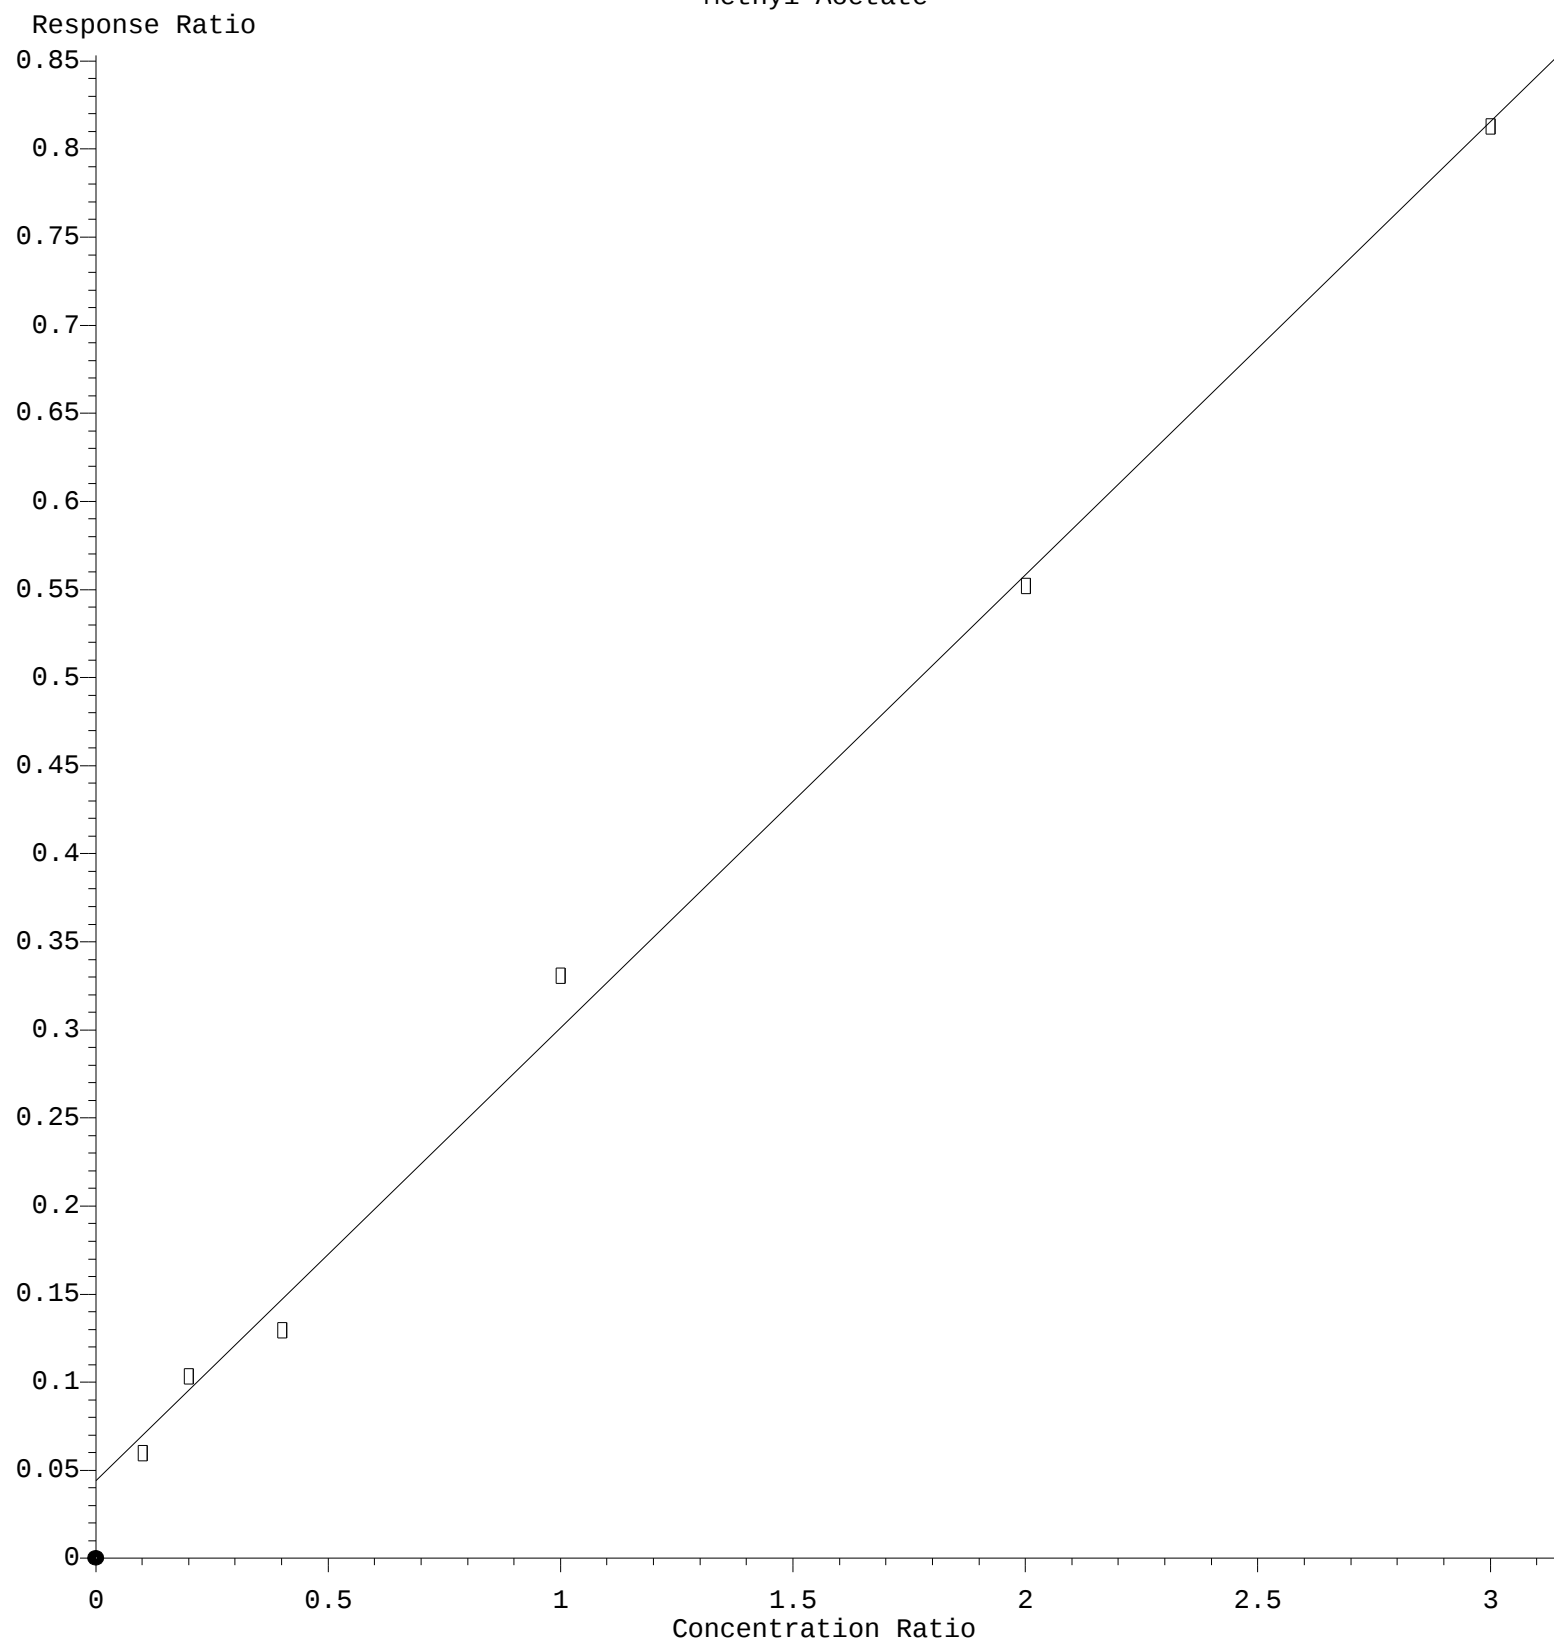

Response = $2.573 \times 10^{-1} \times \text{Amt} + 4.393 \times 10^{-2}$
Coef of Det (r^2) = 0.996897 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032522S.M
Calibration Table Last Updated: Sat Mar 26 03:24:51 2022

Methylene Chloride

Response Ratio

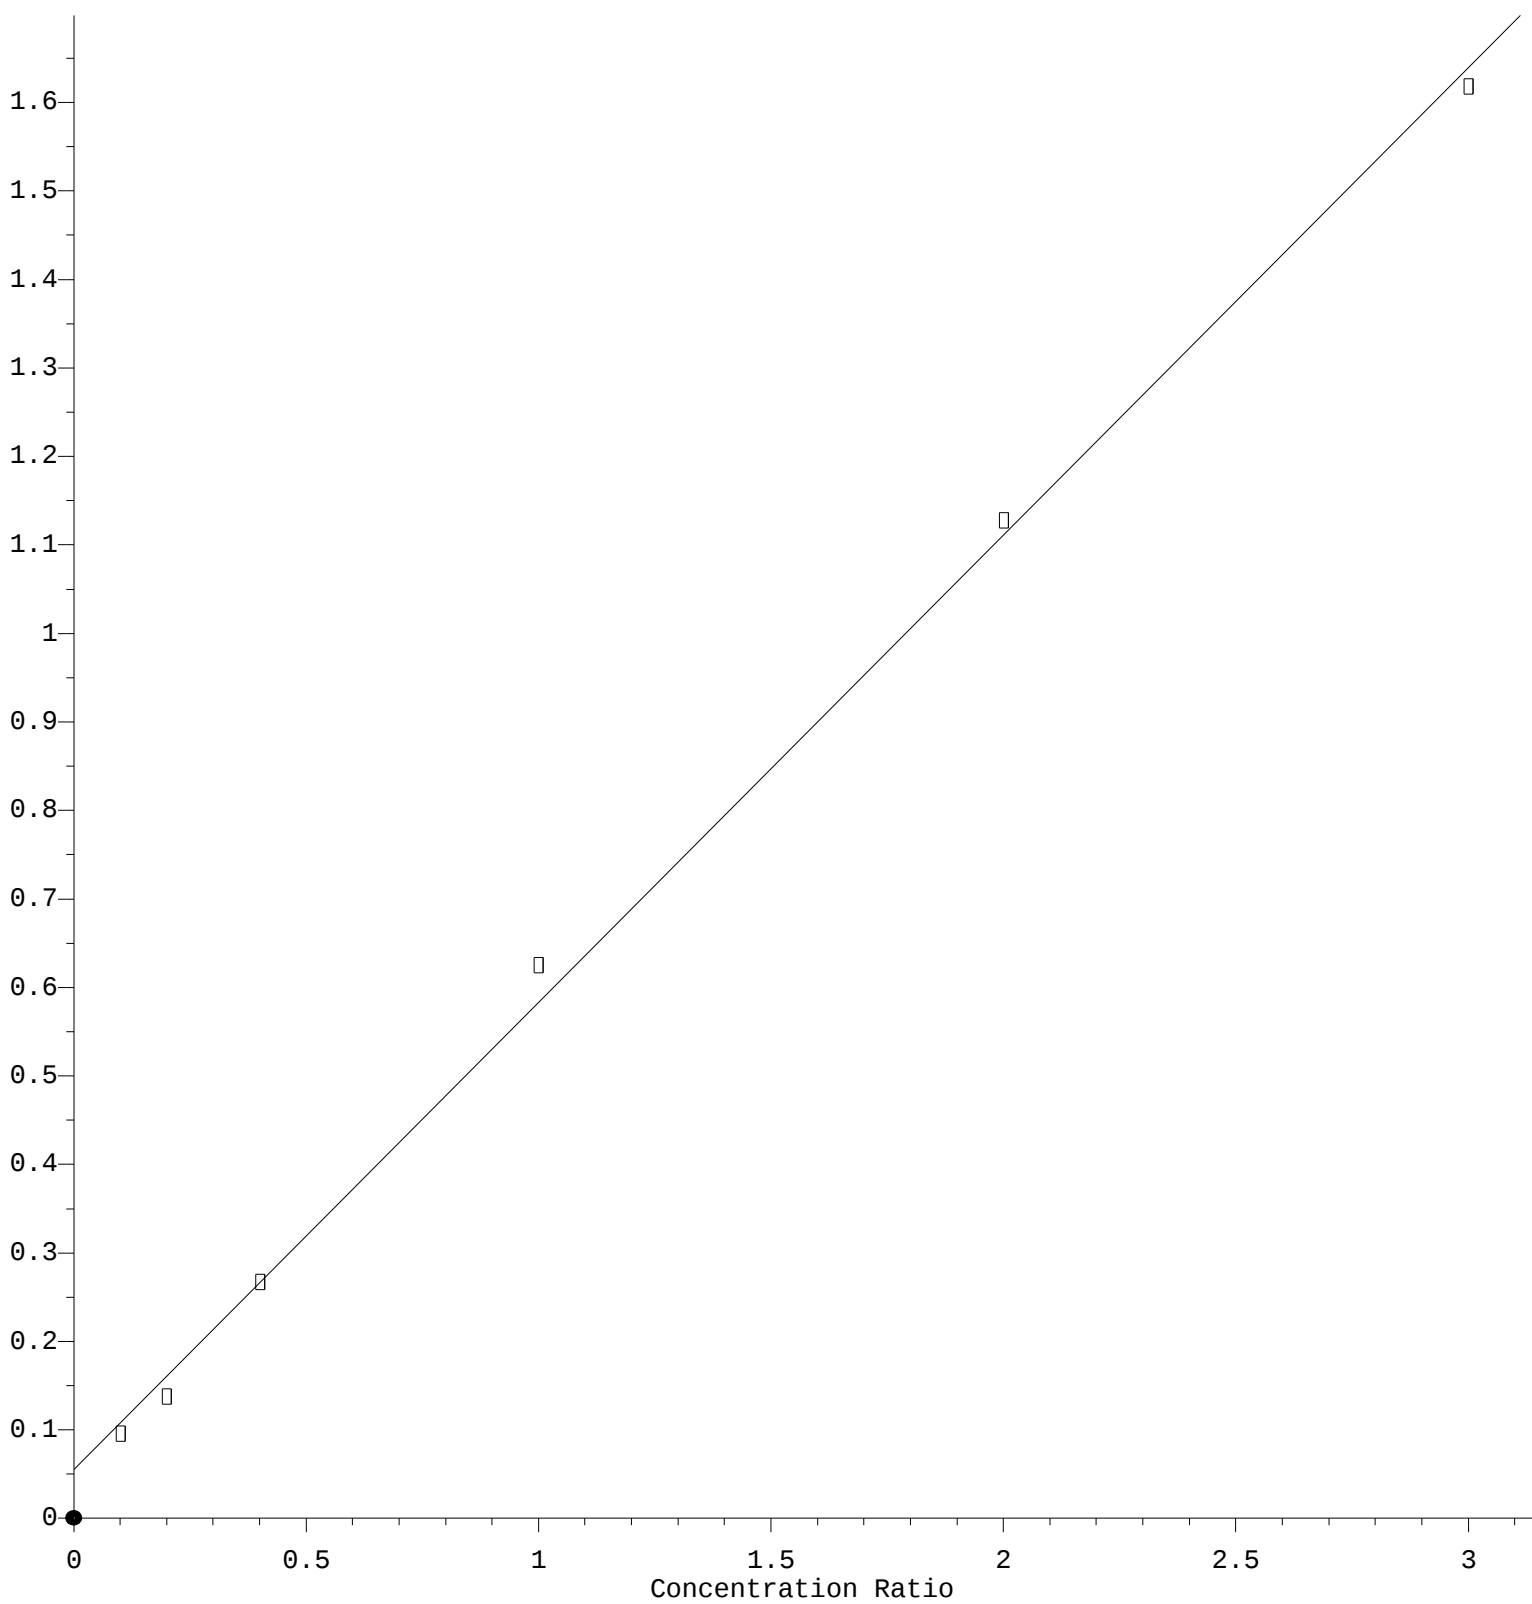

$$\text{Response} = 5.285\text{e-}001 * \text{Amt} + 5.487\text{e-}002$$


Coef of Det (r^2) = 0.998344 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032522S.M

Calibration Table Last Updated: Sat Mar 26 03:24:51 2022

Bromochloromethane

Response Ratio

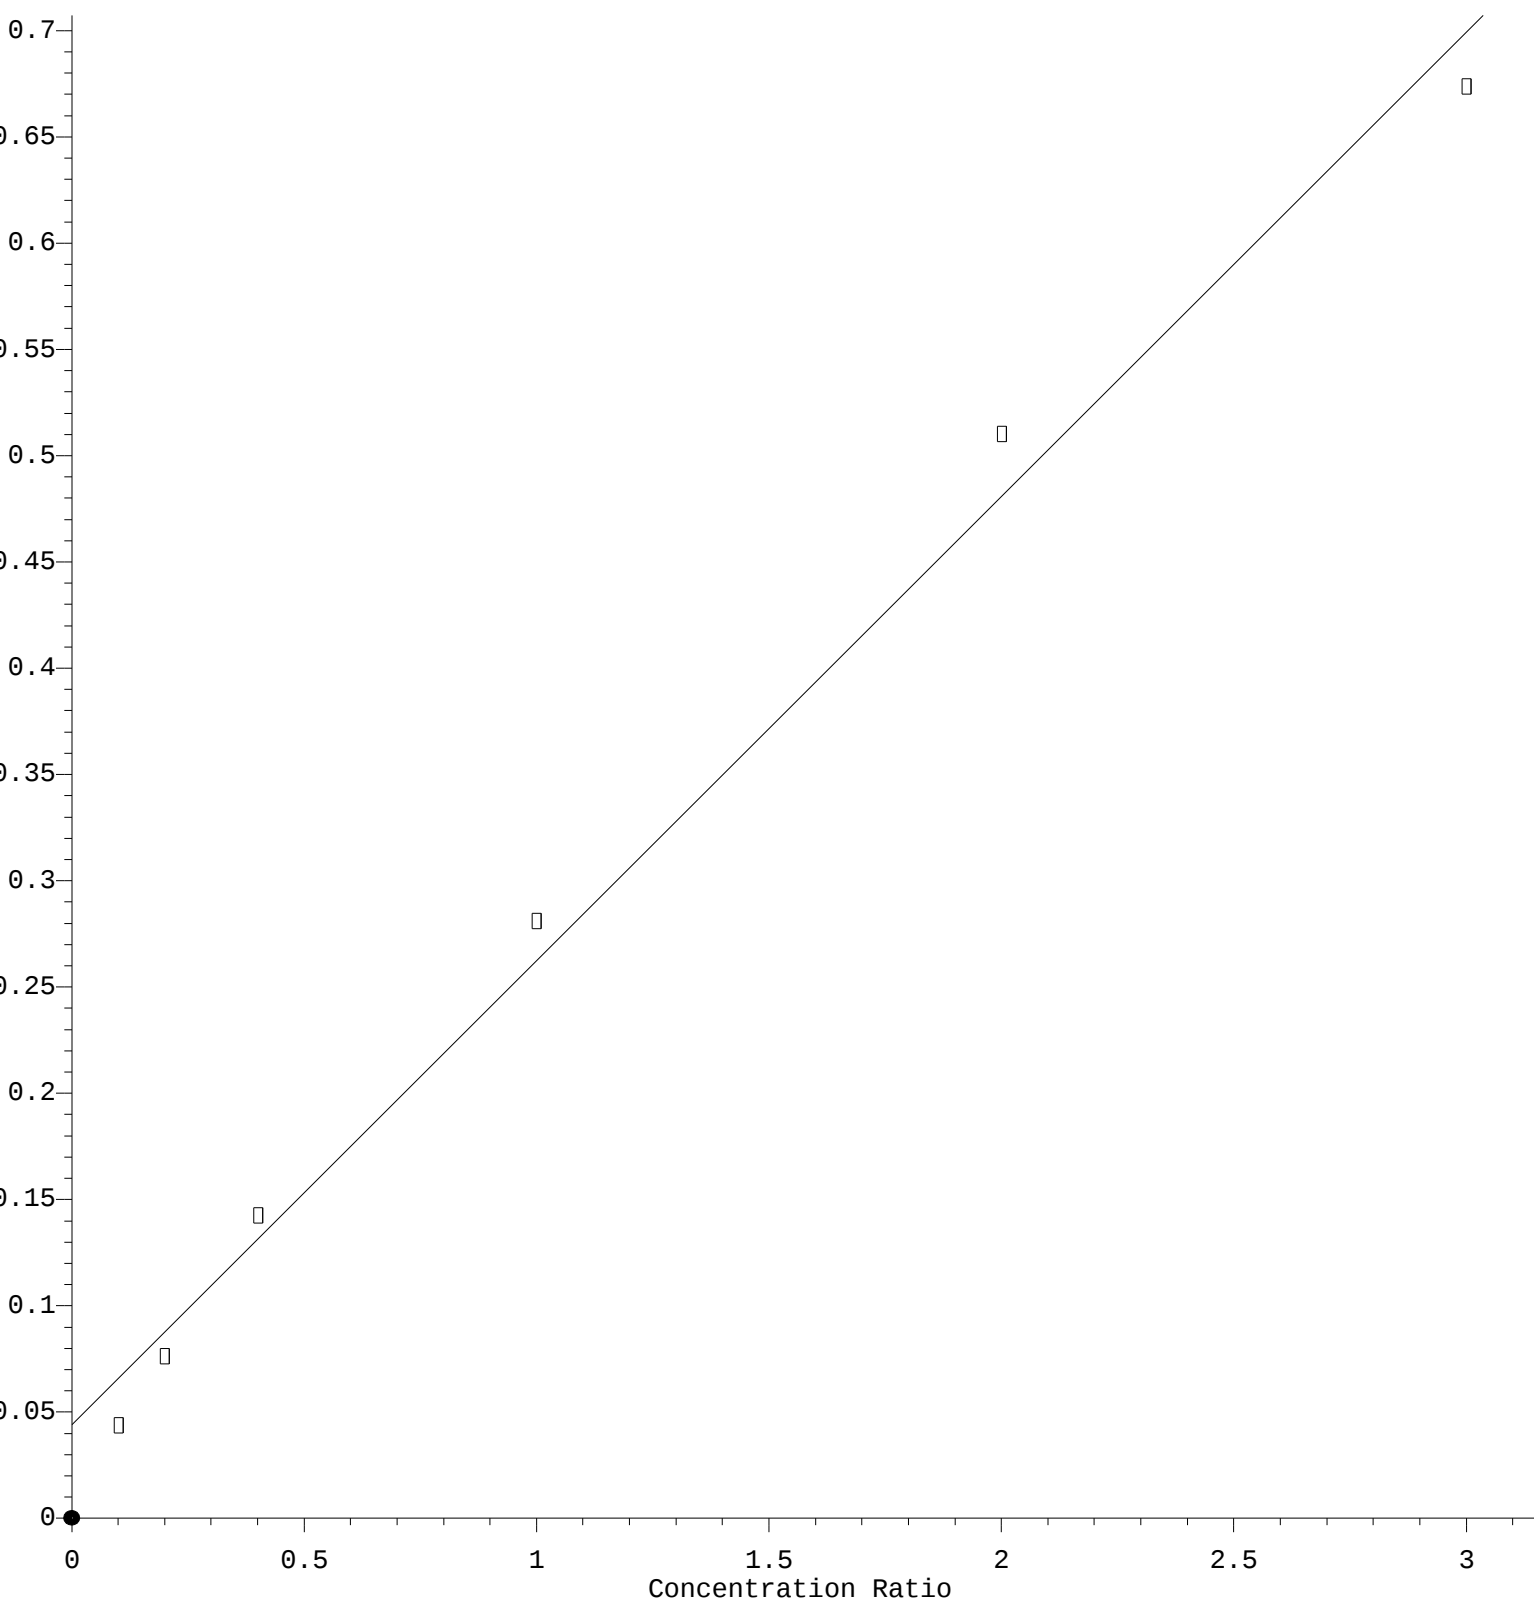

$$\text{Response} = 2.185\text{e-}001 * \text{Amt} + 4.382\text{e-}002$$

Coef of Det (r^2) = 0.991966 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032522S.M

Calibration Table Last Updated: Sat Mar 26 03:24:51 2022