


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY032620\
 Data File : VY002084.D
 Acq On : 26 Mar 2020 13:04
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y032620S.M
 Title : SW846 8260
 Last Update : Fri Mar 27 07:11:05 2020

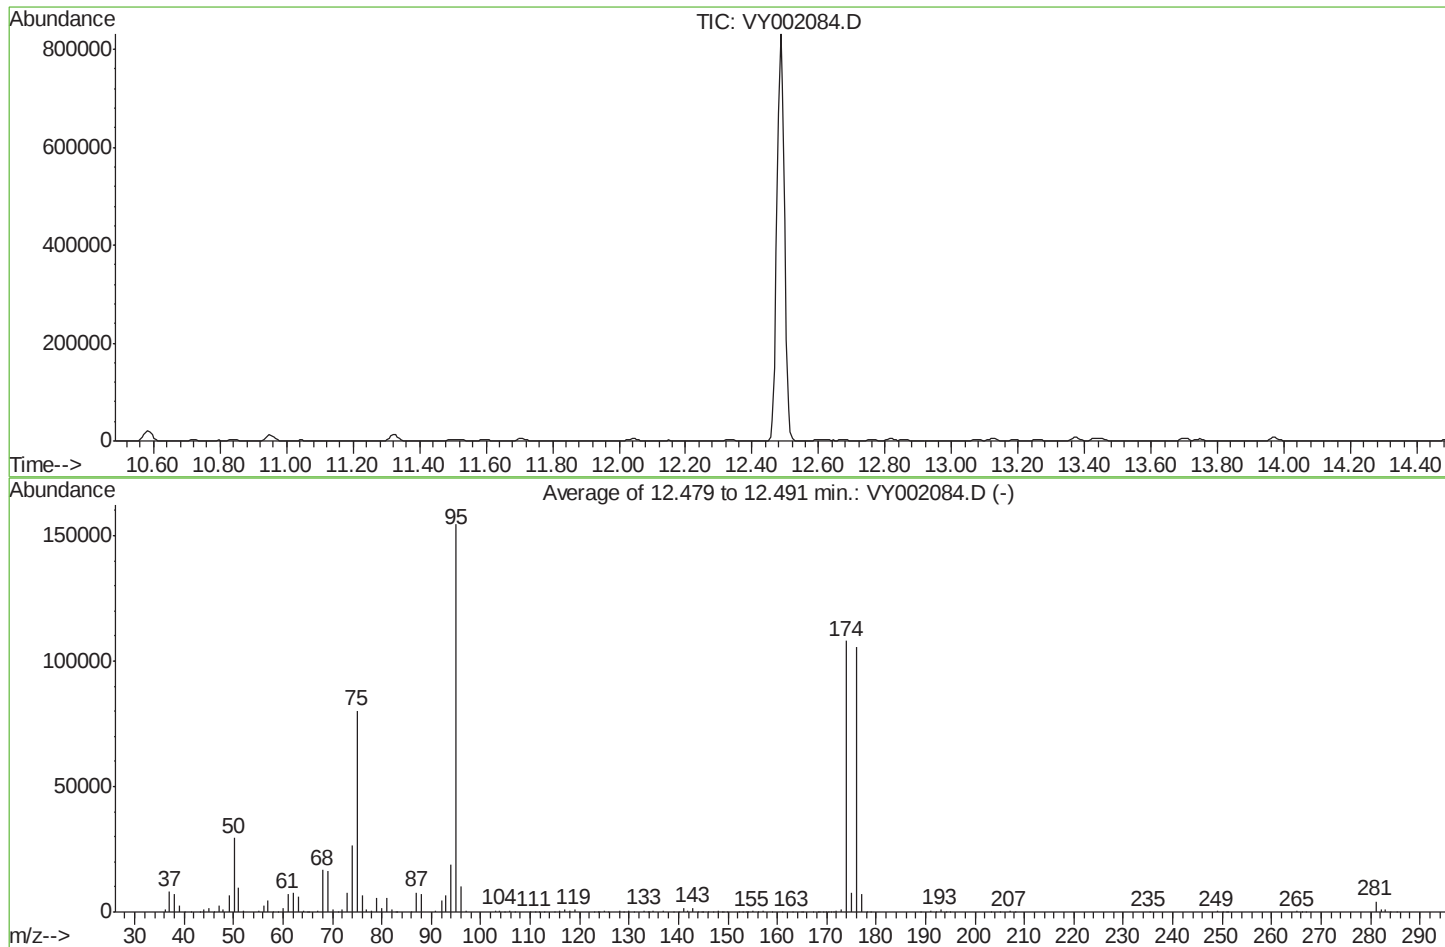

AutoFind: Scans 1762, 1763, 1764; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	29528	PASS
75	95	30	60	51.9	80173	PASS
95	95	100	100	100.0	154517	PASS
96	95	5	9	6.6	10148	PASS
173	174	0.00	2	1.0	1078	PASS
174	95	50	100	70.0	108093	PASS
175	174	5	9	7.2	7763	PASS
176	174	95	101	97.7	105573	PASS
177	176	5	9	6.8	7143	PASS