
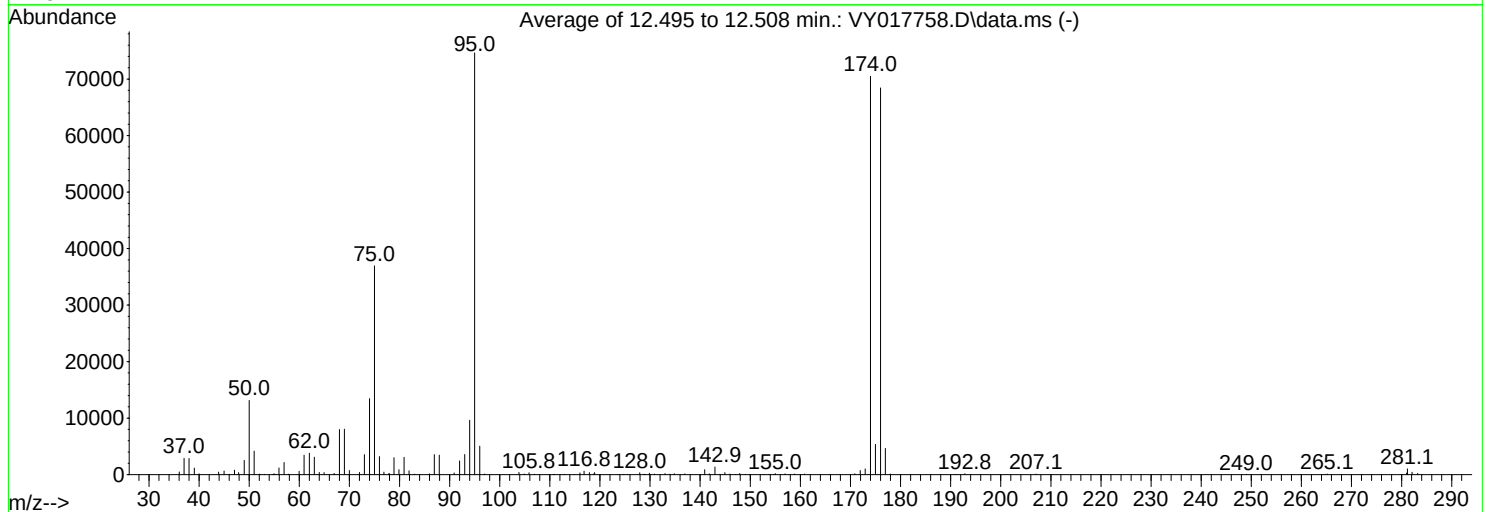


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY032624\
Data File : VY017758.D
Acq On : 26 Mar 2024 08:35
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032224S.M
Title : SW846 8260
Last Update : Sat Mar 23 04:03:52 2024

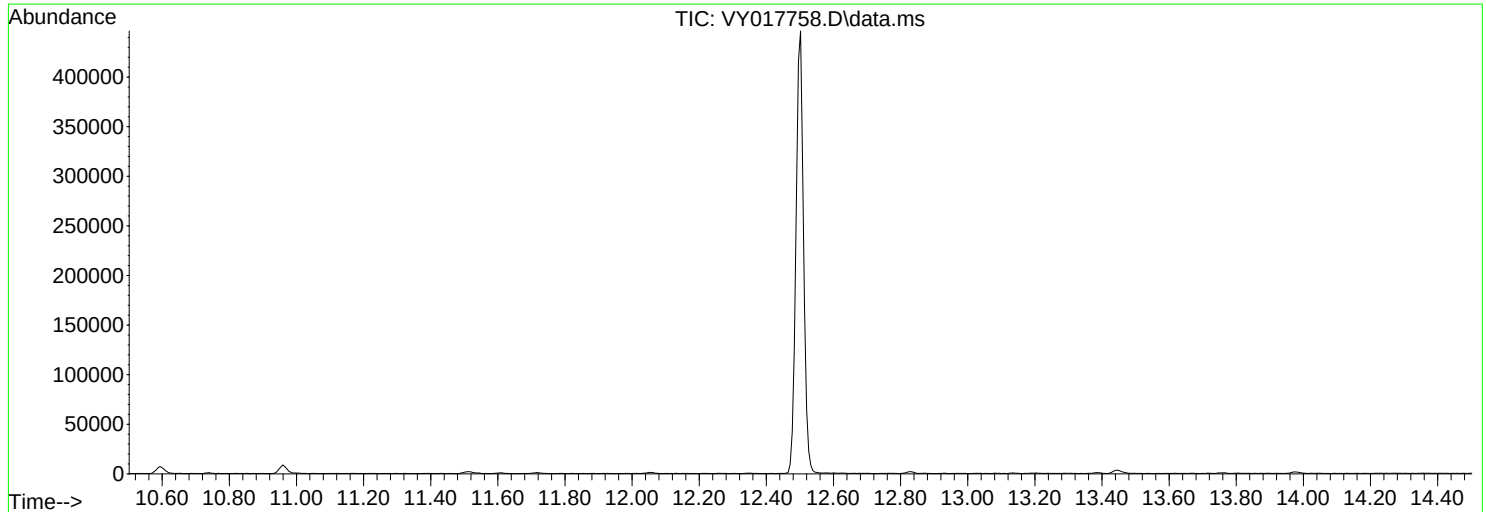

AutoFind: Scans 1751, 1752, 1753; Background Corrected with Scan 1742

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	13149	PASS
75	95	30	60	49.5	36955	PASS
95	95	100	100	100.0	74637	PASS
96	95	5	9	6.8	5047	PASS
173	174	0.00	2	1.5	1034	PASS
174	95	50	100	94.5	70515	PASS
175	174	5	9	7.6	5346	PASS
176	174	95	101	97.0	68429	PASS
177	176	5	9	6.8	4636	PASS