


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY032720\
 Data File : VY002093.D
 Acq On : 27 Mar 2020 10:03
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y032620S.M
 Title : SW846 8260
 Last Update : Fri Mar 27 07:11:05 2020

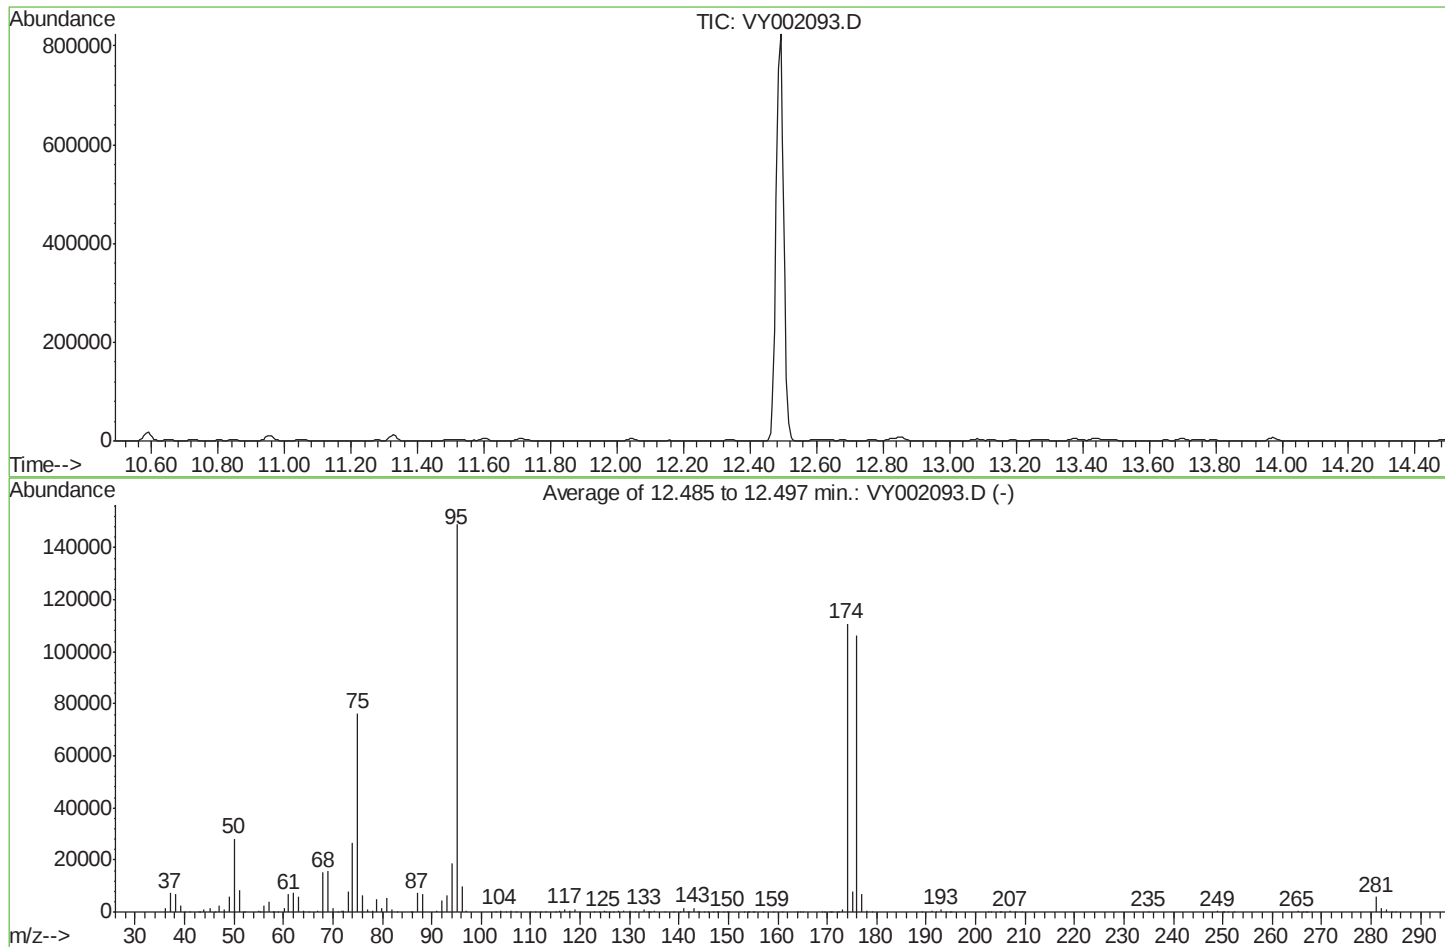

AutoFind: Scans 1763, 1764, 1765; Background Corrected with Scan 1755

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	28250	PASS
75	95	30	60	51.2	76205	PASS
95	95	100	100	100.0	148965	PASS
96	95	5	9	6.7	9919	PASS
173	174	0.00	2	0.9	1004	PASS
174	95	50	100	74.4	110904	PASS
175	174	5	9	7.0	7799	PASS
176	174	95	101	95.8	106277	PASS
177	176	5	9	6.5	6900	PASS