
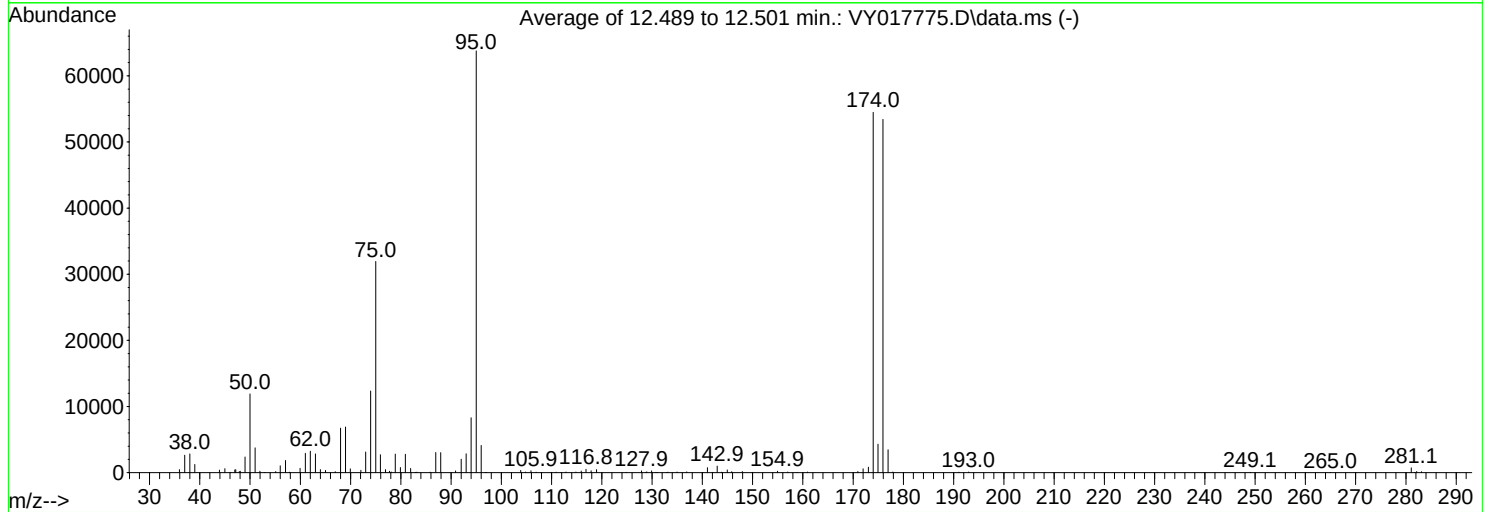


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY032724\
Data File : VY017775.D
Acq On : 27 Mar 2024 08:24
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032224S.M
Title : SW846 8260
Last Update : Sat Mar 23 04:03:52 2024

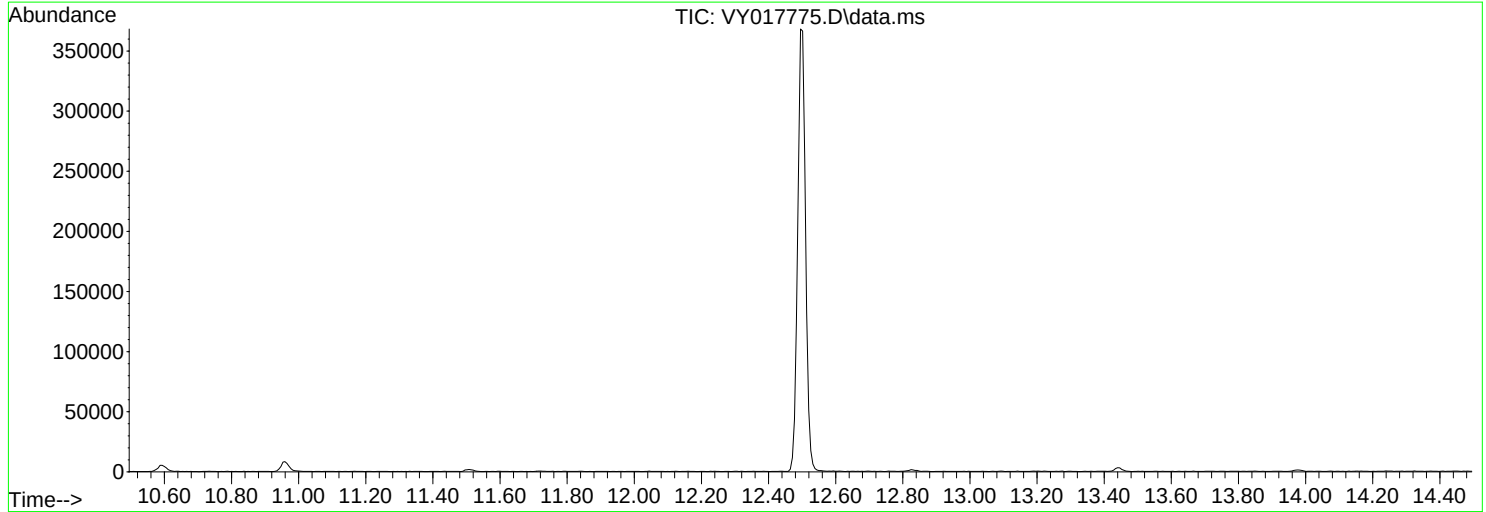

AutoFind: Scans 1750, 1751, 1752; Background Corrected with Scan 1742

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	11892	PASS
75	95	30	60	50.1	31931	PASS
95	95	100	100	100.0	63781	PASS
96	95	5	9	6.4	4112	PASS
173	174	0.00	2	1.5	820	PASS
174	95	50	100	85.4	54493	PASS
175	174	5	9	7.9	4314	PASS
176	174	95	101	98.0	53421	PASS
177	176	5	9	6.5	3471	PASS