

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY032822\
 Data File : VY008060.D
 Acq On : 28 Mar 2022 12:23
 Operator : SY/MD
 Sample : VY0328SBS01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0328SBS01

Quant Time: Mar 28 18:37:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 25 16:26:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	0.000	168	0	0.000	ug/l	-5.56
34) 1,4-Difluorobenzene	0.000	114	0	0.000	ug/l	-6.76
63) Chlorobenzene-d5	0.000	117	0	0.000	ug/l	-10.06
72) 1,4-Dichlorobenzene-d4	0.000	152	0	0.000	ug/l	-12.02
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.027	65	18326	0.000	ug/l	0.06
Spiked Amount 50.000			Recovery	=	0.000%	
35) Dibromofluoromethane	0.000	113	0	0.000	ug/l	
Spiked Amount 50.000			Recovery	=	0.000%	
50) Toluene-d8	0.000	98	0	0.000	ug/l	
Spiked Amount 50.000			Recovery	=	0.000%	
62) 4-Bromofluorobenzene	11.093	95	1643	0.000	ug/l	0.00
Spiked Amount 50.000			Recovery	=	0.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY032822\
Data File : VY008060.D
Acq On : 28 Mar 2022 12:23
Operator : SY/MD
Sample : VY0328SBS01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0328SBS01

Quant Time: Mar 28 18:37:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M
Quant Title : SW846 8260
QLast Update : Fri Mar 25 16:26:59 2022
Response via : Initial Calibration

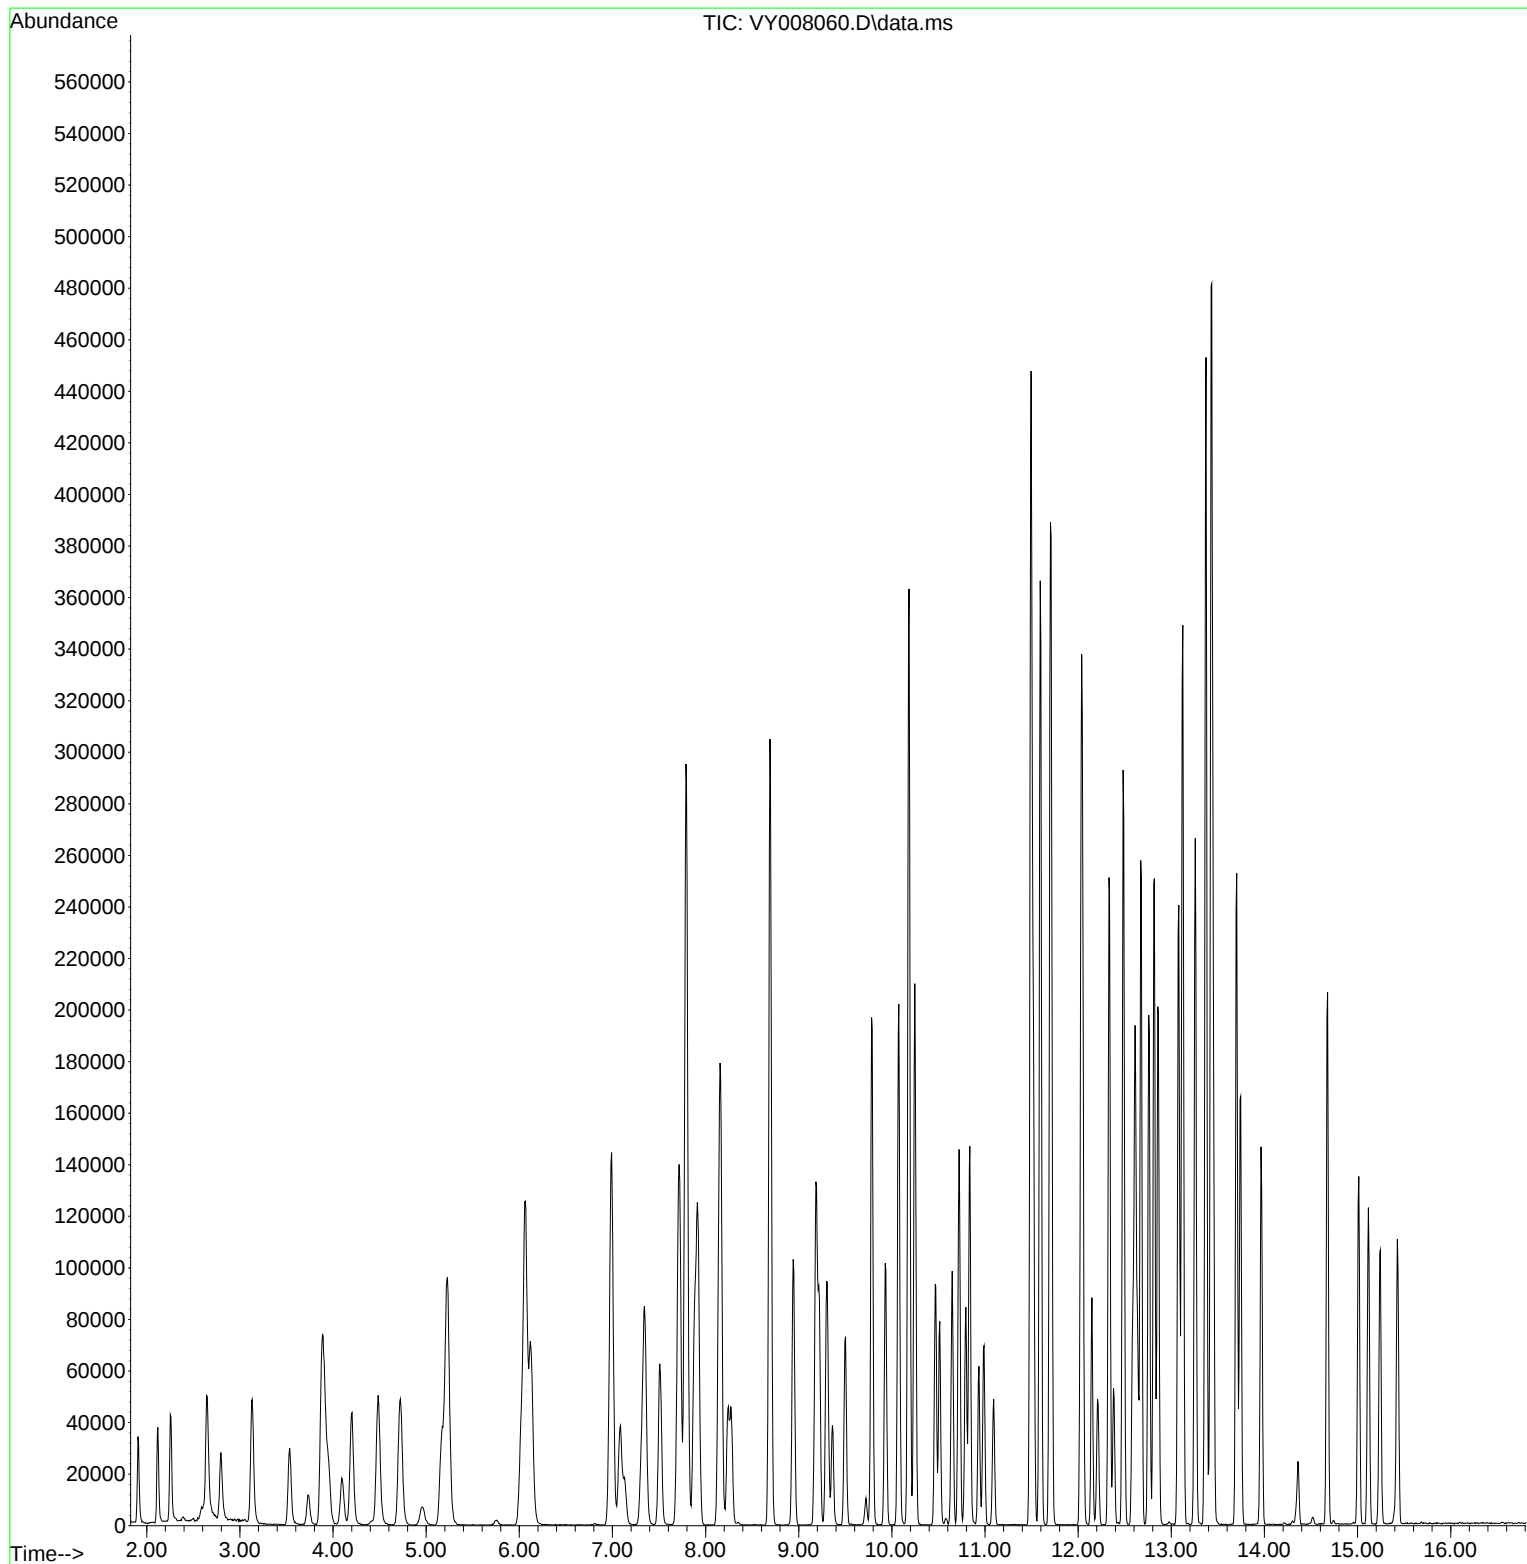


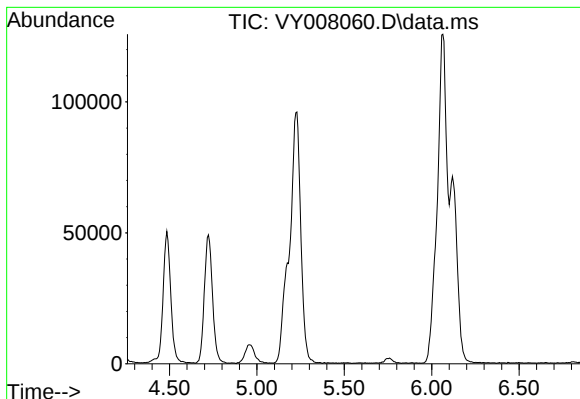


#1
Pentafluorobenzene
Concen: 0.000 ug/l
Expected RT: 5.56 min

Lab File: VY008060.D
Acq: 28 Mar 2022 12:23




Instrument :
MSVOA_Y
ClientSampleId :
VY0328SBS01


Tgt Ion: 168
Sig Exp Ratio
168 100
99 52.1

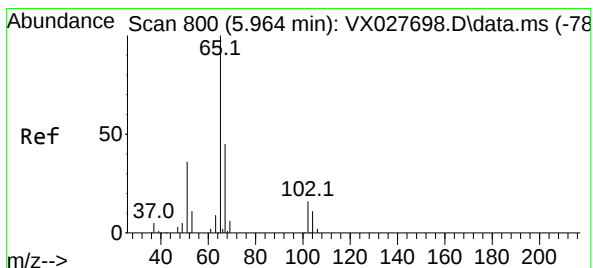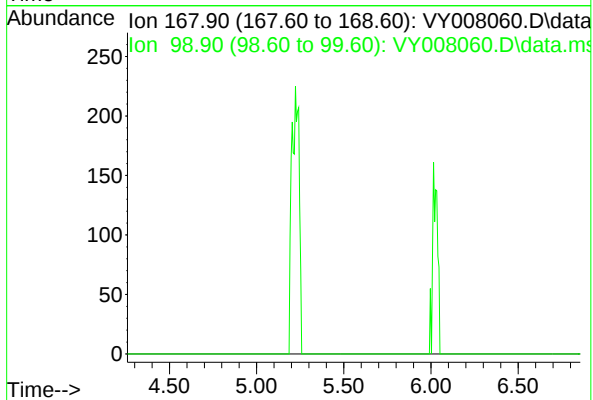

#33
1,2-Dichloroethane-d4
Concen: 0.000 ug/l
RT: 6.027 min Scan# 690
Delta R.T. 0.063 min
Lab File: VY008060.D
Acq: 28 Mar 2022 12:23

Tgt Ion: 65 Resp: 18326
Ion Ratio Lower Upper
65 100
67 0.0 0.0 107.4

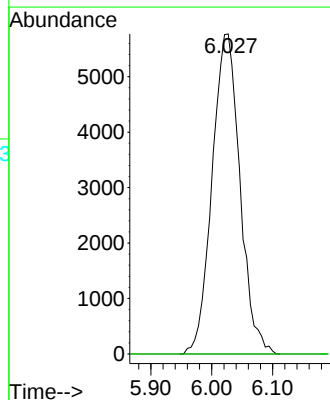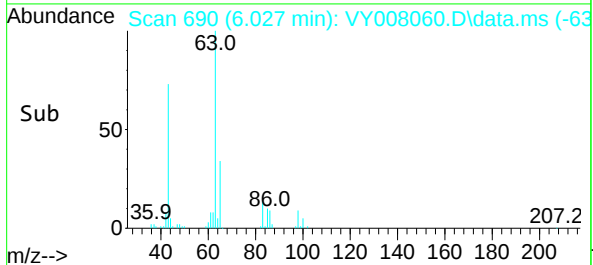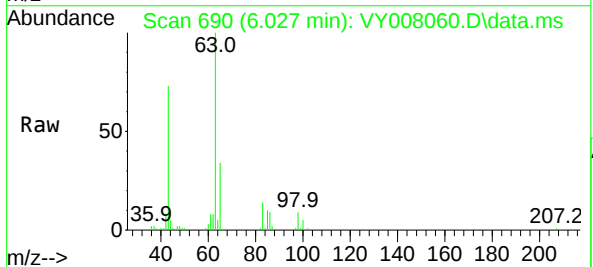


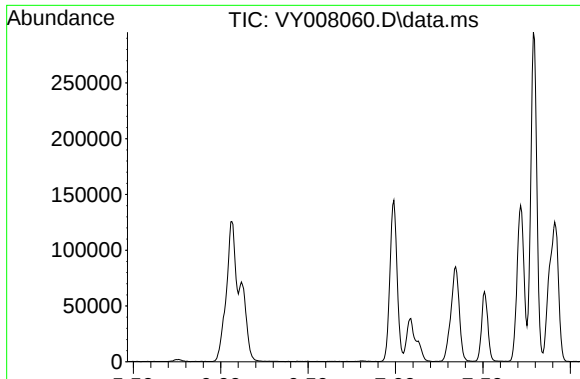


#34
 1,4-Difluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 6.76 min
 Lab File: VY008060.D
 Acq: 28 Mar 2022 12:23

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0328SBS01

Tgt Ion: 114


Sig	Exp Ratio
114	100
63	18.4
88	16.2

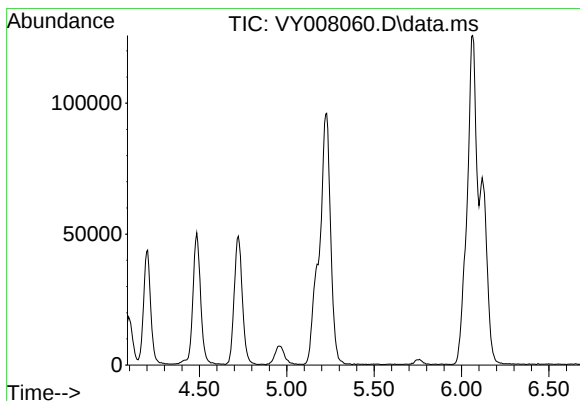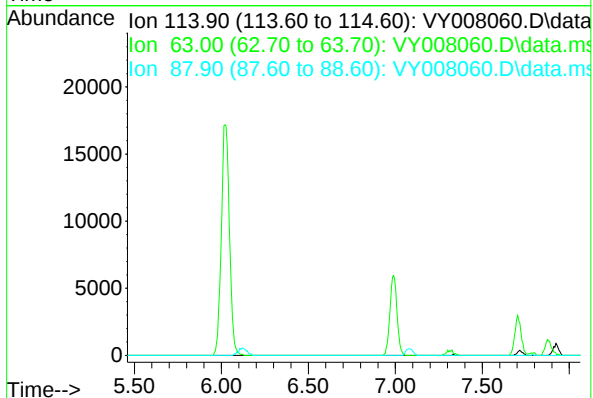


#35
 Dibromofluoromethane
 Concen: 0.000 ug/l
 Expected RT: 5.38 min
 Lab File: VY008060.D
 Acq: 28 Mar 2022 12:23

Tgt Ion: 113

Sig	Exp Ratio
113	100
111	103.5
192	21.1


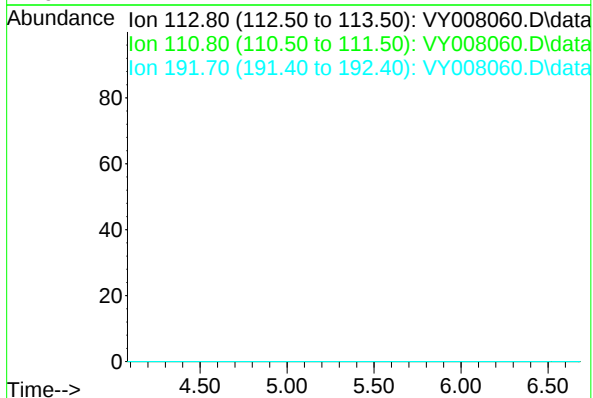


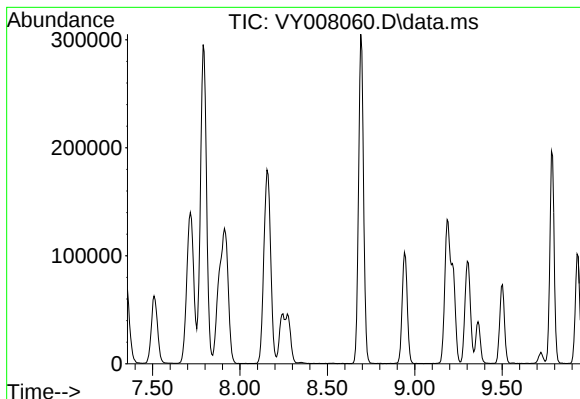

#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 8.65 min
Lab File: VY008060.D
Acq: 28 Mar 2022 12:23




Instrument :
MSVOA_Y
ClientSampleId :
VY0328SBS01


Tgt Ion: 98
Sig Exp Ratio
98 100
100 65.7

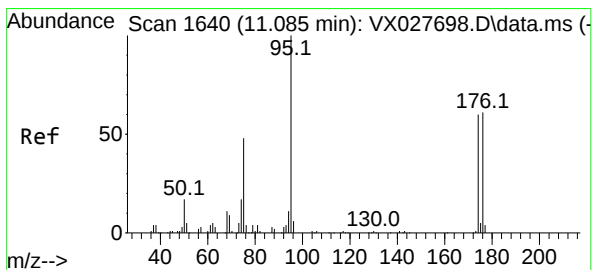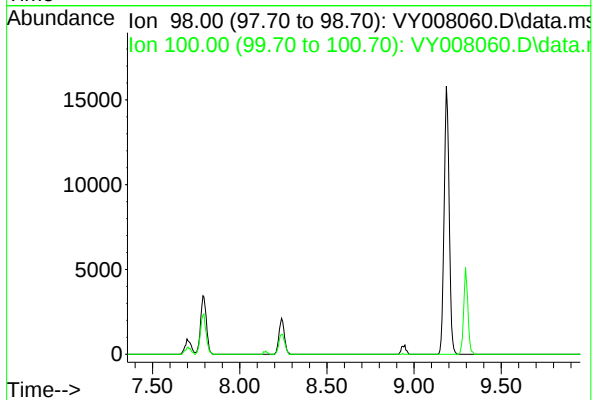

#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
RT: 11.093 min Scan# 1521
Delta R.T. 0.008 min
Lab File: VY008060.D
Acq: 28 Mar 2022 12:23

Tgt Ion: 95 Resp: 1643
Ion Ratio Lower Upper
95 100
174 0.0 0.0 163.0
176 0.0 0.0 155.0

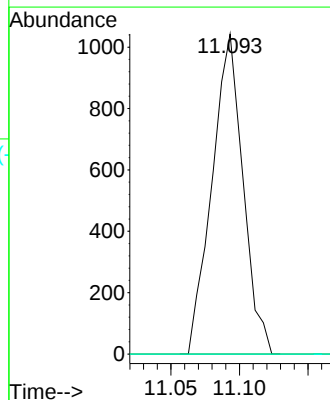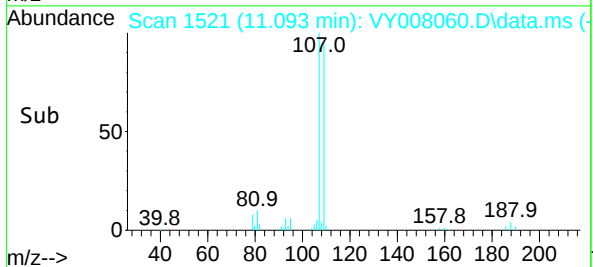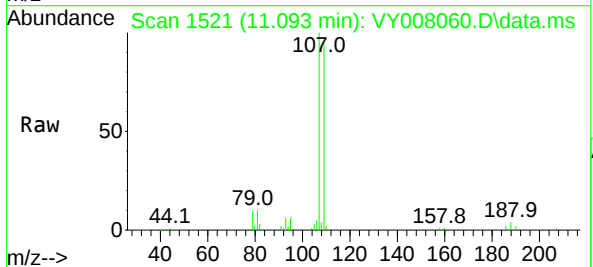


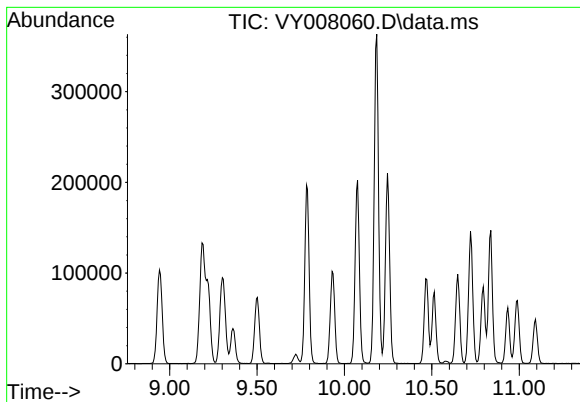


#63
 Chlorobenzene-d5
 Concen: 0.000 ug/l
 Expected RT: 10.06 min
 Lab File: VY008060.D
 Acq: 28 Mar 2022 12:23

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0328SBS01

Tgt Ion: 117

Sig	Exp Ratio
117	100
82	52.3
119	31.0

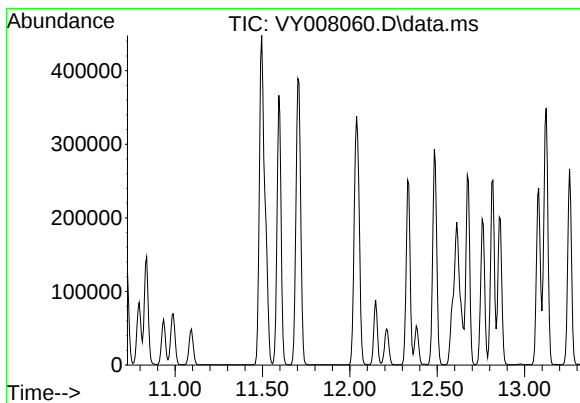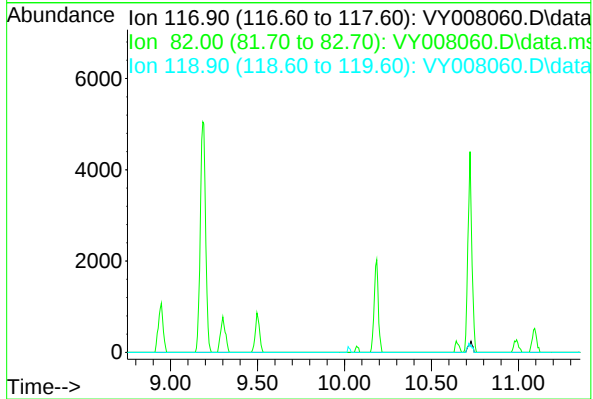

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ug/l
 Expected RT: 12.02 min
 Lab File: VY008060.D
 Acq: 28 Mar 2022 12:23

Tgt Ion: 152

Sig	Exp Ratio
152	100
115	75.1
150	169.1

