

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY032822\
 Data File : VY008059.D
 Acq On : 28 Mar 2022 11:56
 Operator : SY/MD
 Sample : VY0328SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0328SBL01

Quant Time: Mar 28 18:56:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032522S.M
 Quant Title : SW846 8260
 QLast Update : Sat Mar 26 03:24:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.795	168	144683	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	261300	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.496	117	240031	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	104062	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	78875	54.336	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	108.680%
35) Dibromofluoromethane	7.722	113	81958	50.027	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.060%
50) Toluene-d8	10.185	98	311030	50.392	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	100.780%
62) 4-Bromofluorobenzene	12.483	95	106623	48.964	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	97.920%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY032822\
Data File : VY008059.D
Acq On : 28 Mar 2022 11:56
Operator : SY/MD
Sample : VY0328SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0328SBL01

Quant Time: Mar 28 18:56:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032522S.M
Quant Title : SW846 8260
QLast Update : Sat Mar 26 03:24:51 2022
Response via : Initial Calibration




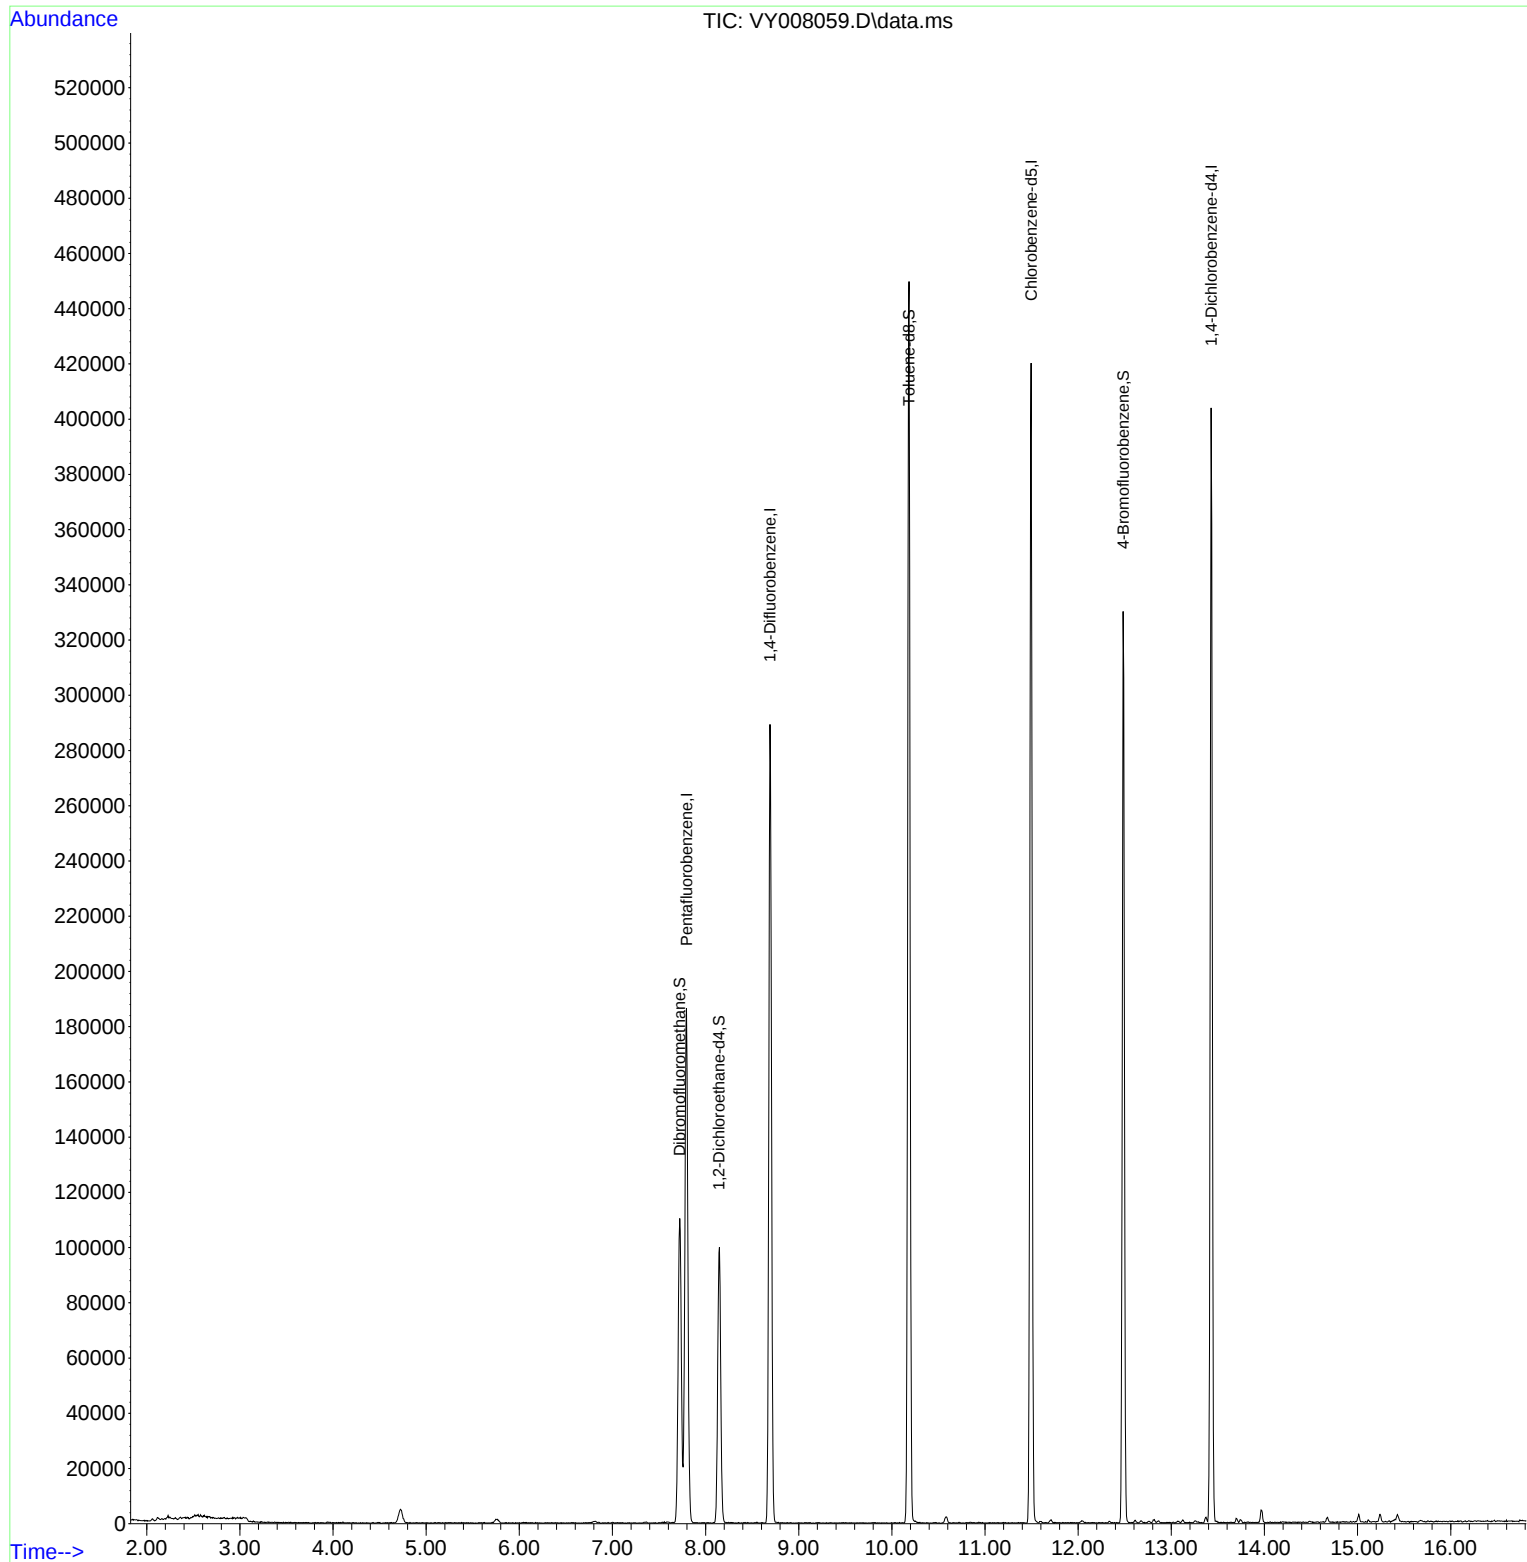


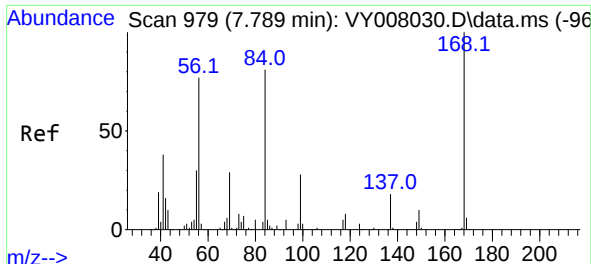

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.795 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY008059.D
Acq: 28 Mar 2022 11:56




Instrument :
MSVOA_Y
ClientSampleId :
VY0328SBL01

Tgt Ion:168 Resp: 144683
Ion Ratio Lower Upper
168 100
99 56.6 46.9 70.3

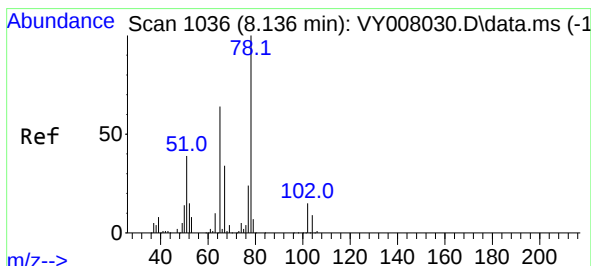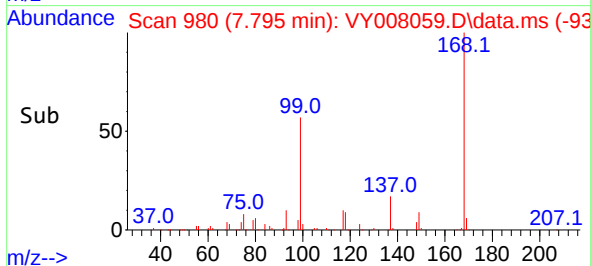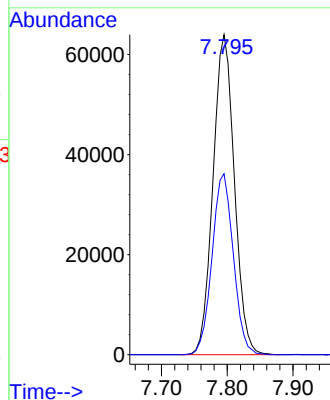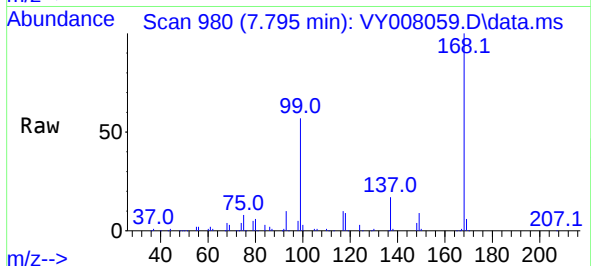

#33
1,2-Dichloroethane-d4
Concen: 54.336 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. 0.007 min
Lab File: VY008059.D
Acq: 28 Mar 2022 11:56

Tgt Ion: 65 Resp: 78875
Ion Ratio Lower Upper
65 100
67 53.6 0.0 99.4

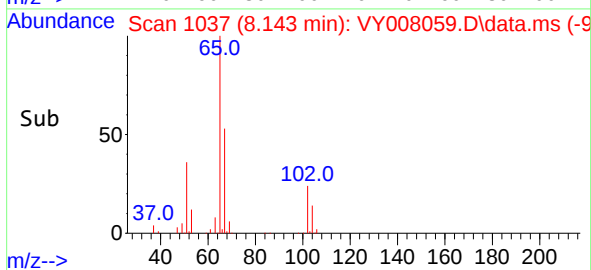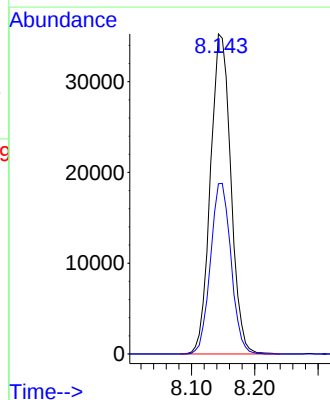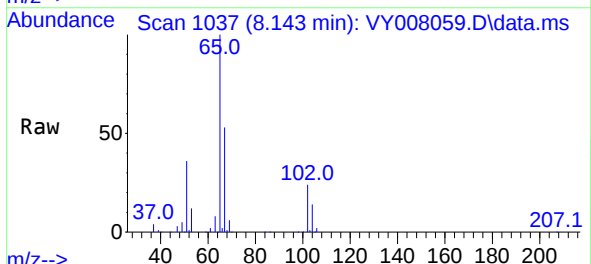



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.006 min

Lab File: VY008059.D

Acq: 28 Mar 2022 11:56

Instrument :

MSVOA_Y

ClientSampleId :

VY0328SBL01




Tgt Ion:114 Resp: 261300

Ion Ratio Lower Upper

114 100

63 18.0 0.0 43.2

88 14.6 0.0 31.8

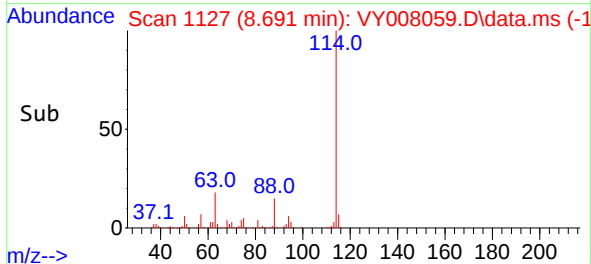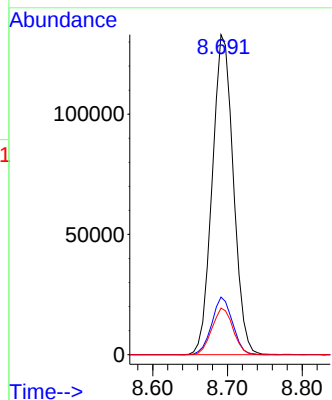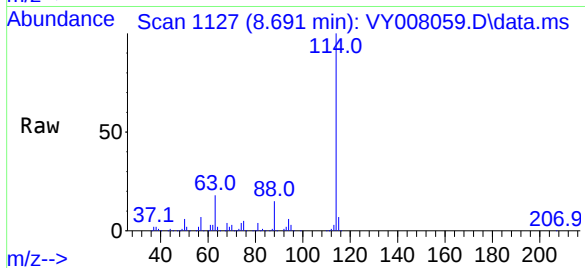

#35

Dibromofluoromethane

Concen: 50.027 ug/l

RT: 7.722 min Scan# 968

Delta R.T. 0.006 min

Lab File: VY008059.D

Acq: 28 Mar 2022 11:56




Tgt Ion:113 Resp: 81958


Ion Ratio Lower Upper

113 100

111 100.3 82.6 124.0

192 17.9 17.6 26.4

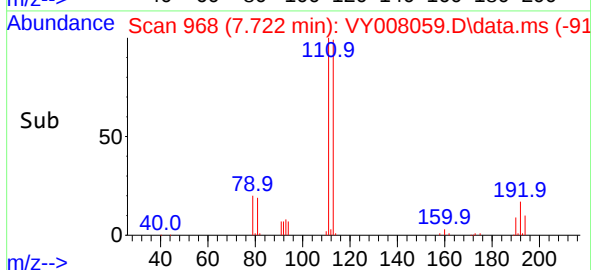
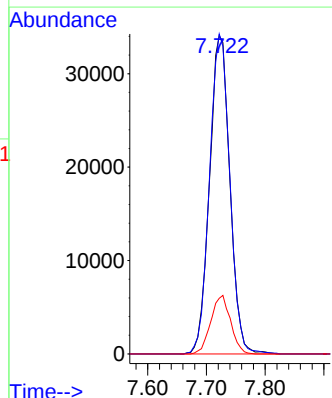
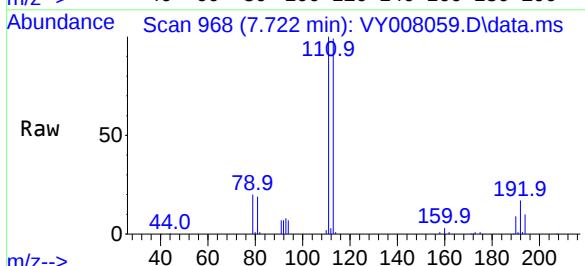


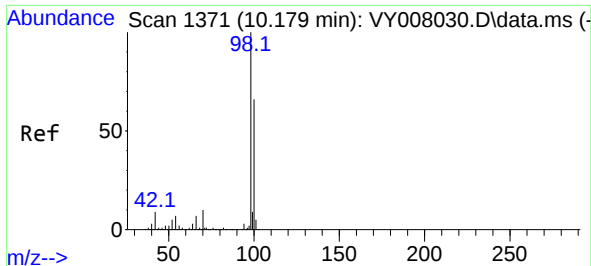

#50
Toluene-d8
Concen: 50.392 ug/l
RT: 10.185 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY008059.D
Acq: 28 Mar 2022 11:56




Instrument :
MSVOA_Y
ClientSampleId :
VY0328SBL01


Tgt Ion: 98 Resp: 311030
Ion Ratio Lower Upper
98 100
100 65.5 50.2 75.2

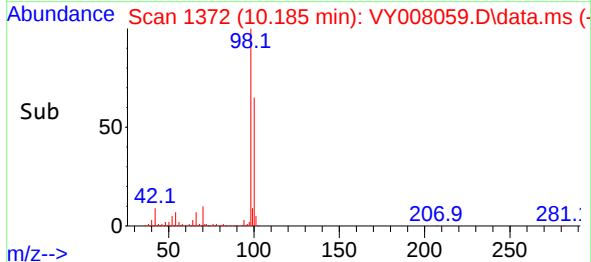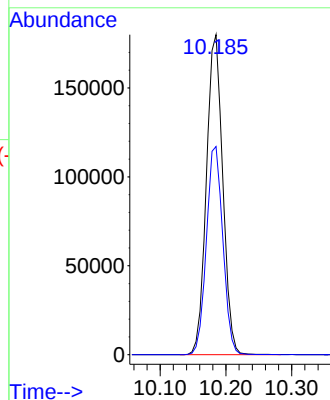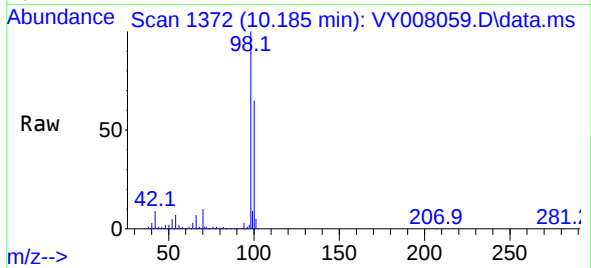

#62
4-Bromofluorobenzene
Concen: 48.964 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY008059.D
Acq: 28 Mar 2022 11:56

Tgt Ion: 95 Resp: 106623
Ion Ratio Lower Upper
95 100
174 78.7 0.0 177.0
176 77.2 0.0 175.8


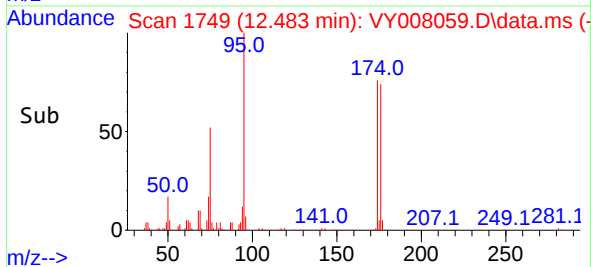
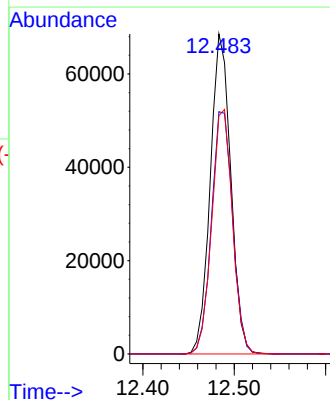
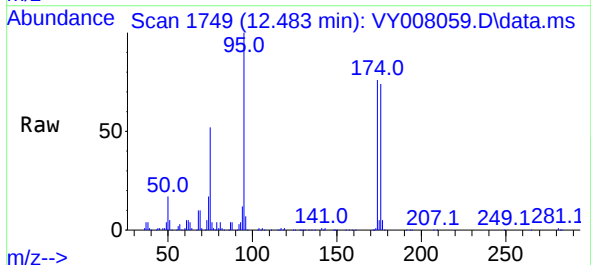


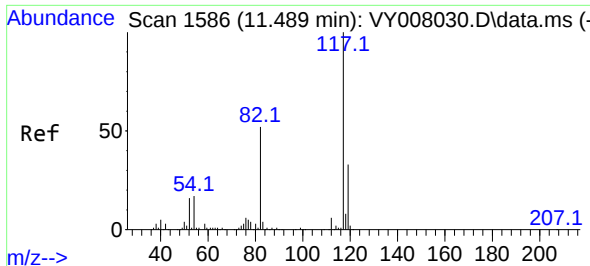

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.496 min Scan# 11
Delta R.T. 0.007 min
Lab File: VY008059.D
Acq: 28 Mar 2022 11:56

Instrument :
MSVOA_Y
ClientSampleId :
VY0328SBL01

Tgt Ion:117 Resp: 240031
Ion Ratio Lower Upper
117 100
82 51.7 43.0 64.4
119 31.5 25.4 38.0

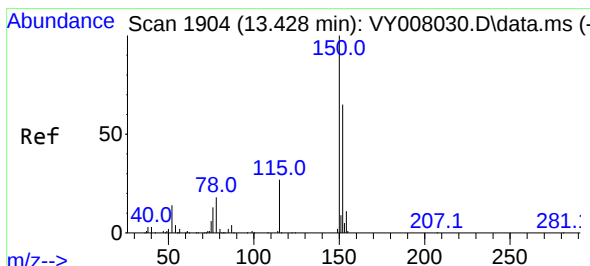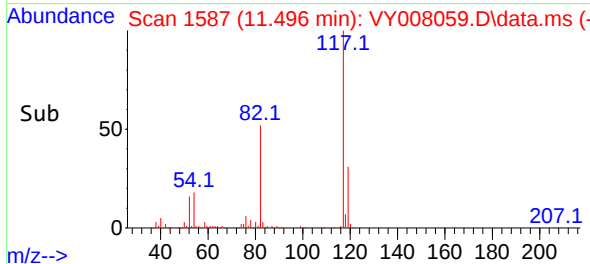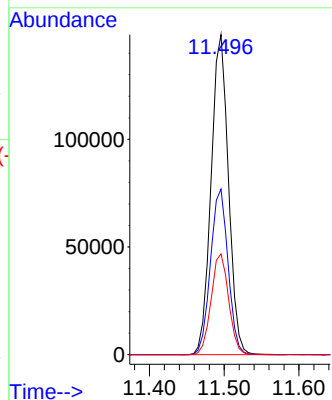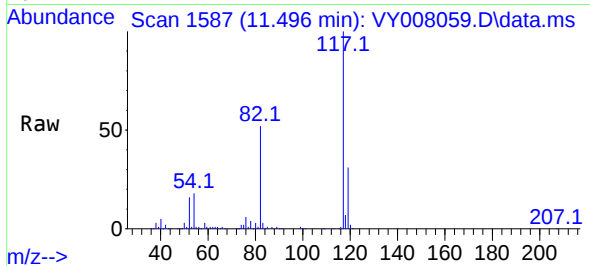

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY008059.D
Acq: 28 Mar 2022 11:56

Tgt Ion:152 Resp: 104062
Ion Ratio Lower Upper
152 100
115 59.9 28.2 84.7
150 156.1 0.0 347.6

