



Acrolein

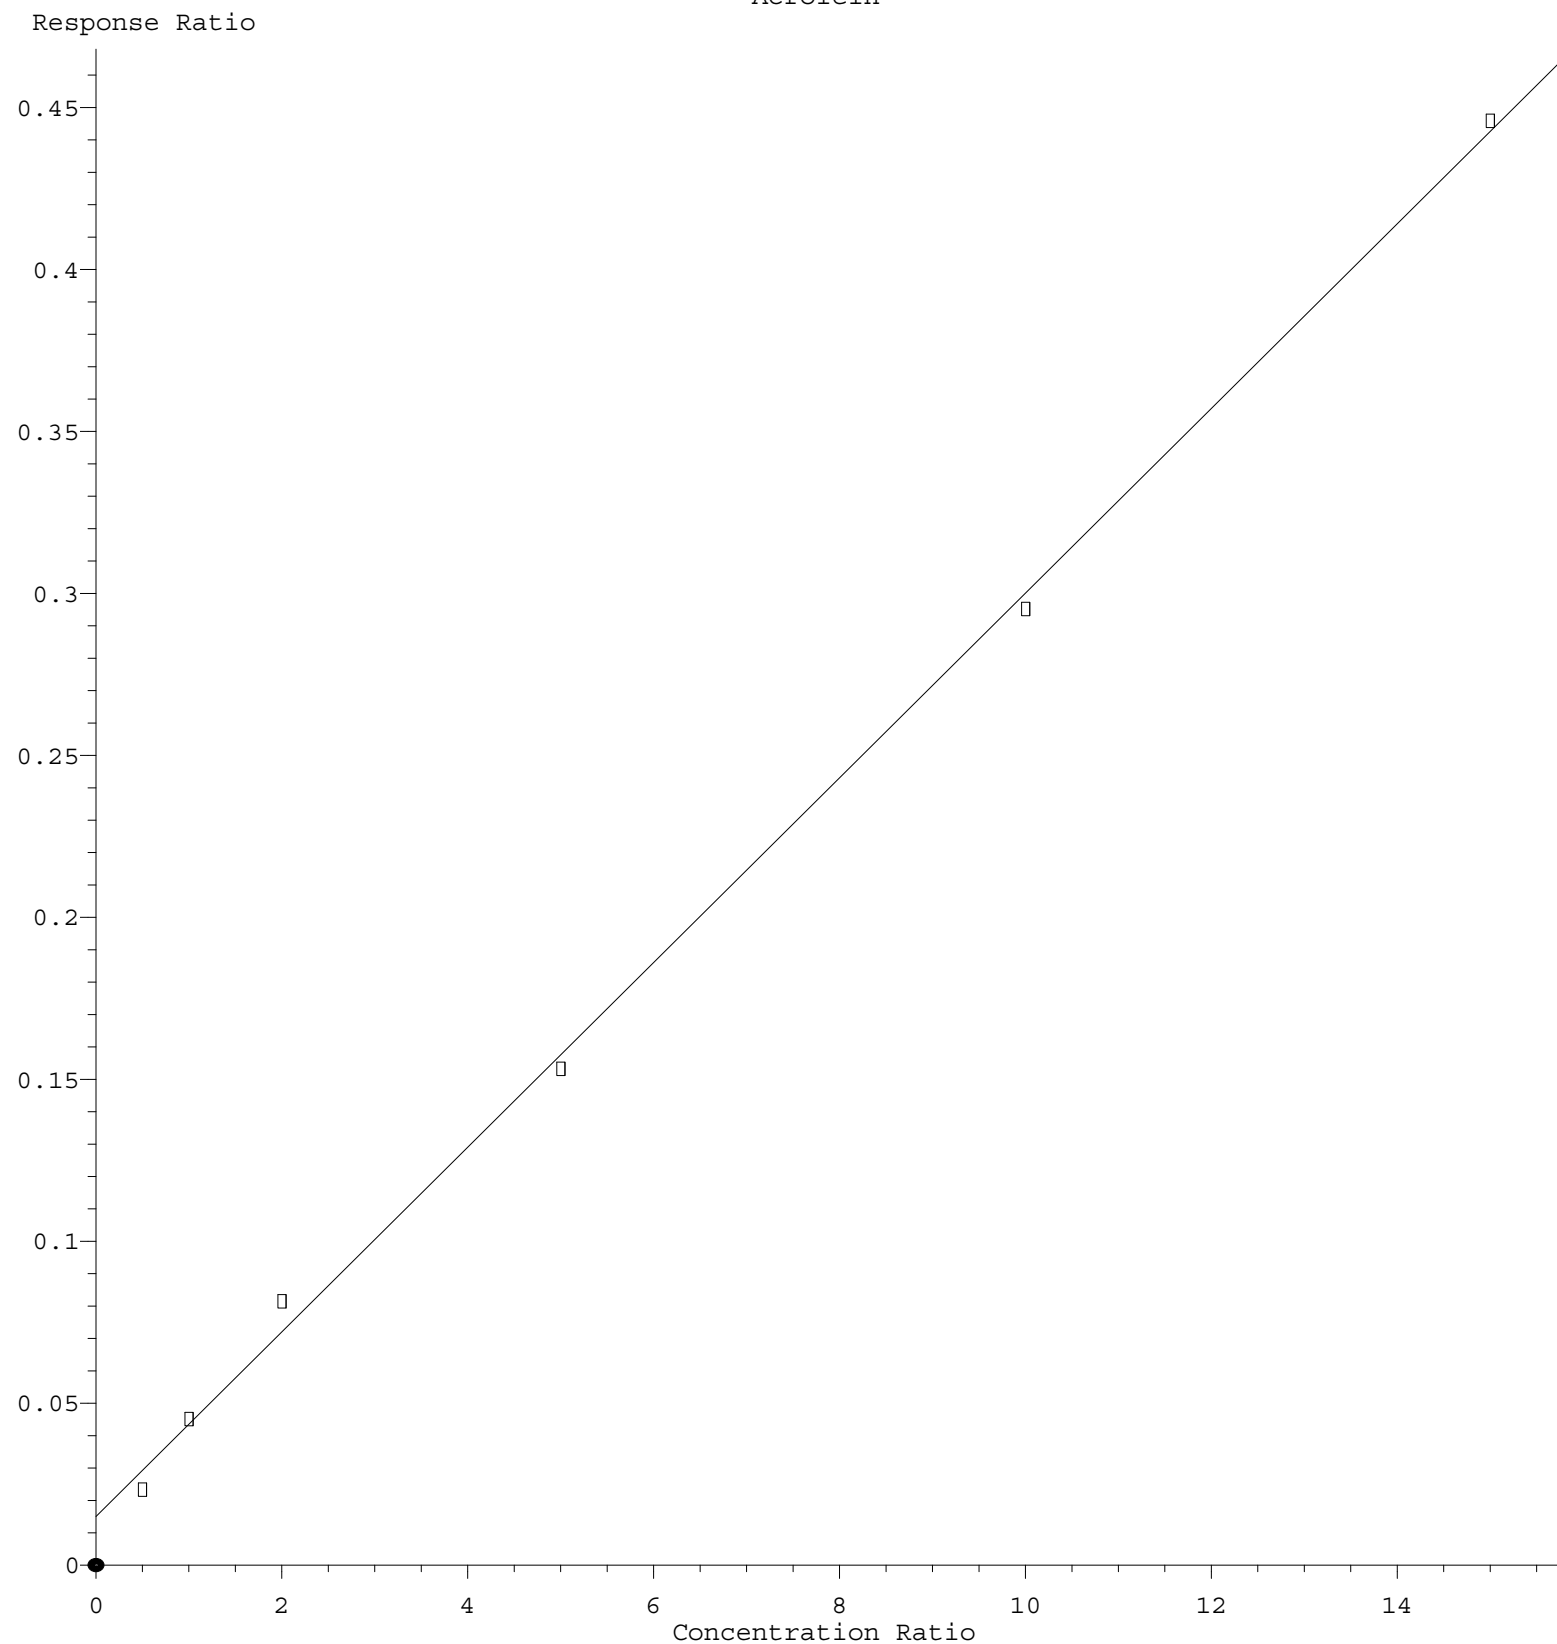

$\text{Response} = 2.851\text{e-}002 * \text{Amt} + 1.484\text{e-}002$
 Coef of Det (r^2) = 0.998682 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y032921S.M
 Calibration Table Last Updated: Tue Mar 30 06:38:14 2021

Methylene Chloride

Response Ratio

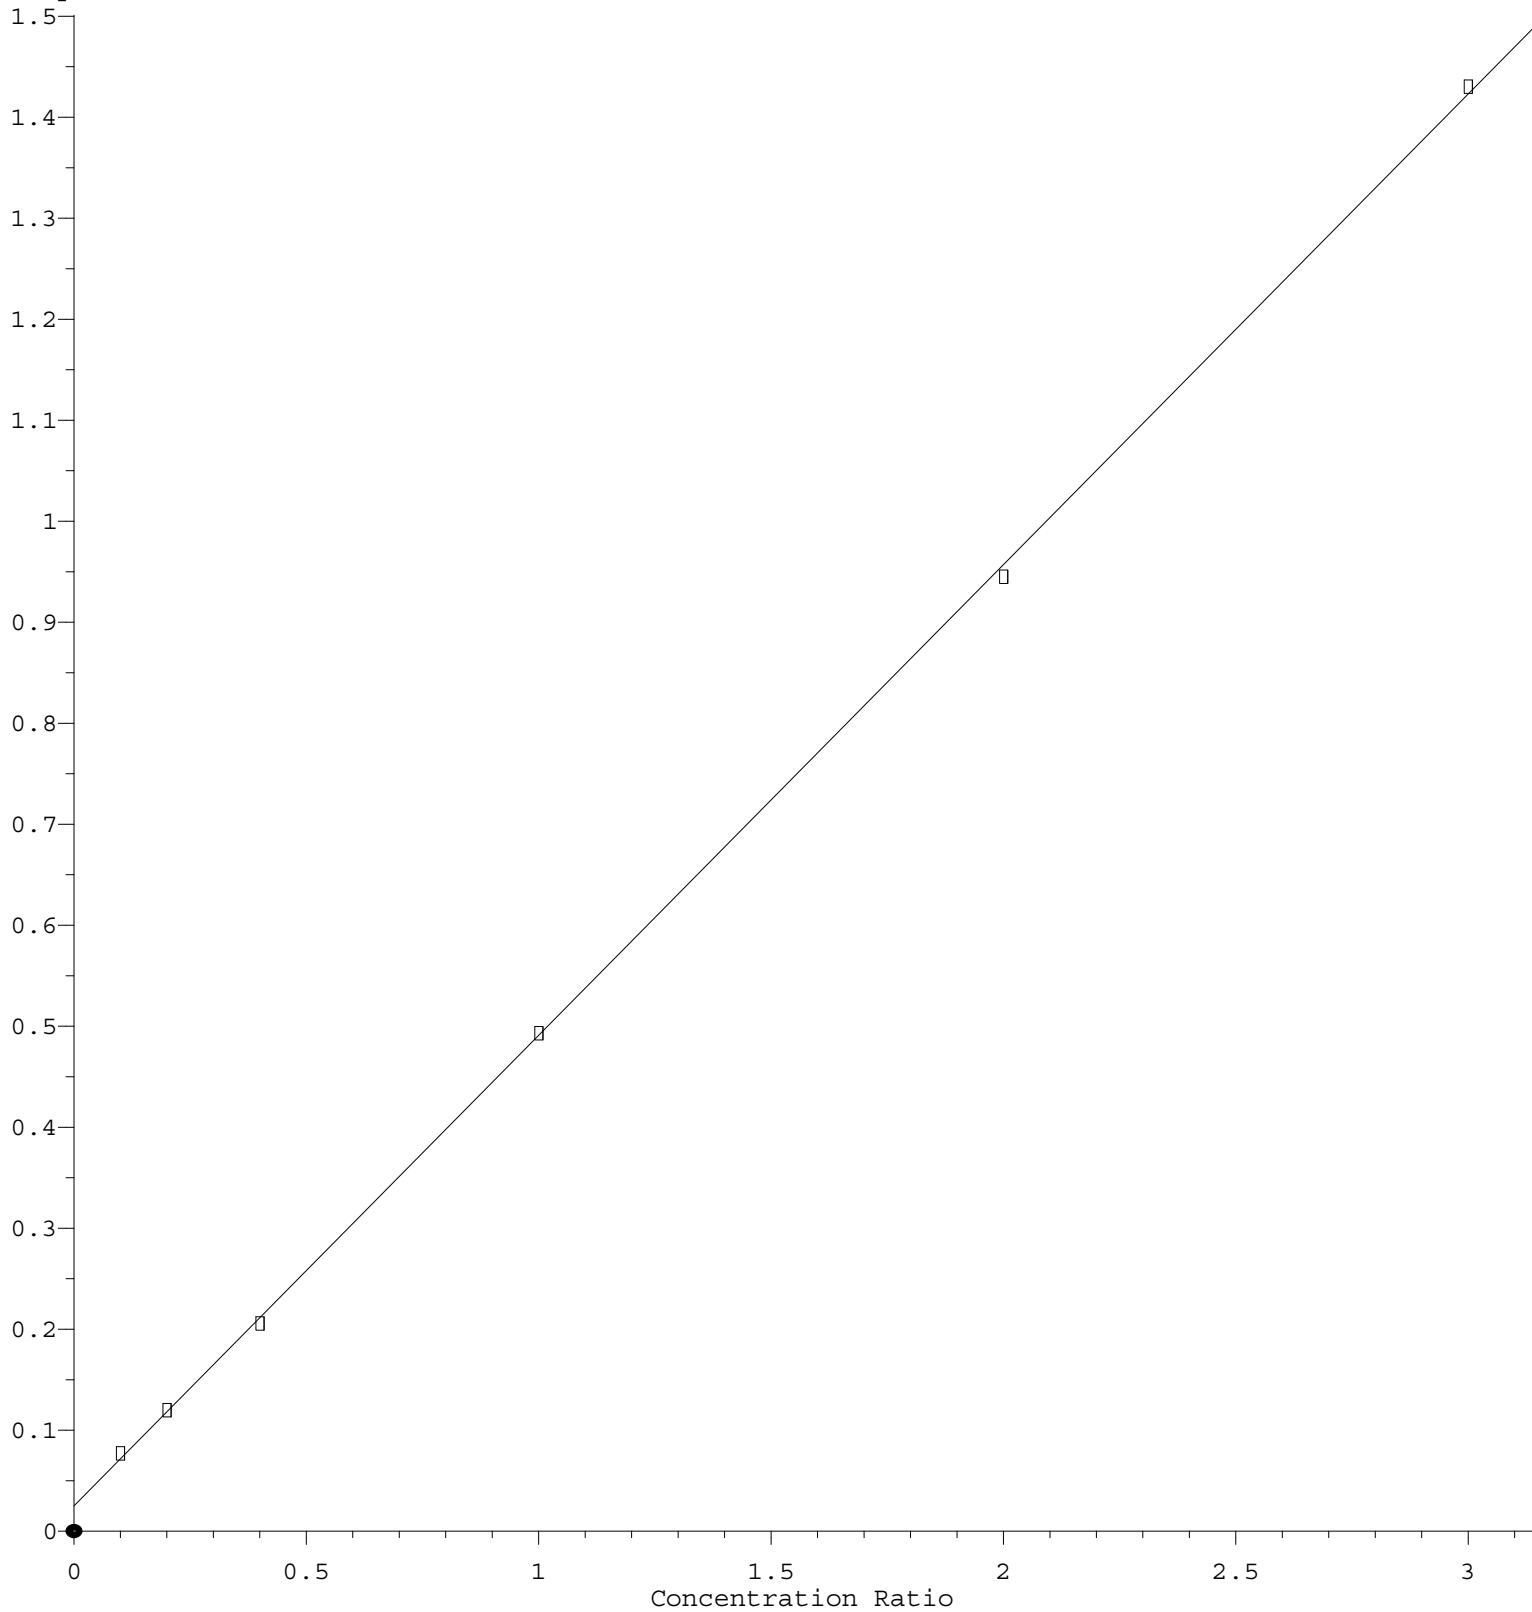


$$\text{Response} = 4.660\text{e-}001 * \text{Amt} + 2.474\text{e-}002$$

Coef of Det (r^2) = 0.999820 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y032921S.M

Calibration Table Last Updated: Tue Mar 30 06:38:14 2021


1,4-Dioxane

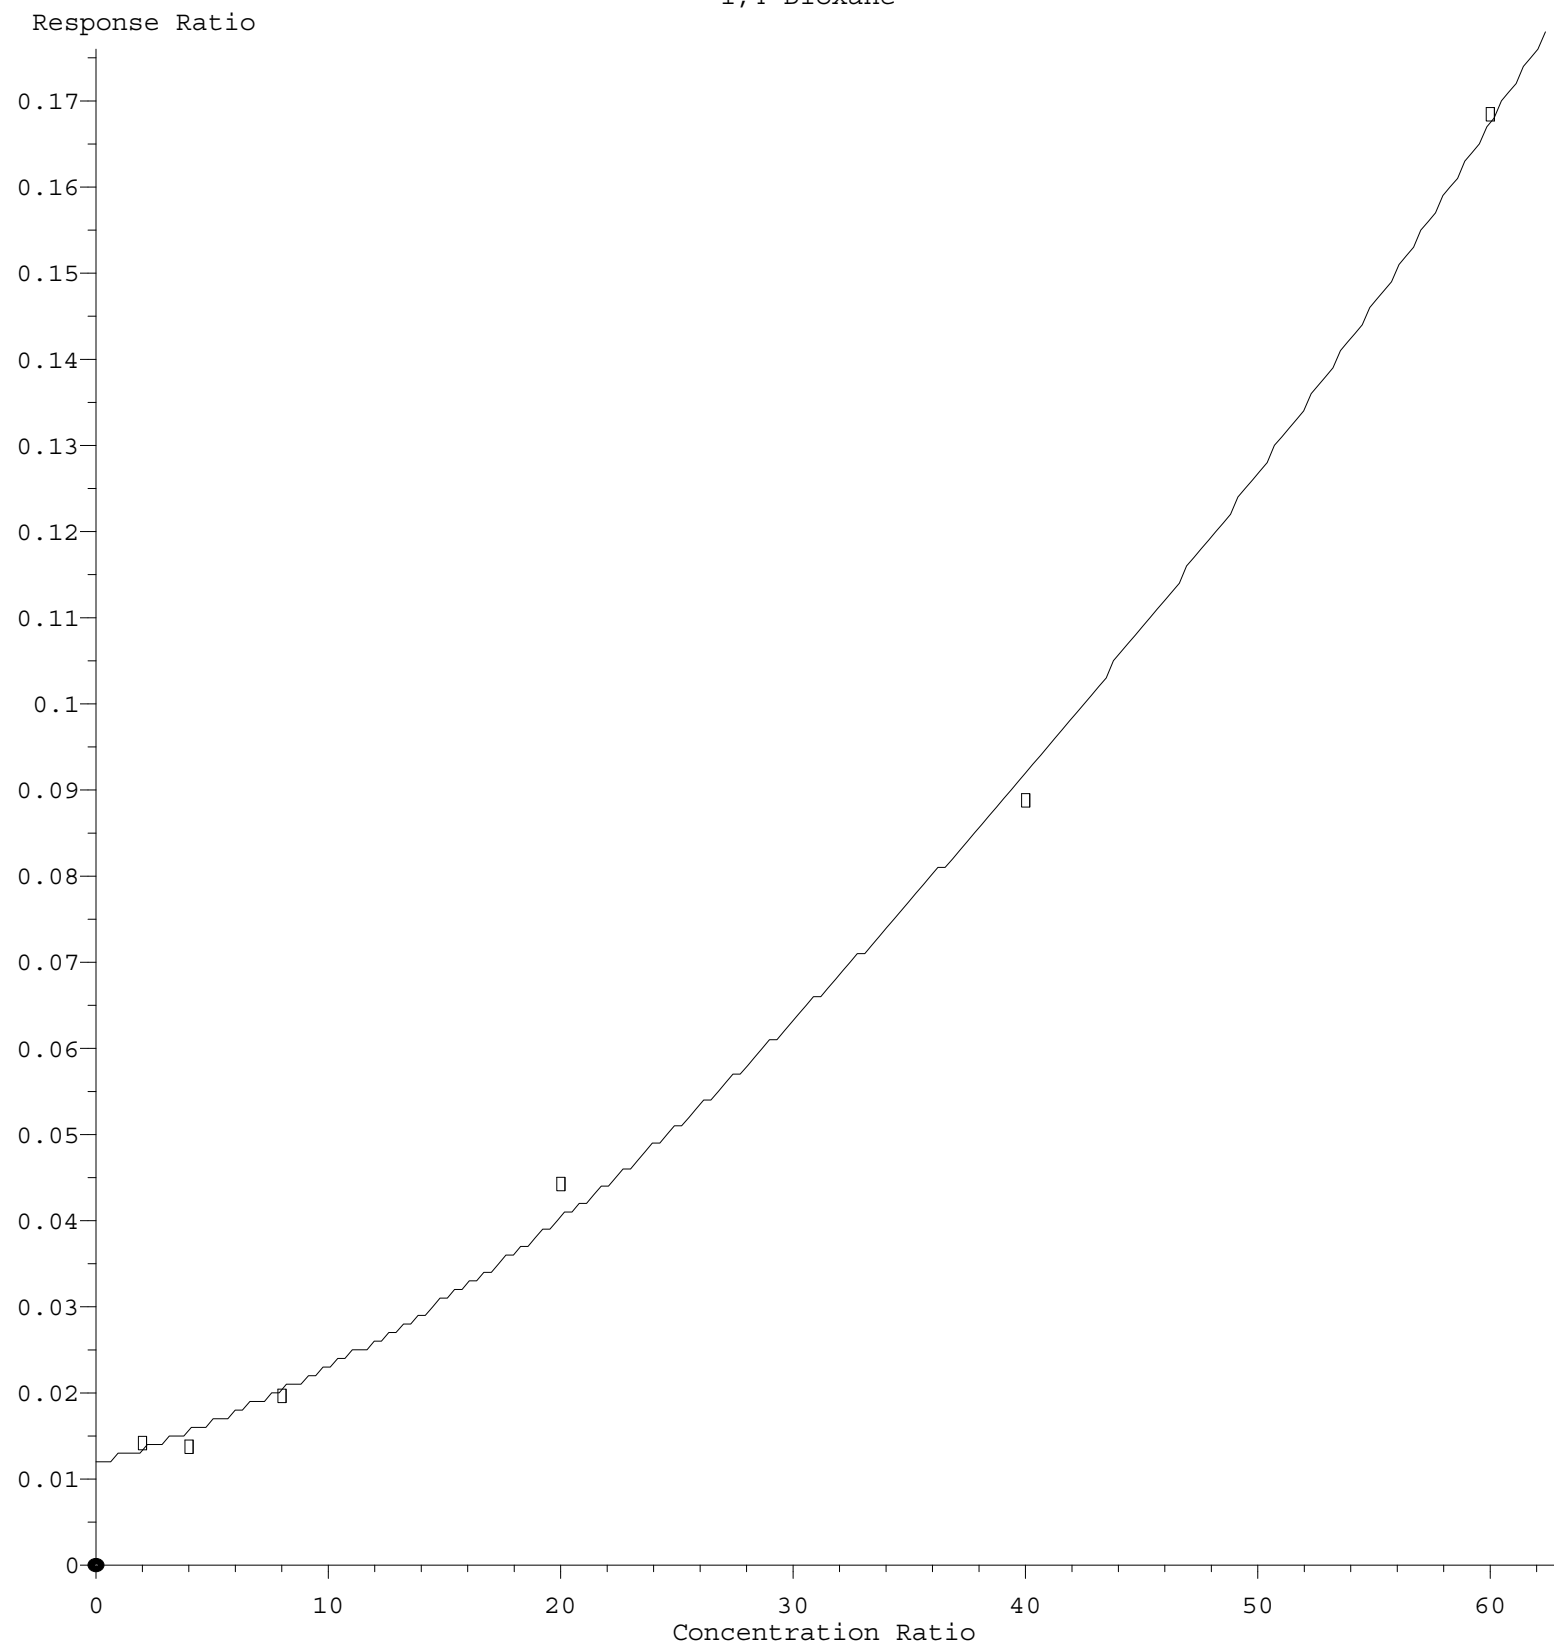

$R = 2.926e-005 A^2 + 8.391e-004 A + 1.171e-002$
Coef of Det (r^2) = 0.998259 Curve Fit: Quadratic
Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y032921S.M
Calibration Table Last Updated: Tue Mar 30 06:38:14 2021

Hexachloroethane

Response Ratio

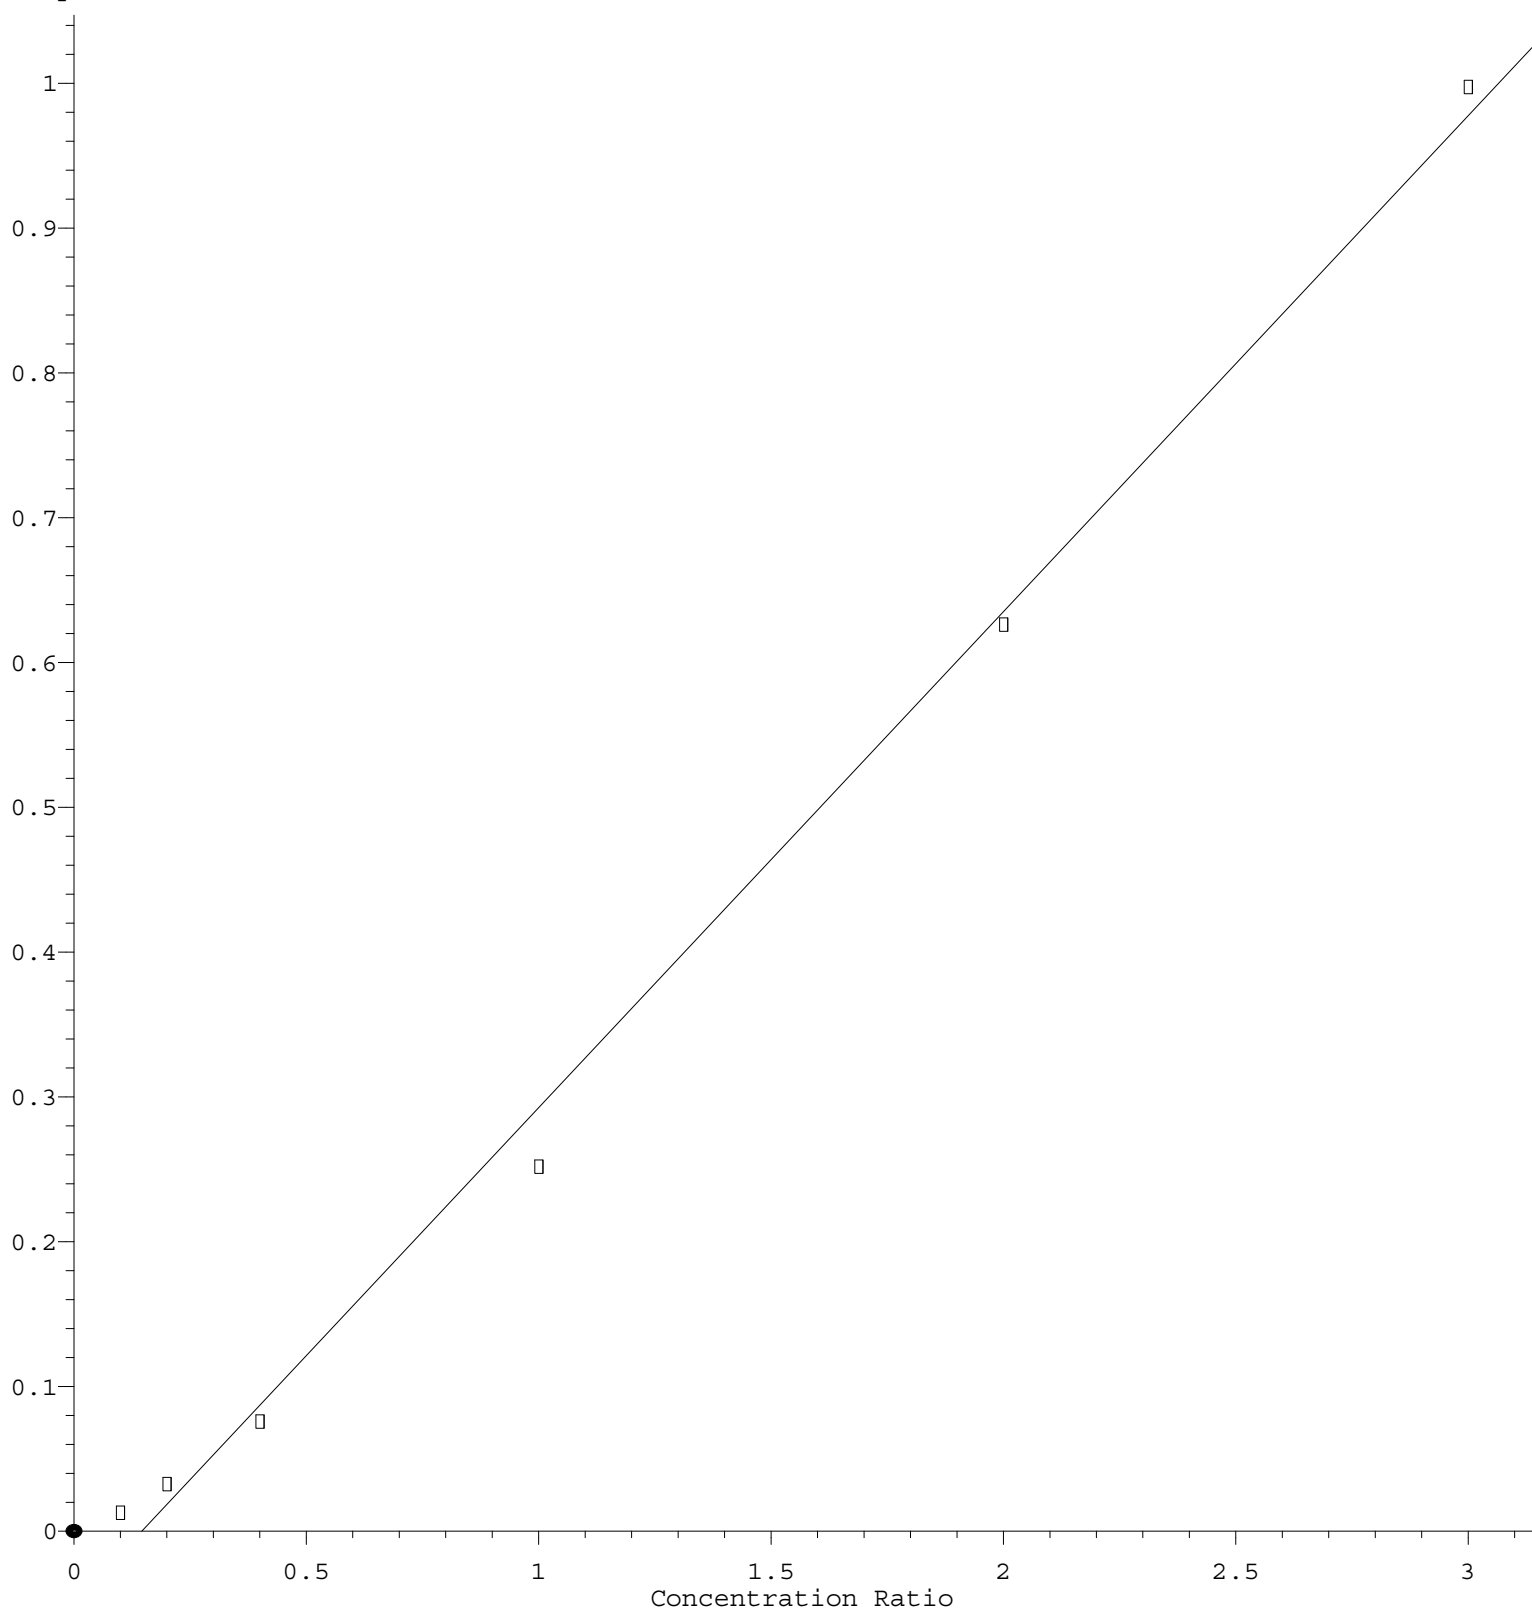

$$\text{Response} = 3.426\text{e-}001 * \text{Amt} - 4.991\text{e-}002$$

Coef of Det (r^2) = 0.995878 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y032921S.M

Calibration Table Last Updated: Tue Mar 30 06:38:14 2021