

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY033120\
 Data File : VY002135.D
 Acq On : 31 Mar 2020 15:59
 Operator : SY/MD
 Sample : L2054-01
 Misc : 7.68G/5ML/MSVOA Y/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 239-SB-07-1-2

Quant Time: Apr 01 05:12:33 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y032620S.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 27 07:11:05 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.82	168	119875	50.00	ug/l	0.01
34) 1,4-Difluorobenzene	8.71	114	238721	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.50	117	225547	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.44	152	94657	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.17	65	77028	58.13	ug/l	0.00
Spiked Amount	50.000		Recovery	=	116.26%	
35) Dibromofluoromethane	7.75	113	70867	52.98	ug/l	0.01
Spiked Amount	50.000		Recovery	=	105.96%	
50) Toluene-d8	10.19	98	291602	52.48	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.96%	
62) 4-Bromofluorobenzene	12.49	95	98303	50.58	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.16%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY033120\
Data File : VY002135.D
Acq On : 31 Mar 2020 15:59
Operator : SY/MD
Sample : L2054-01
Misc : 7.68G/5ML/MSVOA Y/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
239-SB-07-1-2

Quant Time: Apr 01 05:12:33 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y032620S.M
Quant Title : SW846 8260
QLast Update : Fri Mar 27 07:11:05 2020
Response via : Initial Calibration

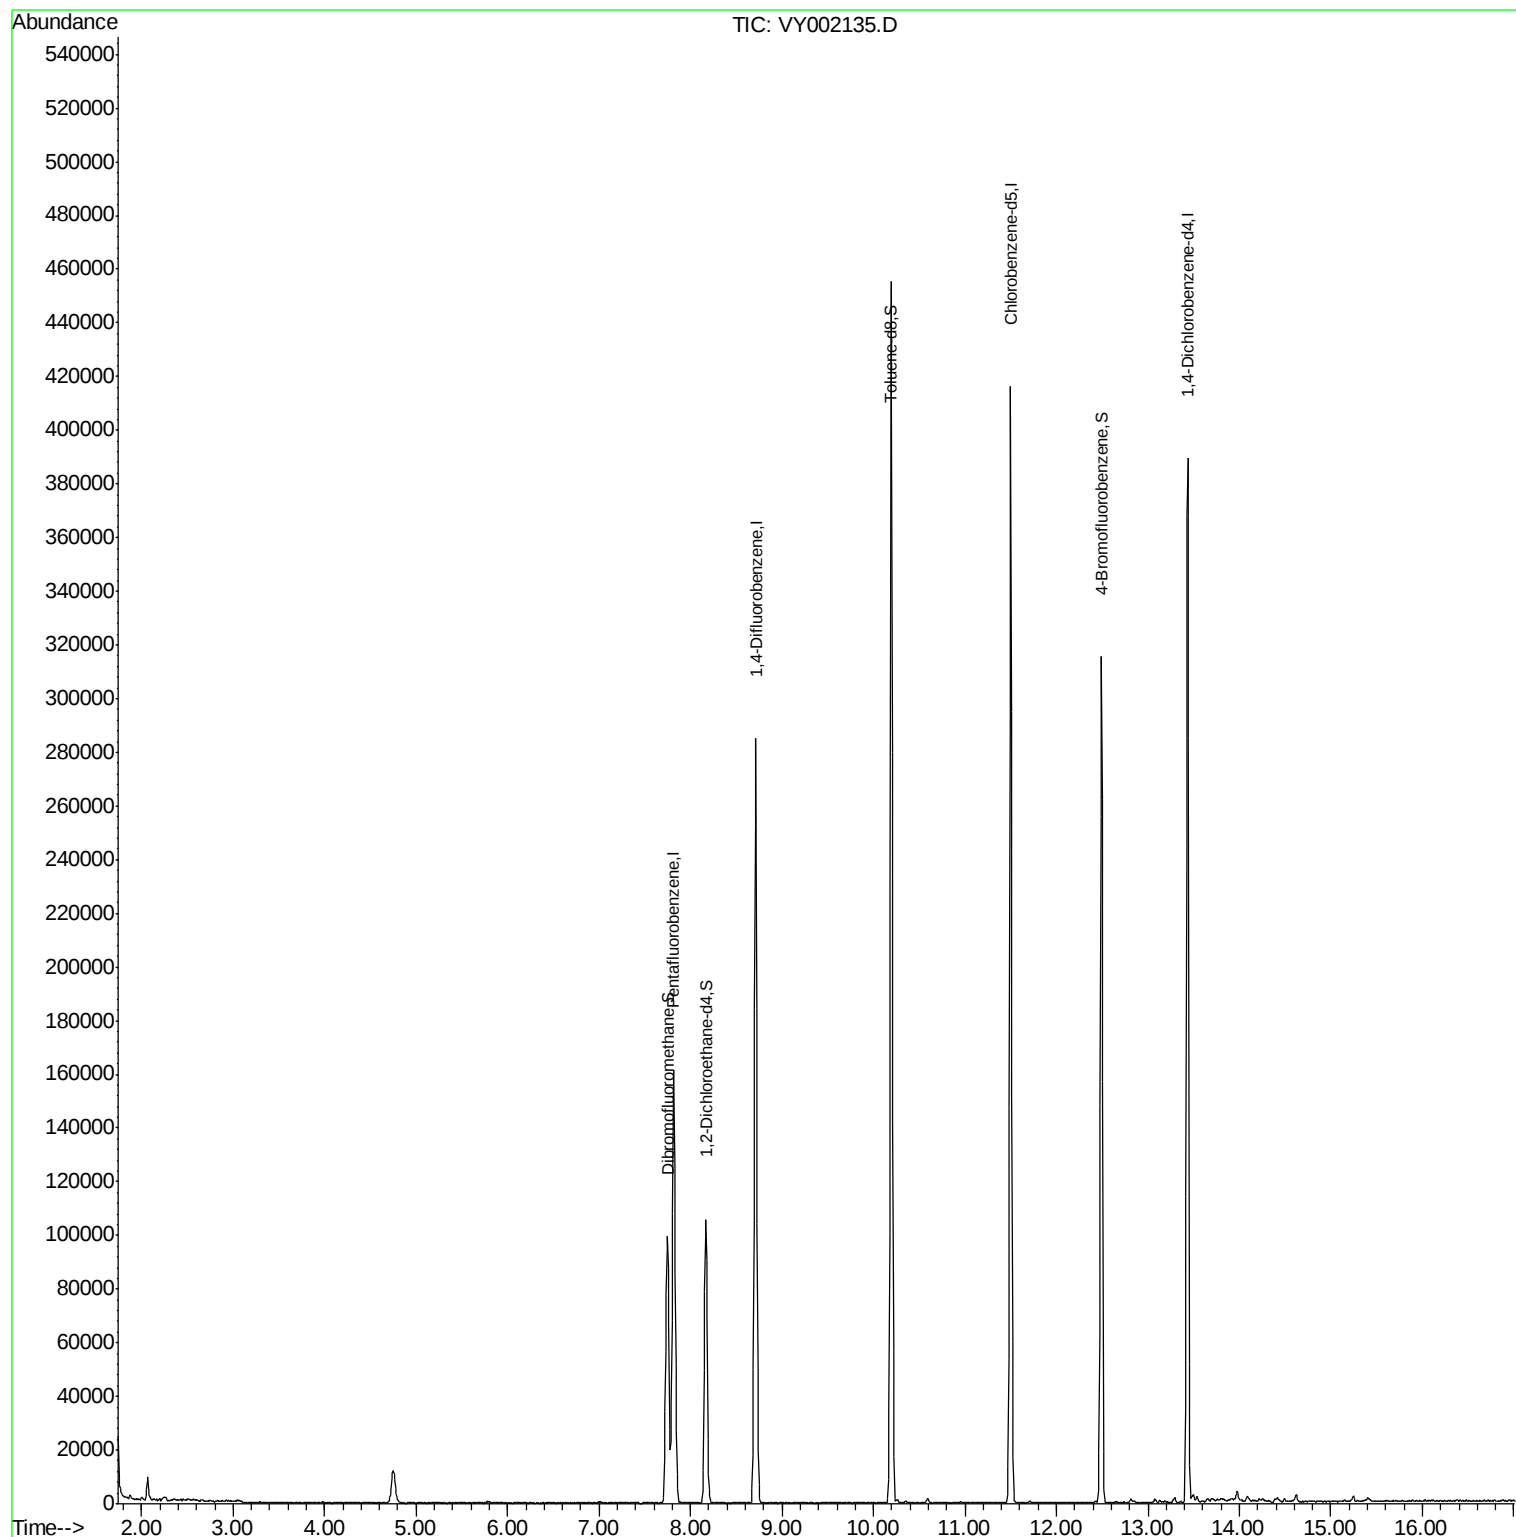

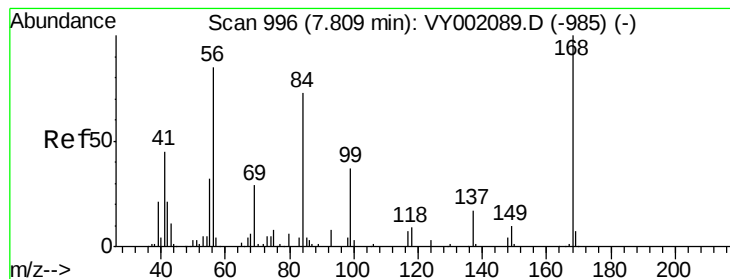

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.82 min Scan# 998

Delta R.T. 0.01 min

Lab File: VY002135.D

Acq: 31 Mar 2020 15:59

Instrument :

MSVOA_Y

ClientSampleId :


239-SB-07-1-2

Tot Ion:168 Resp: 119875




Ion Ratio Lower Upper

168 100

99 59.1 47.6 71.4

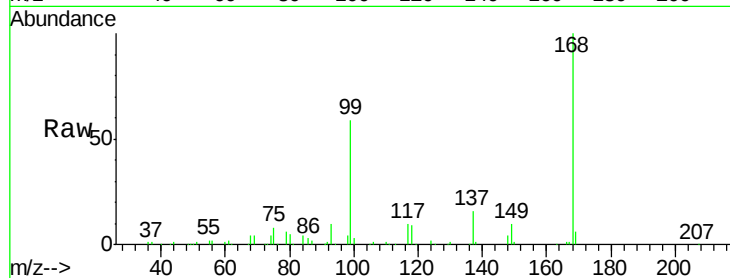

Abundance Ion 167.90 (167.60 to 168.60): VY002135.D (-947) (-)

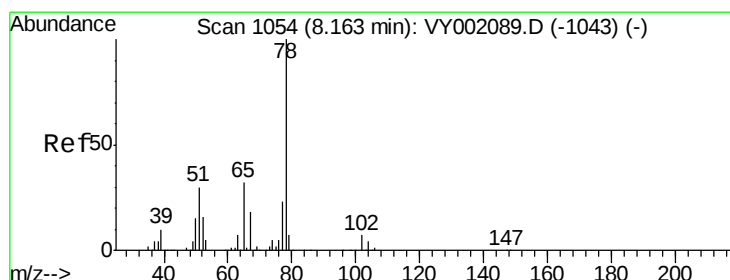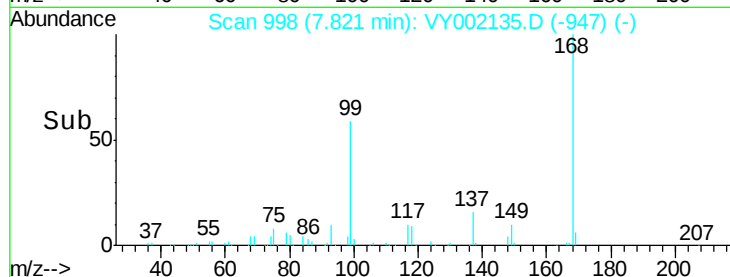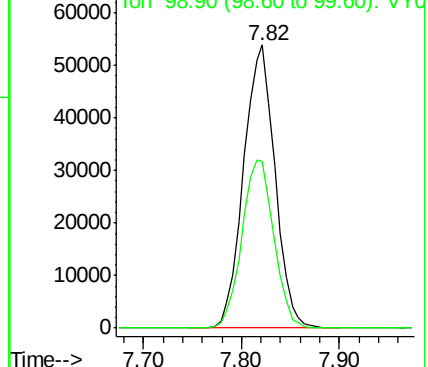

#33

1,2-Dichloroethane-d4

Concen: 58.126 ug/l

RT: 8.17 min Scan# 1055

Delta R.T. 0.01 min

Lab File: VY002135.D


Acq: 31 Mar 2020 15:59

Tgt Ion: 65 Resp: 77028



Ion Ratio Lower Upper


65 100

67 54.0 0.0 112.8

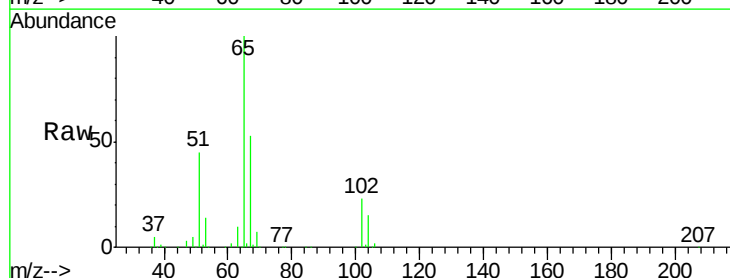

Abundance Ion 64.90 (64.60 to 65.60): VY002135.D (-1005) (-)



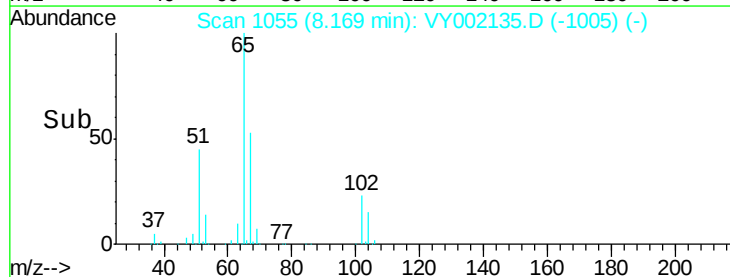
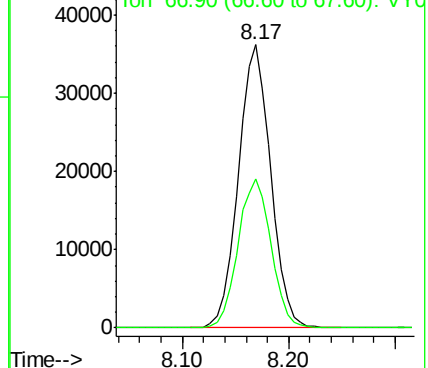


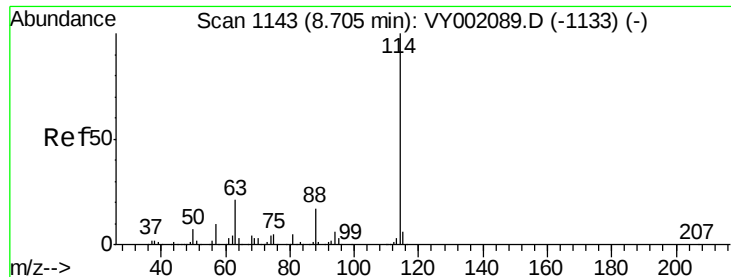

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.71 min Scan# 1144
 Delta R.T. 0.01 min
 Lab File: VY002135.D
 Acq: 31 Mar 2020 15:59




Instrument :
 MSVOA_Y
 ClientSampleId :
 239-SB-07-1-2


Tot Ion	Ratio	Lower	Upper
114	100		
63	21.3	0.0	41.4
88	16.0	0.0	33.0

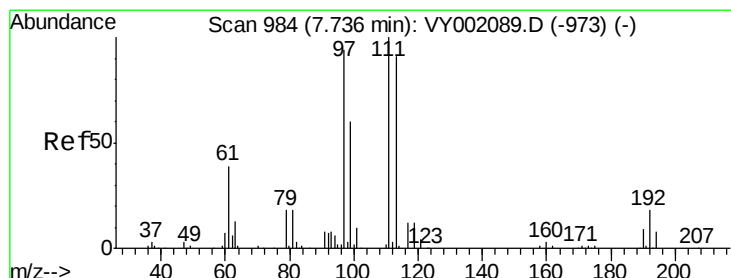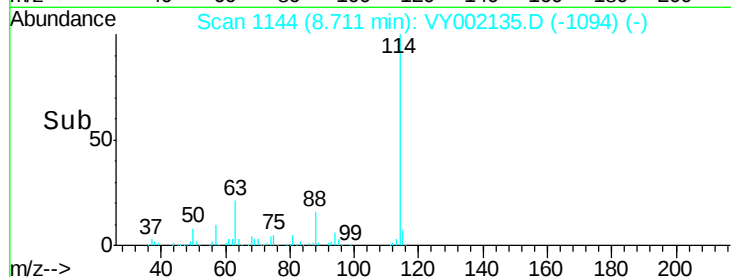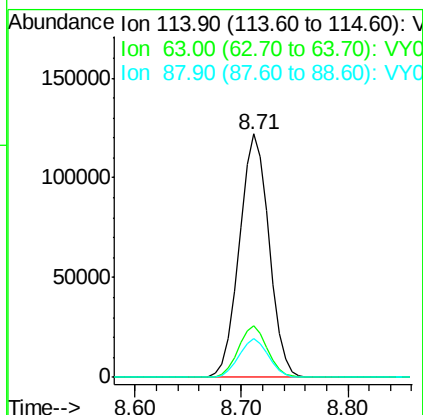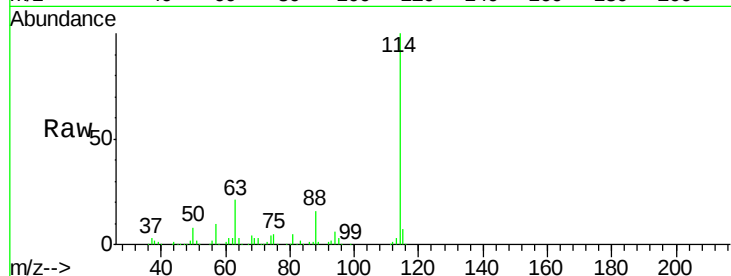

#35
 Dibromofluoromethane
 Concen: 52.981 ug/l
 RT: 7.75 min Scan# 986
 Delta R.T. 0.01 min
 Lab File: VY002135.D
 Acq: 31 Mar 2020 15:59

Tgt Ion	Ratio	Lower	Upper
113	100		
111	103.5	84.4	126.6
192	18.0	14.6	21.8

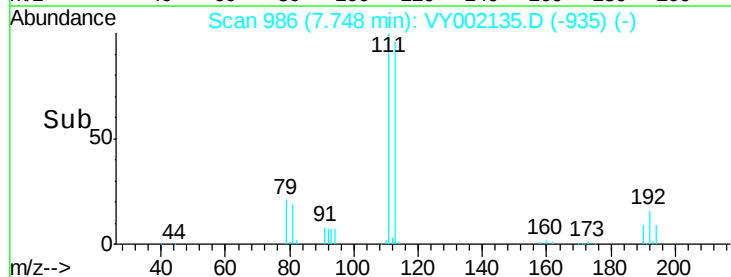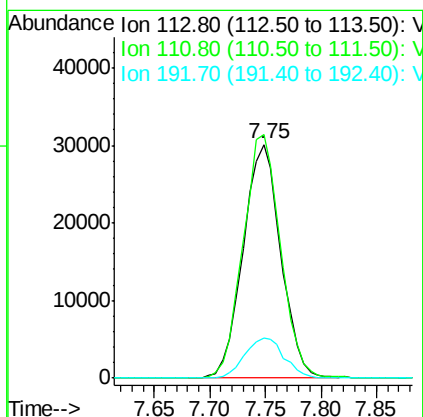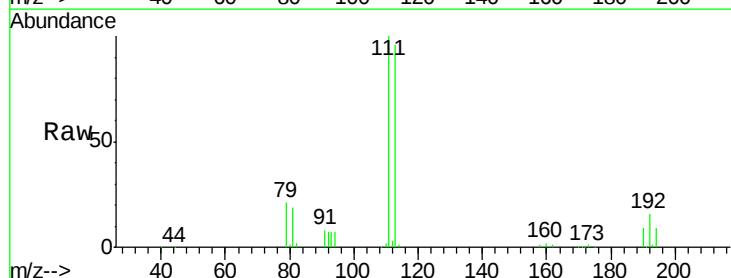

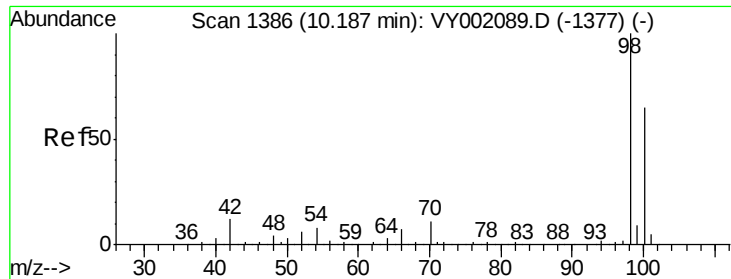

#50

Toluene-d8

Concen: 52.478 ug/l

RT: 10.19 min Scan# 1387

Delta R.T. 0.01 min

Lab File: VY002135.D

Acq: 31 Mar 2020 15:59

Instrument :

MSVOA_Y

ClientSampleId :


239-SB-07-1-2

Tot Ion: 98 Resp: 291602

Ion Ratio Lower Upper

98 100

100 66.0 51.6 77.4

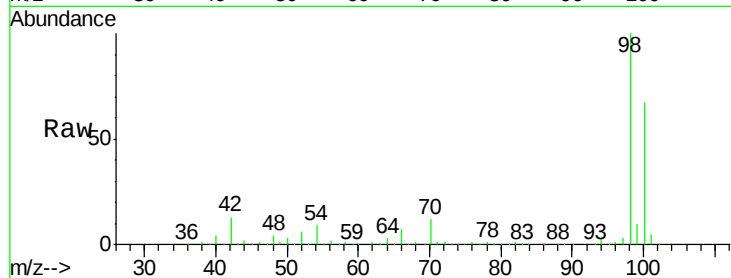

Abundance Ion 98.00 (97.70 to 98.70): VY0

Ion 100.00 (99.70 to 100.70): VY

10.19



150000

100000

50000

0

Time-->

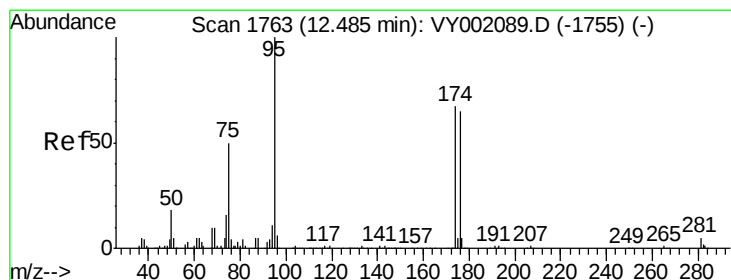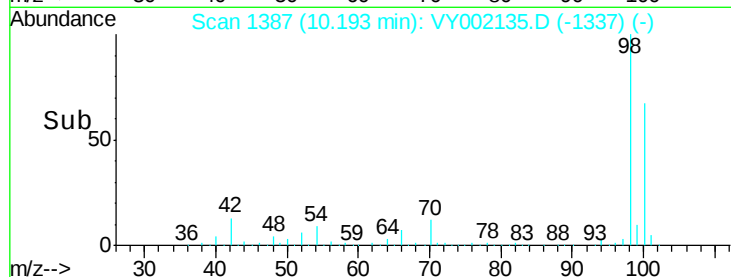

#62

4-Bromofluorobenzene

Concen: 50.584 ug/l

RT: 12.49 min Scan# 1764

Delta R.T. 0.01 min

Lab File: VY002135.D

Acq: 31 Mar 2020 15:59


Tgt Ion: 95 Resp: 98303

Ion Ratio Lower Upper

95 100

174 74.9 0.0 143.4

176 70.8 0.0 137.0

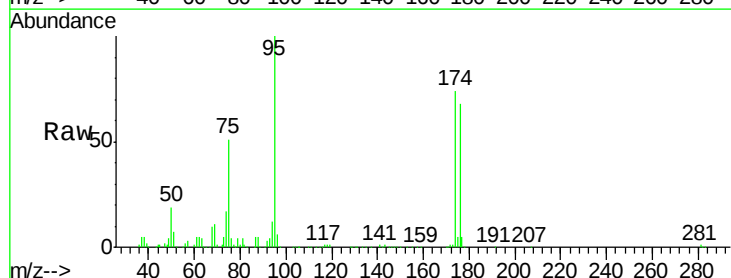

Abundance Ion 94.90 (94.60 to 95.60): VY0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

12.49

80000


60000


40000

20000

0

Time-->

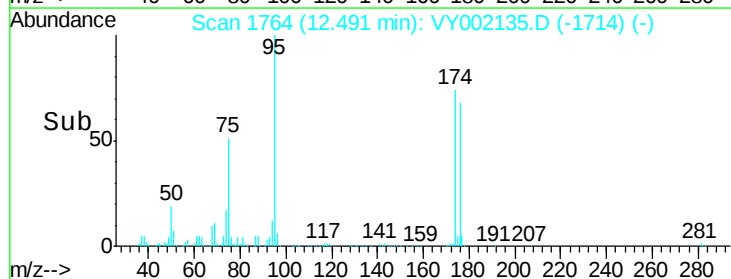


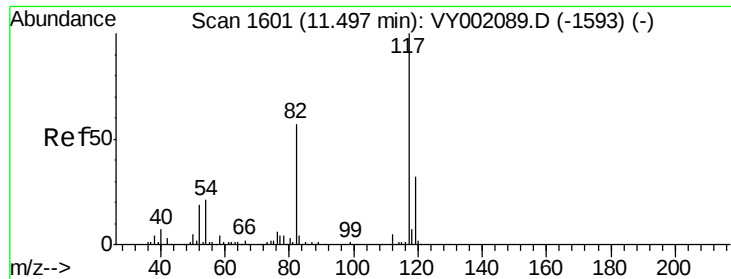




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.50 min Scan# 1602
Delta R.T. 0.01 min
Lab File: VY002135.D
Acq: 31 Mar 2020 15:59

Instrument :
MSVOA_Y
ClientSampleId :
239-SB-07-1-2

Tot Ion	Ratio	Lower	Upper
117	100		
82	56.0	45.4	68.2
119	31.6	25.3	37.9

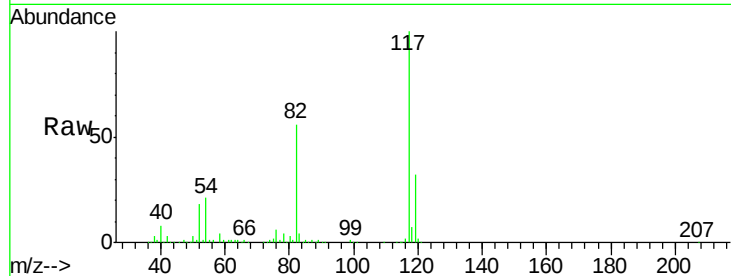


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VY0
Ion 118.90 (118.60 to 119.60): V

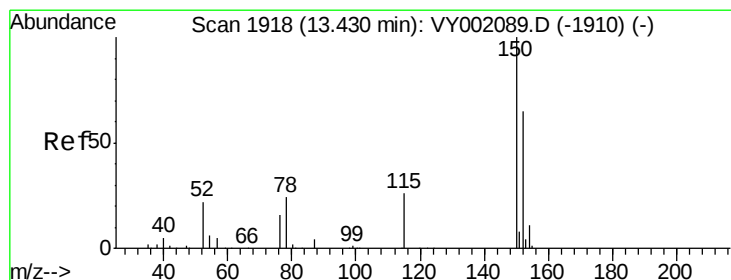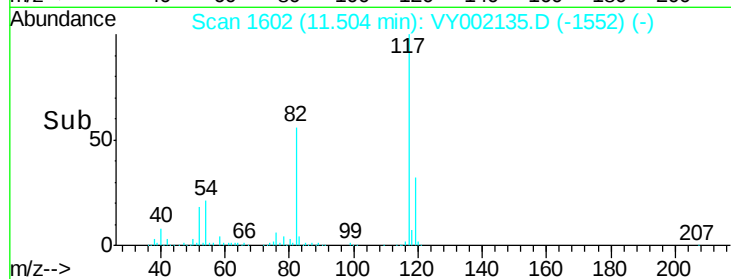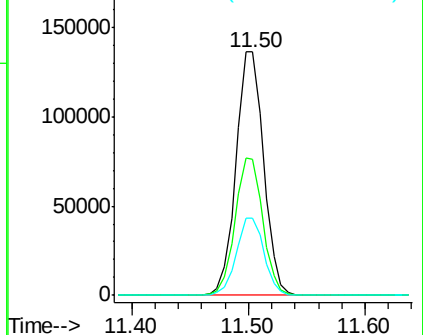

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.44 min Scan# 1919
Delta R.T. 0.01 min
Lab File: VY002135.D
Acq: 31 Mar 2020 15:59

Tgt Ion	Ratio	Lower	Upper
152	100		
115	59.8	31.2	93.6
150	158.7	0.0	354.8

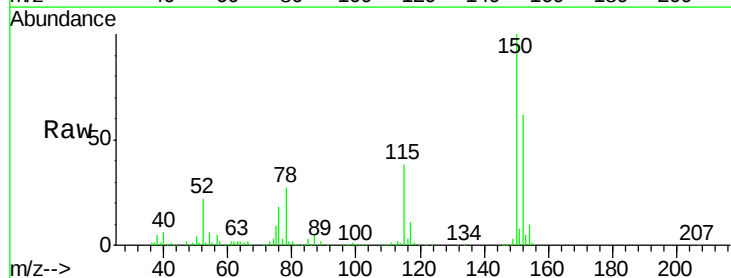

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

