

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY033122\
 Data File : VY008133.D
 Acq On : 31 Mar 2022 12:48
 Operator : SY/MD
 Sample : N2176-03
 Misc : 5.79g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 TT-156-IDWSO-20220329-3

Quant Time: Mar 31 14:23:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032522S.M
 Quant Title : SW846 8260
 QLast Update : Sat Mar 26 03:24:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	130515	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	236554	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	217734	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	89491	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	73932	56.460	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	112.920%
35) Dibromofluoromethane	7.722	113	74898	50.500	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	101.000%
50) Toluene-d8	10.179	98	285046	51.013	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	102.020%
62) 4-Bromofluorobenzene	12.483	95	93288	47.322	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	94.640%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY033122\
Data File : VY008133.D
Acq On : 31 Mar 2022 12:48
Operator : SY/MD
Sample : N2176-03
Misc : 5.79g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
TT-156-IDWSO-20220329-3

Quant Time: Mar 31 14:23:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032522S.M
Quant Title : SW846 8260
QLast Update : Sat Mar 26 03:24:51 2022
Response via : Initial Calibration




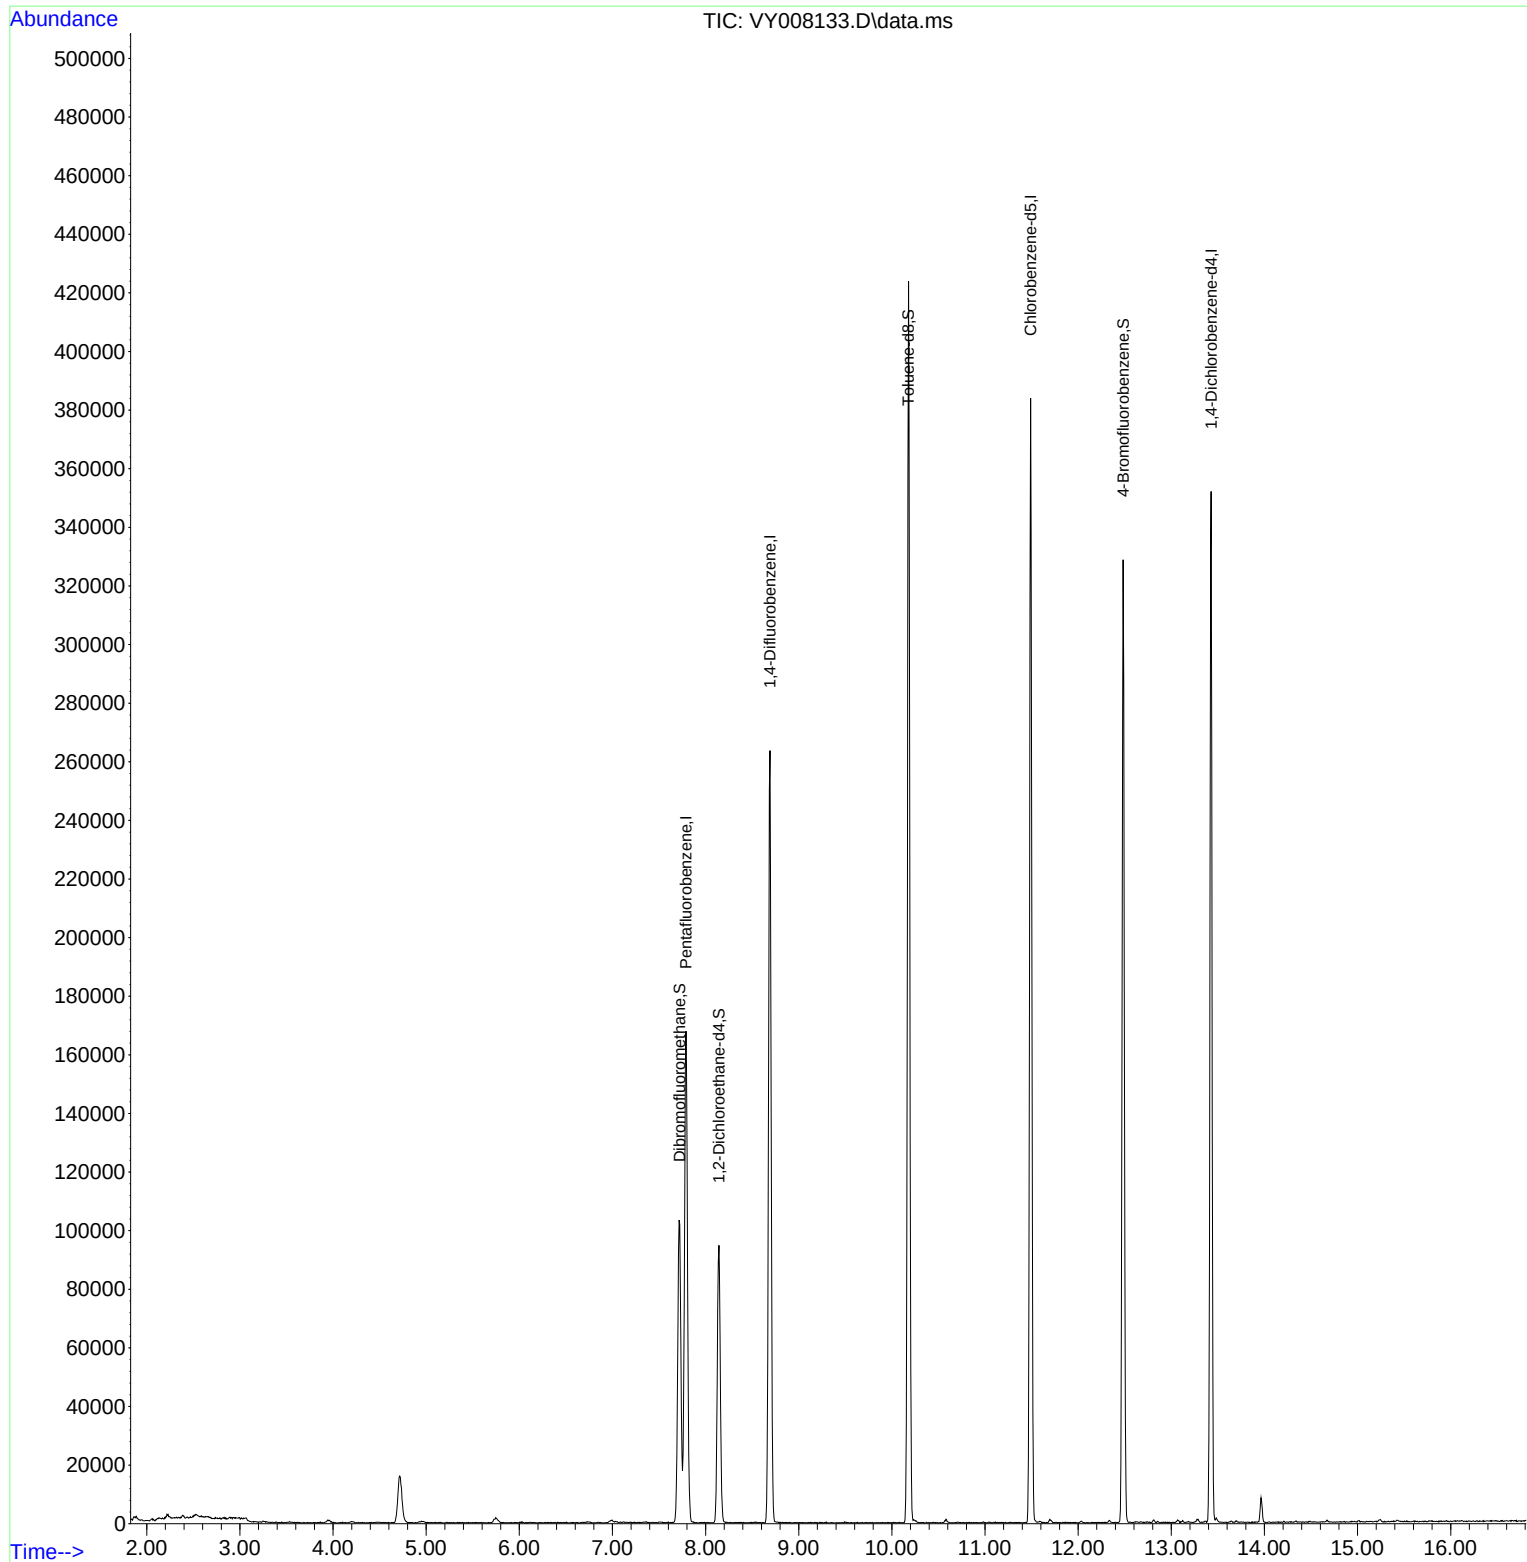


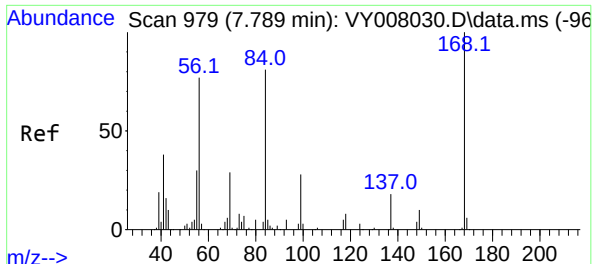

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY008133.D
Acq: 31 Mar 2022 12:48




Instrument :
MSVOA_Y
ClientSampleId :
TT-156-IDWSO-20220329-3


Tgt Ion:168 Resp: 130515
Ion Ratio Lower Upper
168 100
99 58.0 46.9 70.3

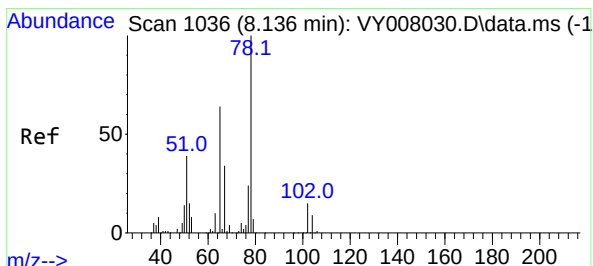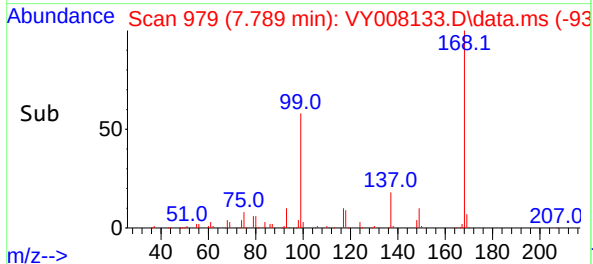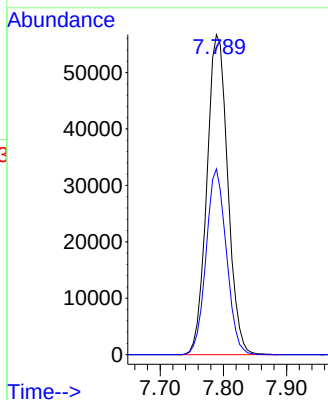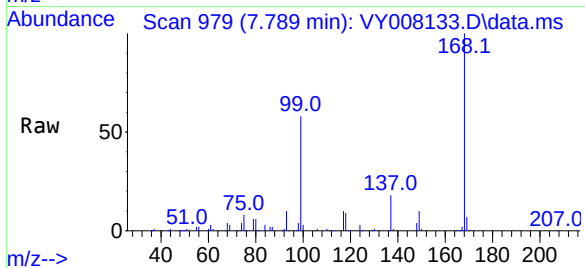

#33
1,2-Dichloroethane-d4
Concen: 56.460 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. 0.007 min
Lab File: VY008133.D
Acq: 31 Mar 2022 12:48

Tgt Ion: 65 Resp: 73932
Ion Ratio Lower Upper
65 100
67 53.2 0.0 99.4

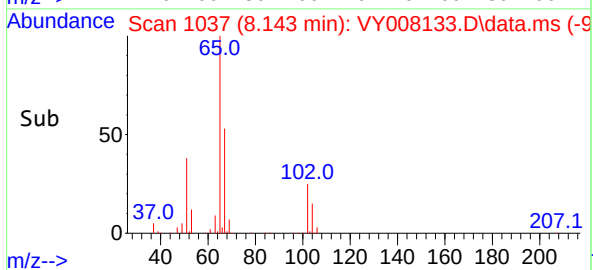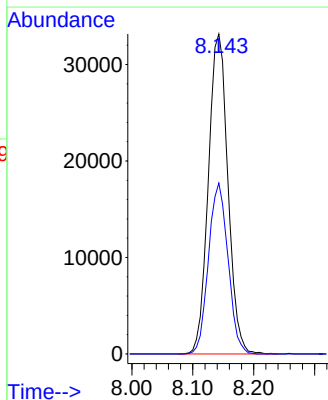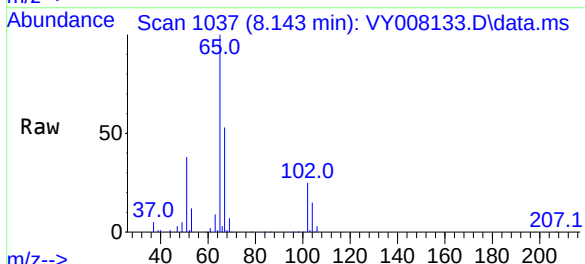

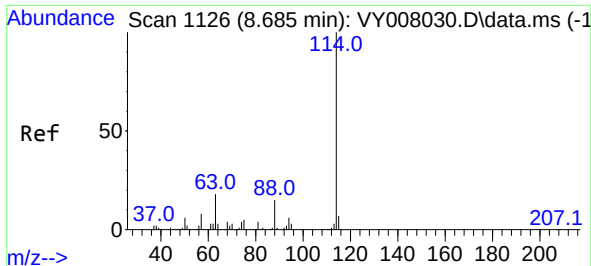

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1126

Delta R.T. 0.006 min

Lab File: VY008133.D

Acq: 31 Mar 2022 12:48

Instrument :

MSVOA_Y

ClientSampleId :

TT-156-IDWSO-20220329-3





Tgt Ion:114 Resp: 236554

Ion Ratio Lower Upper

114 100

63 17.3 0.0 43.2

88 14.8 0.0 31.8

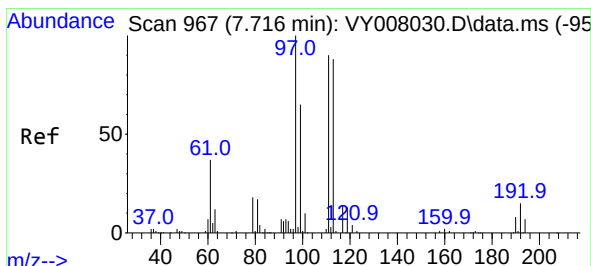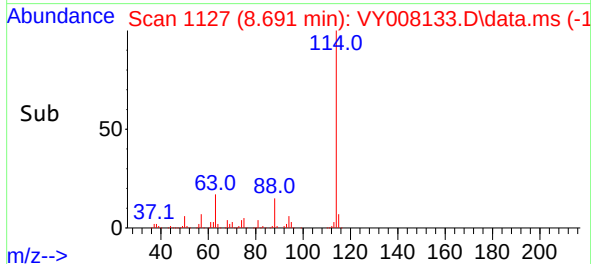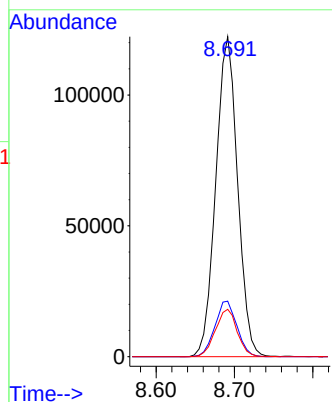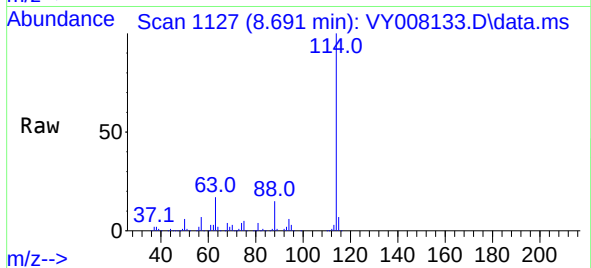

#35

Dibromofluoromethane

Concen: 50.500 ug/l

RT: 7.722 min Scan# 968

Delta R.T. 0.006 min

Lab File: VY008133.D

Acq: 31 Mar 2022 12:48




Tgt Ion:113 Resp: 74898


Ion Ratio Lower Upper

113 100

111 102.8 82.6 124.0

192 18.0 17.6 26.4


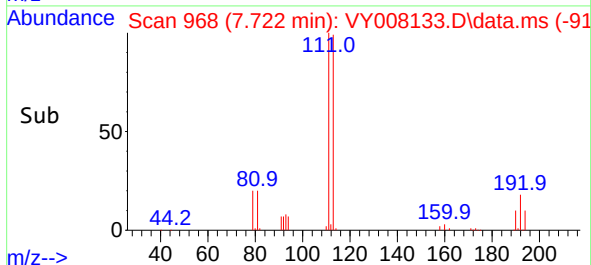
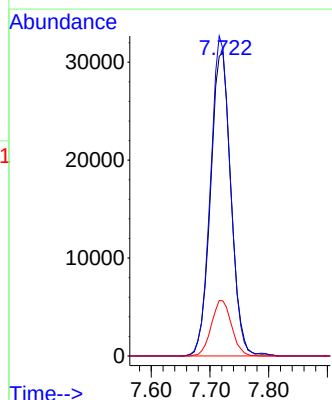
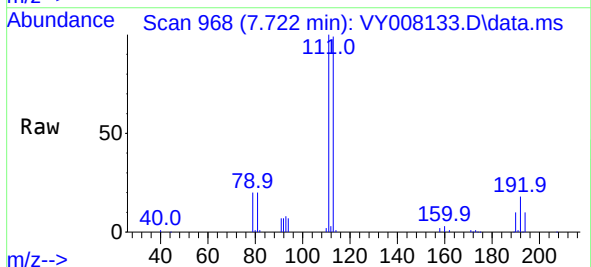


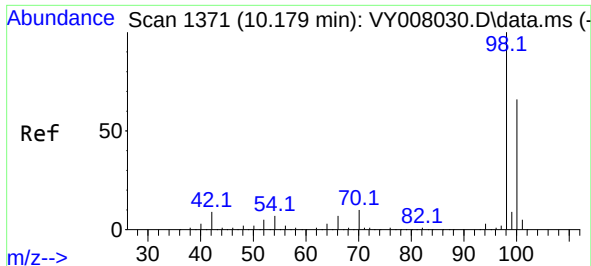

#50
Toluene-d8
Concen: 51.013 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY008133.D
Acq: 31 Mar 2022 12:48




Instrument :
MSVOA_Y
ClientSampleId :
TT-156-IDWSO-20220329-3


Tgt Ion: 98 Resp: 285046
Ion Ratio Lower Upper
98 100
100 65.3 50.2 75.2

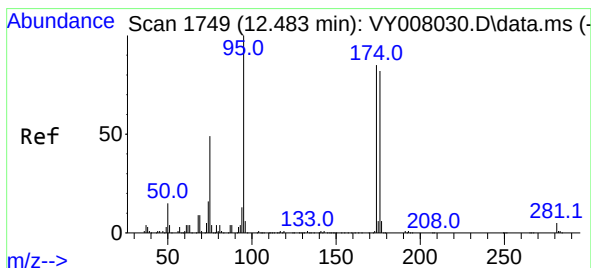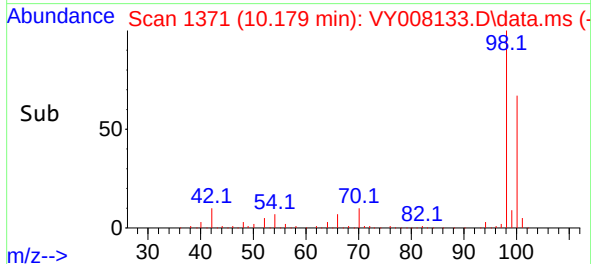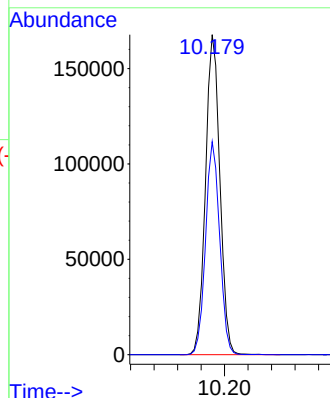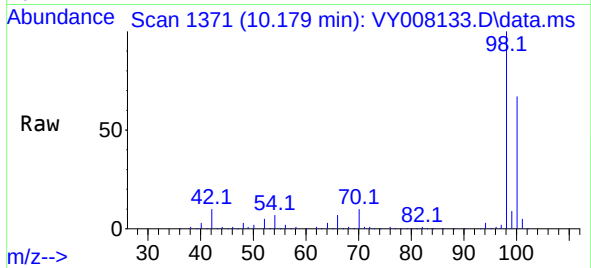

#62
4-Bromofluorobenzene
Concen: 47.322 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY008133.D
Acq: 31 Mar 2022 12:48

Tgt Ion: 95 Resp: 93288
Ion Ratio Lower Upper
95 100
174 80.2 0.0 177.0
176 77.5 0.0 175.8


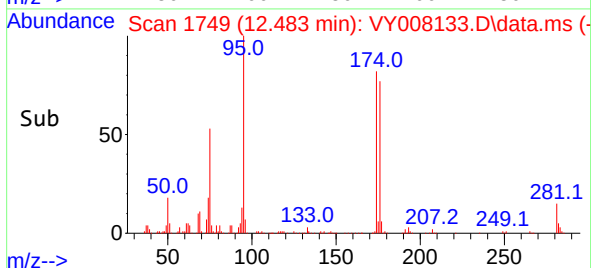
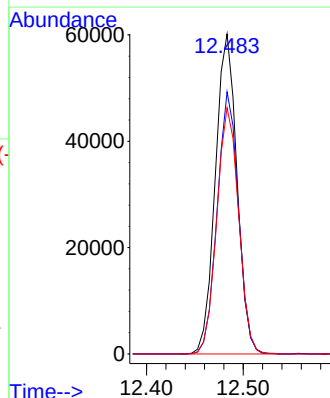
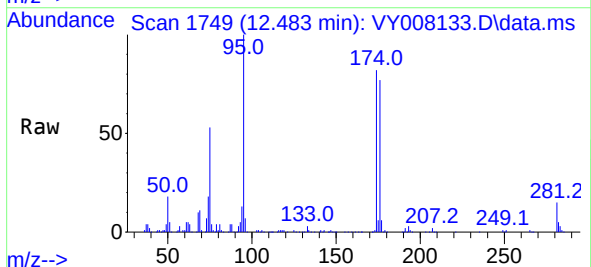


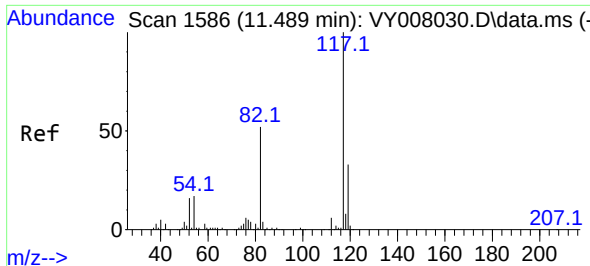

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 117
Delta R.T. 0.001 min
Lab File: VY008133.D
Acq: 31 Mar 2022 12:48

Instrument :
MSVOA_Y
ClientSampleId :
TT-156-IDWSO-20220329-3

Tgt Ion:117 Resp: 217734
Ion Ratio Lower Upper
117 100
82 53.6 43.0 64.4
119 32.1 25.4 38.0

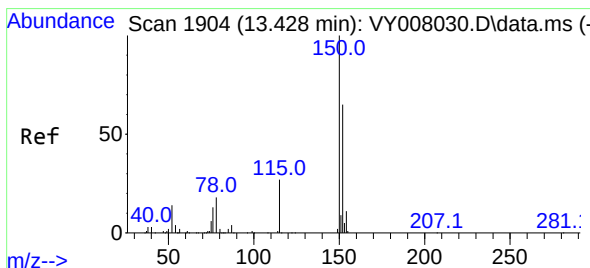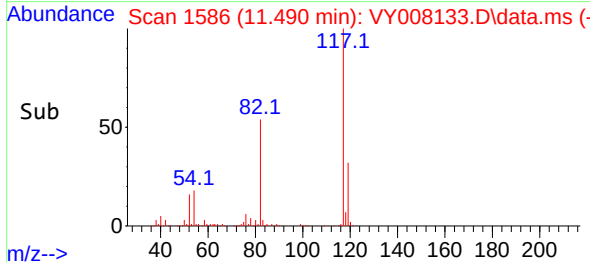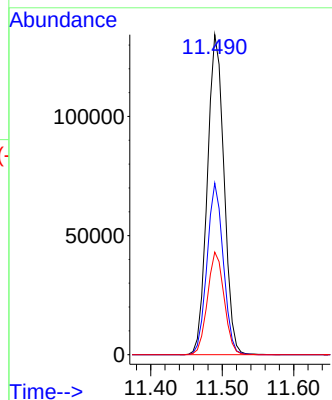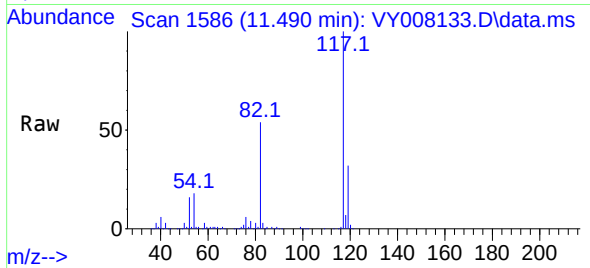

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY008133.D
Acq: 31 Mar 2022 12:48

Tgt Ion:152 Resp: 89491
Ion Ratio Lower Upper
152 100
115 59.5 28.2 84.7
150 158.5 0.0 347.6

