

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY033122\
 Data File : VY008144.D
 Acq On : 31 Mar 2022 17:29
 Operator : SY/MD
 Sample : N2195-01
 Misc : 5.02g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 TP-1-1-5FT

Quant Time: Apr 01 04:34:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032522S.M
 Quant Title : SW846 8260
 QLast Update : Sat Mar 26 03:24:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	164310	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	272666	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	261923	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	127996	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	77873	47.238	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	94.480%
35) Dibromofluoromethane	7.716	113	85410	49.961	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	99.920%
50) Toluene-d8	10.179	98	320836	49.814	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	99.620%
62) 4-Bromofluorobenzene	12.483	95	117304	51.623	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	103.240%
Target Compounds						
16) Acetone	3.948	43	22253	59.057	ug/l	Qvalue # 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY033122\
Data File : VY008144.D
Acq On : 31 Mar 2022 17:29
Operator : SY/MD
Sample : N2195-01
Misc : 5.02g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
TP-1-1-5FT

Quant Time: Apr 01 04:34:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032522S.M
Quant Title : SW846 8260
QLast Update : Sat Mar 26 03:24:51 2022
Response via : Initial Calibration




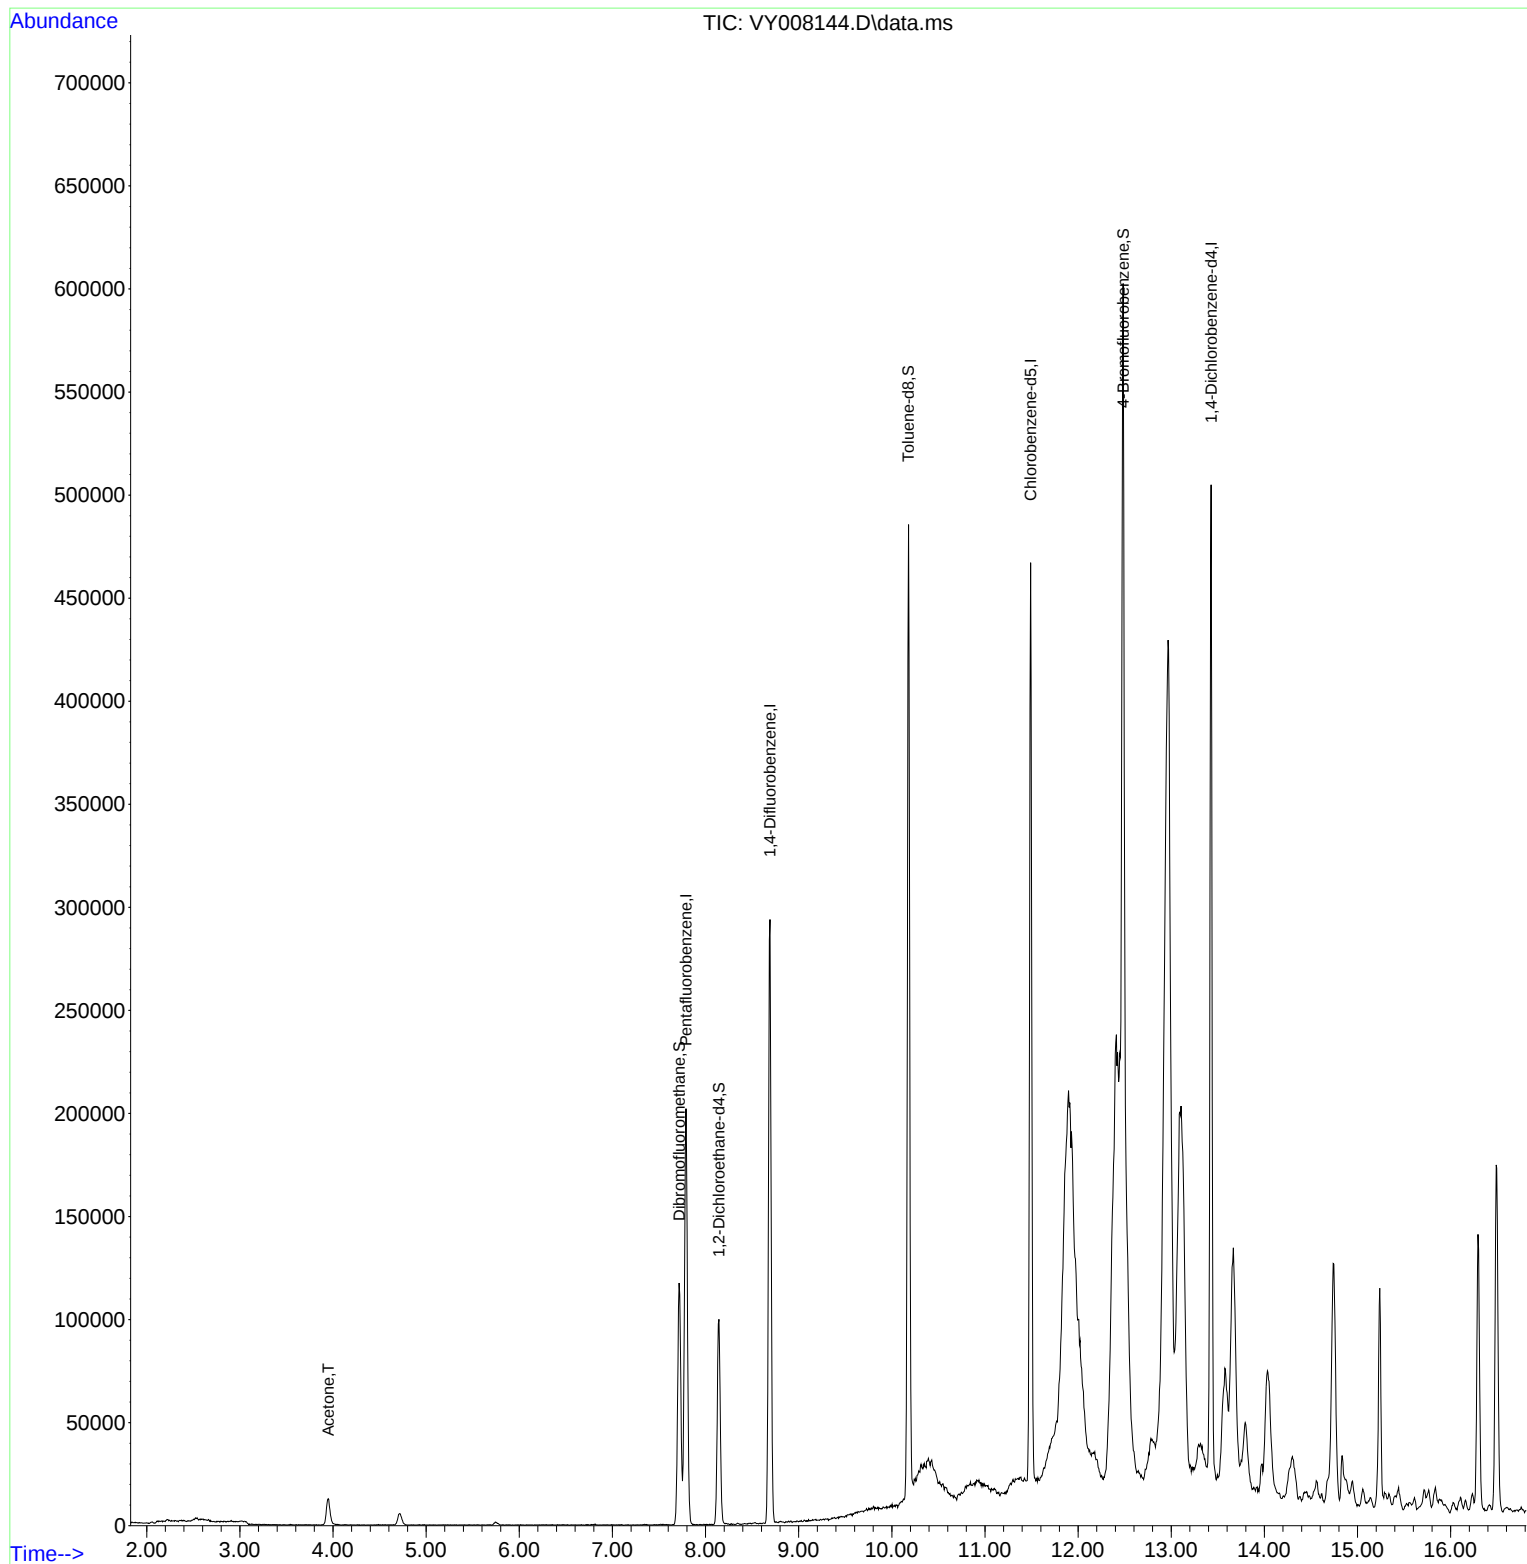


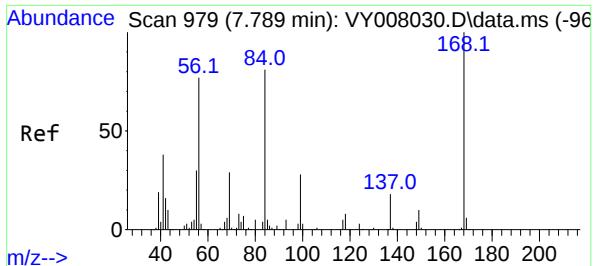

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY008144.D
Acq: 31 Mar 2022 17:29




Instrument :
MSVOA_Y
ClientSampleId :
TP-1-1-5FT


Tgt Ion:168 Resp: 164310
Ion Ratio Lower Upper
168 100
99 53.0 46.9 70.3

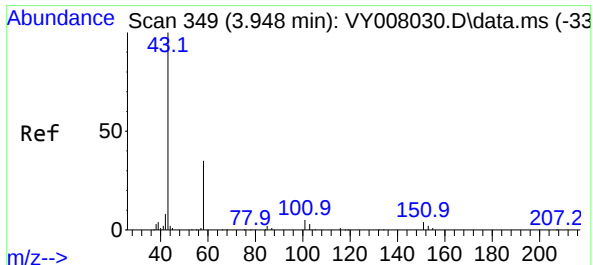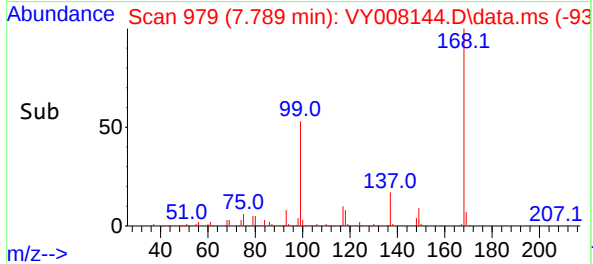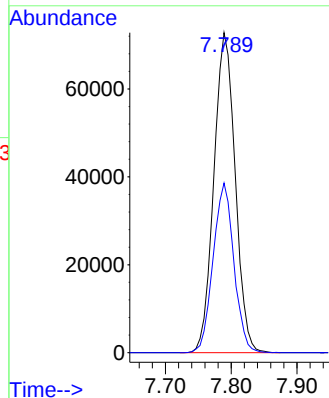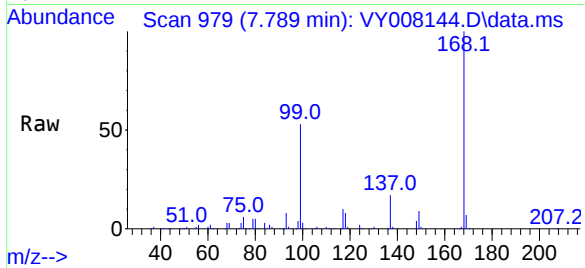

#16
Acetone
Concen: 59.057 ug/l
RT: 3.948 min Scan# 349
Delta R.T. 0.000 min
Lab File: VY008144.D
Acq: 31 Mar 2022 17:29

Tgt Ion: 43 Resp: 22253
Ion Ratio Lower Upper
43 100
58 36.4 22.0 33.0#

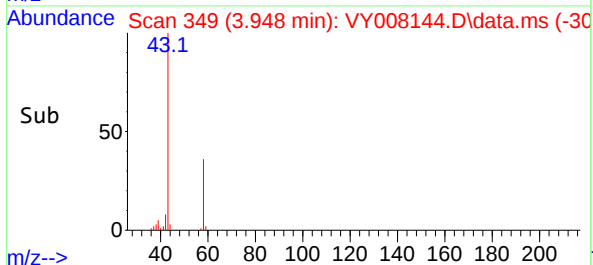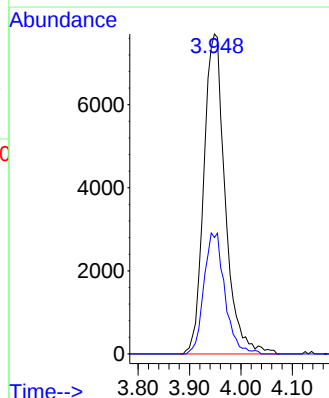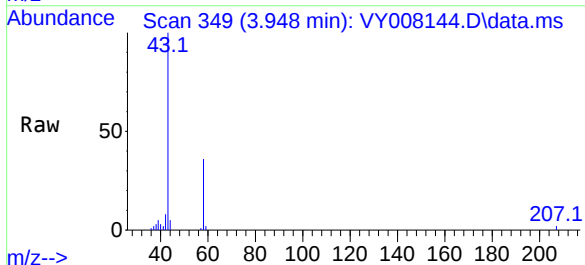

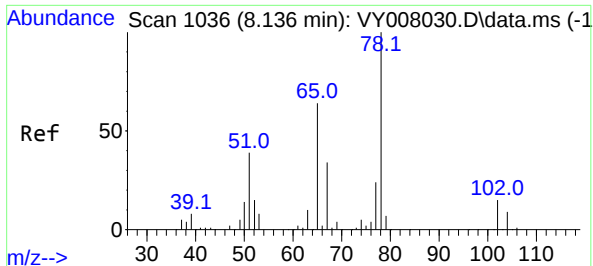

#33

1,2-Dichloroethane-d4

Concen: 47.238 ug/l

RT: 8.143 min Scan# 1037

Delta R.T. 0.007 min

Lab File: VY008144.D

Acq: 31 Mar 2022 17:29

Instrument :

MSVOA_Y

ClientSampleId :





TP-1-1-5FT

Tgt Ion: 65 Resp: 77873

Ion Ratio Lower Upper

65 100

67 53.3 0.0 99.4

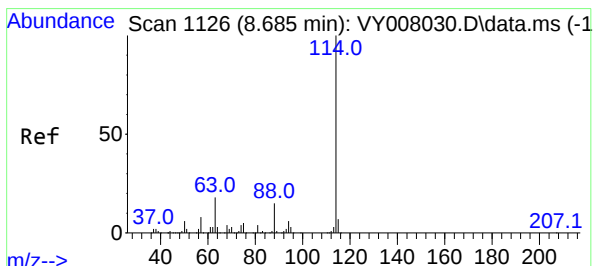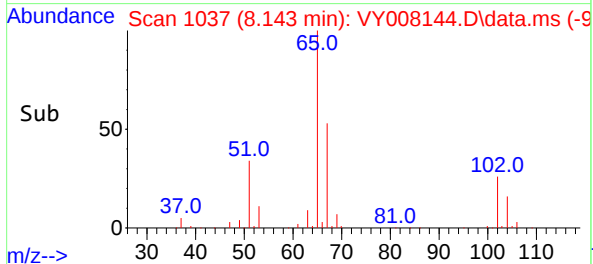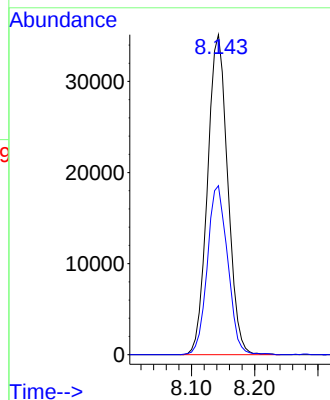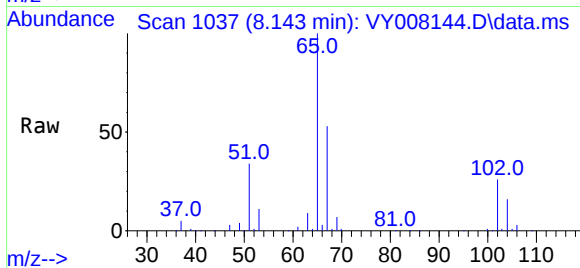

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.006 min

Lab File: VY008144.D

Acq: 31 Mar 2022 17:29




Tgt Ion:114 Resp: 272666


Ion Ratio Lower Upper

114 100

63 16.0 0.0 43.2

88 14.0 0.0 31.8


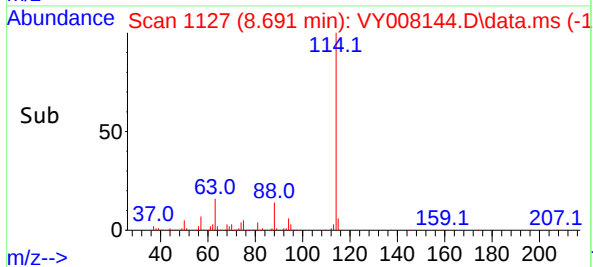
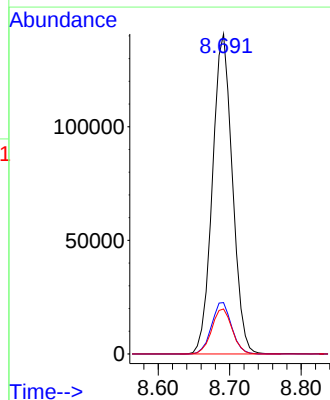
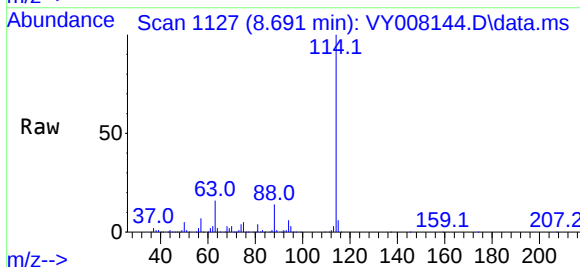


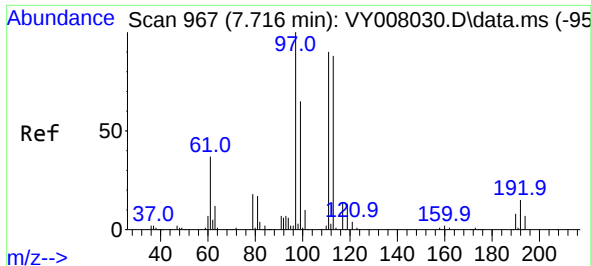

#35
Dibromofluoromethane
Concen: 49.961 ug/l
RT: 7.716 min Scan# 90
Delta R.T. -0.000 min
Lab File: VY008144.D
Acq: 31 Mar 2022 17:29




Instrument :
MSVOA_Y
ClientSampleId :
TP-1-1-5FT


Tgt Ion:113 Resp: 85410
Ion Ratio Lower Upper
113 100
111 101.6 82.6 124.0
192 20.5 17.6 26.4

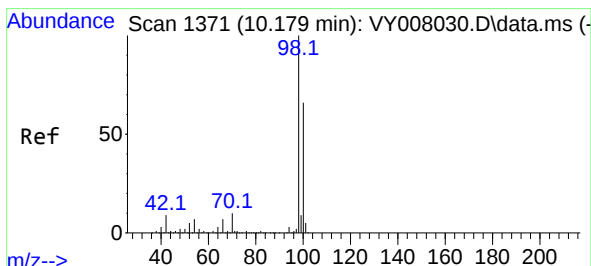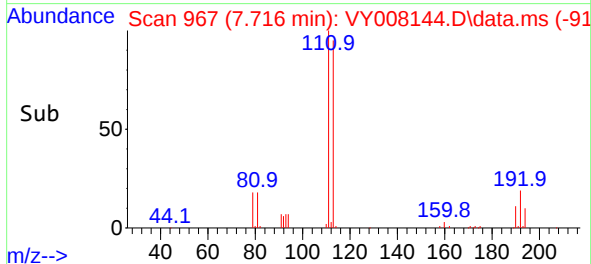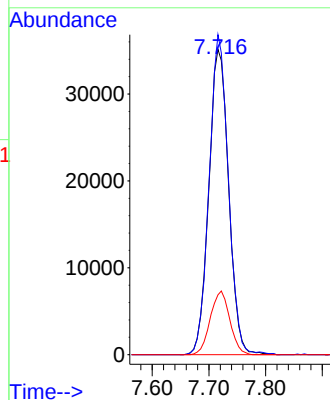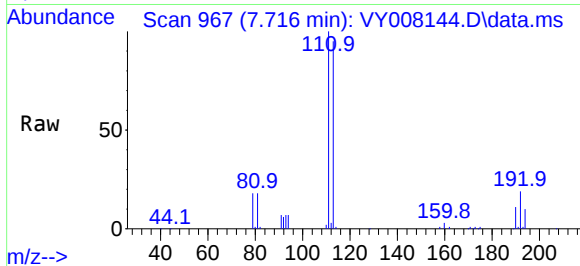

#50
Toluene-d8
Concen: 49.814 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY008144.D
Acq: 31 Mar 2022 17:29

Tgt Ion: 98 Resp: 320836
Ion Ratio Lower Upper
98 100
100 65.8 50.2 75.2


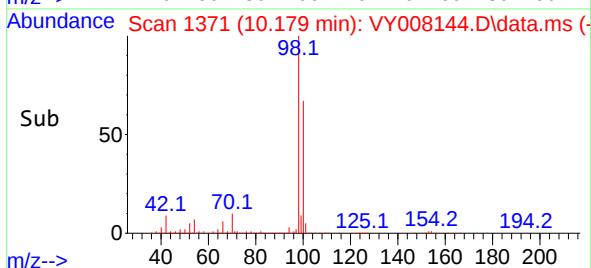
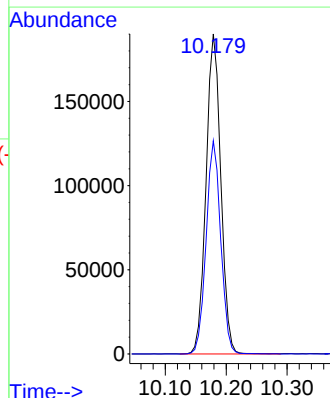
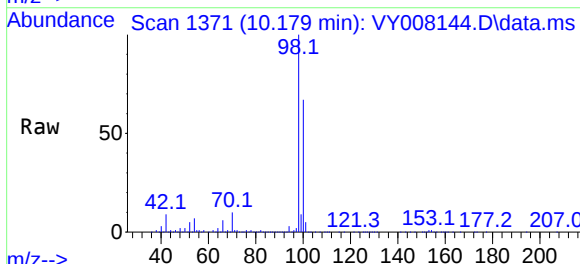


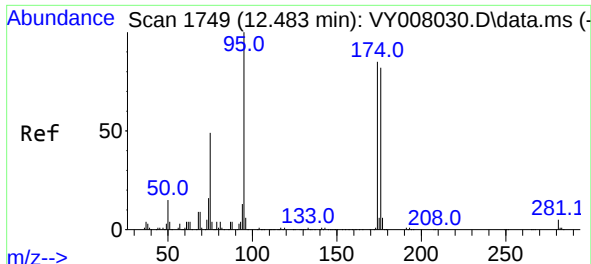

#62
4-Bromofluorobenzene
Concen: 51.623 ug/l
RT: 12.483 min Scan# 117304
Delta R.T. 0.000 min
Lab File: VY008144.D
Acq: 31 Mar 2022 17:29




Instrument :
MSVOA_Y
ClientSampleId :
TP-1-1-5FT


Tgt Ion: 95 Resp: 117304
Ion Ratio Lower Upper
95 100
174 88.2 0.0 177.0
176 86.2 0.0 175.8

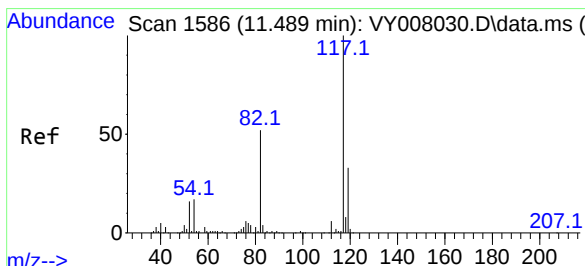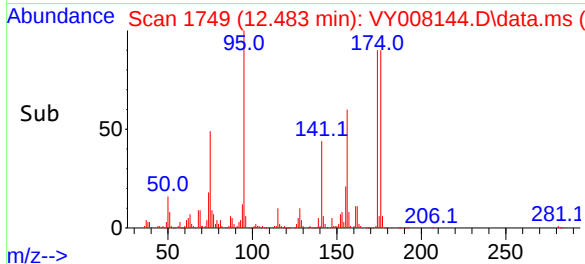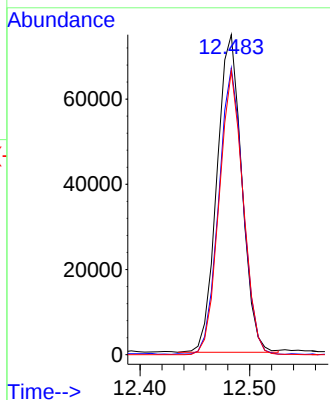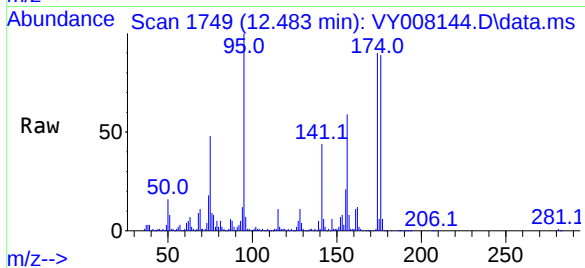

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 1586
Delta R.T. 0.001 min
Lab File: VY008144.D
Acq: 31 Mar 2022 17:29


Tgt Ion: 117 Resp: 261923
Ion Ratio Lower Upper
117 100
82 49.8 43.0 64.4
119 32.7 25.4 38.0

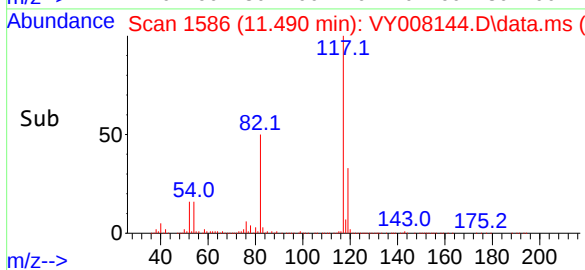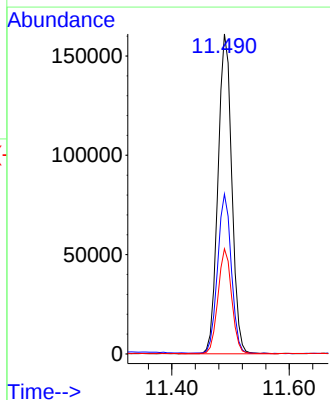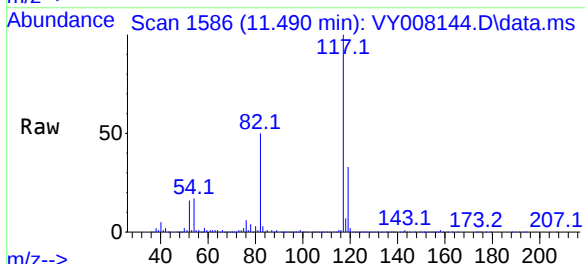

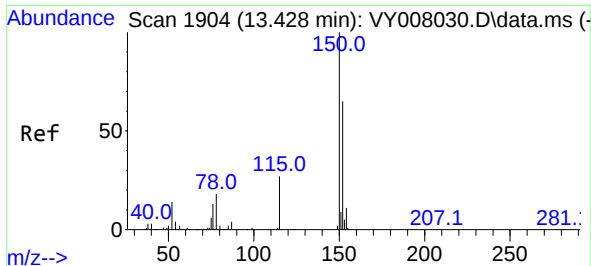

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.428 min Scan# 1904
 Delta R.T. 0.000 min
 Lab File: VY008144.D
 Acq: 31 Mar 2022 17:29

Instrument :
 MSVOA_Y
 ClientSampleId :
 TP-1-1-5FT

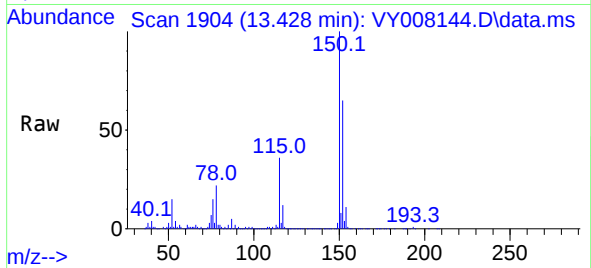

Tgt Ion:152 Resp: 127996

Ion	Ratio	Lower	Upper
152	100		
115	56.1	28.2	84.7
150	156.1	0.0	347.6

