

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY033122\  
 Data File : VY008145.D  
 Acq On : 31 Mar 2022 17:52  
 Operator : SY/MD  
 Sample : N2195-03  
 Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
 ALS Vial : 21 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 TP-2-1-5FT

Quant Time: Apr 01 04:35:08 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y032522S.M  
 Quant Title : SW846 8260  
 QLast Update : Sat Mar 26 03:24:51 2022  
 Response via : Initial Calibration

| Compound                   | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|----------------------------|--------|------|----------|--------|-------|----------|
| -----                      |        |      |          |        |       |          |
| Internal Standards         |        |      |          |        |       |          |
| 1) Pentafluorobenzene      | 7.789  | 168  | 155684   | 50.000 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 8.691  | 114  | 270246   | 50.000 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 11.490 | 117  | 253787   | 50.000 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 13.428 | 152  | 116158   | 50.000 | ug/l  | 0.00     |

|                             |        |       |          |          |      |          |
|-----------------------------|--------|-------|----------|----------|------|----------|
| System Monitoring Compounds |        |       |          |          |      |          |
| 33) 1,2-Dichloroethane-d4   | 8.143  | 65    | 78403    | 50.195   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 50 - 163 | Recovery | =    | 100.380% |
| 35) Dibromofluoromethane    | 7.722  | 113   | 84161    | 49.671   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 54 - 147 | Recovery | =    | 99.340%  |
| 50) Toluene-d8              | 10.179 | 98    | 320730   | 50.243   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 49 - 140 | Recovery | =    | 100.480% |
| 62) 4-Bromofluorobenzene    | 12.483 | 95    | 113206   | 50.266   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 25 - 144 | Recovery | =    | 100.540% |


| Target Compounds | Qvalue |
|------------------|--------|
| -----            |        |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY033122\  
Data File : VY008145.D  
Acq On : 31 Mar 2022 17:52  
Operator : SY/MD  
Sample : N2195-03  
Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
TP-2-1-5FT

Quant Time: Apr 01 04:35:08 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y032522S.M  
Quant Title : SW846 8260  
QLast Update : Sat Mar 26 03:24:51 2022  
Response via : Initial Calibration




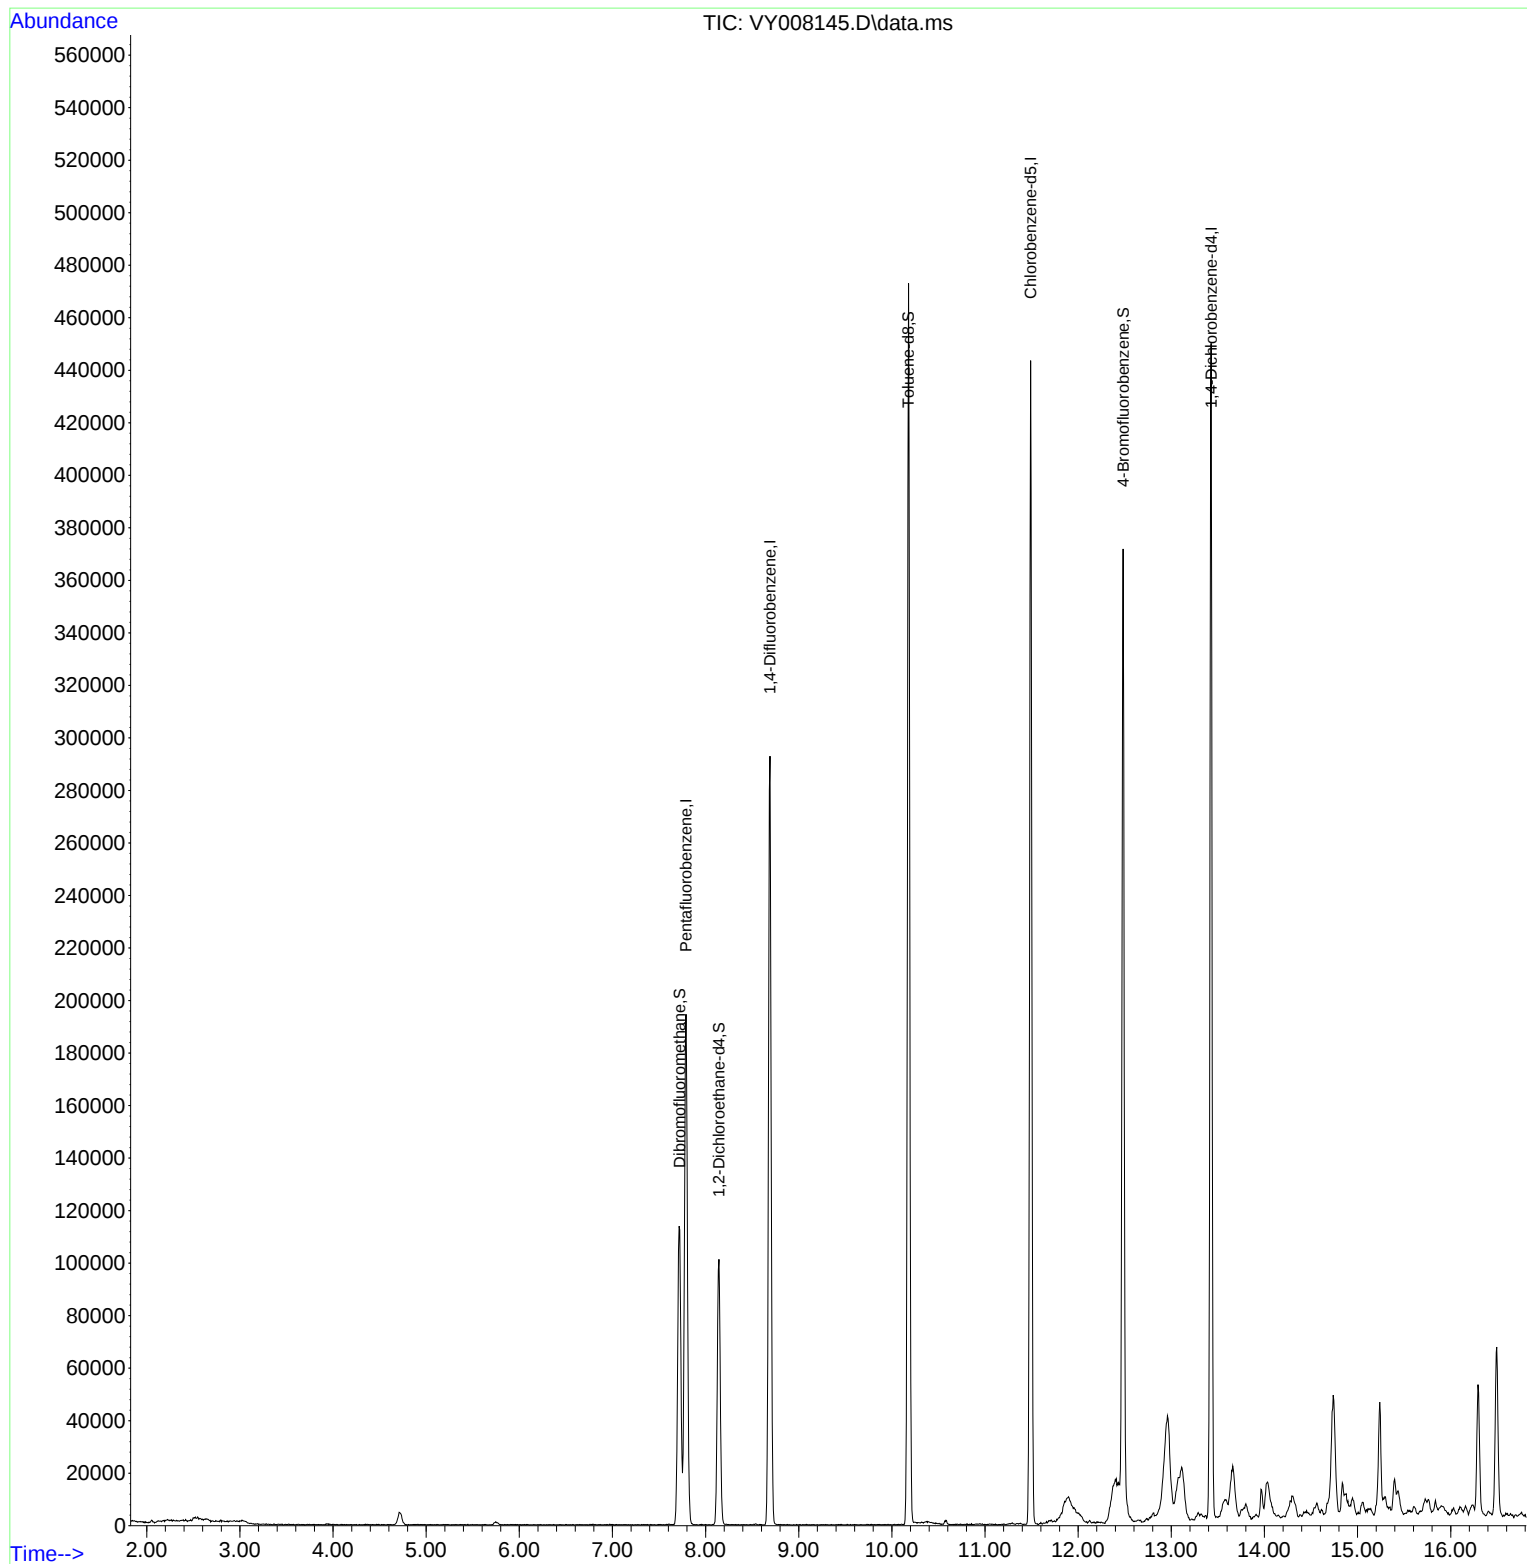


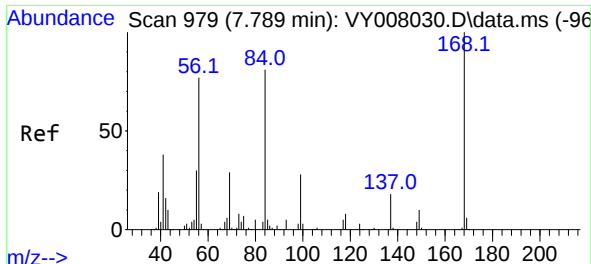

#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 7.789 min Scan# 91  
Delta R.T. -0.000 min  
Lab File: VY008145.D  
Acq: 31 Mar 2022 17:52




Instrument :  
MSVOA\_Y  
ClientSampleId :  
TP-2-1-5FT


Tgt Ion:168 Resp: 155684  
Ion Ratio Lower Upper  
168 100  
99 53.4 46.9 70.3

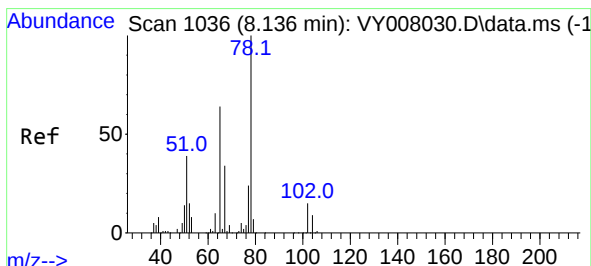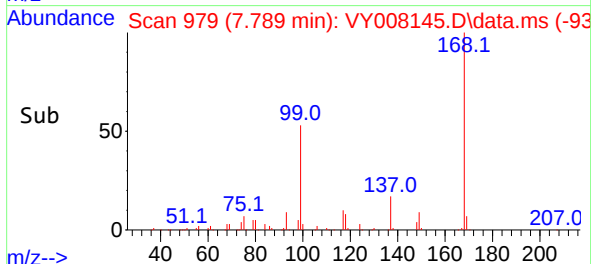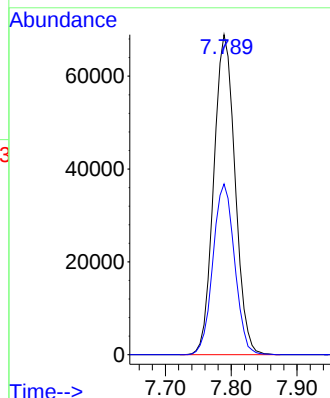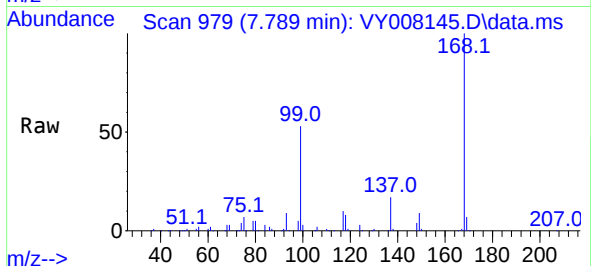

#33  
1,2-Dichloroethane-d4  
Concen: 50.195 ug/l  
RT: 8.143 min Scan# 1037  
Delta R.T. 0.007 min  
Lab File: VY008145.D  
Acq: 31 Mar 2022 17:52

Tgt Ion: 65 Resp: 78403  
Ion Ratio Lower Upper  
65 100  
67 54.0 0.0 99.4

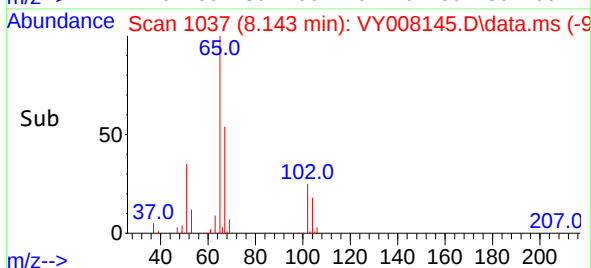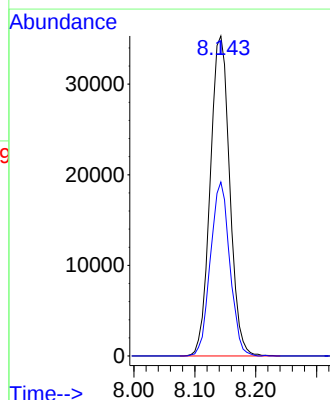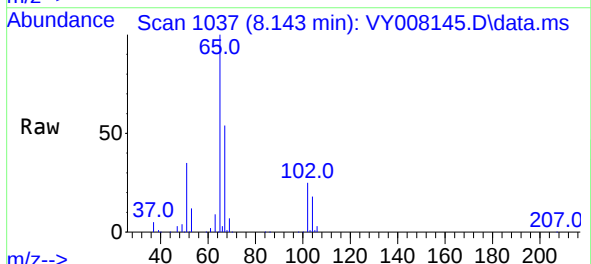

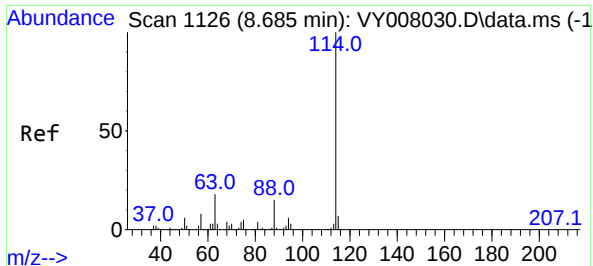

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1126

Delta R.T. 0.006 min

Lab File: VY008145.D

Acq: 31 Mar 2022 17:52

Instrument :

MSVOA\_Y

ClientSampleId :

TP-2-1-5FT





Tgt Ion:114 Resp: 270246

Ion Ratio Lower Upper

114 100

63 16.8 0.0 43.2

88 14.6 0.0 31.8

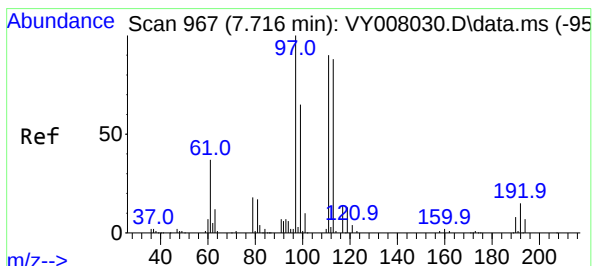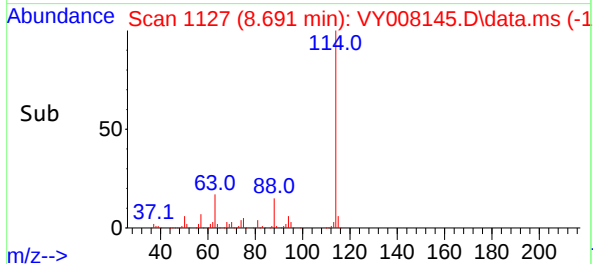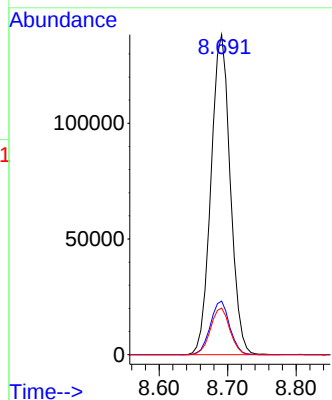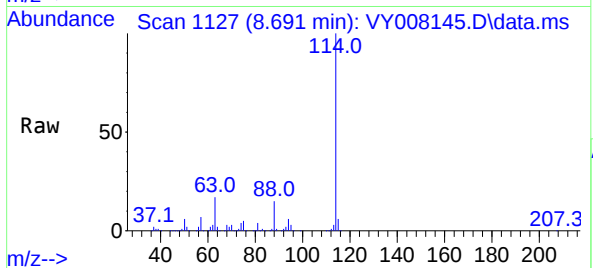

#35

Dibromofluoromethane

Concen: 49.671 ug/l

RT: 7.722 min Scan# 968

Delta R.T. 0.006 min

Lab File: VY008145.D

Acq: 31 Mar 2022 17:52




Tgt Ion:113 Resp: 84161


Ion Ratio Lower Upper

113 100

111 102.6 82.6 124.0

192 18.9 17.6 26.4

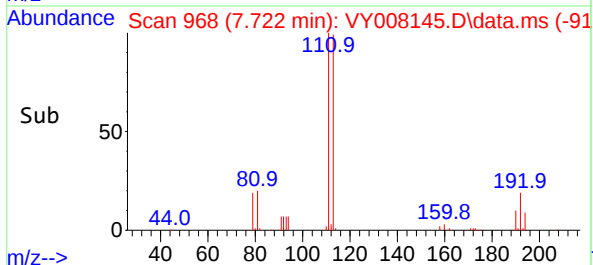
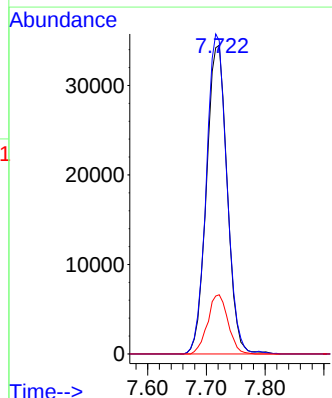
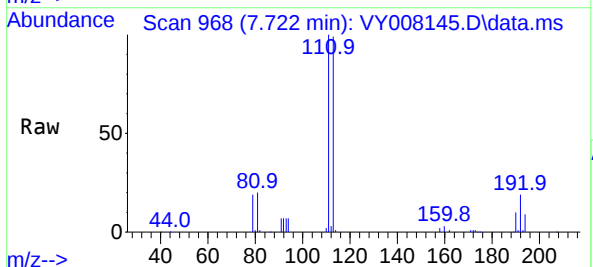


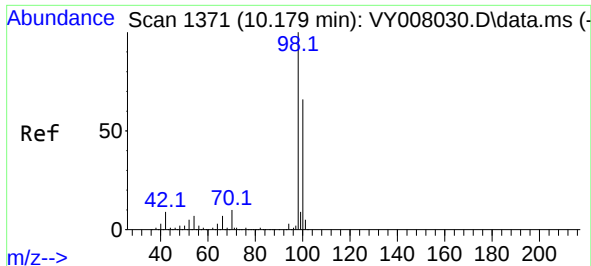

#50  
Toluene-d8  
Concen: 50.243 ug/l  
RT: 10.179 min Scan# 1371  
Delta R.T. -0.000 min  
Lab File: VY008145.D  
Acq: 31 Mar 2022 17:52




Instrument :  
MSVOA\_Y  
ClientSampleId :  
TP-2-1-5FT

Tgt Ion: 98 Resp: 320730  
Ion Ratio Lower Upper  
98 100  
100 65.5 50.2 75.2

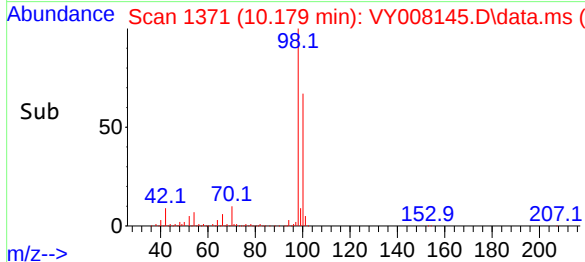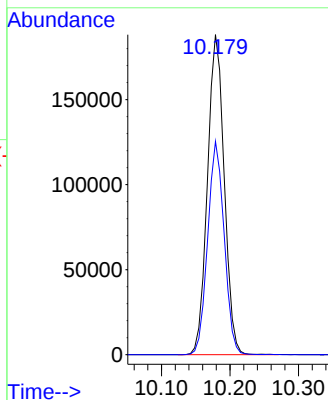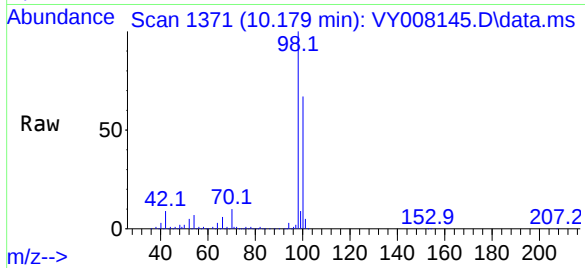

#62  
4-Bromofluorobenzene  
Concen: 50.266 ug/l  
RT: 12.483 min Scan# 1749  
Delta R.T. 0.000 min  
Lab File: VY008145.D  
Acq: 31 Mar 2022 17:52

Tgt Ion: 95 Resp: 113206  
Ion Ratio Lower Upper  
95 100  
174 83.3 0.0 177.0  
176 80.5 0.0 175.8


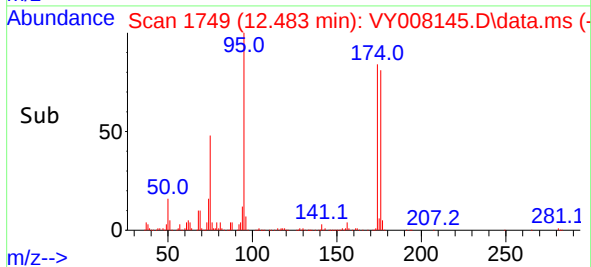
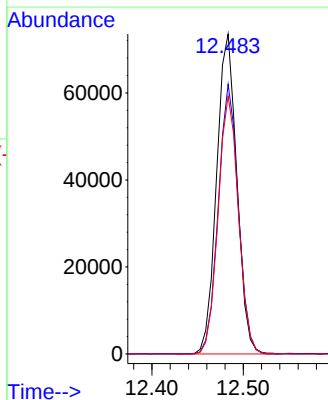
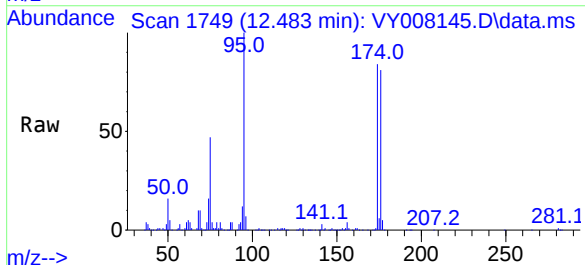




#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.490 min Scan# 117  
Delta R.T. 0.001 min  
Lab File: VY008145.D  
Acq: 31 Mar 2022 17:52

Instrument :  
MSVOA\_Y  
ClientSampleId :  
TP-2-1-5FT

Tgt Ion:117 Resp: 253787  
Ion Ratio Lower Upper  
117 100  
82 51.4 43.0 64.4  
119 31.2 25.4 38.0

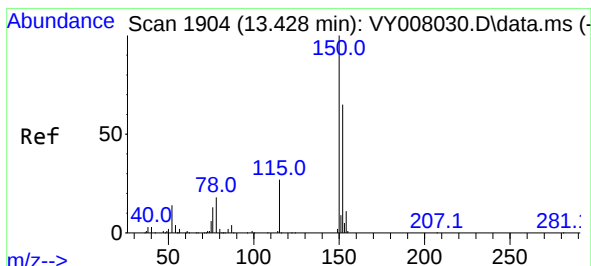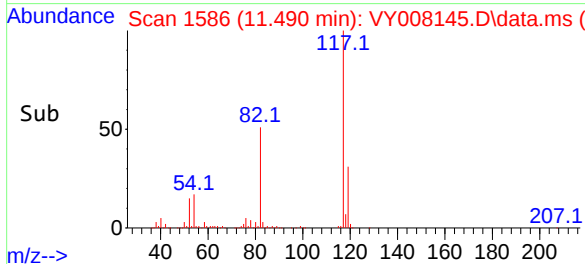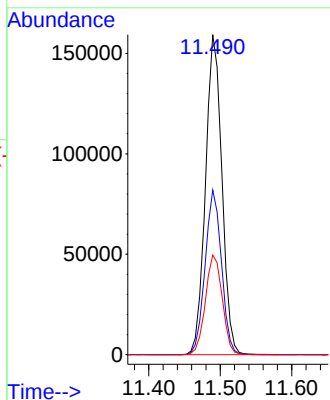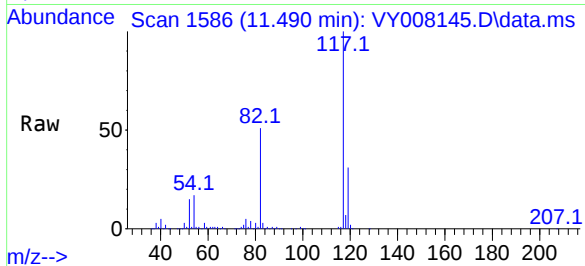

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 13.428 min Scan# 1904  
Delta R.T. 0.000 min  
Lab File: VY008145.D  
Acq: 31 Mar 2022 17:52

Tgt Ion:152 Resp: 116158  
Ion Ratio Lower Upper  
152 100  
115 59.8 28.2 84.7  
150 158.9 0.0 347.6

