
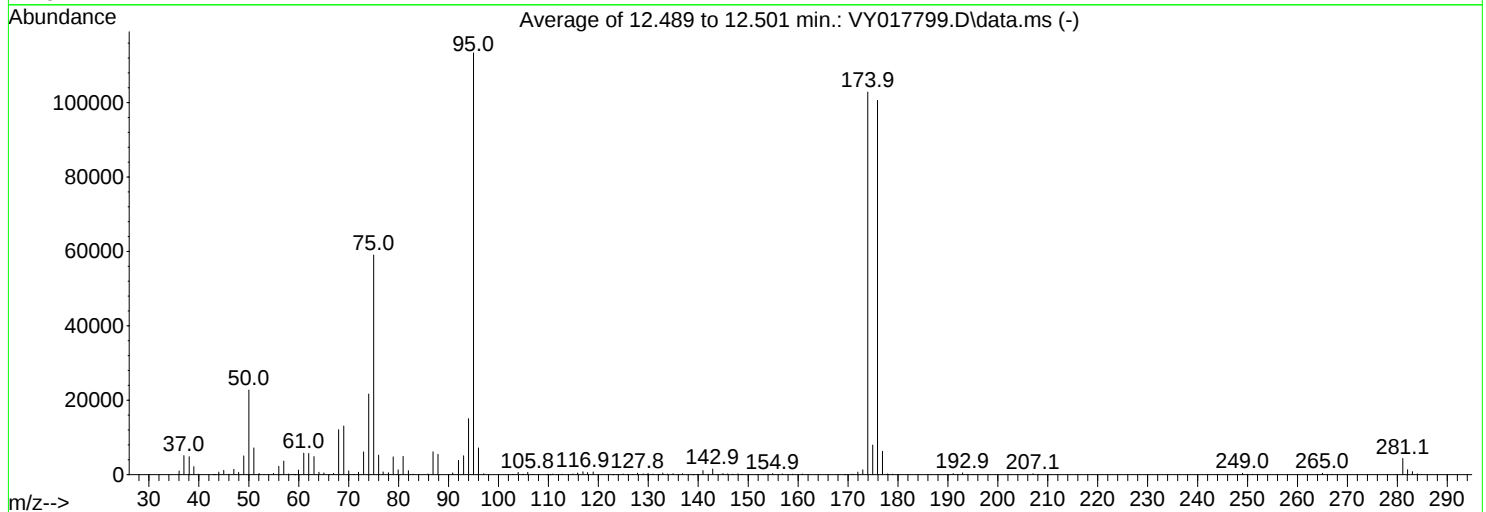


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY040124\  
Data File : VY017799.D  
Acq On : 01 Apr 2024 08:33  
Operator : SY/MD  
Sample : BFB  
Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y032924S.M  
Title : SW846 8260  
Last Update : Sat Mar 30 05:58:13 2024

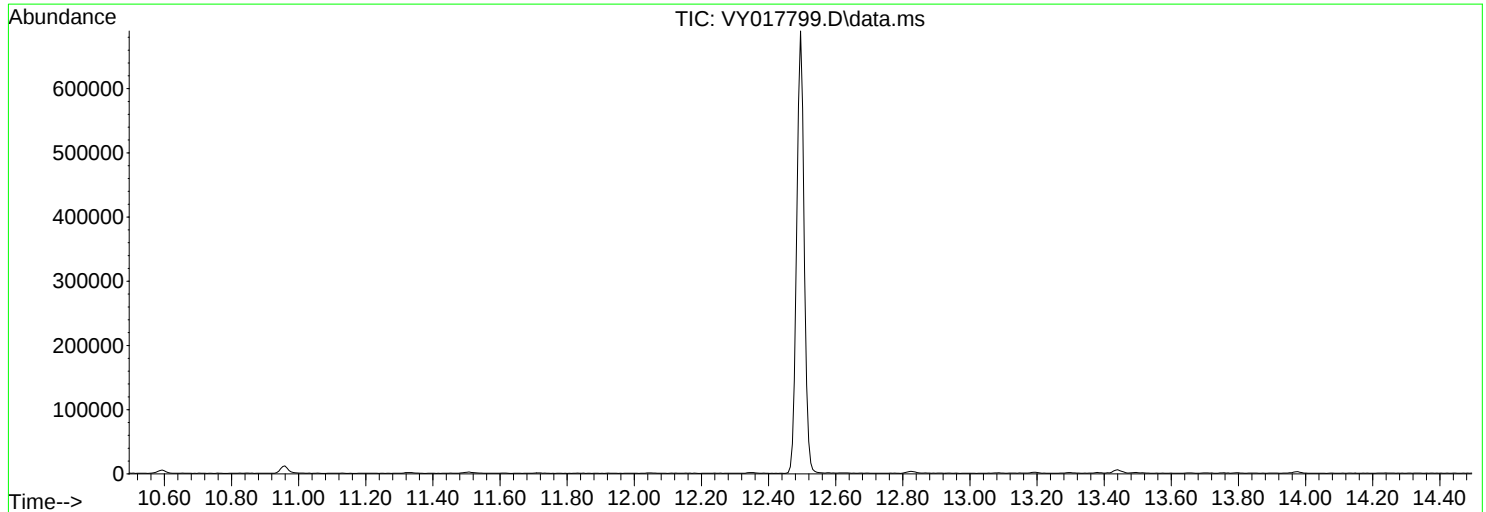

AutoFind: Scans 1750, 1751, 1752; Background Corrected with Scan 1742

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 20.1         | 22768      | PASS                |
| 75             | 95              | 30              | 60              | 52.1         | 59032      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 113381     | PASS                |
| 96             | 95              | 5               | 9               | 6.3          | 7190       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.3          | 1312       | PASS                |
| 174            | 95              | 50              | 100             | 90.7         | 102816     | PASS                |
| 175            | 174             | 5               | 9               | 7.7          | 7956       | PASS                |
| 176            | 174             | 95              | 101             | 97.8         | 100605     | PASS                |
| 177            | 176             | 5               | 9               | 6.2          | 6268       | PASS                |