

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY040220\
 Data File : VY002191.D
 Acq On : 02 Apr 2020 14:54
 Operator : SY/MD
 Sample : L2135-04
 Misc : 7.11G/5ML/MSVOA Y/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-2E-(7-9)

Quant Time: Apr 03 03:14:55 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y032620S.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 27 07:11:05 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-7.81
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-8.71
63) Chlorobenzene-d5	0.00	117	0	0.00	ug/l	-11.50
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-13.43
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	0.00	65	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
35) Dibromofluoromethane	0.00	113	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
62) 4-Bromofluorobenzene	0.00	95	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY040220\
Data File : VY002191.D
Acq On : 02 Apr 2020 14:54
Operator : SY/MD
Sample : L2135-04
Misc : 7.11G/5ML/MSVOA Y/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SB-2E-(7-9)

Quant Time: Apr 03 03:14:55 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y032620S.M
Quant Title : SW846 8260
QLast Update : Fri Mar 27 07:11:05 2020
Response via : Initial Calibration

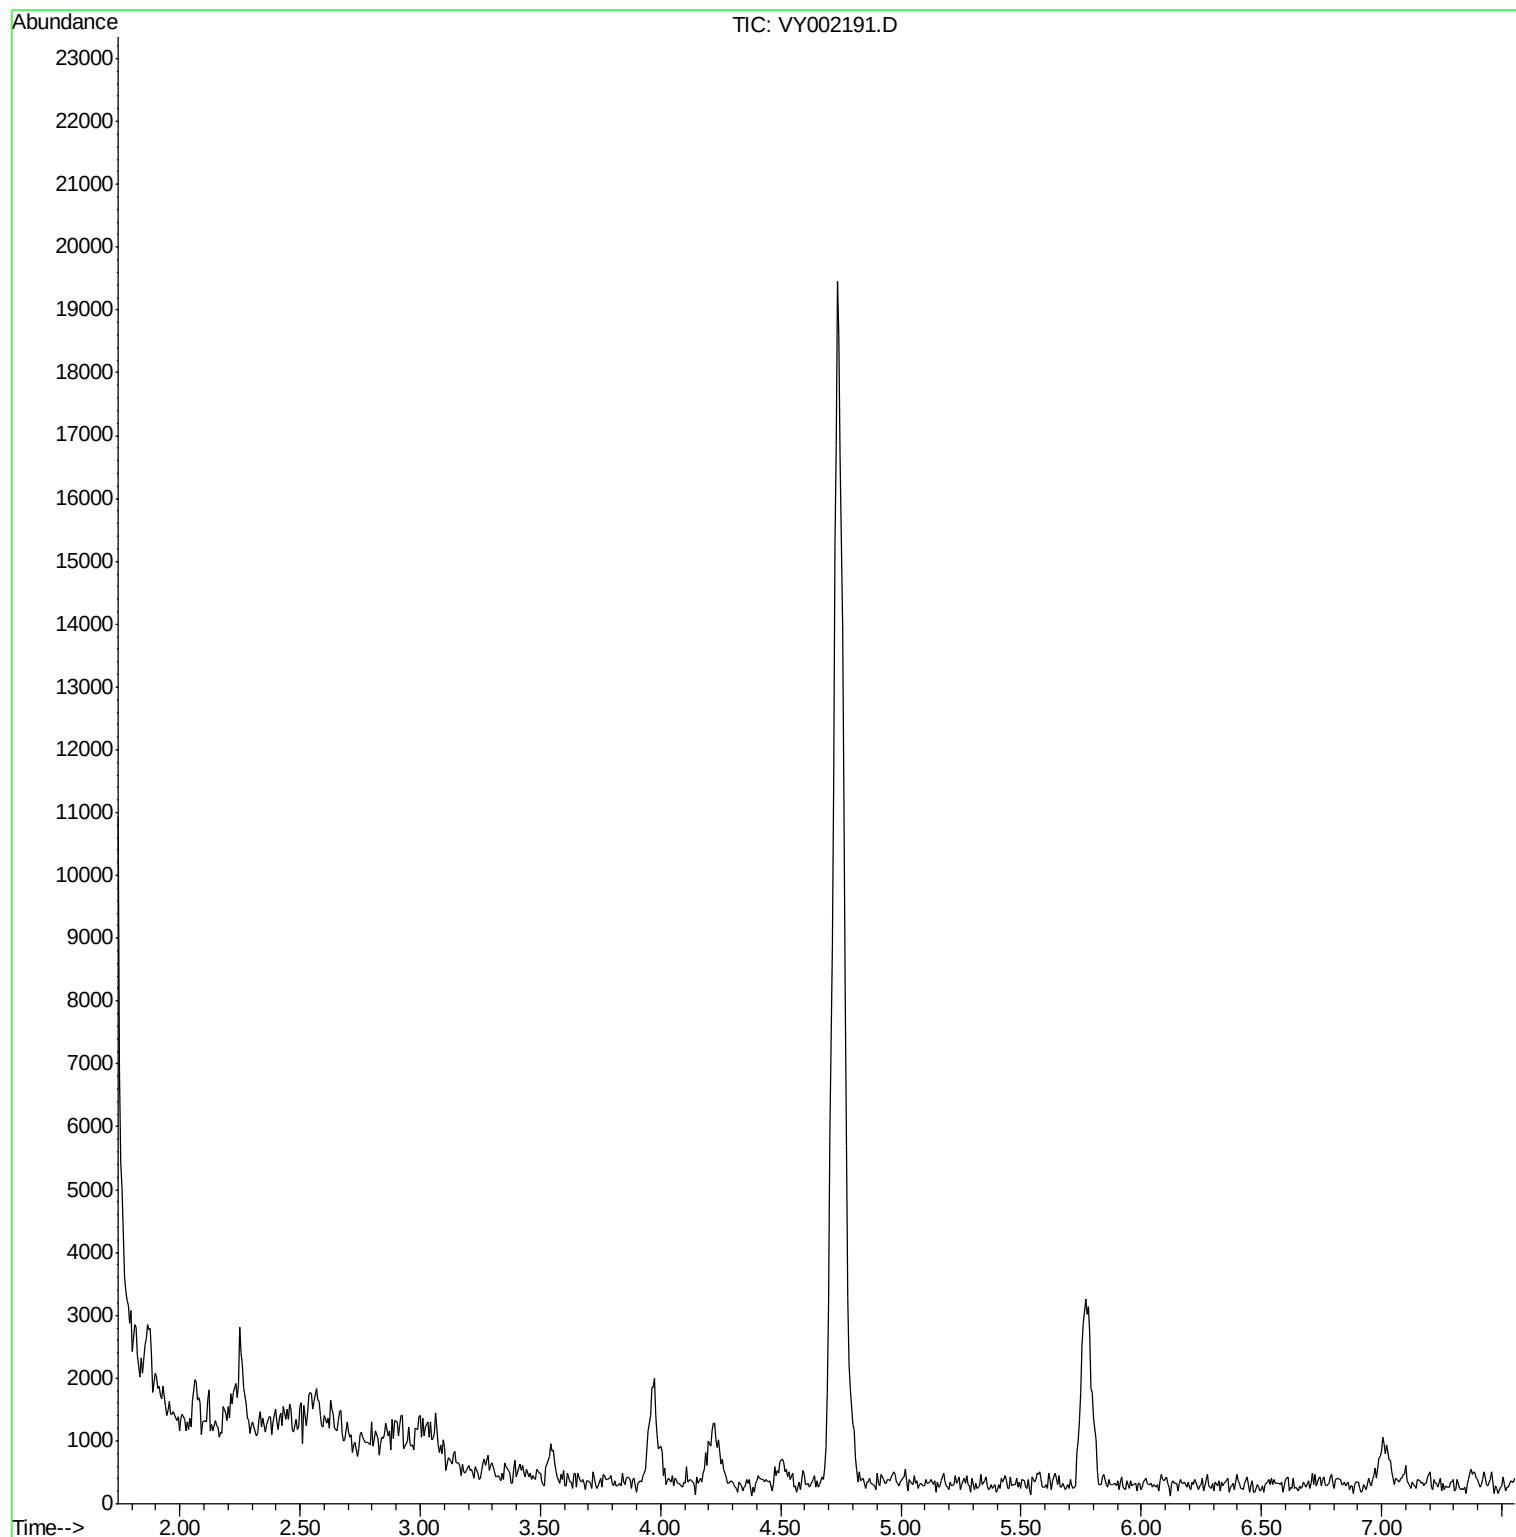

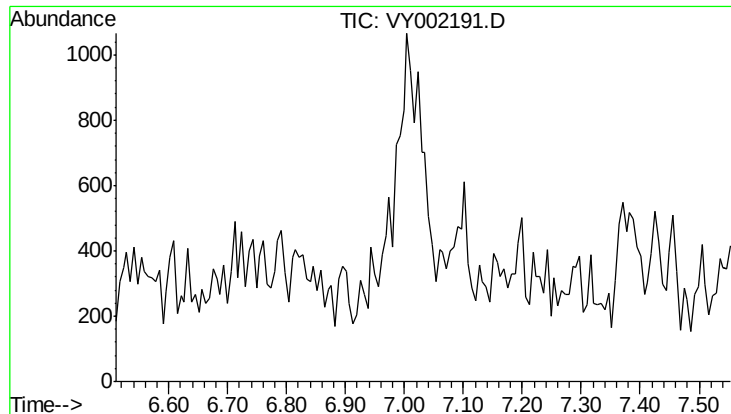

#1

Pentafluorobenzene

Concen: 0.000 ug/l

Expected RT: 7.81 min

Lab File: VY002191.D

Acq: 02 Apr 2020 14:54

Tot Ion: 168

Sig Exp Ratio

168 100



99 59.5

Instrument :

MSVOA_Y

ClientSampleId :

SB-2E-(7-9)

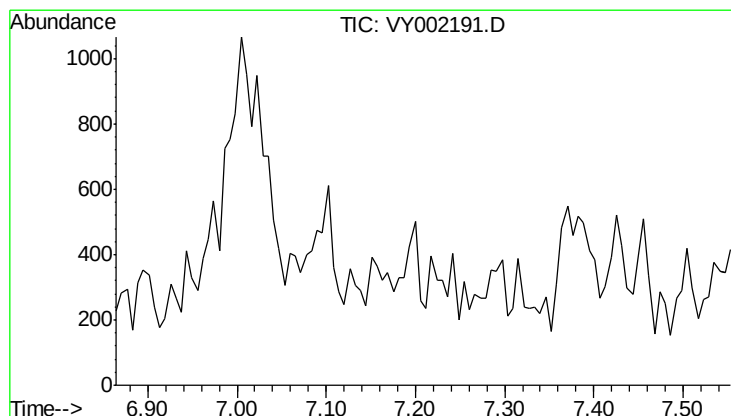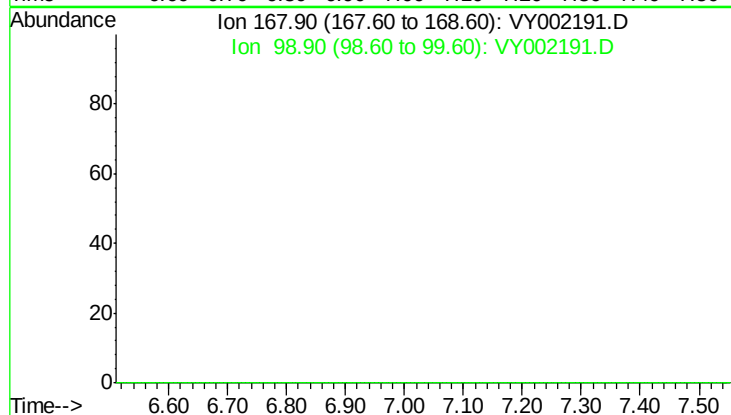

#33

1,2-Dichloroethane-d4

Concen: 0.000 ug/l

Expected RT: 8.16 min

Lab File: VY002191.D


Acq: 02 Apr 2020 14:54


Tgt Ion: 65

Sig Exp Ratio

65 100

67 56.4


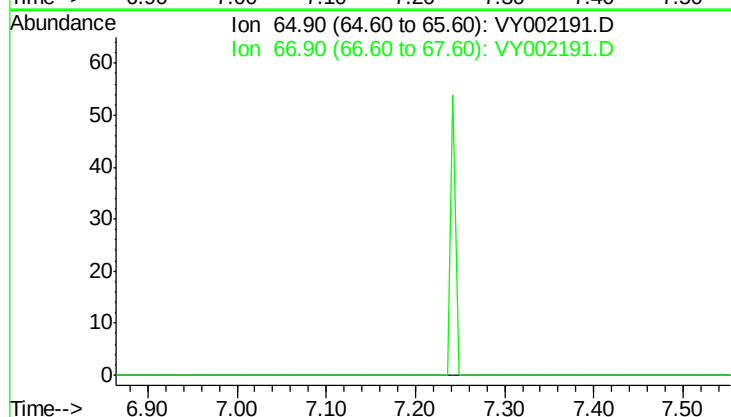


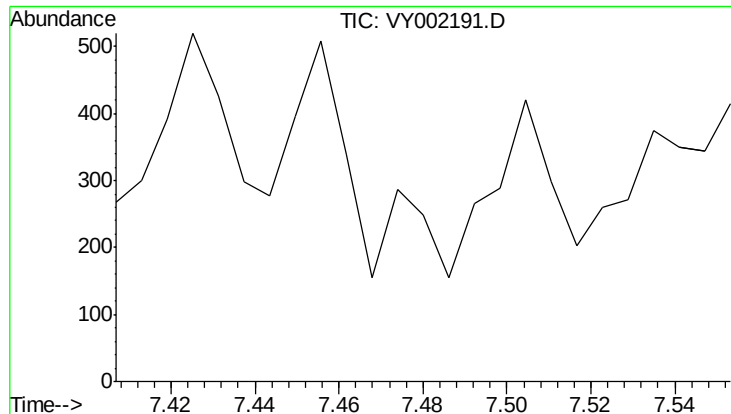

#34
 1,4-Difluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 8.71 min
 Lab File: VY002191.D
 Acq: 02 Apr 2020 14:54


Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-2E-(7-9)


Tot Ion	114
Sig	Exp Ratio
114	100
63	20.7
88	16.5

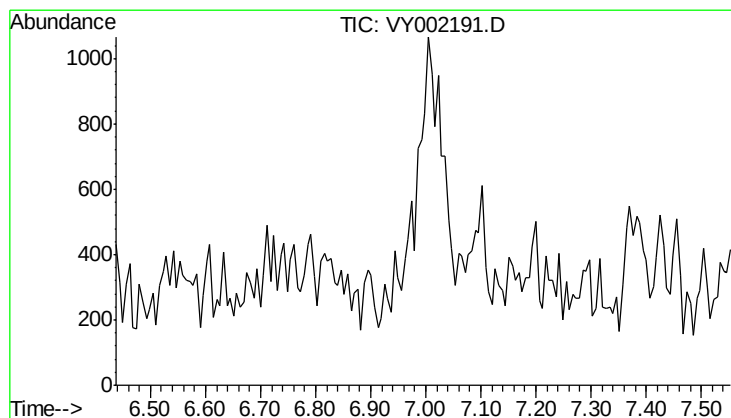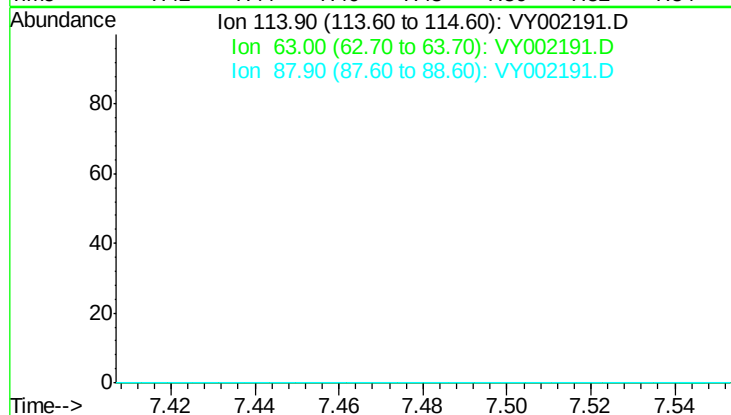

#35
 Dibromofluoromethane
 Concen: 0.000 ug/l
 Expected RT: 7.74 min
 Lab File: VY002191.D
 Acq: 02 Apr 2020 14:54

Tgt Ion	113
Sig	Exp Ratio
113	100
111	105.5
192	18.2

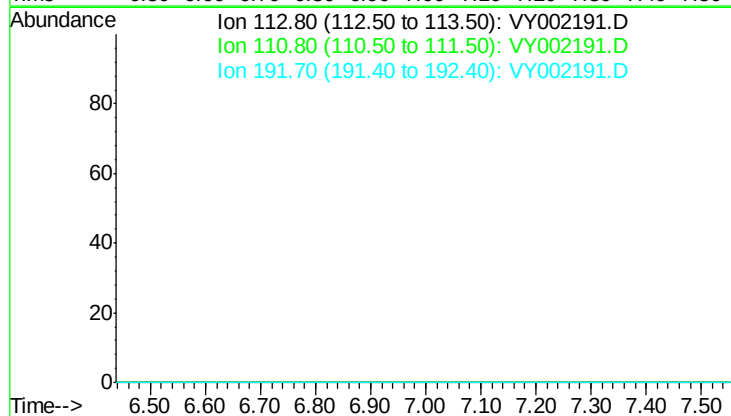


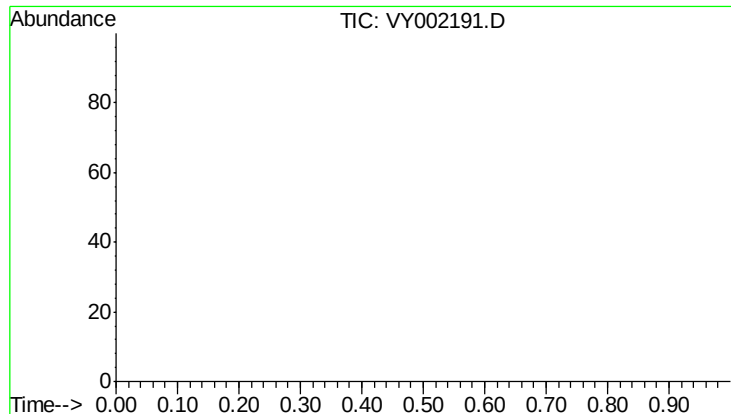


#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 10.19 min

Lab File: VY002191.D
Acq: 02 Apr 2020 14:54

Instrument :
MSVOA_Y
ClientSampleId :
SB-2E-(7-9)


Tot Ion	Sig	Exp Ratio
98	100	64.5
100	64.5	

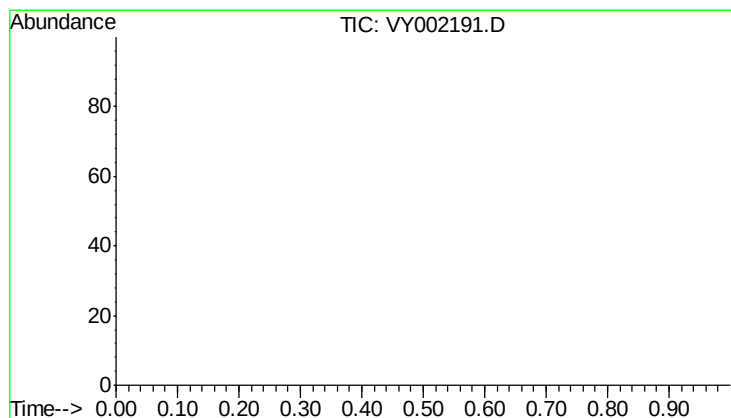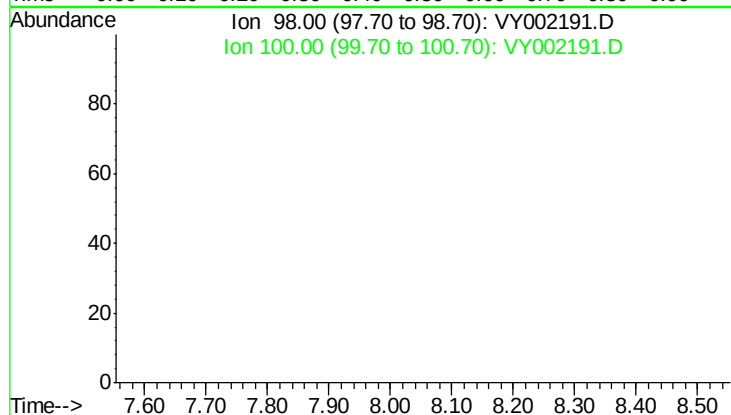


#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
Expected RT: 12.48 min

Lab File: VY002191.D
Acq: 02 Apr 2020 14:54

Tgt Ion	Sig	Exp Ratio
95	100	71.7
174	71.7	68.5
176	68.5	


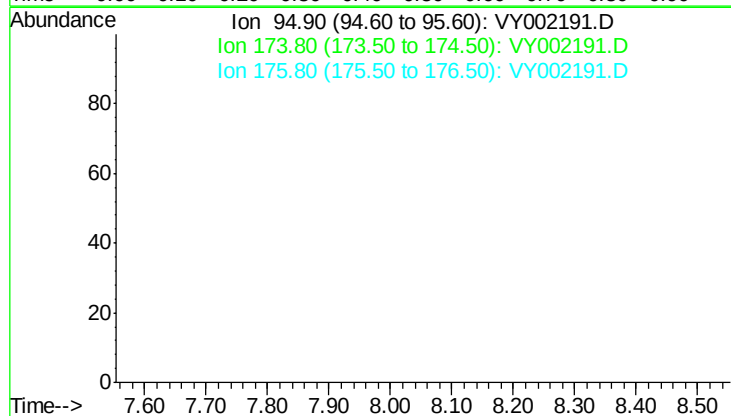


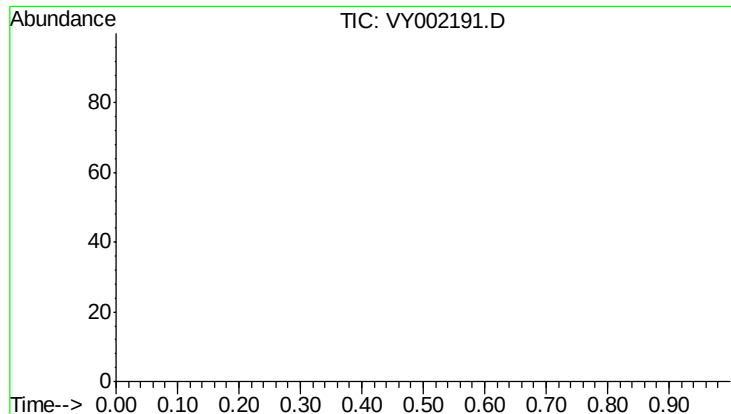

#63
 Chlorobenzene-d5
 Concen: 0.000 ug/l
 Expected RT: 11.50 min
 Lab File: VY002191.D
 Acq: 02 Apr 2020 14:54

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-2E-(7-9)

Tot Ion: 117
 Sig Exp Ratio
 117 100
 82 56.8
 119 31.6

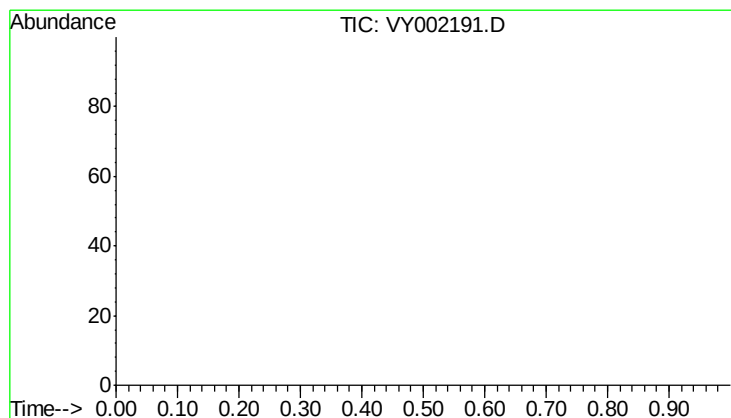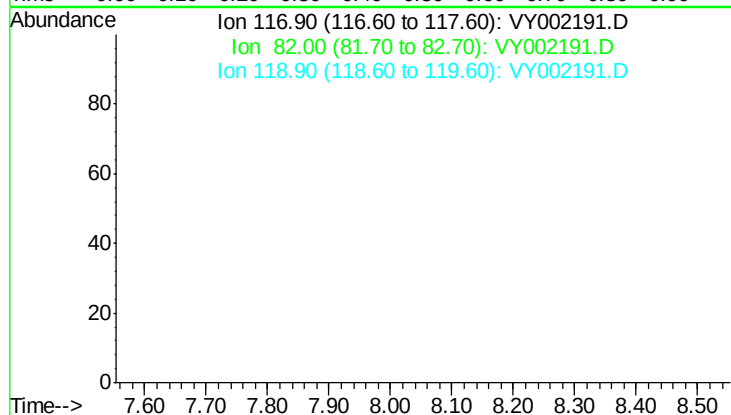

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ug/l
 Expected RT: 13.43 min
 Lab File: VY002191.D
 Acq: 02 Apr 2020 14:54

Tgt Ion: 152
 Sig Exp Ratio
 152 100
 115 62.4
 150 177.4

