

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY040221\
 Data File : VY004267.D
 Acq On : 02 Apr 2021 16:58
 Operator : SY/MD
 Sample : M1909-03
 Misc : 6.02g/5mL/MSVOA_Y/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 FS-SB-17-12-13

Quant Time: Apr 02 23:02:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032921S.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 30 06:38:14 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.801	168	252905	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	434085	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.496	117	386466	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	175118	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.155	65	150768	62.01	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery = 124.02%			
35) Dibromofluoromethane	7.734	113	131515	54.37	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery = 108.74%			
50) Toluene-d8	10.185	98	526049	57.83	ug/l	0.00
Spiked Amount 50.000	Range 49 - 140		Recovery = 115.66%			
62) 4-Bromofluorobenzene	12.483	95	178208	57.16	ug/l	0.00
Spiked Amount 50.000	Range 25 - 144		Recovery = 114.32%			
Target Compounds						Qvalue
39) Methylcyclohexane	9.191	83	6257	1.28	ug/l	95
40) Benzene	8.173	78	197934	17.62	ug/l	98
52) Toluene	10.252	92	121203	16.78	ug/l	99
67) Ethyl Benzene	11.599	91	209278	14.95	ug/l	99
68) m/p-Xylenes	11.703	106	217239	40.42	ug/l	97
69) o-Xylene	12.032	106	77523	15.42	ug/l	96
73) Isopropylbenzene	12.331	105	13243	1.04	ug/l	95
78) n-propylbenzene	12.672	91	24476	1.65	ug/l	97
80) 1,3,5-Trimethylbenzene	12.819	105	54729	5.24	ug/l	99
84) 1,2,4-Trimethylbenzene	13.123	105	188020	17.96	ug/l	100
95) Naphthalene	15.239	128	2918412	385.90	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY040221\
Data File : VY004267.D
Acq On : 02 Apr 2021 16:58
Operator : SY/MD
Sample : M1909-03
Misc : 6.02g/5mL/MSVOA_Y/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
FS-SB-17-12-13

Quant Time: Apr 02 23:02:28 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032921S.M
Quant Title : SW846 8260
QLast Update : Tue Mar 30 06:38:14 2021
Response via : Initial Calibration




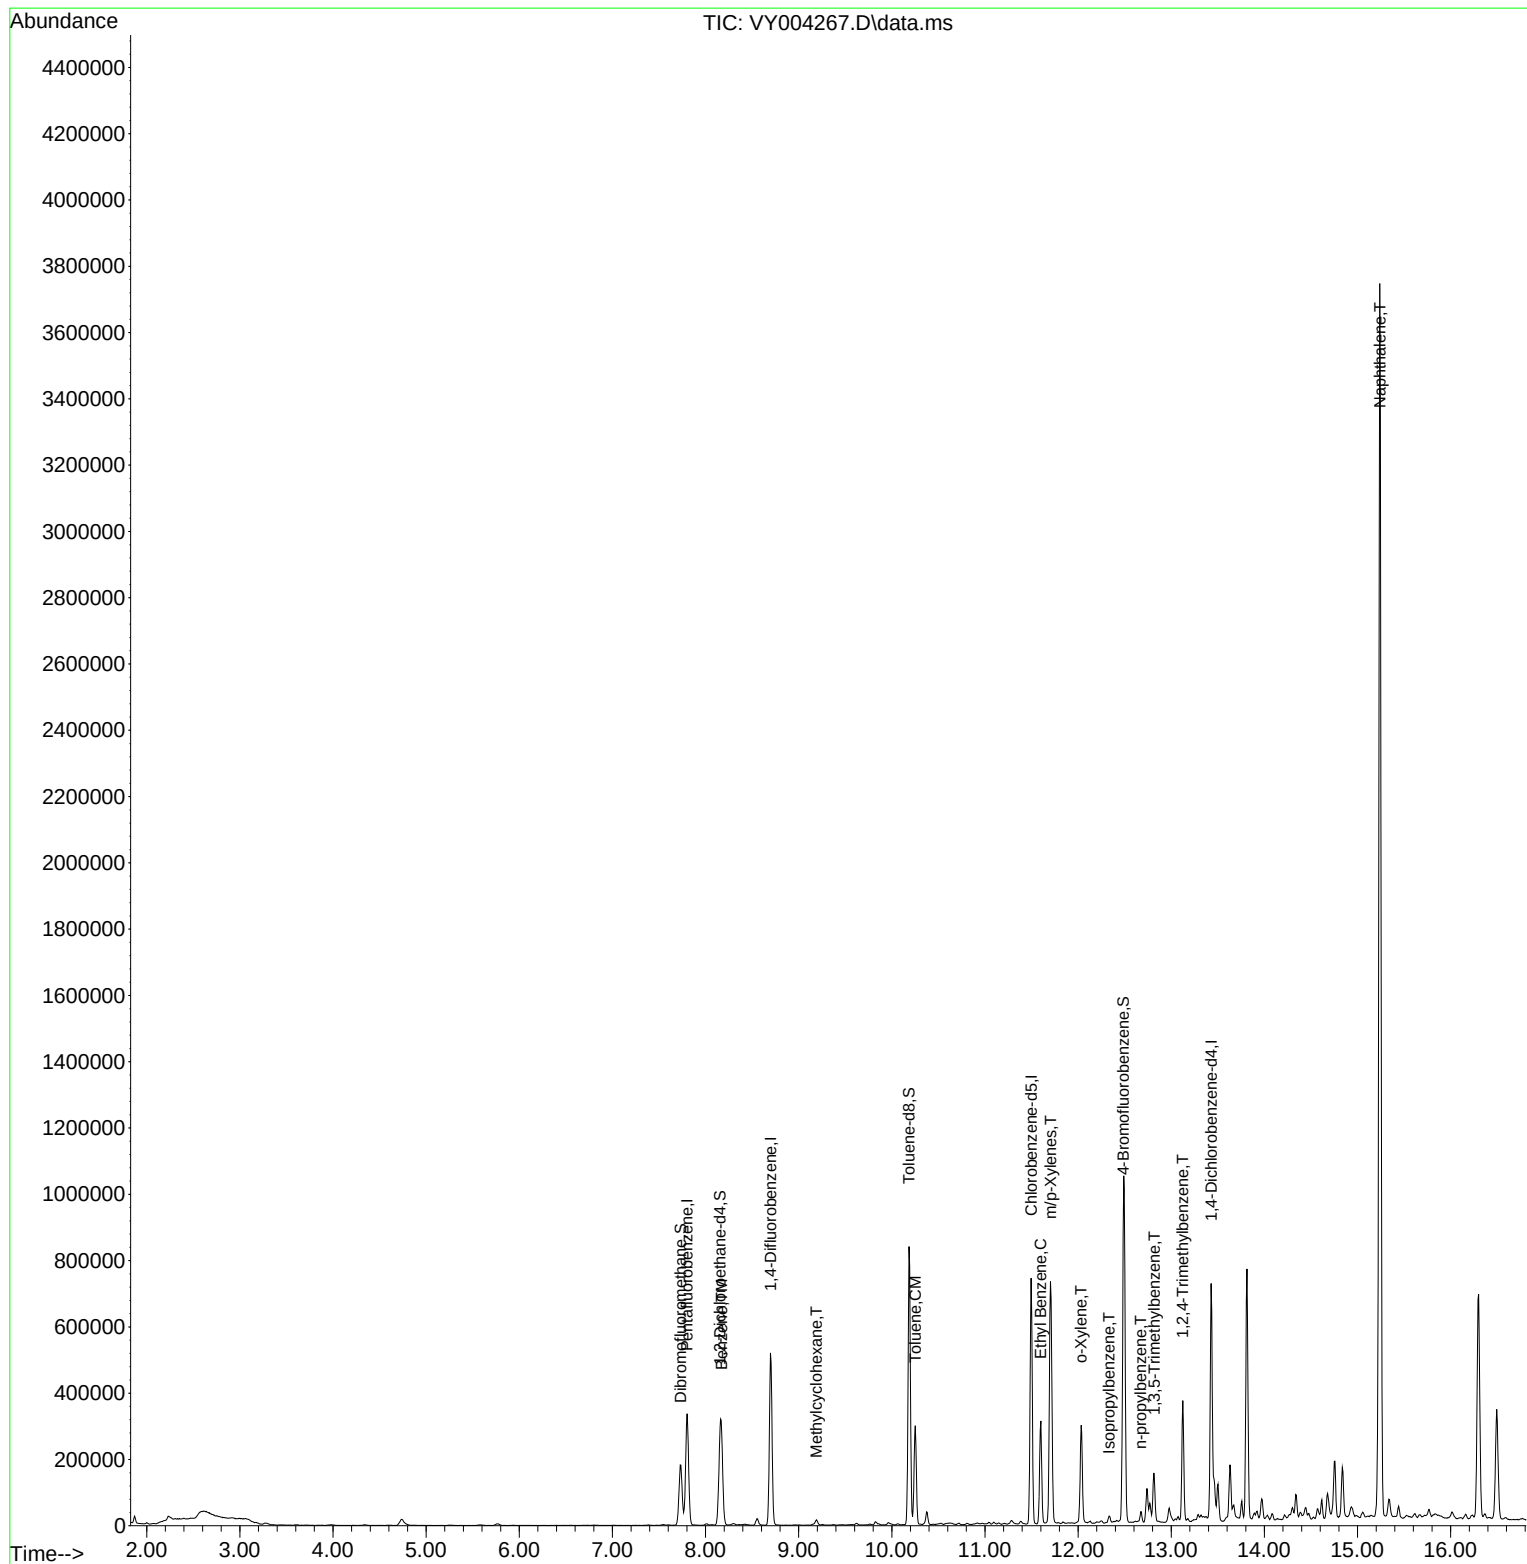


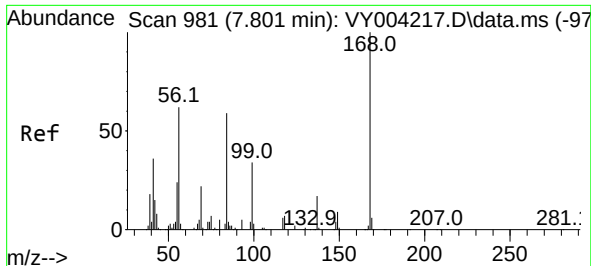

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.801 min Scan# 981
Delta R.T. 0.000 min
Lab File: VY004267.D
Acq: 02 Apr 2021 16:58




Instrument :
MSVOA_Y
ClientSampleId :
FS-SB-17-12-13


Tgt Ion:168 Resp: 252905
Ion Ratio Lower Upper
168 100
99 57.9 42.6 64.0

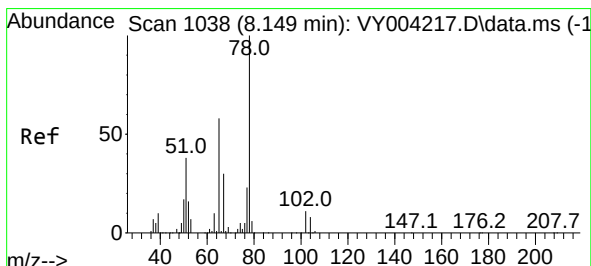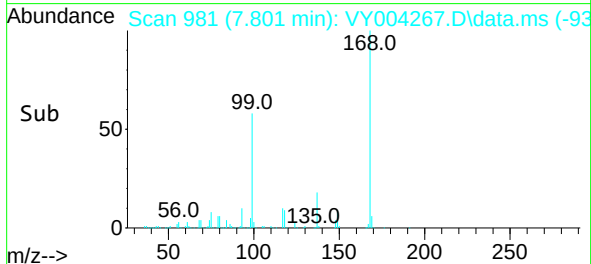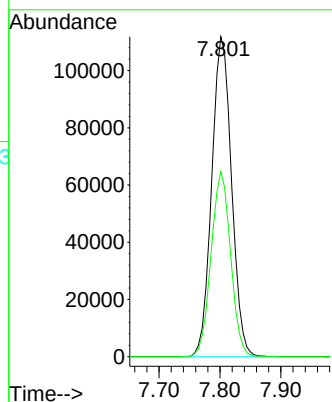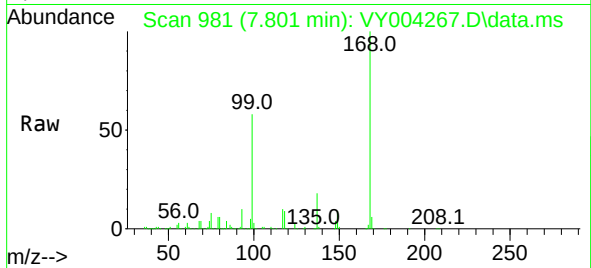

#33
1,2-Dichloroethane-d4
Concen: 62.01 ug/l
RT: 8.155 min Scan# 1039
Delta R.T. 0.006 min
Lab File: VY004267.D
Acq: 02 Apr 2021 16:58

Tgt Ion: 65 Resp: 150768
Ion Ratio Lower Upper
65 100
67 53.0 0.0 103.2


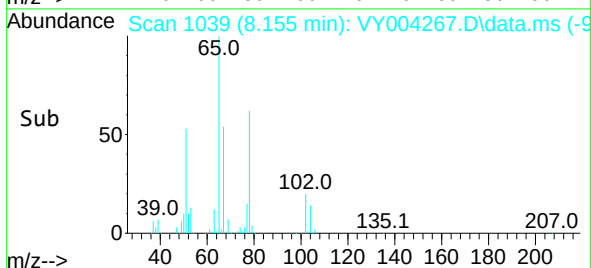
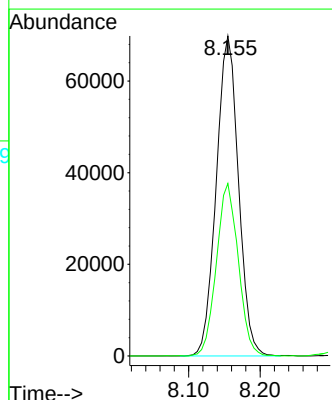
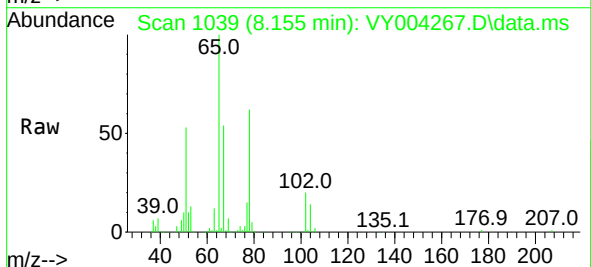


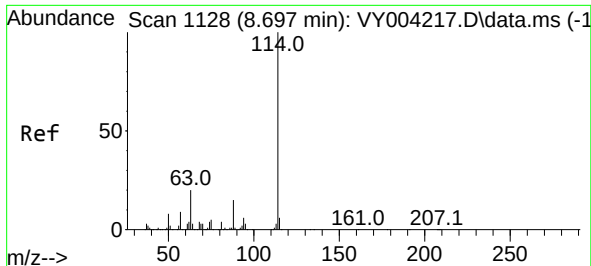

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. 0.000 min
Lab File: VY004267.D
Acq: 02 Apr 2021 16:58




Instrument :
MSVOA_Y
ClientSampleId :
FS-SB-17-12-13


Tgt Ion:	114	Resp:	434085
Ion Ratio	Lower	Upper	
114	100		
63	21.3	0.0	40.4
88	15.6	0.0	30.8

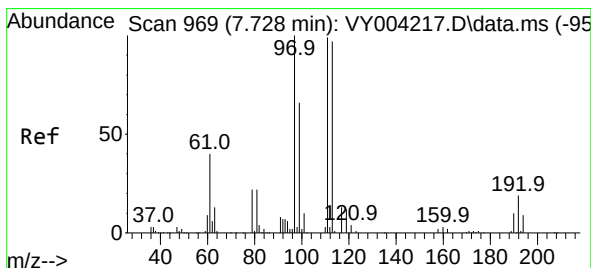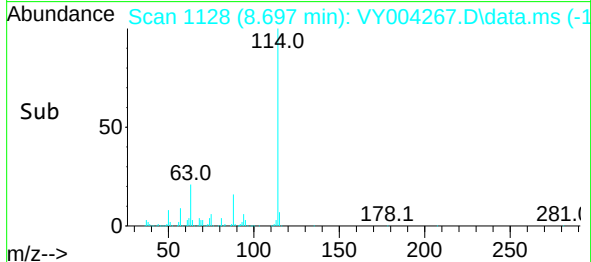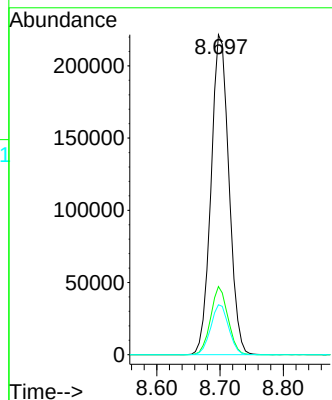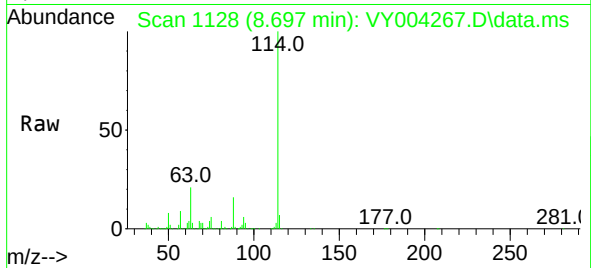

#35
Dibromofluoromethane
Concen: 54.37 ug/l
RT: 7.734 min Scan# 970
Delta R.T. 0.006 min
Lab File: VY004267.D
Acq: 02 Apr 2021 16:58

Tgt Ion:	113	Resp:	131515
Ion Ratio	Lower	Upper	
113	100		
111	102.8	82.6	124.0
192	19.4	16.4	24.6

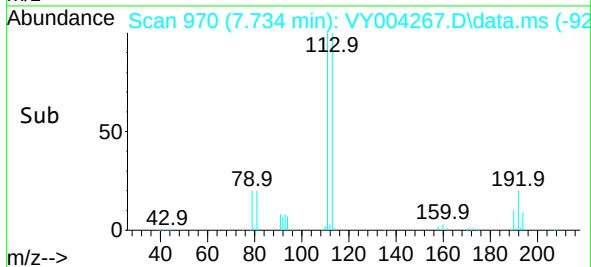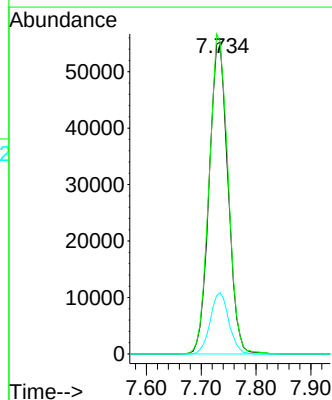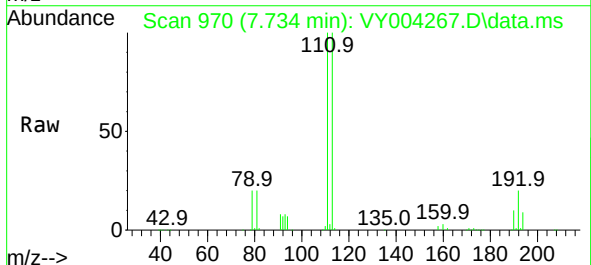

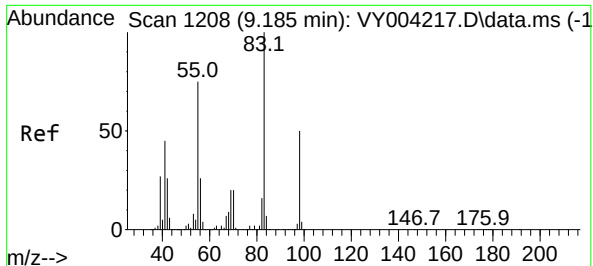

#39

Methylcyclohexane

Concen: 1.28 ug/l

RT: 9.191 min Scan# 1209

Delta R.T. 0.006 min

Lab File: VY004267.D

Acq: 02 Apr 2021 16:58





Tgt Ion: 83 Resp: 6257

Ion Ratio Lower Upper

83 100

55 80.3 60.0 90.0

98 51.7 40.2 60.2

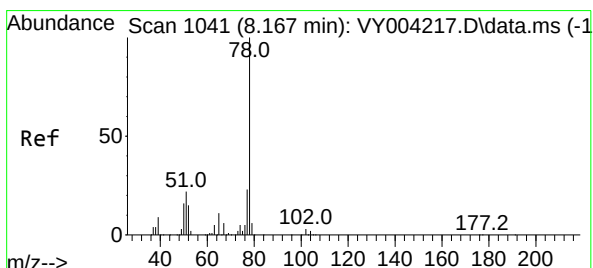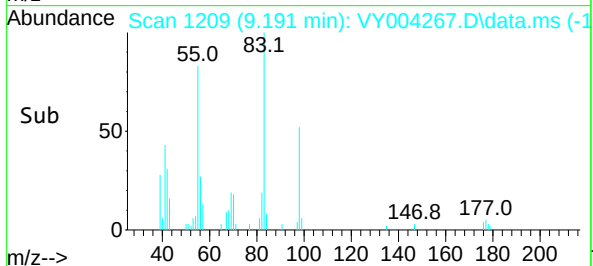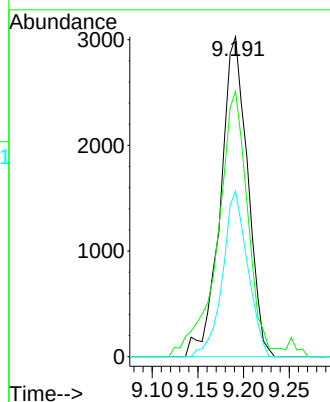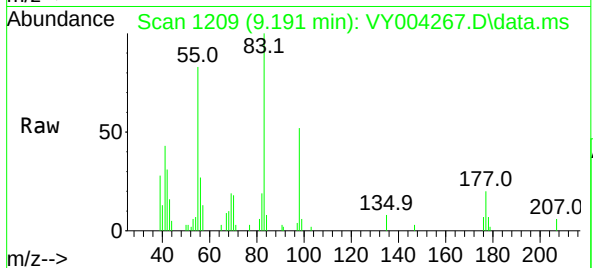

#40

Benzene

Concen: 17.62 ug/l

RT: 8.173 min Scan# 1042

Delta R.T. 0.006 min

Lab File: VY004267.D




Acq: 02 Apr 2021 16:58


Tgt Ion: 78 Resp: 197934

Ion Ratio Lower Upper

78 100

77 23.8 18.3 27.5


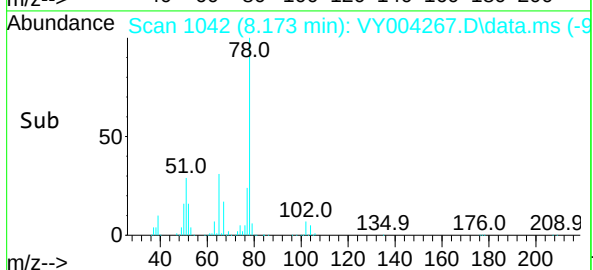
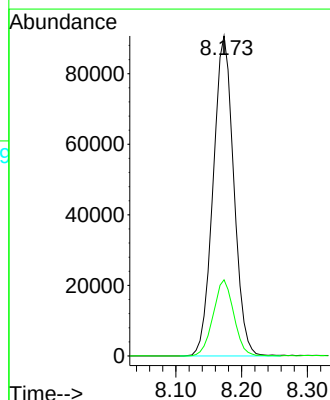
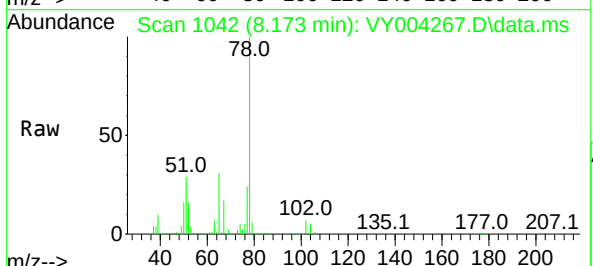


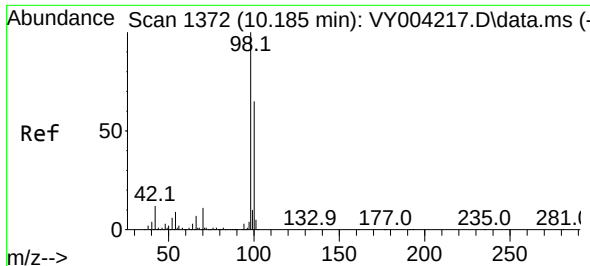

#50
Toluene-d8
Concen: 57.83 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. 0.000 min
Lab File: VY004267.D
Acq: 02 Apr 2021 16:58




Instrument :
MSVOA_Y
ClientSampleId :
FS-SB-17-12-13


Tgt Ion: 98 Resp: 526049
Ion Ratio Lower Upper
98 100
100 65.0 52.5 78.7

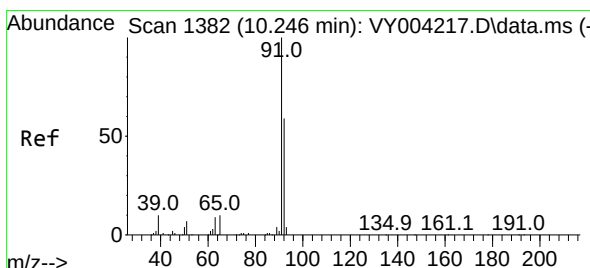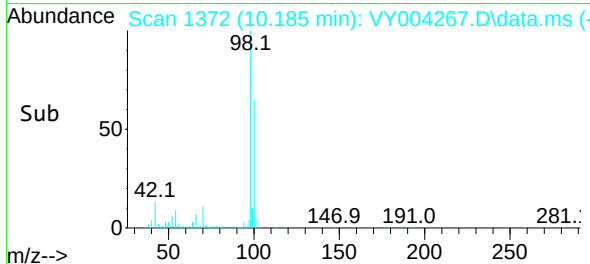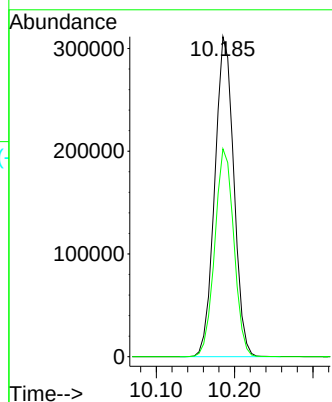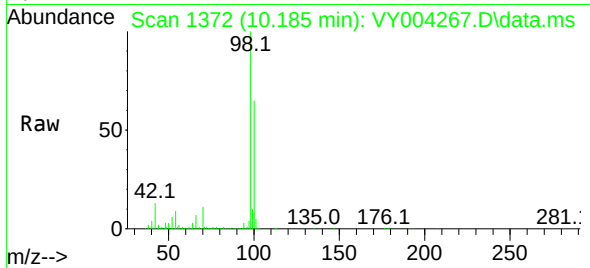

#52
Toluene
Concen: 16.78 ug/l
RT: 10.252 min Scan# 1383
Delta R.T. 0.006 min
Lab File: VY004267.D
Acq: 02 Apr 2021 16:58

Tgt Ion: 92 Resp: 121203
Ion Ratio Lower Upper
92 100
91 171.6 136.0 204.0


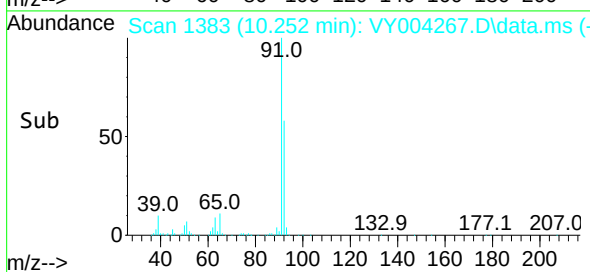
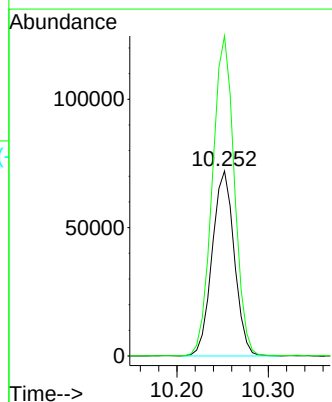
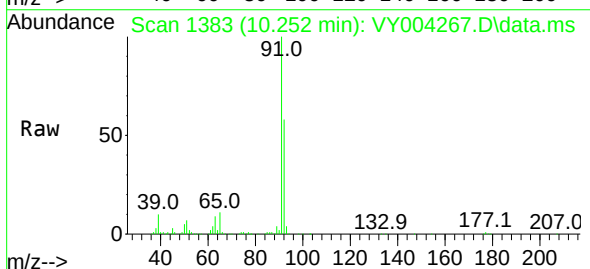


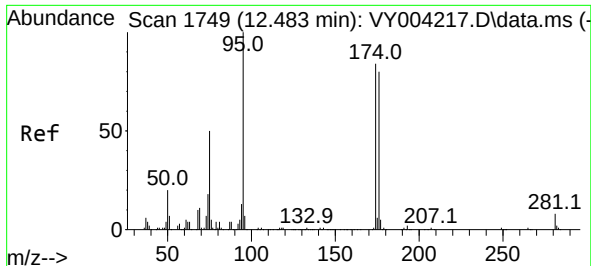

#62
4-Bromofluorobenzene
Concen: 57.16 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY004267.D
Acq: 02 Apr 2021 16:58




Instrument :
MSVOA_Y
ClientSampleId :
FS-SB-17-12-13


Tgt Ion: 95 Resp: 178208
Ion Ratio Lower Upper
95 100
174 80.9 0.0 171.4
176 78.4 0.0 165.6

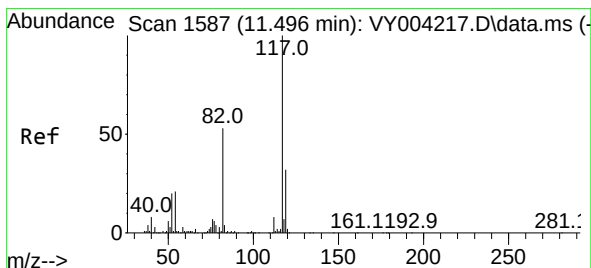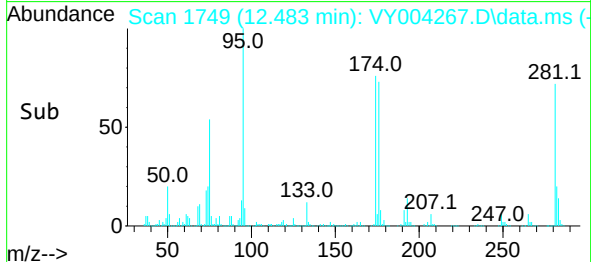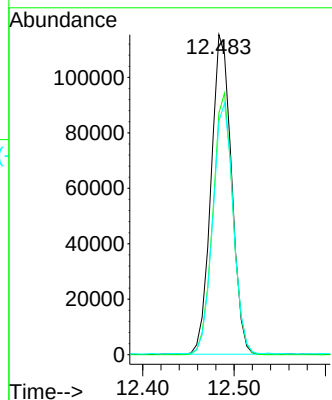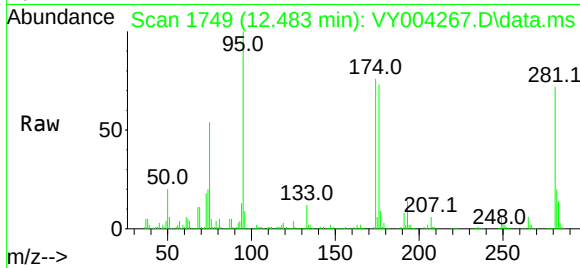

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.496 min Scan# 1587
Delta R.T. 0.000 min
Lab File: VY004267.D
Acq: 02 Apr 2021 16:58

Tgt Ion: 117 Resp: 386466
Ion Ratio Lower Upper
117 100
82 55.9 42.7 64.1
119 32.1 25.7 38.5


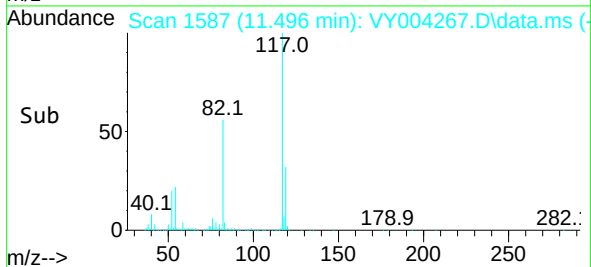
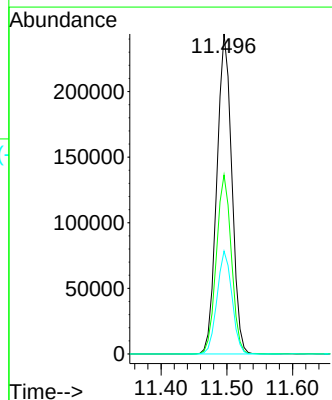
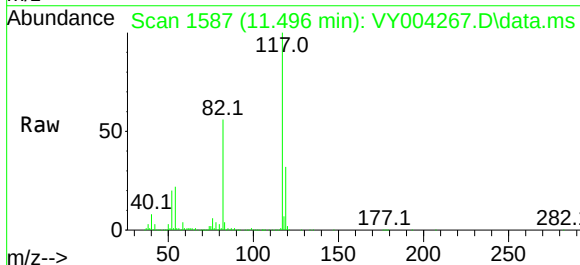


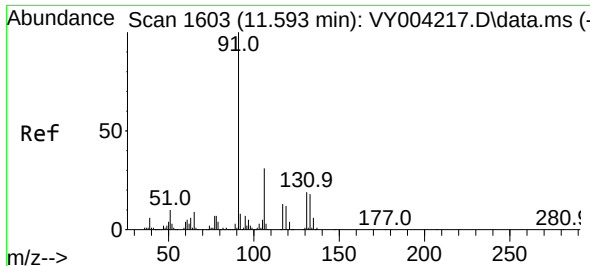

#67
Ethyl Benzene
Concen: 14.95 ug/l
RT: 11.599 min Scan# 1604
Delta R.T. 0.006 min
Lab File: VY004267.D
Acq: 02 Apr 2021 16:58




Instrument :
MSVOA_Y
ClientSampleId :
FS-SB-17-12-13


Tgt Ion: 91 Resp: 209278
Ion Ratio Lower Upper
91 100
106 31.0 25.0 37.6

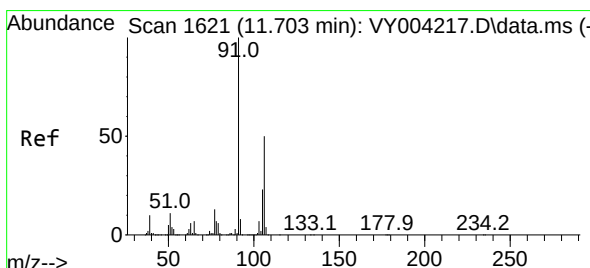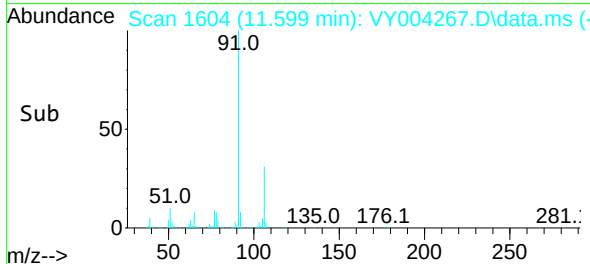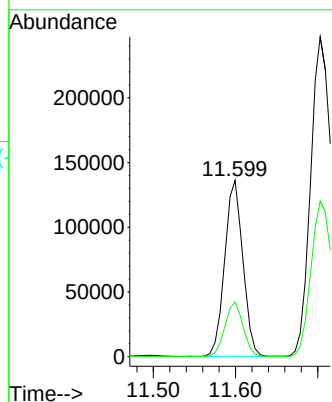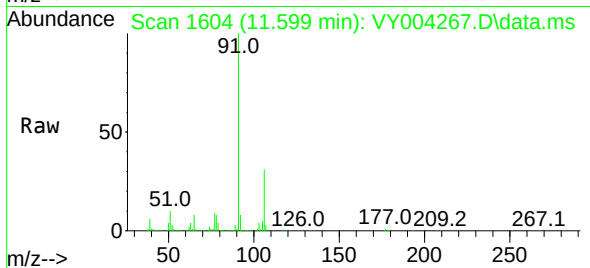

#68
m/p-Xylenes
Concen: 40.42 ug/l
RT: 11.703 min Scan# 1621
Delta R.T. 0.000 min
Lab File: VY004267.D
Acq: 02 Apr 2021 16:58

Tgt Ion: 106 Resp: 217239
Ion Ratio Lower Upper
106 100
91 203.7 159.8 239.6


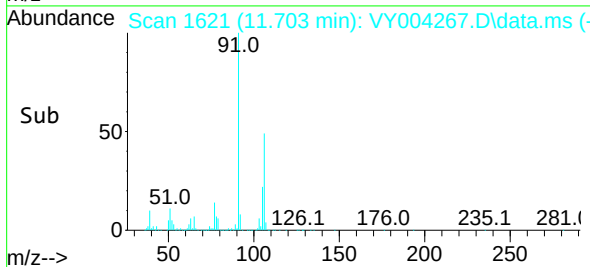
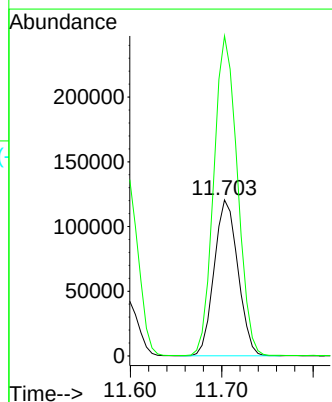
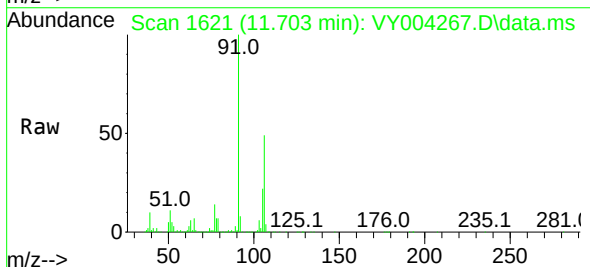


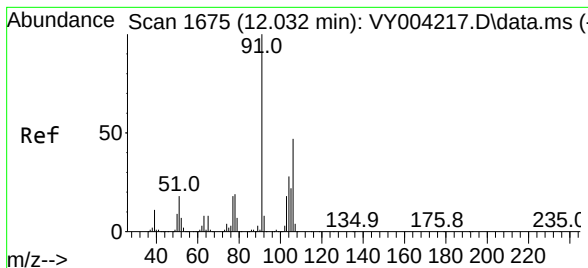

#69
o-Xylene
Concen: 15.42 ug/l
RT: 12.032 min Scan# 1675
Delta R.T. 0.000 min
Lab File: VY004267.D
Acq: 02 Apr 2021 16:58




Instrument :
MSVOA_Y
ClientSampleId :
FS-SB-17-12-13


Tgt Ion:106 Resp: 77523
Ion Ratio Lower Upper
106 100
91 216.7 105.6 316.8

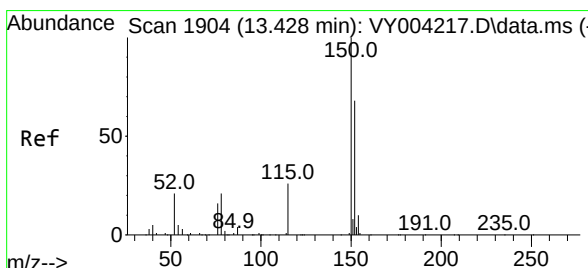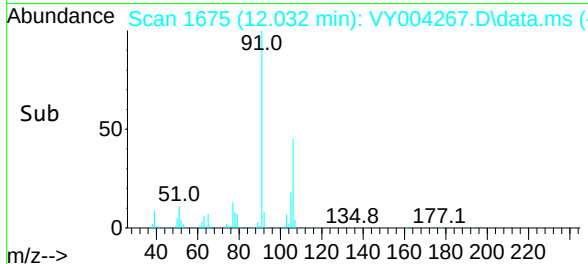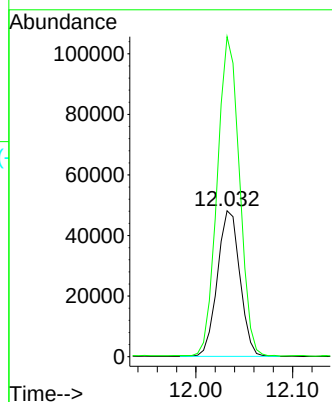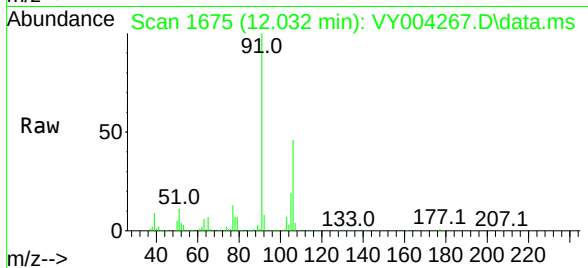

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY004267.D
Acq: 02 Apr 2021 16:58

Tgt Ion:152 Resp: 175118
Ion Ratio Lower Upper
152 100
115 60.3 29.0 87.1
150 158.6 0.0 347.4


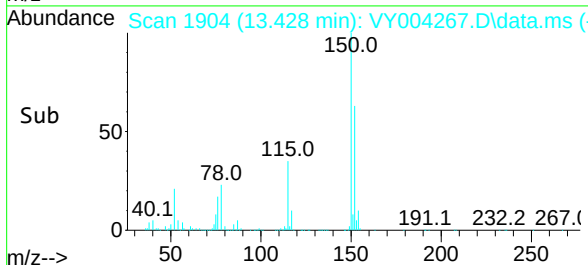
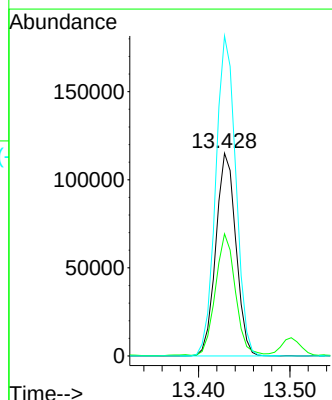
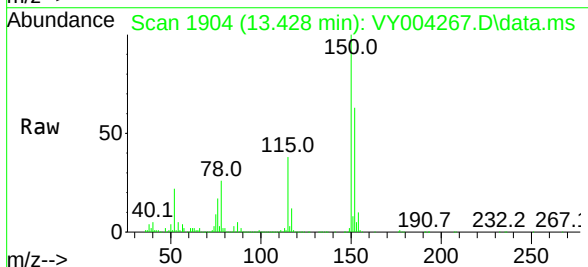


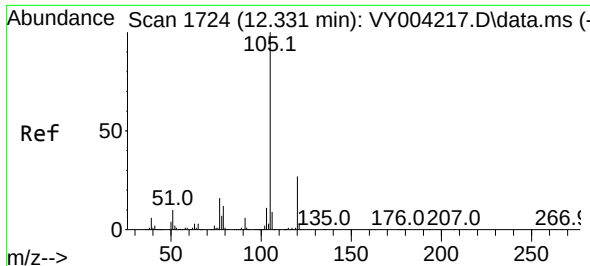

#73
Isopropylbenzene
Concen: 1.04 ug/l
RT: 12.331 min Scan# 1724
Delta R.T. 0.000 min
Lab File: VY004267.D
Acq: 02 Apr 2021 16:58




Instrument :
MSVOA_Y
ClientSampleId :
FS-SB-17-12-13


Tgt Ion: 105 Resp: 13243
Ion Ratio Lower Upper
105 100
120 24.6 13.7 41.0

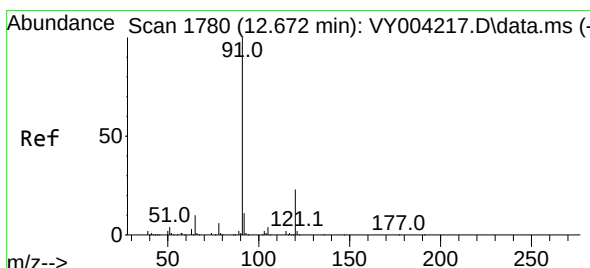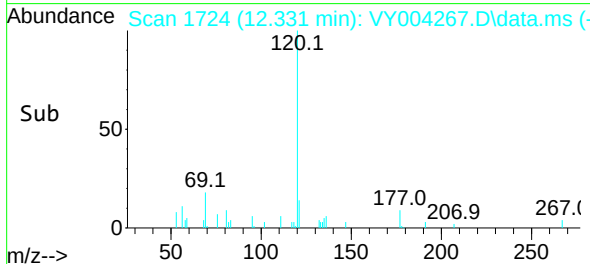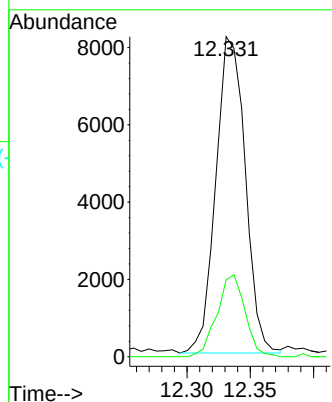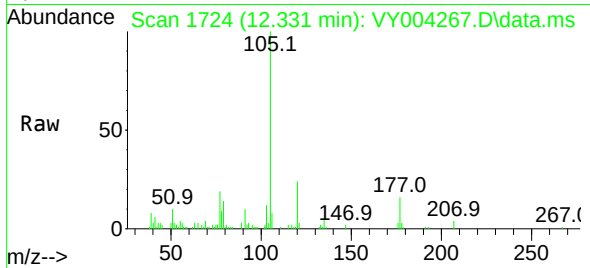

#78
n-propylbenzene
Concen: 1.65 ug/l
RT: 12.672 min Scan# 1780
Delta R.T. 0.000 min
Lab File: VY004267.D
Acq: 02 Apr 2021 16:58

Tgt Ion: 91 Resp: 24476
Ion Ratio Lower Upper
91 100
120 25.2 11.9 35.5


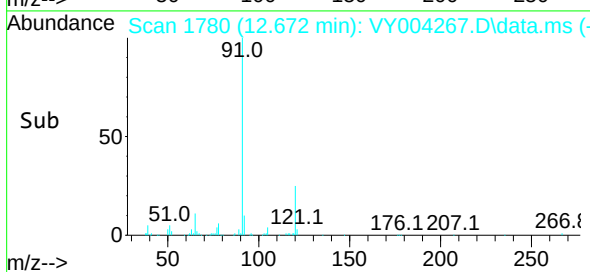
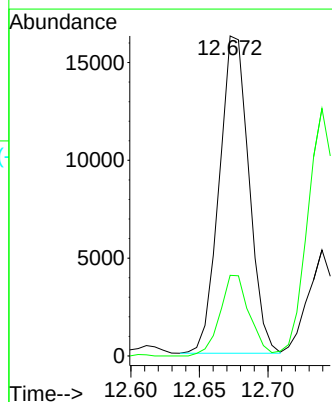
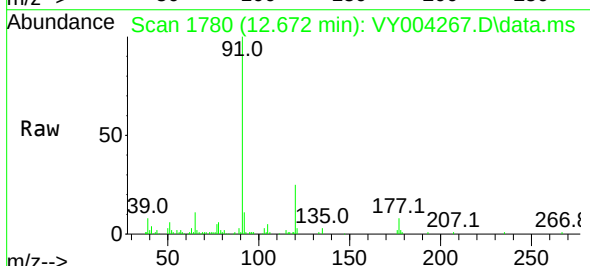


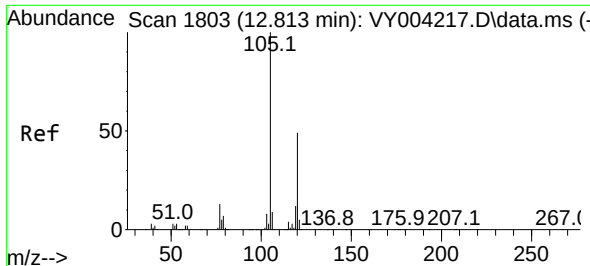

#80
1,3,5-Trimethylbenzene
Concen: 5.24 ug/l
RT: 12.819 min Scan# 1804
Delta R.T. 0.006 min
Lab File: VY004267.D
Acq: 02 Apr 2021 16:58




Instrument :
MSVOA_Y
ClientSampleId :
FS-SB-17-12-13


Tgt Ion:105 Resp: 54729
Ion Ratio Lower Upper
105 100
120 49.4 24.9 74.7

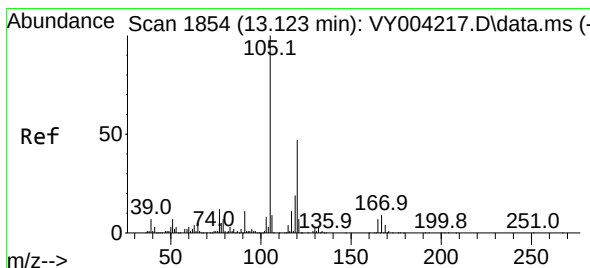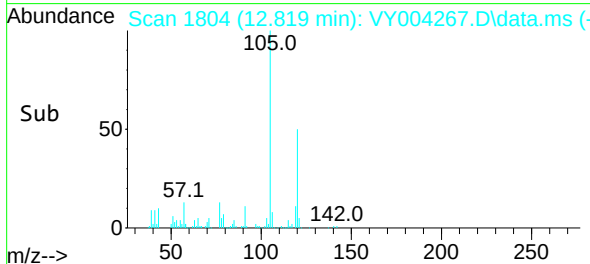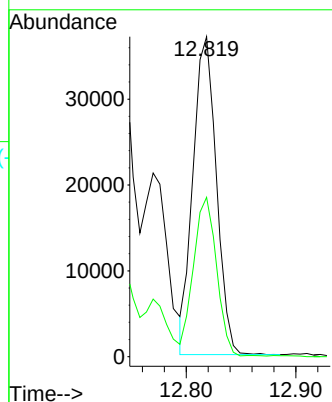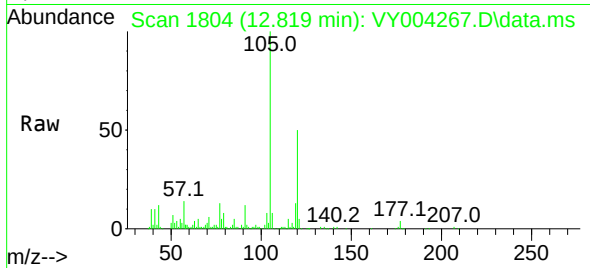

#84
1,2,4-Trimethylbenzene
Concen: 17.96 ug/l
RT: 13.123 min Scan# 1854
Delta R.T. 0.000 min
Lab File: VY004267.D
Acq: 02 Apr 2021 16:58

Tgt Ion:105 Resp: 188020
Ion Ratio Lower Upper
105 100
120 46.0 22.9 68.7

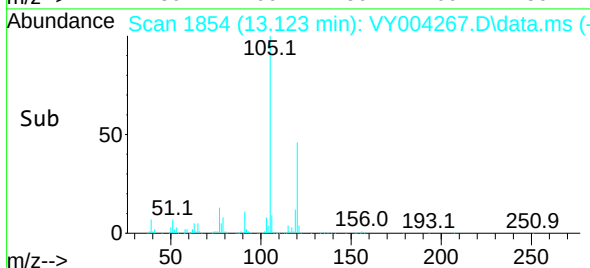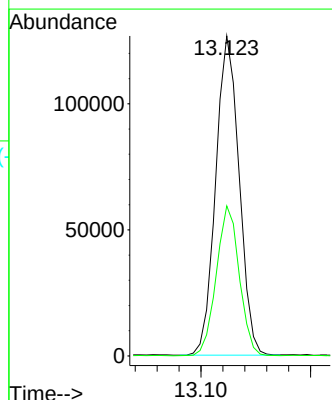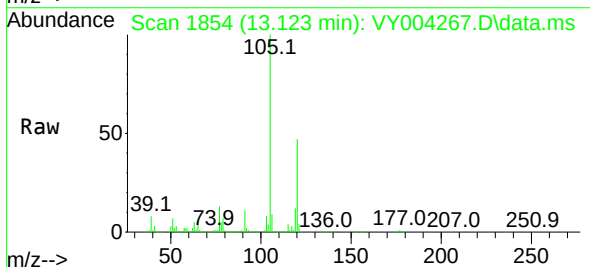

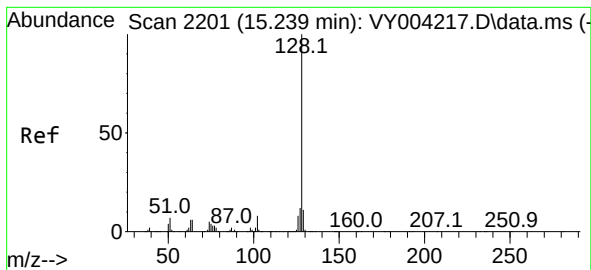

#95
Naphthalene
Concen: 385.90 ug/l
RT: 15.239 min Scan# 2201
Delta R.T. 0.000 min
Lab File: VY004267.D
Acq: 02 Apr 2021 16:58

Instrument :
MSVOA_Y
ClientSampleId :
FS-SB-17-12-13

Tgt Ion:128 Resp: 2918412
Ion Ratio Lower Upper
128 100
127 12.8 10.1 15.1
129 11.0 8.9 13.3

