
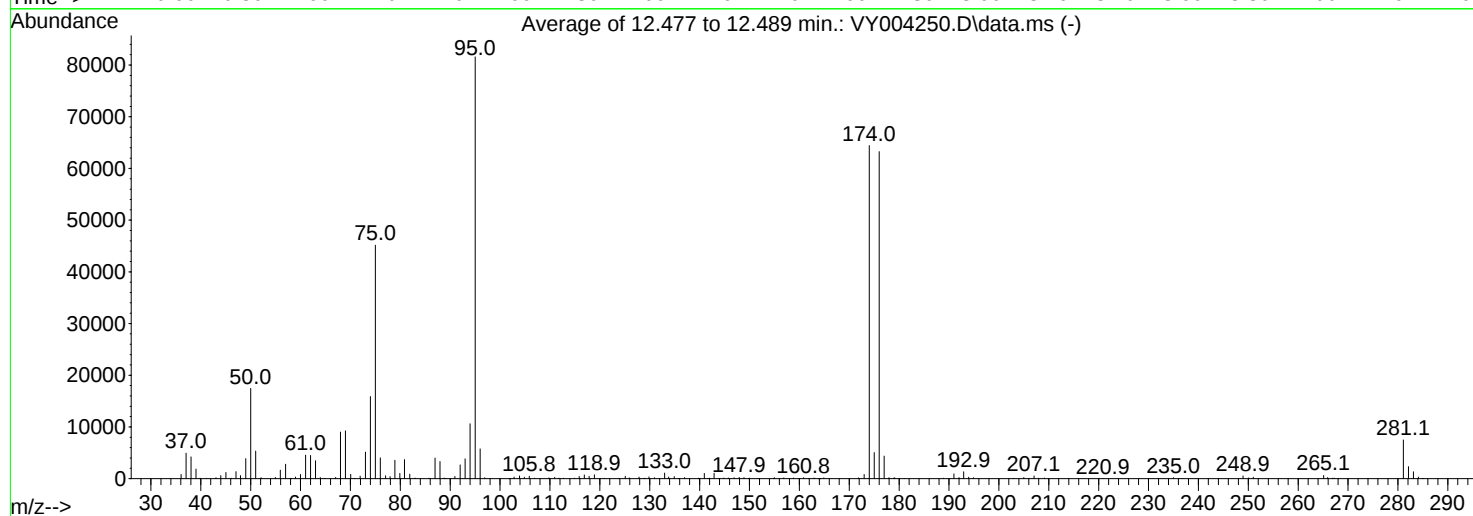


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY040221\
Data File : VY004250.D
Acq On : 02 Apr 2021 09:21
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032921S.M
Title : SW846 8260
Last Update : Tue Mar 30 06:38:14 2021

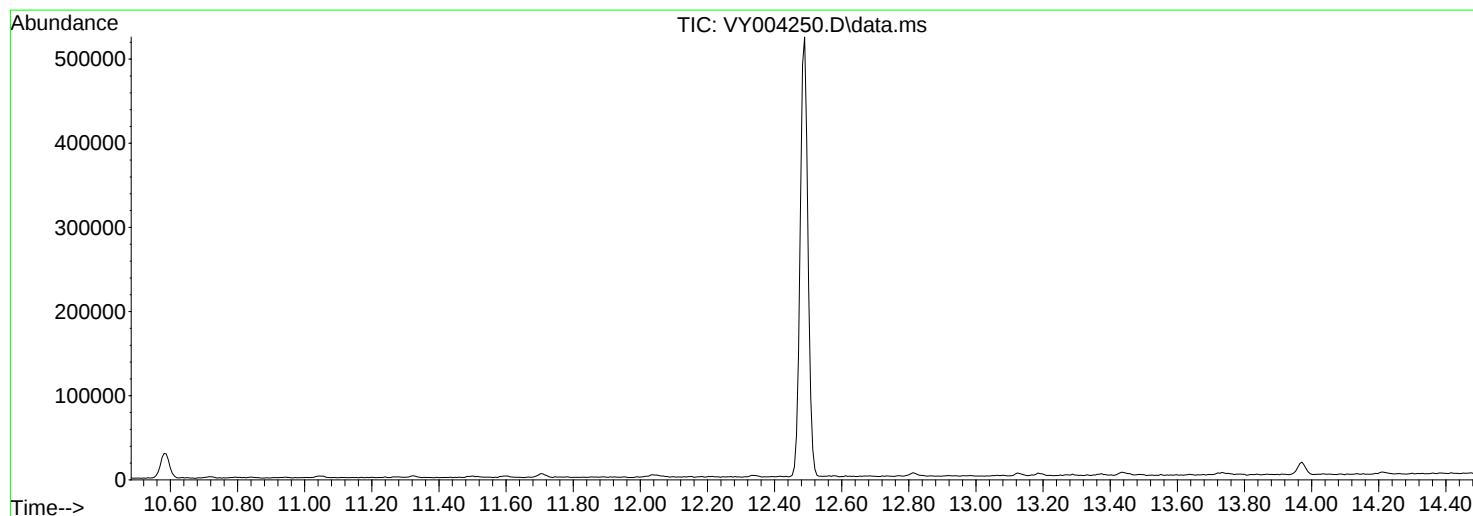

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	17444	PASS
75	95	30	60	55.4	45160	PASS
95	95	100	100	100.0	81587	PASS
96	95	5	9	7.1	5752	PASS
173	174	0.00	2	1.2	792	PASS
174	95	50	100	79.0	64424	PASS
175	174	5	9	7.8	5045	PASS
176	174	95	101	98.2	63262	PASS
177	176	5	9	6.9	4370	PASS