

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY040323\
 Data File : VY013170.D
 Acq On : 03 Apr 2023 13:01
 Operator : KP/MD
 Sample : 02163-01
 Misc : 5.34g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-1A

Quant Time: Apr 03 23:07:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y033023S.M
 Quant Title : SW846 8260
 QLast Update : Mon Apr 03 13:40:57 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	100442	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	161588	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	143224	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	63257	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	54050	50.073	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	100.140%
35) Dibromofluoromethane	7.716	113	52774	49.994	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	99.980%
50) Toluene-d8	10.179	98	188395	47.275	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	94.560%
62) 4-Bromofluorobenzene	12.483	95	56760	43.758	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	87.520%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY040323\
Data File : VY013170.D
Acq On : 03 Apr 2023 13:01
Operator : KP/MD
Sample : 02163-01
Misc : 5.34g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SB-1A

Quant Time: Apr 03 23:07:42 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y033023S.M
Quant Title : SW846 8260
QLast Update : Mon Apr 03 13:40:57 2023
Response via : Initial Calibration




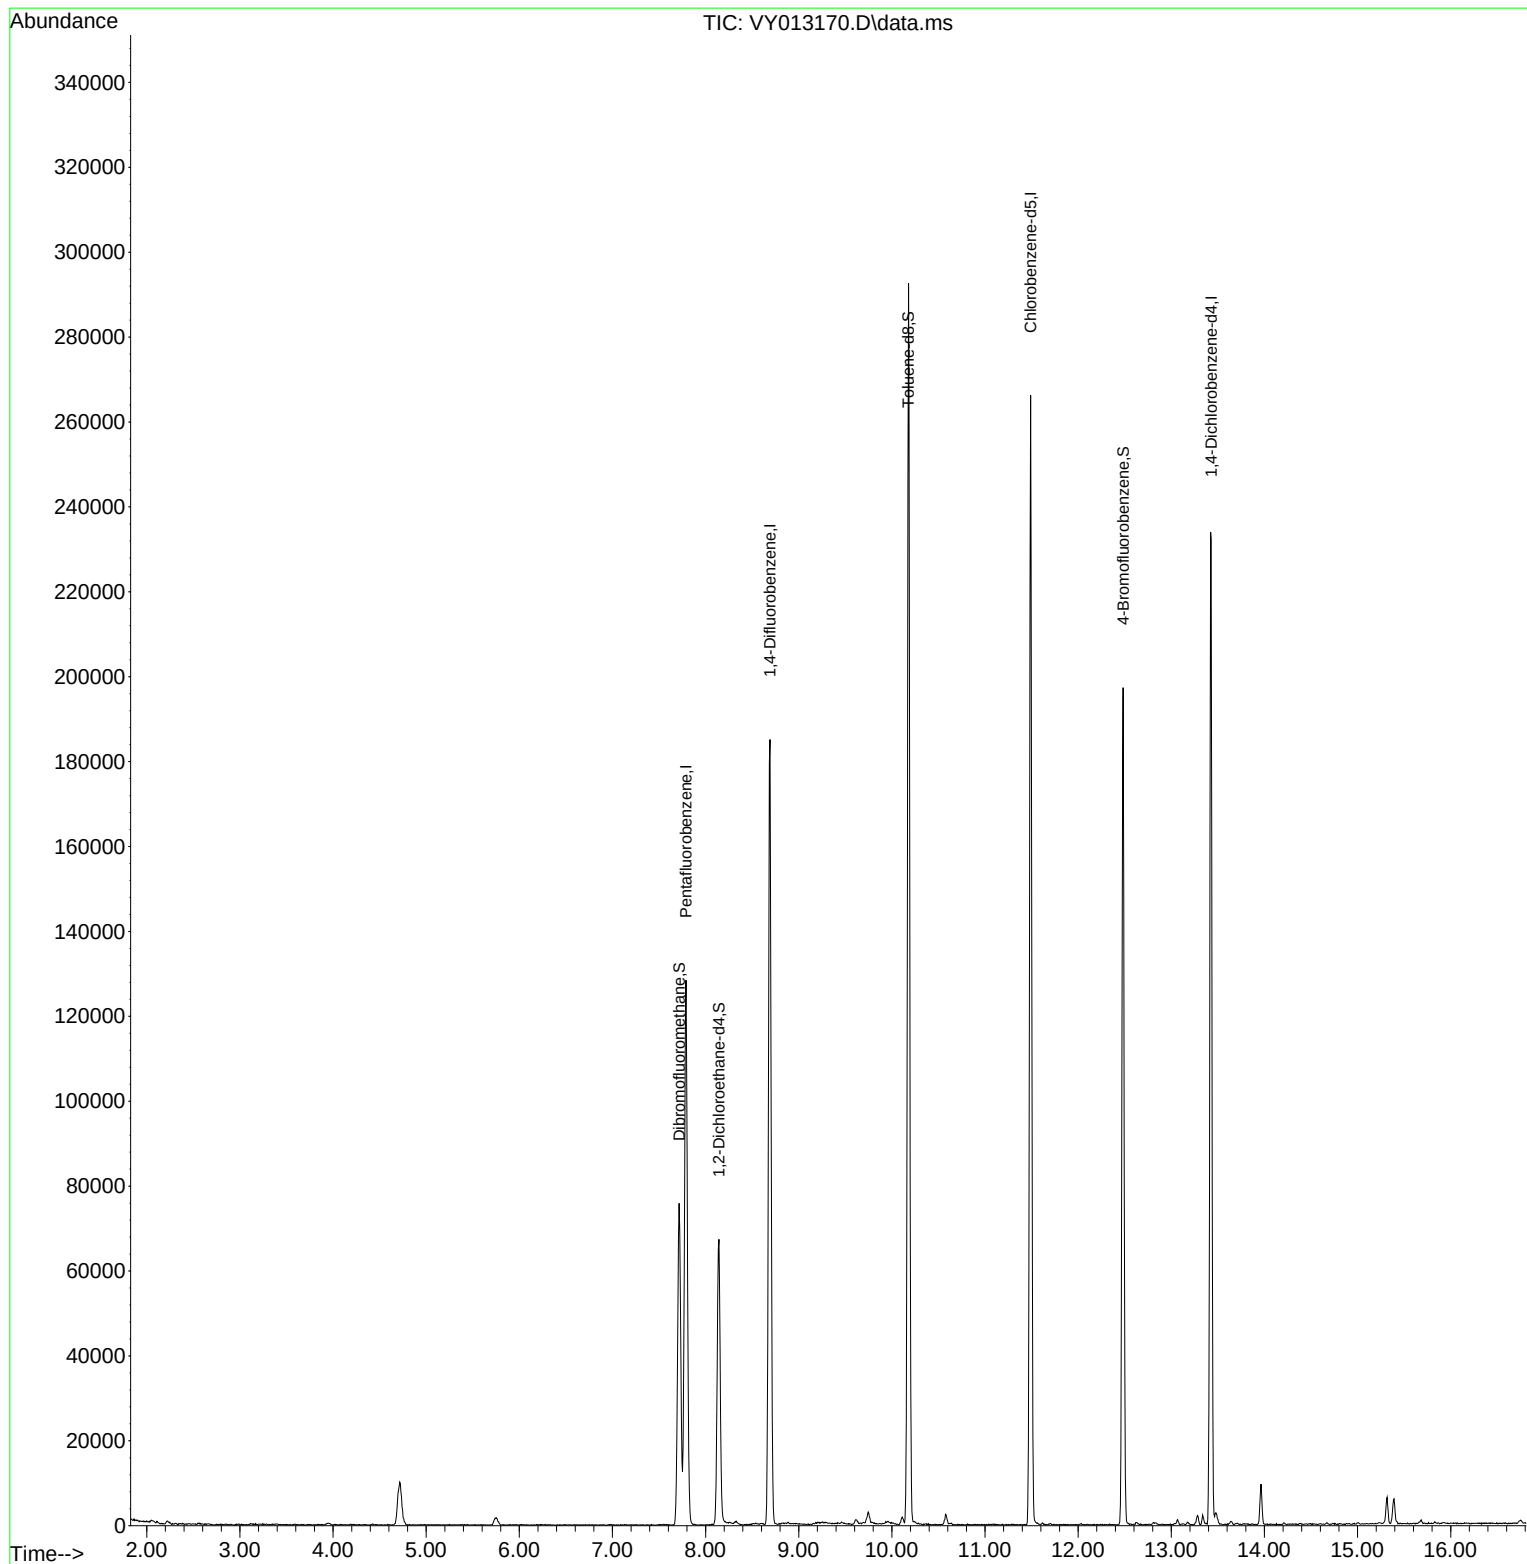


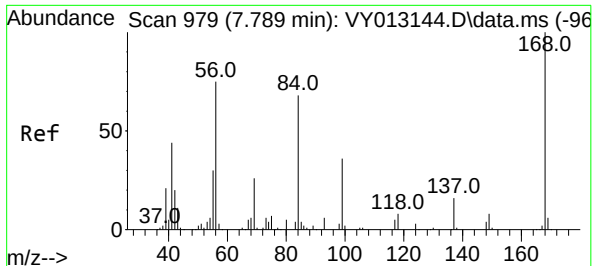

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY013170.D
Acq: 03 Apr 2023 13:01




Instrument :
MSVOA_Y
ClientSampleId :
SB-1A


Tgt Ion:168 Resp: 100442
Ion Ratio Lower Upper
168 100
99 51.3 41.7 62.5

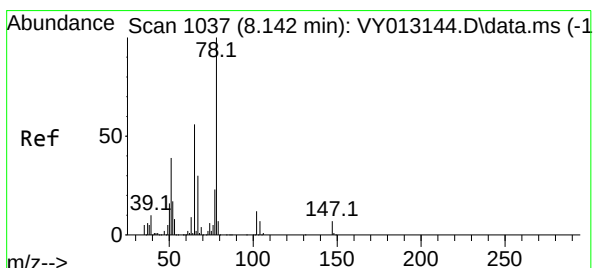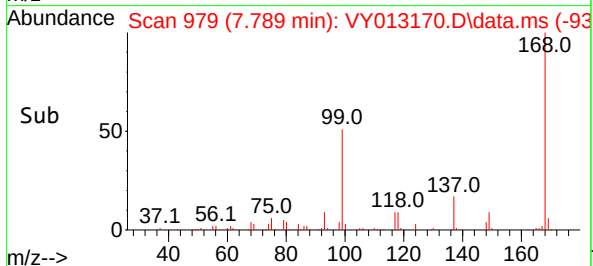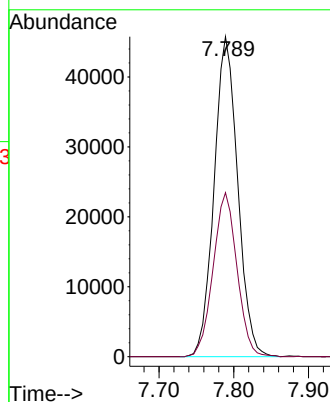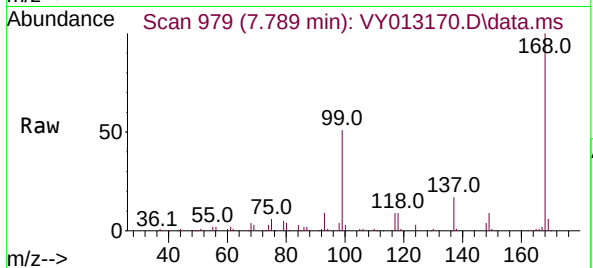

#33
1,2-Dichloroethane-d4
Concen: 50.073 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. 0.001 min
Lab File: VY013170.D
Acq: 03 Apr 2023 13:01

Tgt Ion: 65 Resp: 54050
Ion Ratio Lower Upper
65 100
67 51.9 0.0 104.0

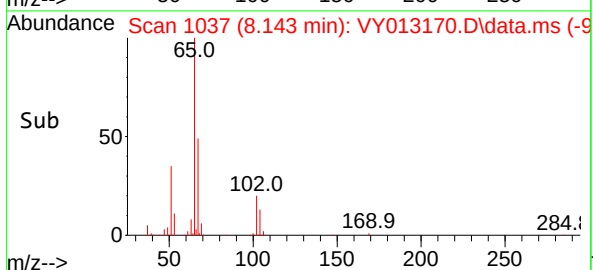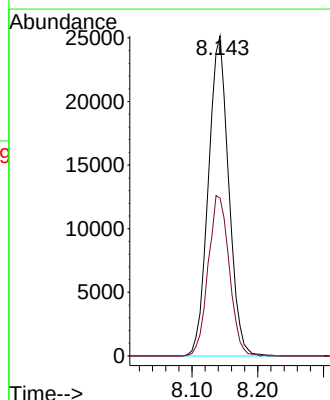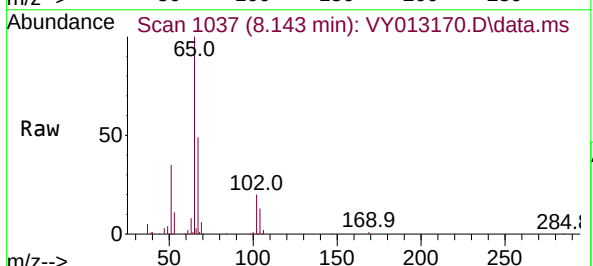

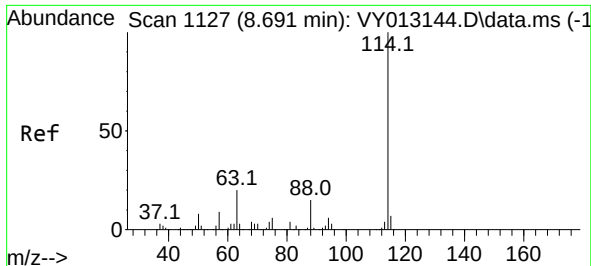

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY013170.D

Acq: 03 Apr 2023 13:01

Instrument :

MSVOA_Y

ClientSampleId :

SB-1A





Tgt Ion:114 Resp: 161588

Ion Ratio Lower Upper

114 100

63 18.3 0.0 37.4

88 15.2 0.0 28.6

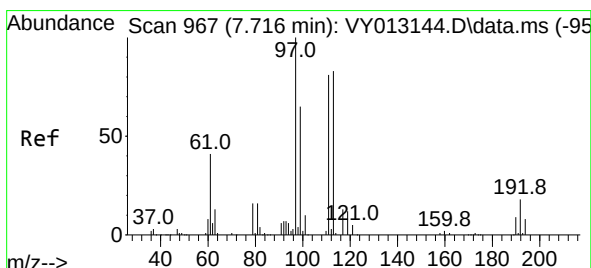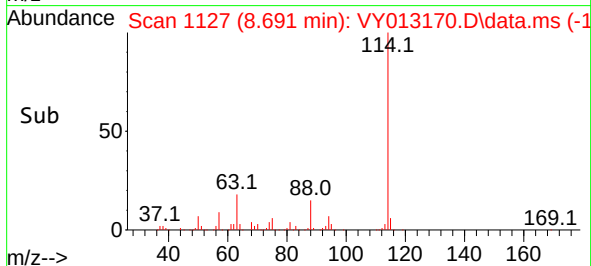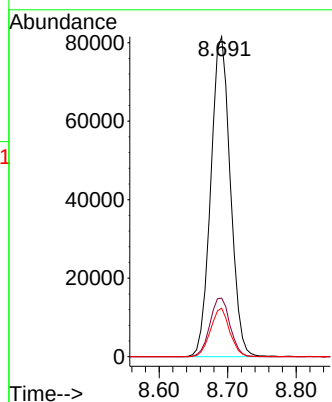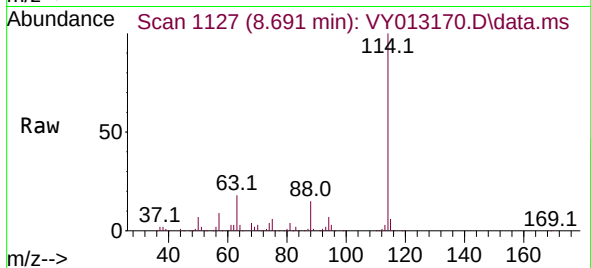

#35

Dibromofluoromethane

Concen: 49.994 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY013170.D

Acq: 03 Apr 2023 13:01




Tgt Ion:113 Resp: 52774


Ion Ratio Lower Upper

113 100

111 102.2 82.2 123.2

192 21.9 16.8 25.2


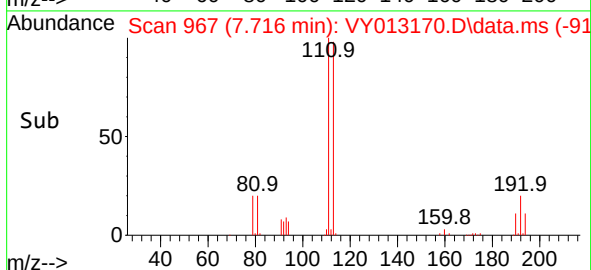
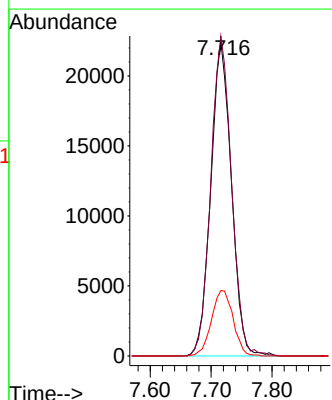
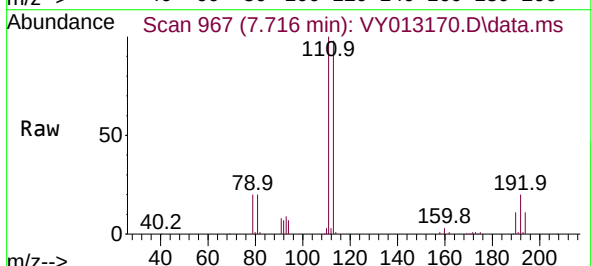


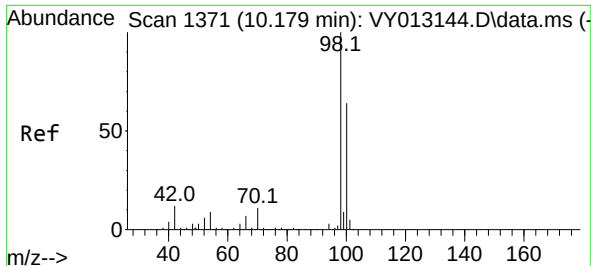

#50
Toluene-d8
Concen: 47.275 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY013170.D
Acq: 03 Apr 2023 13:01




Instrument :
MSVOA_Y
ClientSampleId :
SB-1A


Tgt Ion: 98 Resp: 188395
Ion Ratio Lower Upper
98 100
100 64.3 50.9 76.3

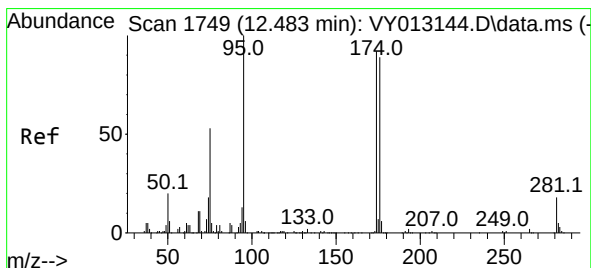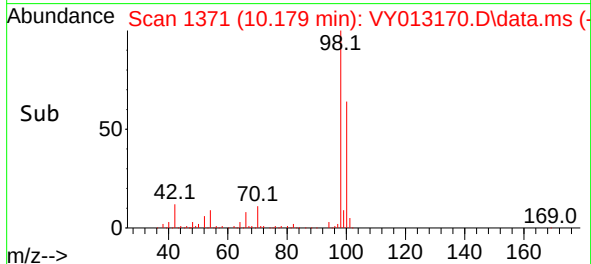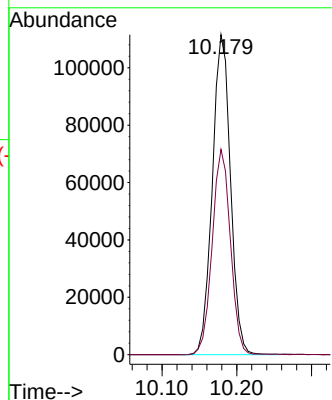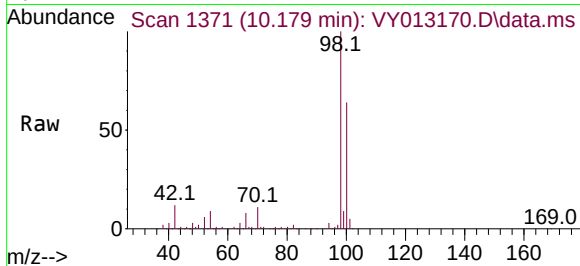

#62
4-Bromofluorobenzene
Concen: 43.758 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY013170.D
Acq: 03 Apr 2023 13:01

Tgt Ion: 95 Resp: 56760
Ion Ratio Lower Upper
95 100
174 93.1 0.0 176.6
176 90.5 0.0 170.2

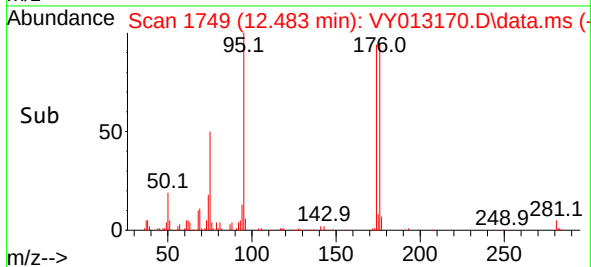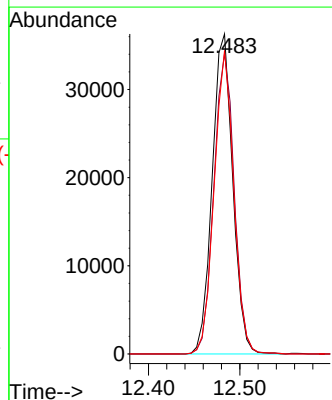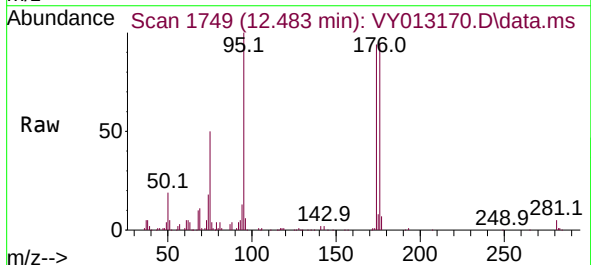

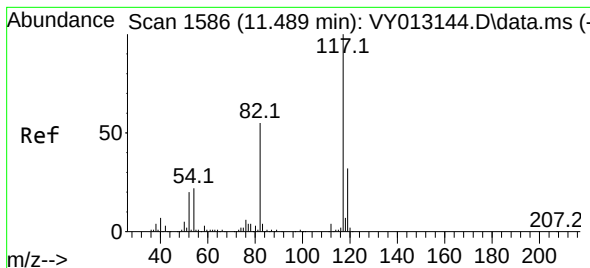

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.490 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY013170.D

Acq: 03 Apr 2023 13:01

Instrument :

MSVOA_Y

ClientSampleId :

SB-1A





Tgt Ion:117 Resp: 143224

Ion Ratio Lower Upper

117 100

82 51.8 45.4 68.0

119 32.7 25.6 38.4

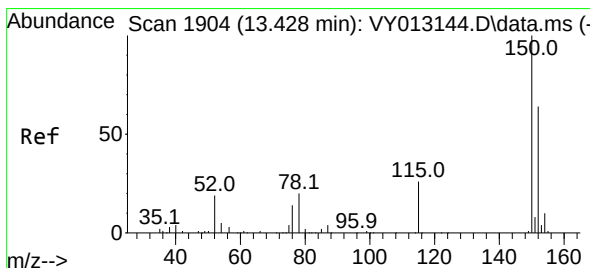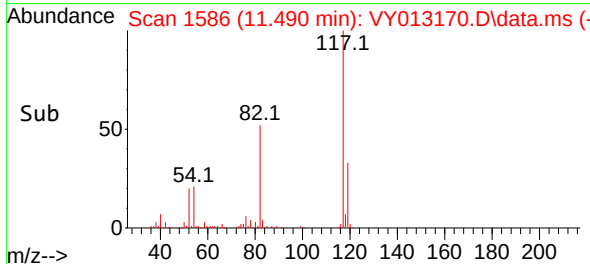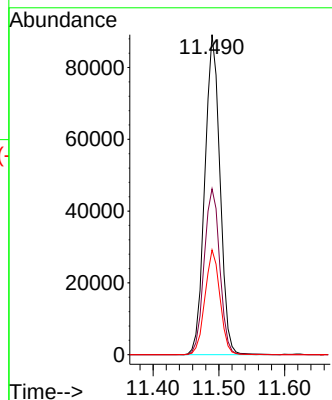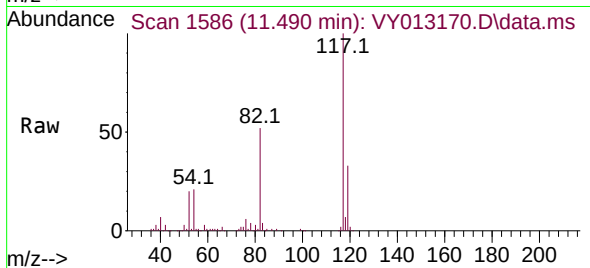

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.428 min Scan# 1904

Delta R.T. 0.000 min

Lab File: VY013170.D

Acq: 03 Apr 2023 13:01

Tgt Ion:152 Resp: 63257

Ion Ratio Lower Upper

152 100

115 55.8 27.1 81.3

150 158.9 0.0 347.8

