
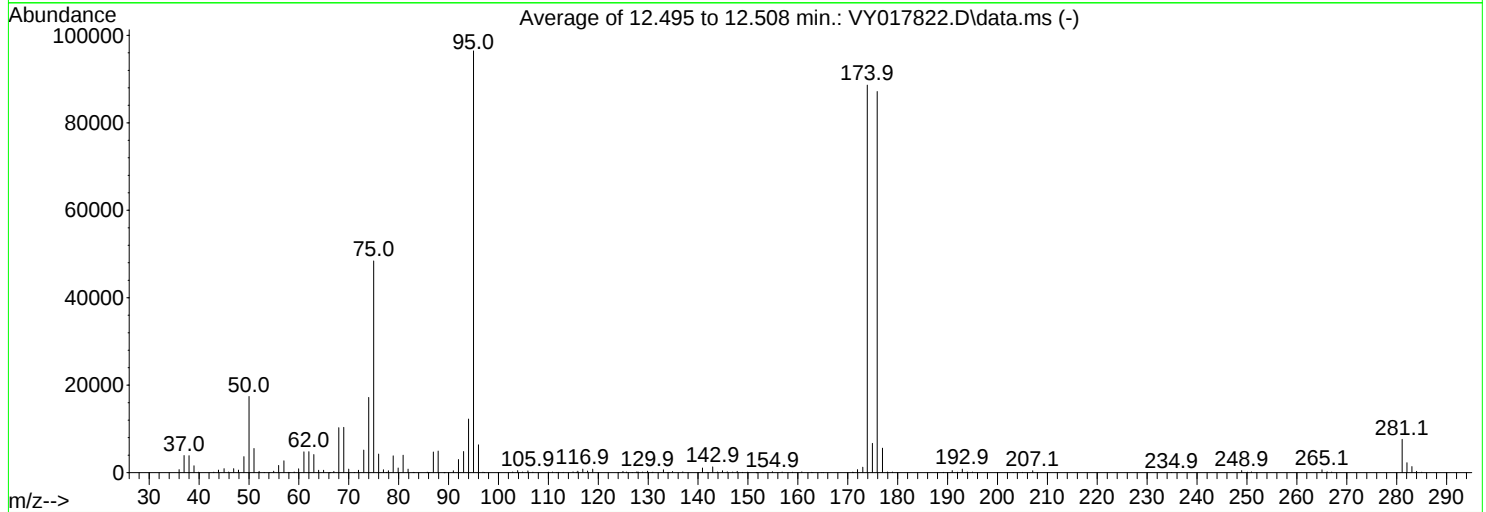


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY040324\
Data File : VY017822.D
Acq On : 03 Apr 2024 08:32
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032924S.M
Title : SW846 8260
Last Update : Sat Mar 30 05:58:13 2024

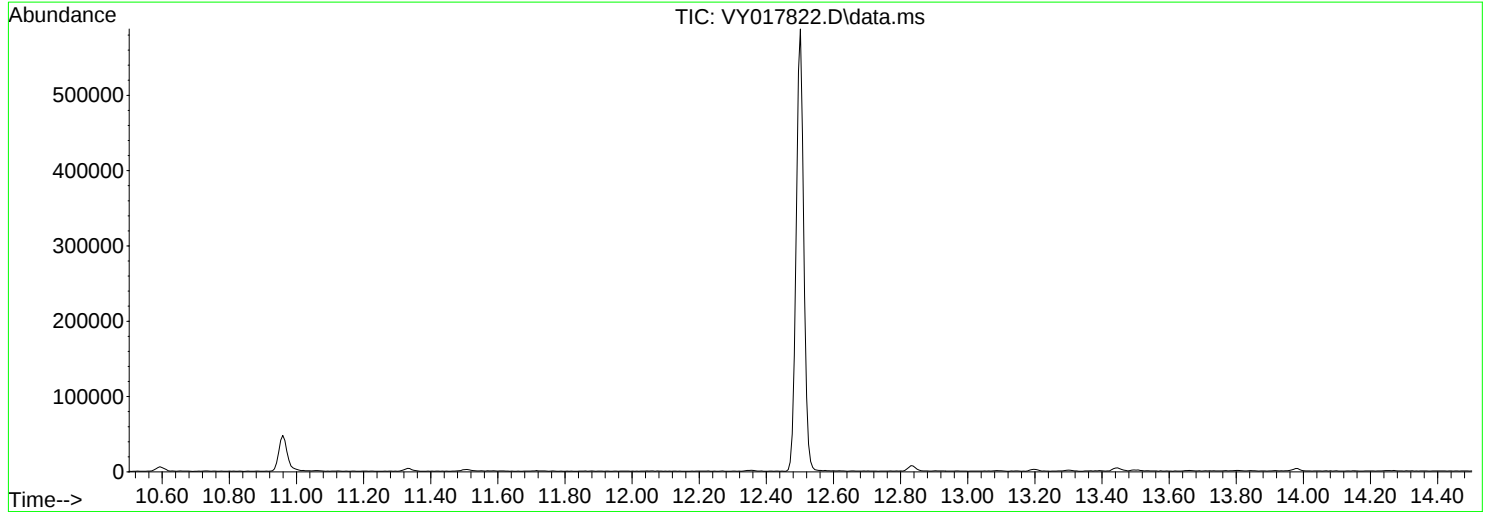

AutoFind: Scans 1751, 1752, 1753; Background Corrected with Scan 1743

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.1	17425	PASS
75	95	30	60	50.2	48408	PASS
95	95	100	100	100.0	96464	PASS
96	95	5	9	6.6	6366	PASS
173	174	0.00	2	1.4	1231	PASS
174	95	50	100	91.9	88613	PASS
175	174	5	9	7.6	6704	PASS
176	174	95	101	98.3	87144	PASS
177	176	5	9	6.4	5594	PASS