

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY040424\
 Data File : VY017848.D
 Acq On : 04 Apr 2024 12:48
 Operator : SY/MD
 Sample : P1974-07
 Misc : 5.09g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SOIL-3

Quant Time: Apr 05 00:45:55 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032924S.M
 Quant Title : SW846 8260
 QLast Update : Sat Mar 30 05:58:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.807	168	64351	50.000	ug/l	0.01
34) 1,4-Difluorobenzene	8.709	114	105735	50.000	ug/l	0.02
63) Chlorobenzene-d5	11.508	117	87858	50.000	ug/l	0.01
72) 1,4-Dichlorobenzene-d4	13.440	152	28899	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.155	65	32102	57.649	ug/l	0.01
Spiked Amount	50.000	Range	50 - 163	Recovery	=	115.300%
35) Dibromofluoromethane	7.734	113	35545	58.177	ug/l	0.02
Spiked Amount	50.000	Range	54 - 147	Recovery	=	116.360%
50) Toluene-d8	10.197	98	119993	52.576	ug/l	0.01
Spiked Amount	50.000	Range	58 - 134	Recovery	=	105.160%
62) 4-Bromofluorobenzene	12.495	95	28348	40.825	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	81.640%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY040424\
Data File : VY017848.D
Acq On : 04 Apr 2024 12:48
Operator : SY/MD
Sample : P1974-07
Misc : 5.09g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SOIL-3

Quant Time: Apr 05 00:45:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032924S.M
Quant Title : SW846 8260
QLast Update : Sat Mar 30 05:58:13 2024
Response via : Initial Calibration




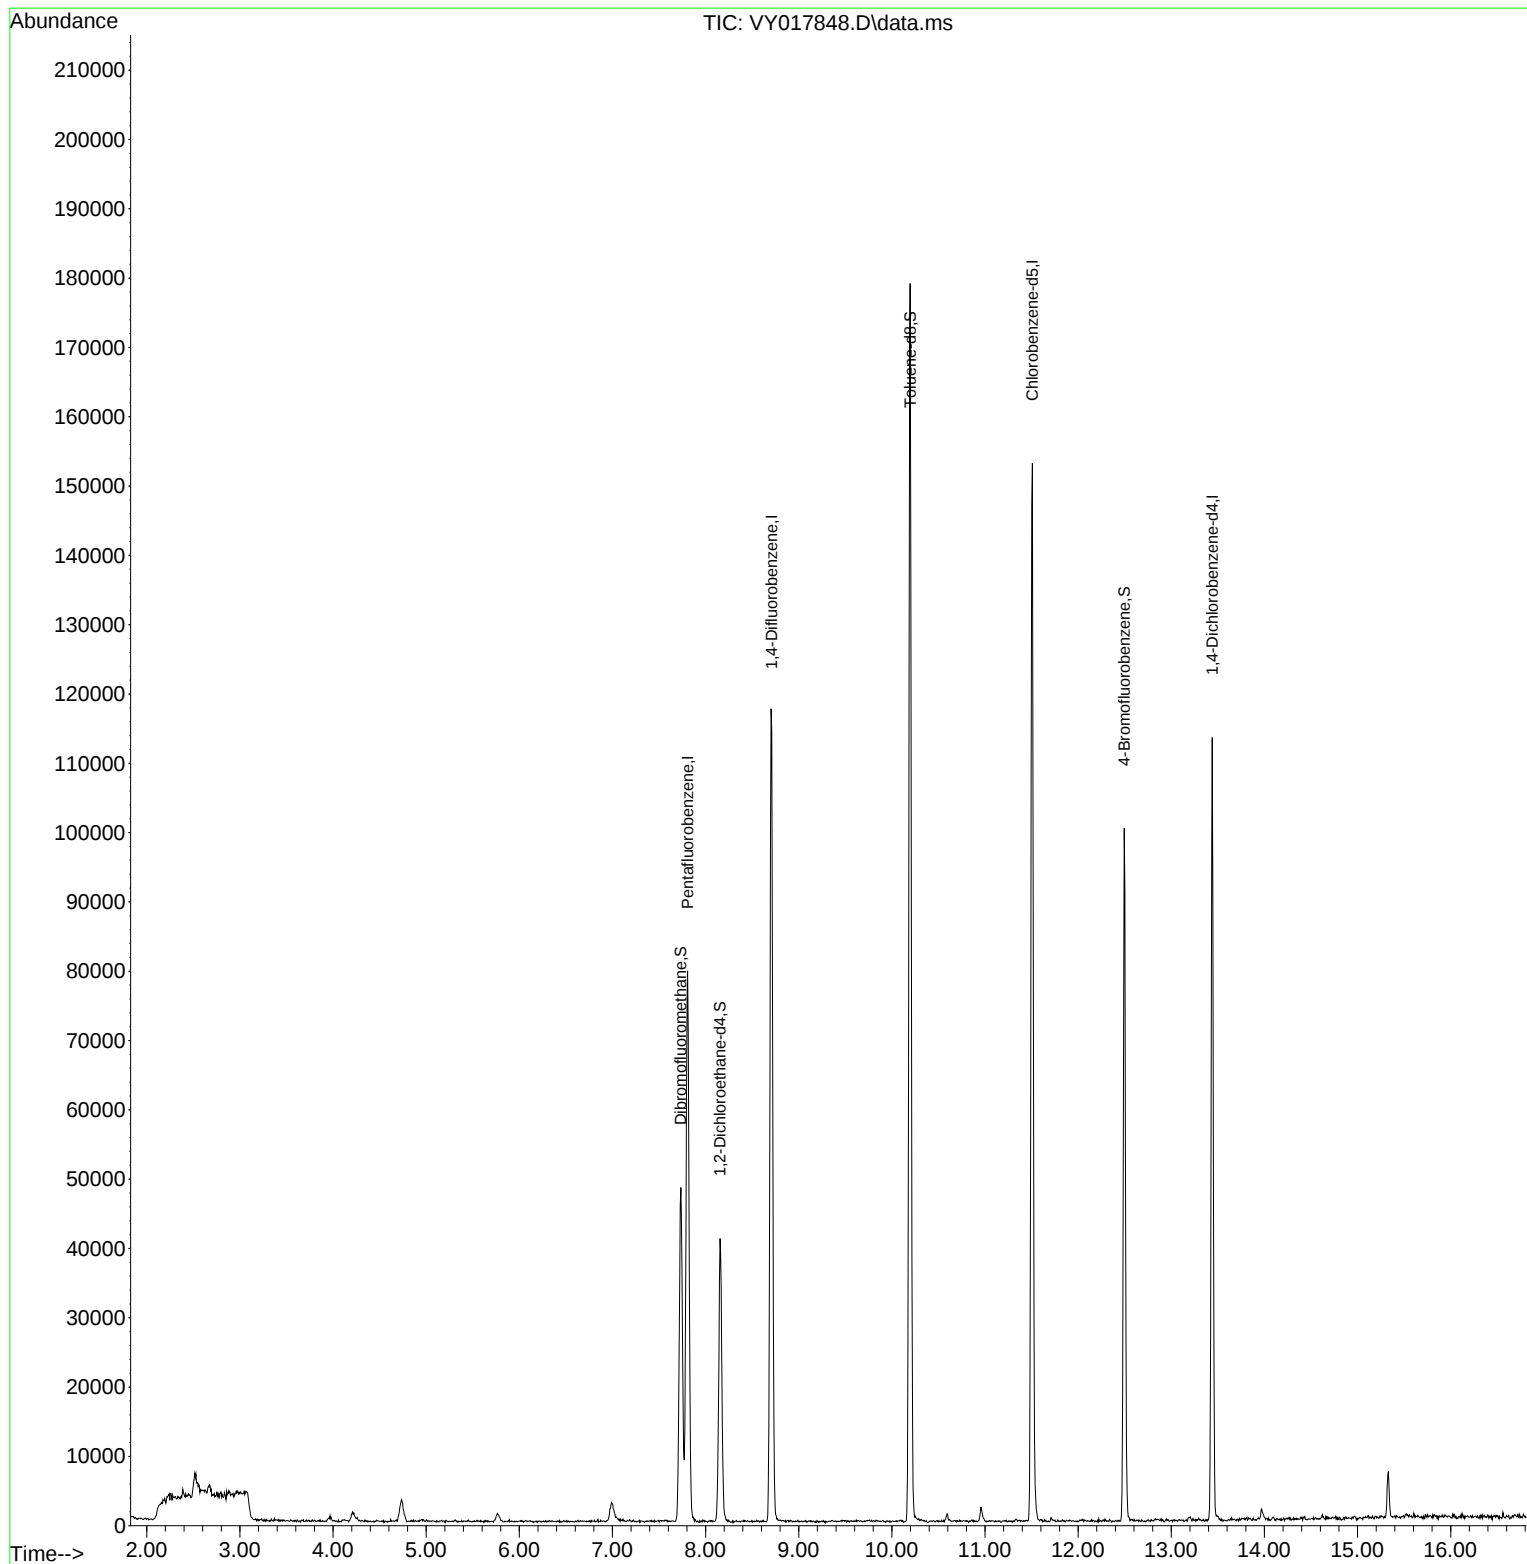




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.807 min Scan# 91
Delta R.T. 0.012 min
Lab File: VY017848.D
Acq: 04 Apr 2024 12:48




Instrument :
MSVOA_Y
ClientSampleId :
SOIL-3


Tgt Ion:168 Resp: 64351
Ion Ratio Lower Upper
168 100
99 47.1 39.1 58.7

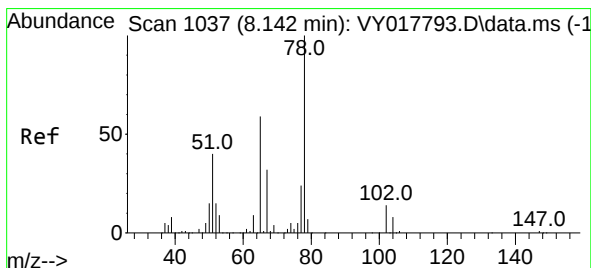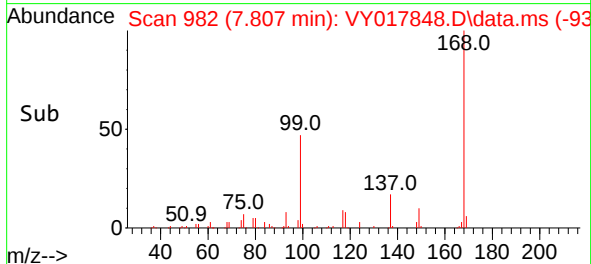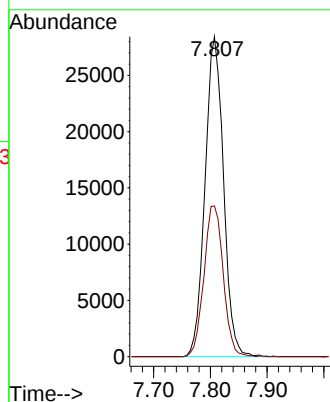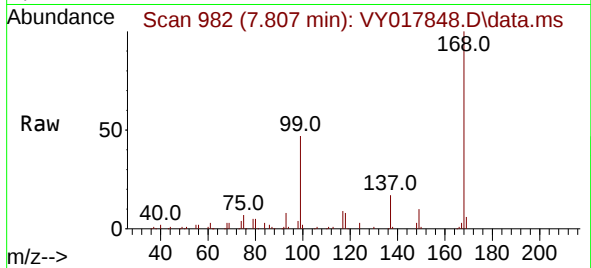

#33
1,2-Dichloroethane-d4
Concen: 57.649 ug/l
RT: 8.155 min Scan# 1039
Delta R.T. 0.012 min
Lab File: VY017848.D
Acq: 04 Apr 2024 12:48

Tgt Ion: 65 Resp: 32102
Ion Ratio Lower Upper
65 100
67 53.1 0.0 109.6

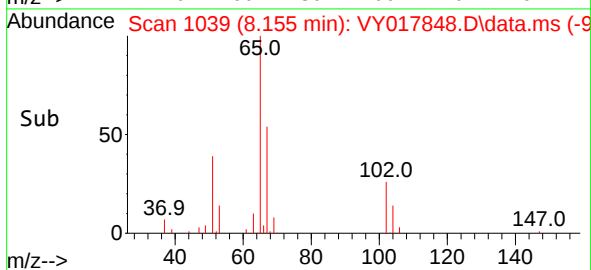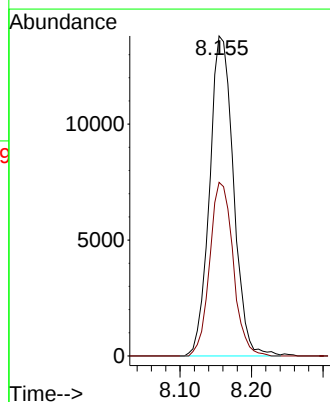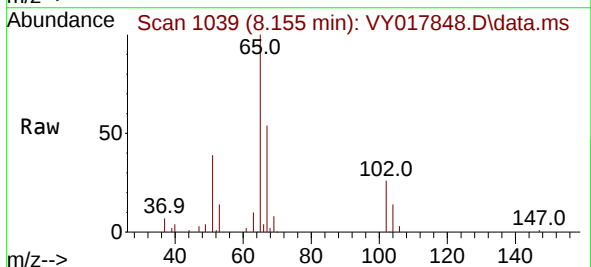

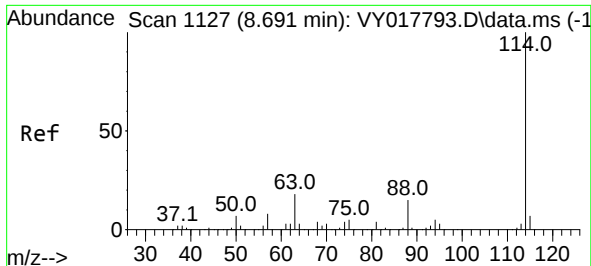

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.709 min Scan# 1127

Delta R.T. 0.018 min

Lab File: VY017848.D

Acq: 04 Apr 2024 12:48

Instrument :

MSVOA_Y

ClientSampleId :

SOIL-3





Tgt Ion:114 Resp: 105735

Ion Ratio Lower Upper

114 100

63 17.3 0.0 35.0

88 14.1 0.0 27.2

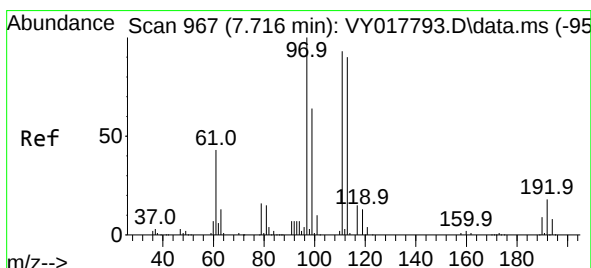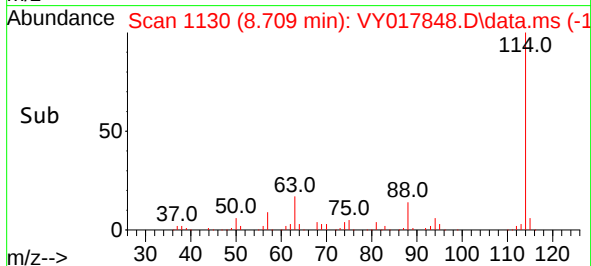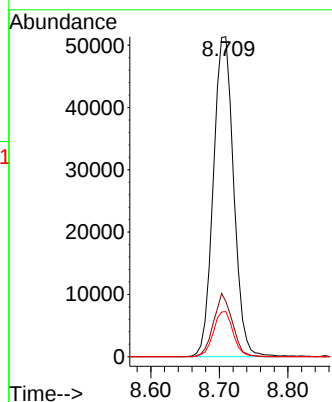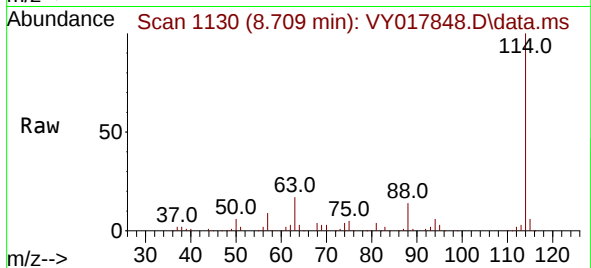

#35

Dibromofluoromethane

Concen: 58.177 ug/l

RT: 7.734 min Scan# 970

Delta R.T. 0.018 min

Lab File: VY017848.D

Acq: 04 Apr 2024 12:48




Tgt Ion:113 Resp: 35545


Ion Ratio Lower Upper

113 100

111 99.7 82.2 123.4

192 20.4 15.9 23.9


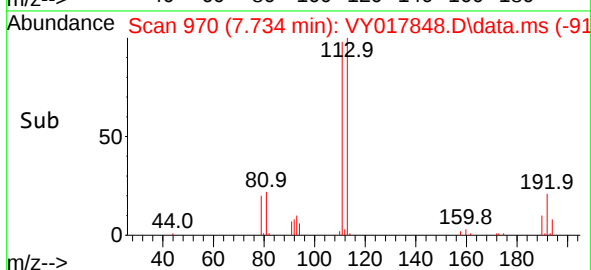
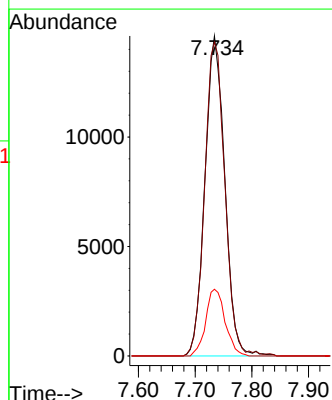
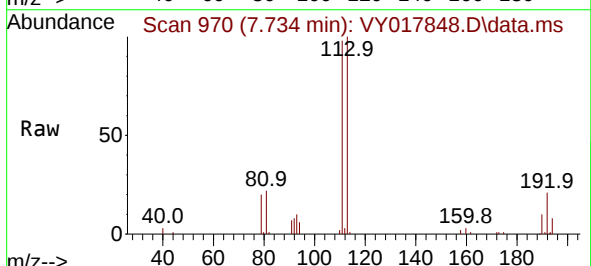


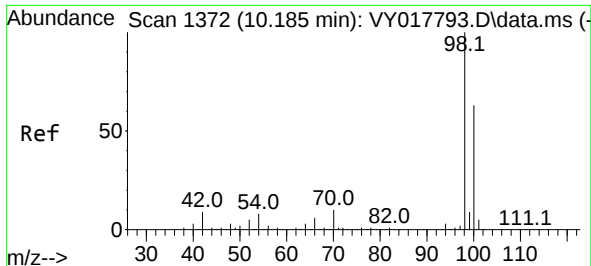

#50
Toluene-d8
Concen: 52.576 ug/l
RT: 10.197 min Scan# 11
Delta R.T. 0.012 min
Lab File: VY017848.D
Acq: 04 Apr 2024 12:48




Instrument :
MSVOA_Y
ClientSampleId :
SOIL-3


Tgt Ion: 98 Resp: 119993
Ion Ratio Lower Upper
98 100
100 64.7 52.0 78.0

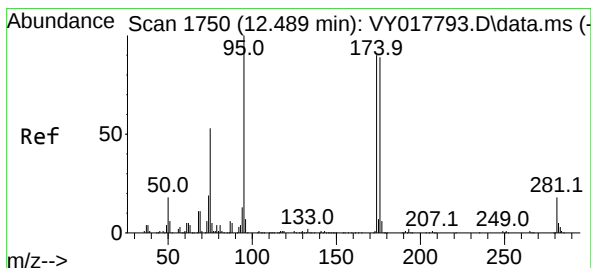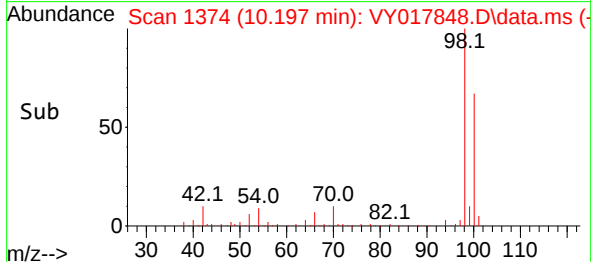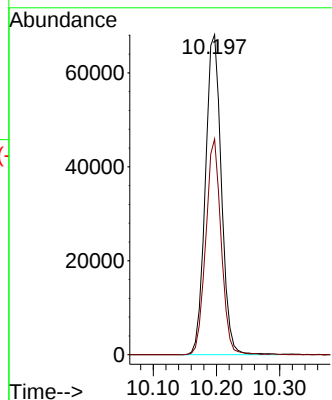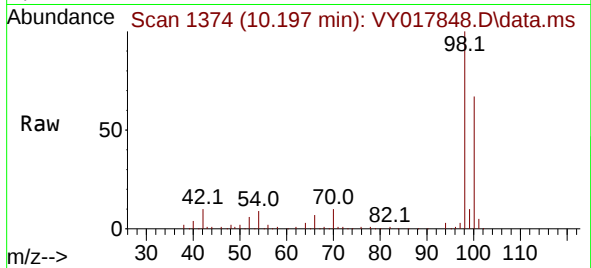

#62
4-Bromofluorobenzene
Concen: 40.825 ug/l
RT: 12.495 min Scan# 1751
Delta R.T. 0.006 min
Lab File: VY017848.D
Acq: 04 Apr 2024 12:48

Tgt Ion: 95 Resp: 28348
Ion Ratio Lower Upper
95 100
174 92.2 0.0 175.6
176 86.6 0.0 171.4


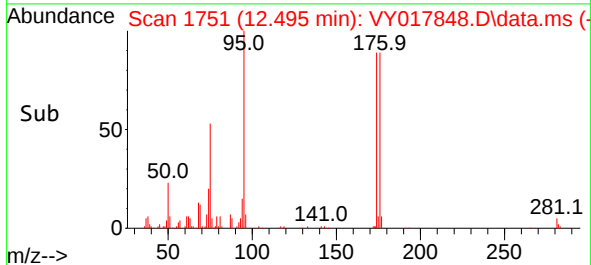
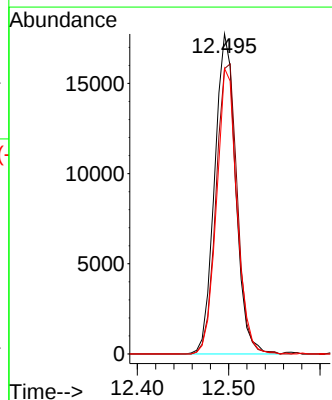
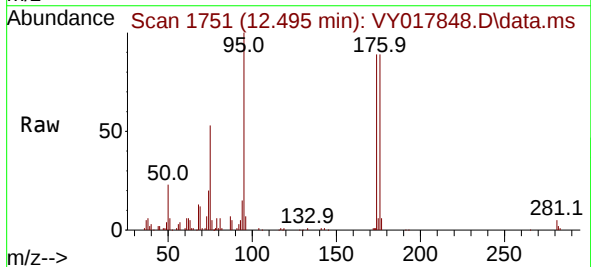


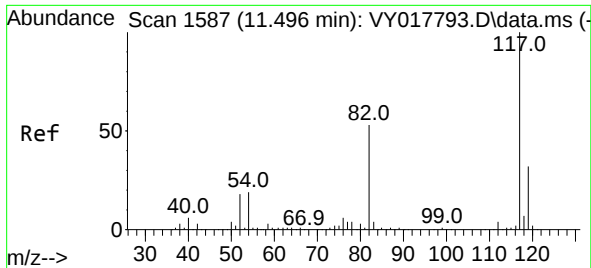

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.508 min Scan# 11
Delta R.T. 0.012 min
Lab File: VY017848.D
Acq: 04 Apr 2024 12:48

Instrument :
MSVOA_Y
ClientSampleId :
SOIL-3

Tgt Ion:117 Resp: 87858
Ion Ratio Lower Upper
117 100
82 52.0 42.4 63.6
119 33.7 25.9 38.9

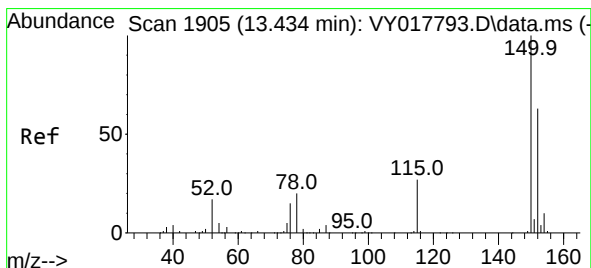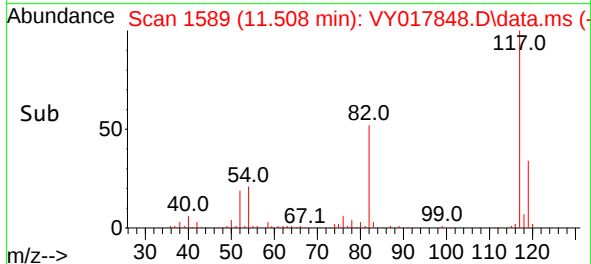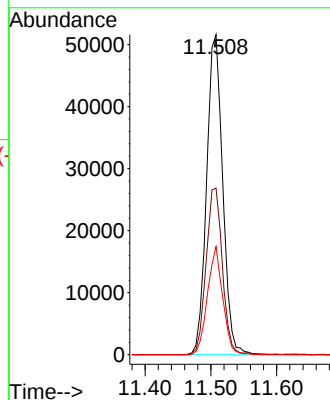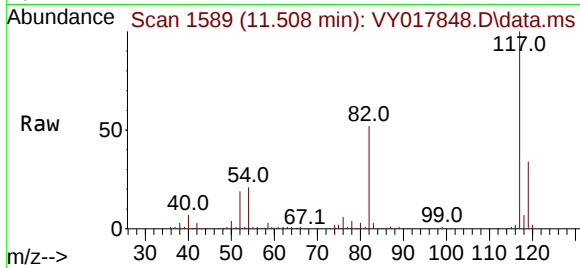

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.440 min Scan# 1906
Delta R.T. 0.006 min
Lab File: VY017848.D
Acq: 04 Apr 2024 12:48

Tgt Ion:152 Resp: 28899
Ion Ratio Lower Upper
152 100
115 54.1 28.2 84.7
150 158.8 0.0 345.6

