

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY040620\
 Data File : VY002237.D
 Acq On : 06 Apr 2020 15:16
 Operator : SY/MD
 Sample : L2172-02
 Misc : 5.09G/5ML/MSVOA Y/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 CC-1A

Quant Time: Apr 07 05:15:01 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y032620S.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 27 07:11:05 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.80	168	132429	50.00	ug/l	-0.01
34) 1,4-Difluorobenzene	8.69	114	263008	50.00	ug/l	-0.01
63) Chlorobenzene-d5	11.49	117	247435	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.42	152	112500	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.15	65	82229	56.17	ug/l	-0.01
Spiked Amount 50.000			Recovery	=	112.34%	
35) Dibromofluoromethane	7.73	113	78393	53.20	ug/l	0.00
Spiked Amount 50.000			Recovery	=	106.40%	
50) Toluene-d8	10.18	98	325543	53.18	ug/l	0.00
Spiked Amount 50.000			Recovery	=	106.36%	
62) 4-Bromofluorobenzene	12.49	95	115113	53.76	ug/l	0.00
Spiked Amount 50.000			Recovery	=	107.52%	
Target Compounds						
16) Acetone	3.96	43	3213	7.812	ug/l	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY040620\
Data File : VY002237.D
Acq On : 06 Apr 2020 15:16
Operator : SY/MD
Sample : L2172-02
Misc : 5.09G/5ML/MSVOA Y/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
CC-1A

Quant Time: Apr 07 05:15:01 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y032620S.M
Quant Title : SW846 8260
QLast Update : Fri Mar 27 07:11:05 2020
Response via : Initial Calibration

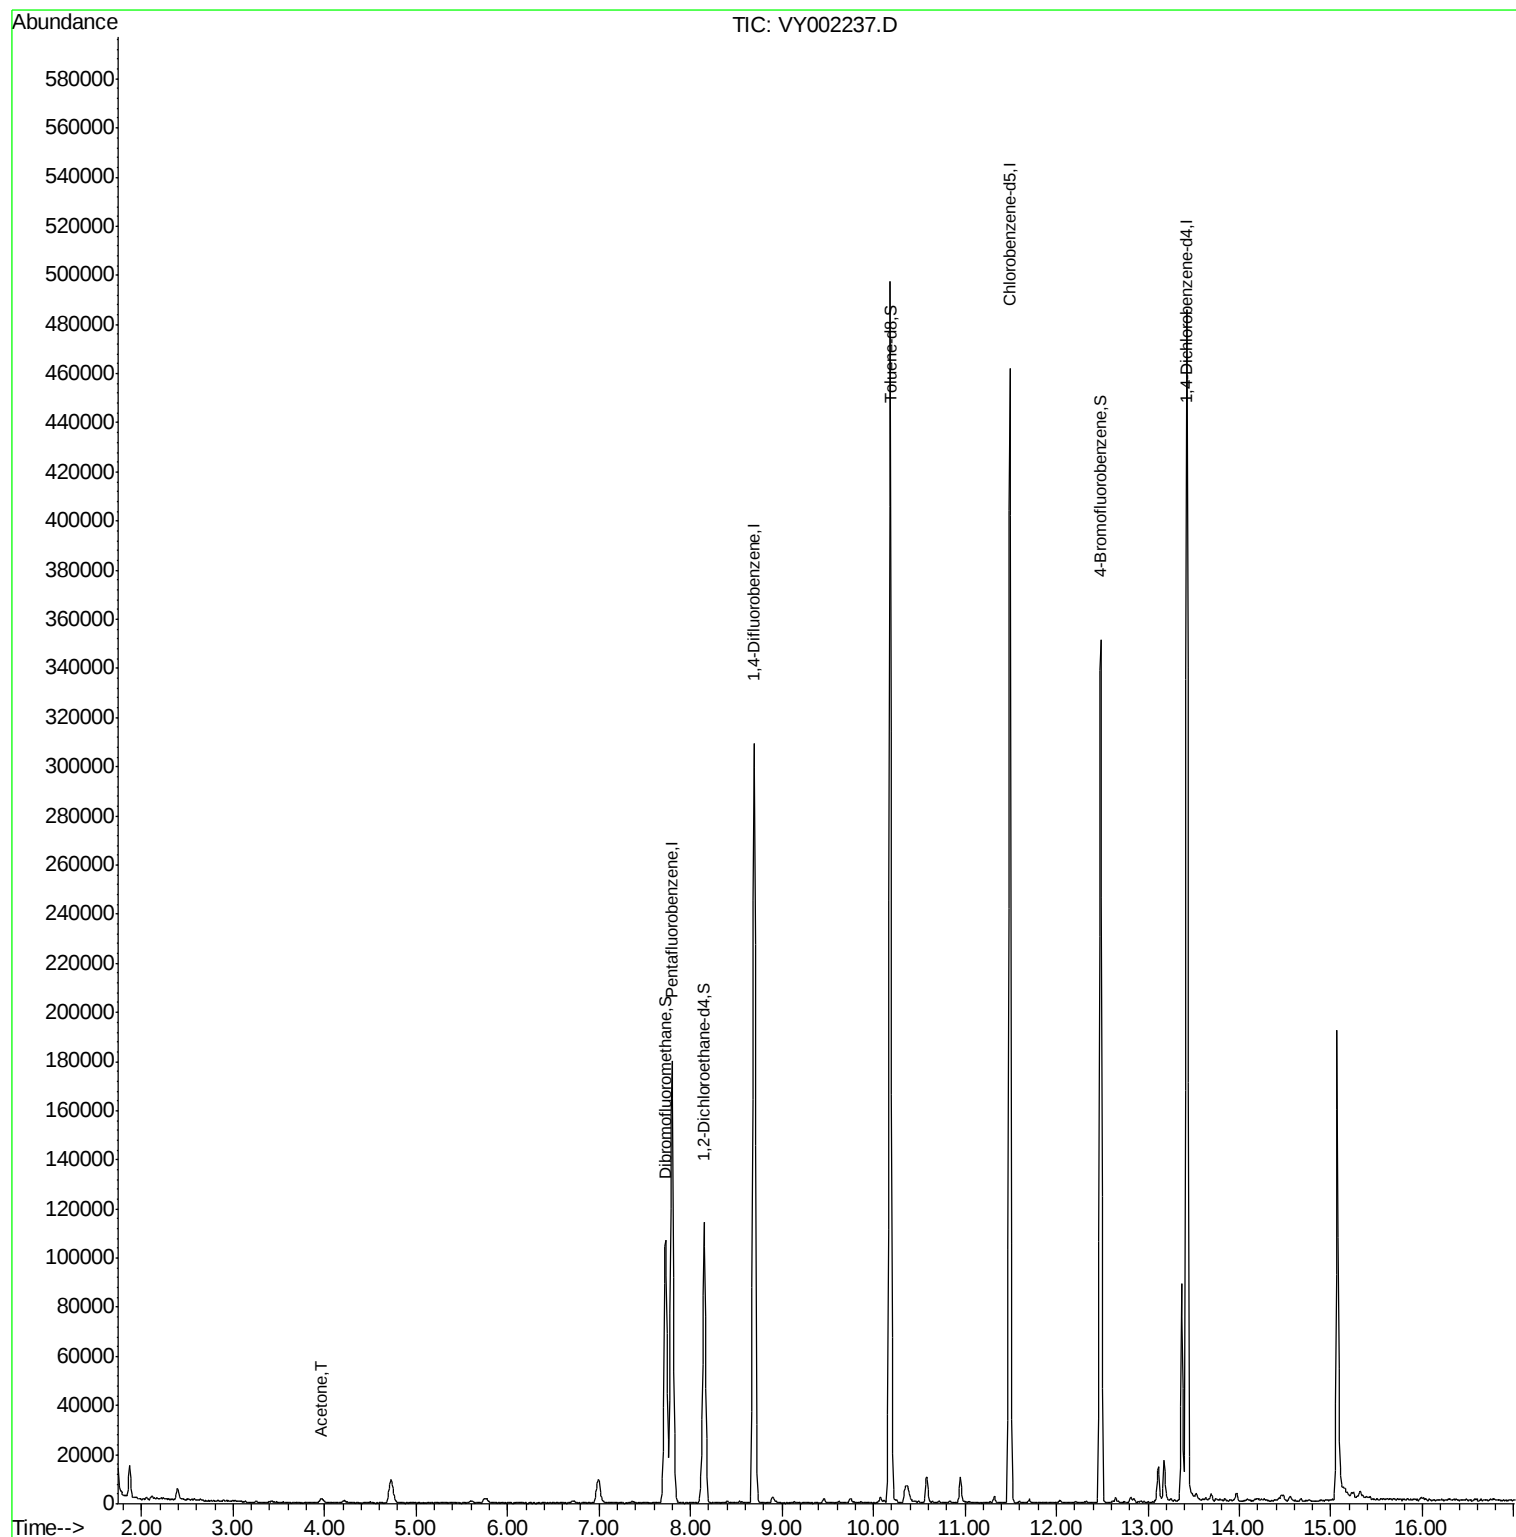

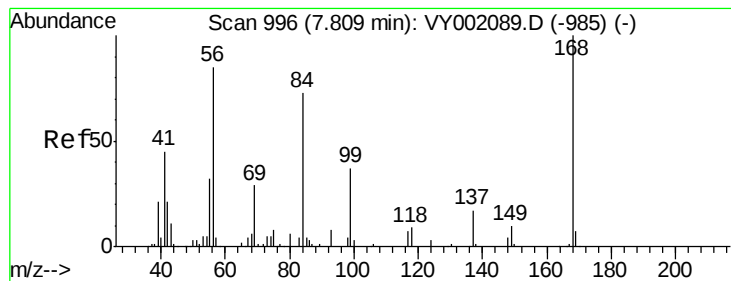

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.80 min Scan# 994

Delta R.T. -0.01 min

Lab File: VY002237.D

Acq: 06 Apr 2020 15:16

Instrument :

MSVOA_Y

ClientSampleId :


CC-1A

Tot Ion:168 Resp: 132429




Ion Ratio Lower Upper

168 100

99 60.9 47.6 71.4

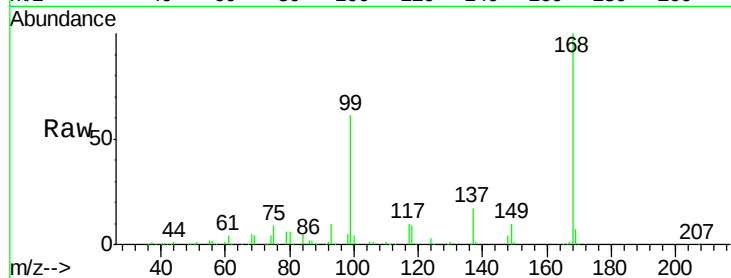

Abundance Ion 167.90 (167.60 to 168.60): VY002237.D (-947) (-)

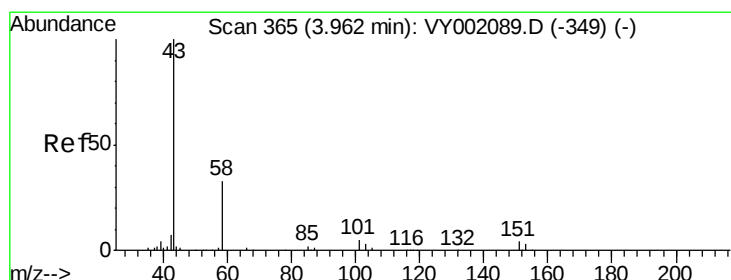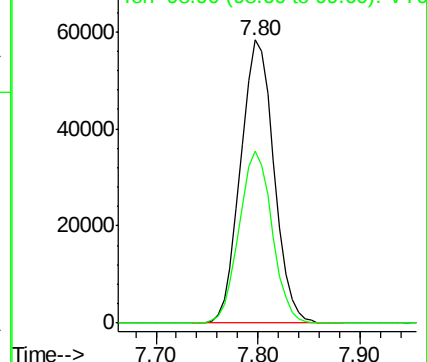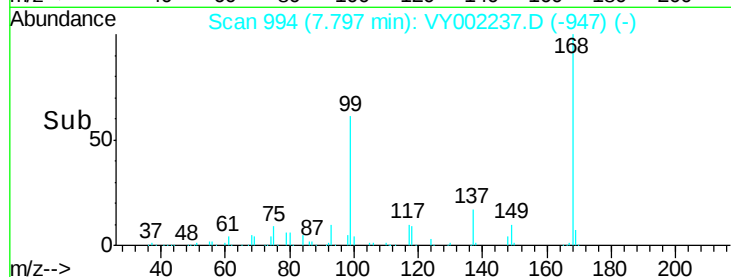

#16

Acetone

Concen: 7.812 ug/l

RT: 3.96 min Scan# 364

Delta R.T. -0.01 min

Lab File: VY002237.D


Acq: 06 Apr 2020 15:16

Tgt Ion: 43 Resp: 3213



Ion Ratio Lower Upper


43 100

58 26.9 26.3 39.5

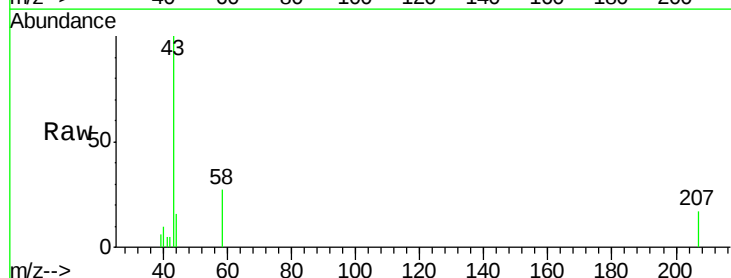

Abundance Ion 43.00 (42.70 to 43.70): VY002237.D (-316) (-)

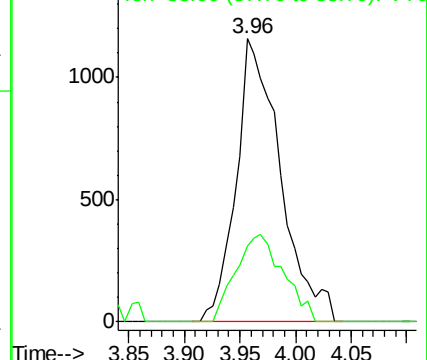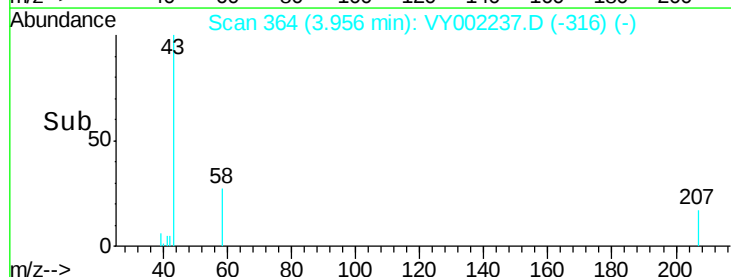

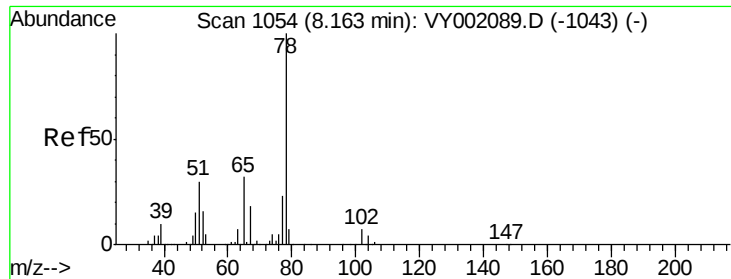

#33

1,2-Dichloroethane-d4

Concen: 56.169 ug/l

RT: 8.15 min Scan# 1052

Delta R.T. -0.01 min

Lab File: VY002237.D

Acq: 06 Apr 2020 15:16

Instrument :

MSVOA_Y

ClientSampleId :


CC-1A

Tot Ion: 65 Resp: 82229

Ion Ratio Lower Upper




65 100

67 55.0 0.0 112.8

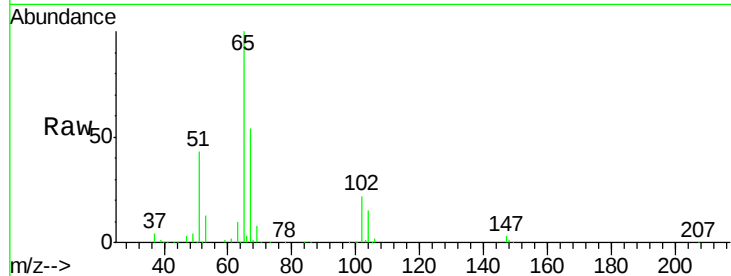

Abundance Ion 64.90 (64.60 to 65.60): VY0

Ion 66.90 (66.60 to 67.60): VY0

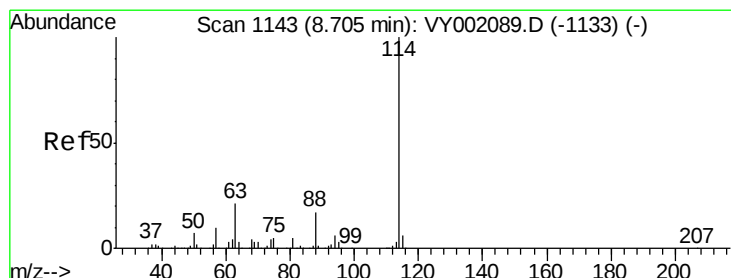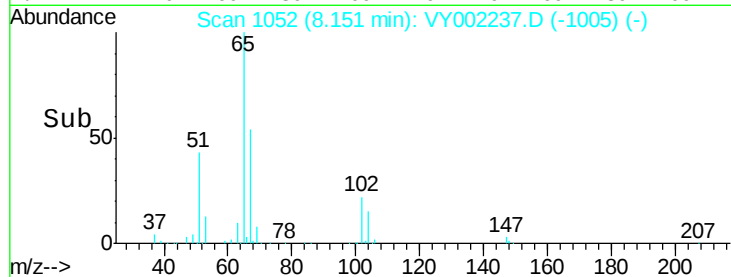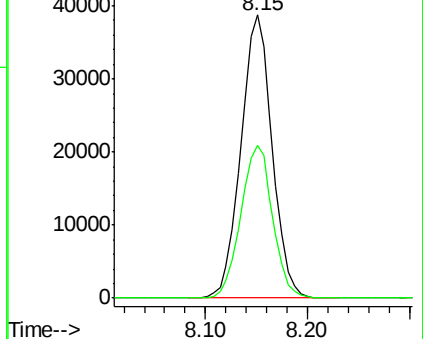

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.69 min Scan# 1141

Delta R.T. -0.01 min

Lab File: VY002237.D

Acq: 06 Apr 2020 15:16


Tgt Ion: 114 Resp: 263008

Ion Ratio Lower Upper

114 100

63 20.6 0.0 41.4



88 15.5 0.0 33.0

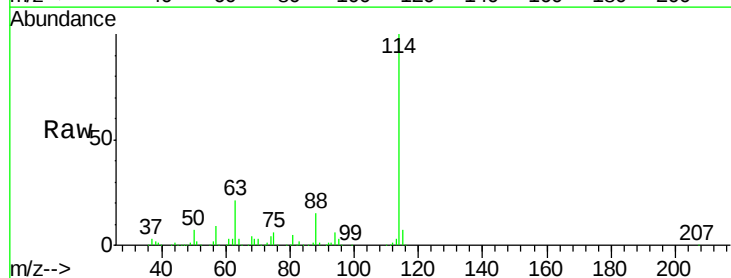


Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VY0

Ion 87.90 (87.60 to 88.60): VY0

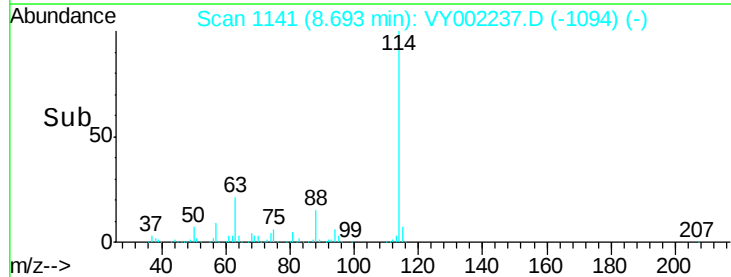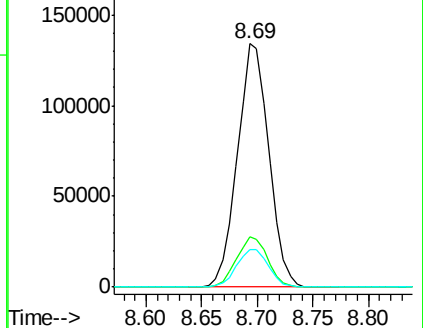

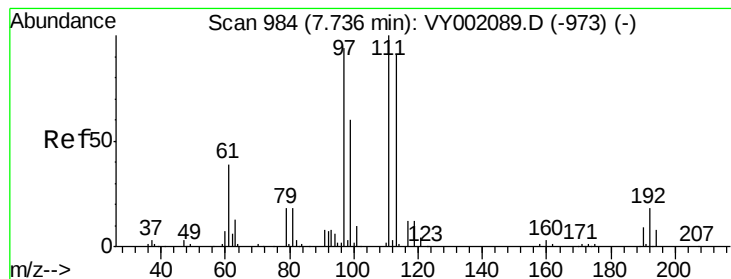

#35

Dibromofluoromethane

Concen: 53.196 ug/l

RT: 7.73 min Scan# 983

Delta R.T. -0.01 min

Lab File: VY002237.D

Acq: 06 Apr 2020 15:16

Instrument :

MSVOA_Y

ClientSampleId :

CC-1A


Tot Ion:113 Resp: 78393

Ion Ratio Lower Upper

113 100

111 102.3 84.4 126.6




192 17.1 14.6 21.8

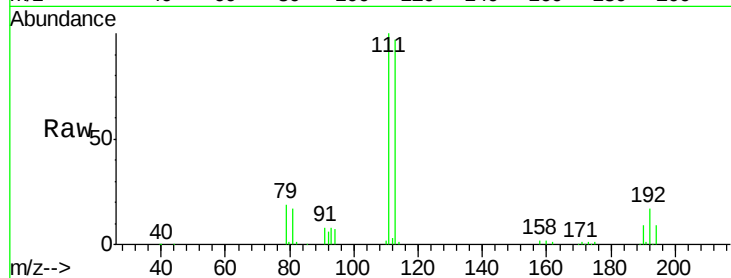

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

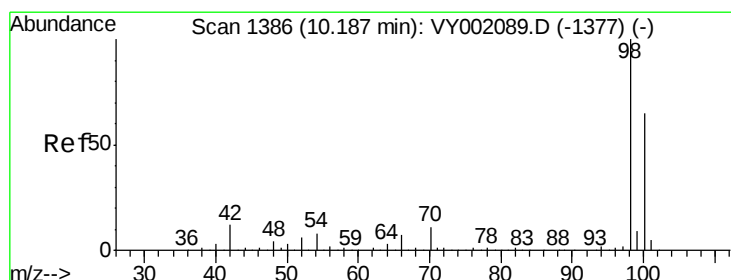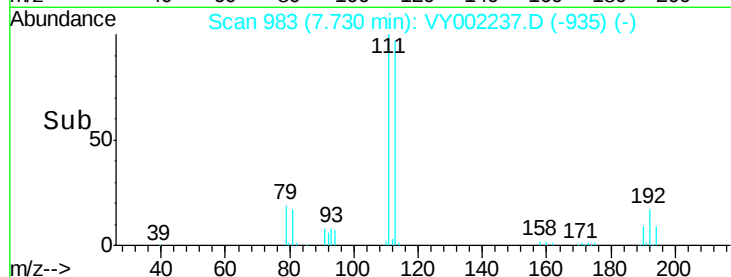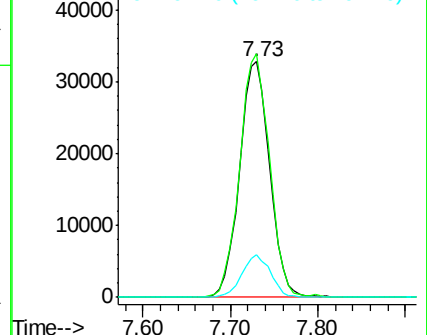

#50

Toluene-d8

Concen: 53.176 ug/l

RT: 10.18 min Scan# 1385

Delta R.T. -0.01 min

Lab File: VY002237.D


Acq: 06 Apr 2020 15:16

Tgt Ion: 98 Resp: 325543

Ion Ratio Lower Upper



98 100


100 65.4 51.6 77.4

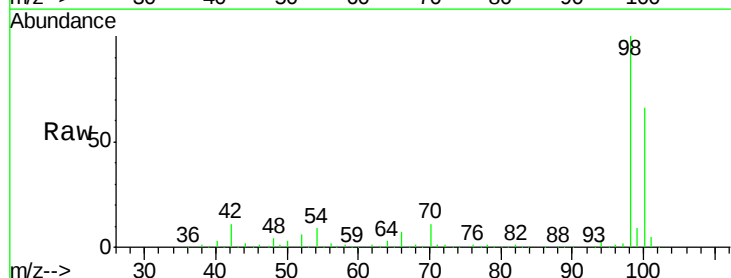

Abundance Ion 98.00 (97.70 to 98.70): VY0

Ion 100.00 (99.70 to 100.70): VY



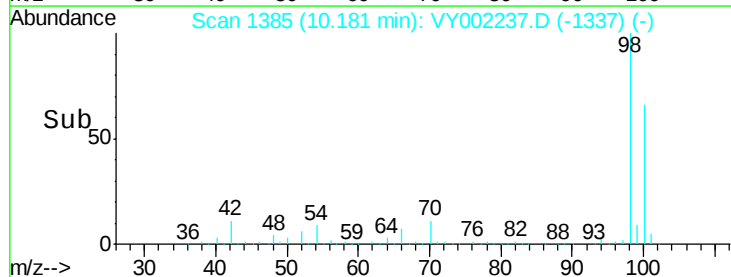
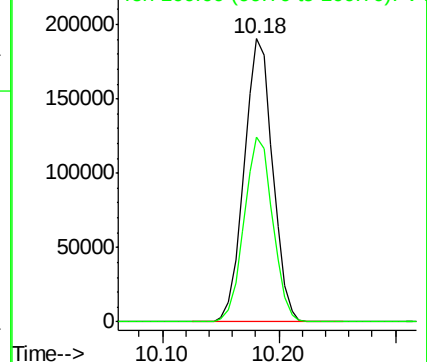


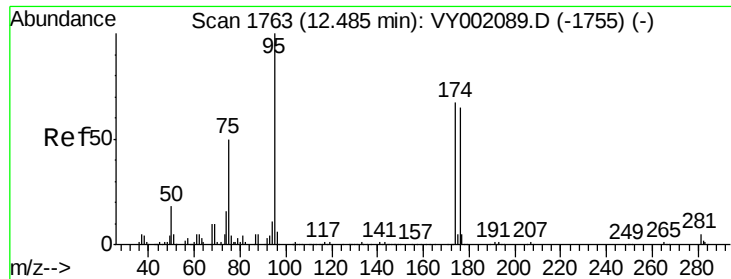

#62
4-Bromofluorobenzene
Concen: 53.764 ug/l
RT: 12.49 min Scan# 1763
Delta R.T. 0.00 min
Lab File: VY002237.D
Acq: 06 Apr 2020 15:16




Instrument :
MSVOA_Y
ClientSampleId :
CC-1A


Tot Ion	Ratio	Lower	Upper
95	100		
174	72.7	0.0	143.4
176	68.4	0.0	137.0

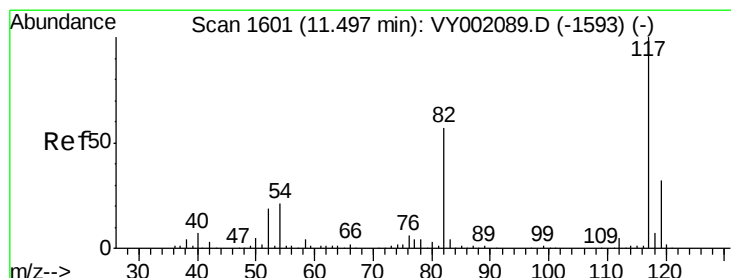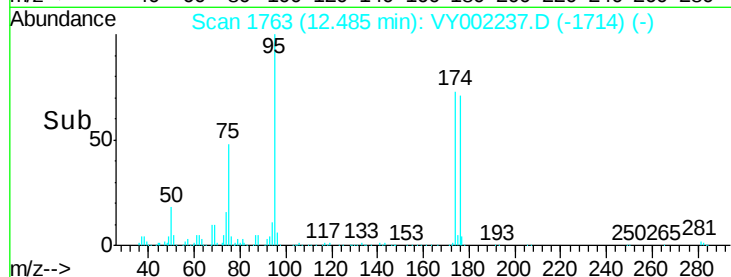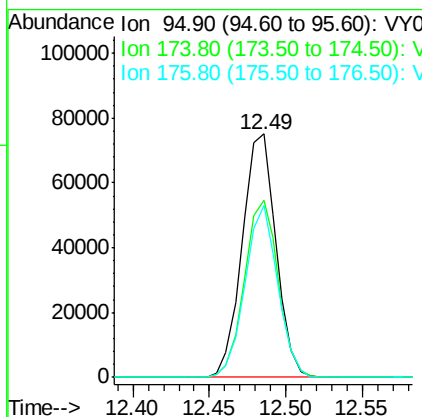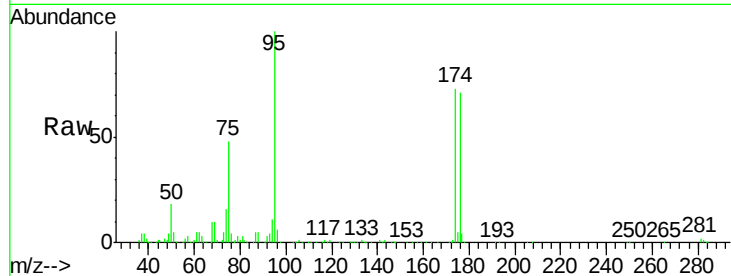

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.49 min Scan# 1600
Delta R.T. -0.01 min
Lab File: VY002237.D
Acq: 06 Apr 2020 15:16

Tgt Ion	Ratio	Lower	Upper
117	100		
82	56.2	45.4	68.2
119	32.2	25.3	37.9

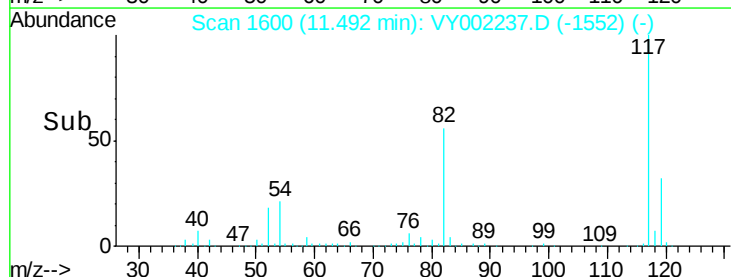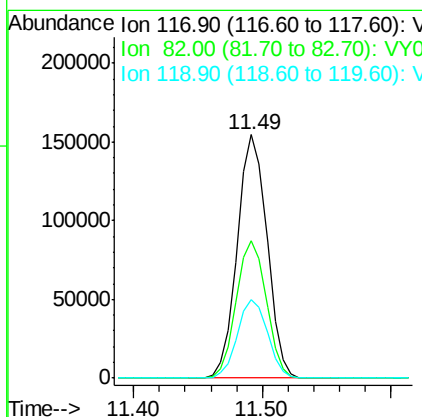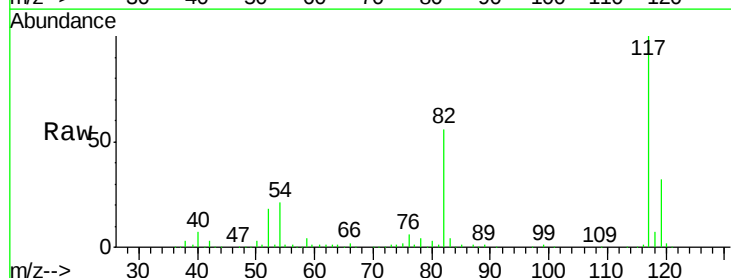

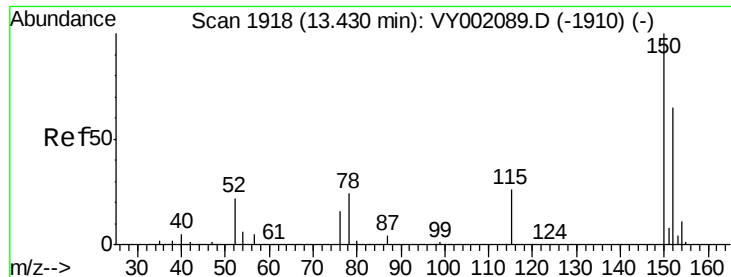


#72

1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.42 min Scan# 1917
 Delta R.T. -0.01 min
 Lab File: VY002237.D
 Acq: 06 Apr 2020 15:16

Instrument :
 MSVOA_Y
 ClientSampleId :
 CC-1A

Tot Ion	Ratio	Lower	Upper
152	100		
115	62.2	31.2	93.6
150	157.8	0.0	354.8

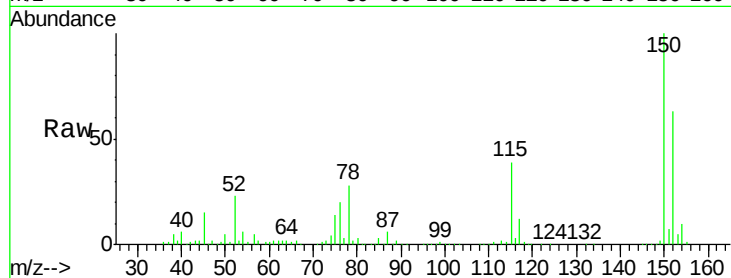

Abundance Ion 151.90 (151.60 to 152.60): V
 Ion 114.90 (114.60 to 115.60): V
 Ion 149.90 (149.60 to 150.60): V

