

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY040621\
 Data File : VY004290.D
 Acq On : 06 Apr 2021 09:52
 Operator : SY/MD
 Sample : VY0406SBL01
 Misc : 5.00g/5mL/MSVOA_Y/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0406SBL01

Quant Time: Apr 07 00:56:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032921S.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 30 06:38:14 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.795	168	191135	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	328233	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.496	117	298881	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	130476	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	113382	61.71	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 123.42%	
35) Dibromofluoromethane	7.728	113	100343	54.87	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 109.74%	
50) Toluene-d8	10.185	98	401642	58.39	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 116.78%	
62) 4-Bromofluorobenzene	12.483	95	130544	55.37	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 110.74%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY040621\
Data File : VY004290.D
Acq On : 06 Apr 2021 09:52
Operator : SY/MD
Sample : VY0406SBL01
Misc : 5.00g/5mL/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0406SBL01

Quant Time: Apr 07 00:56:09 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032921S.M
Quant Title : SW846 8260
QLast Update : Tue Mar 30 06:38:14 2021
Response via : Initial Calibration




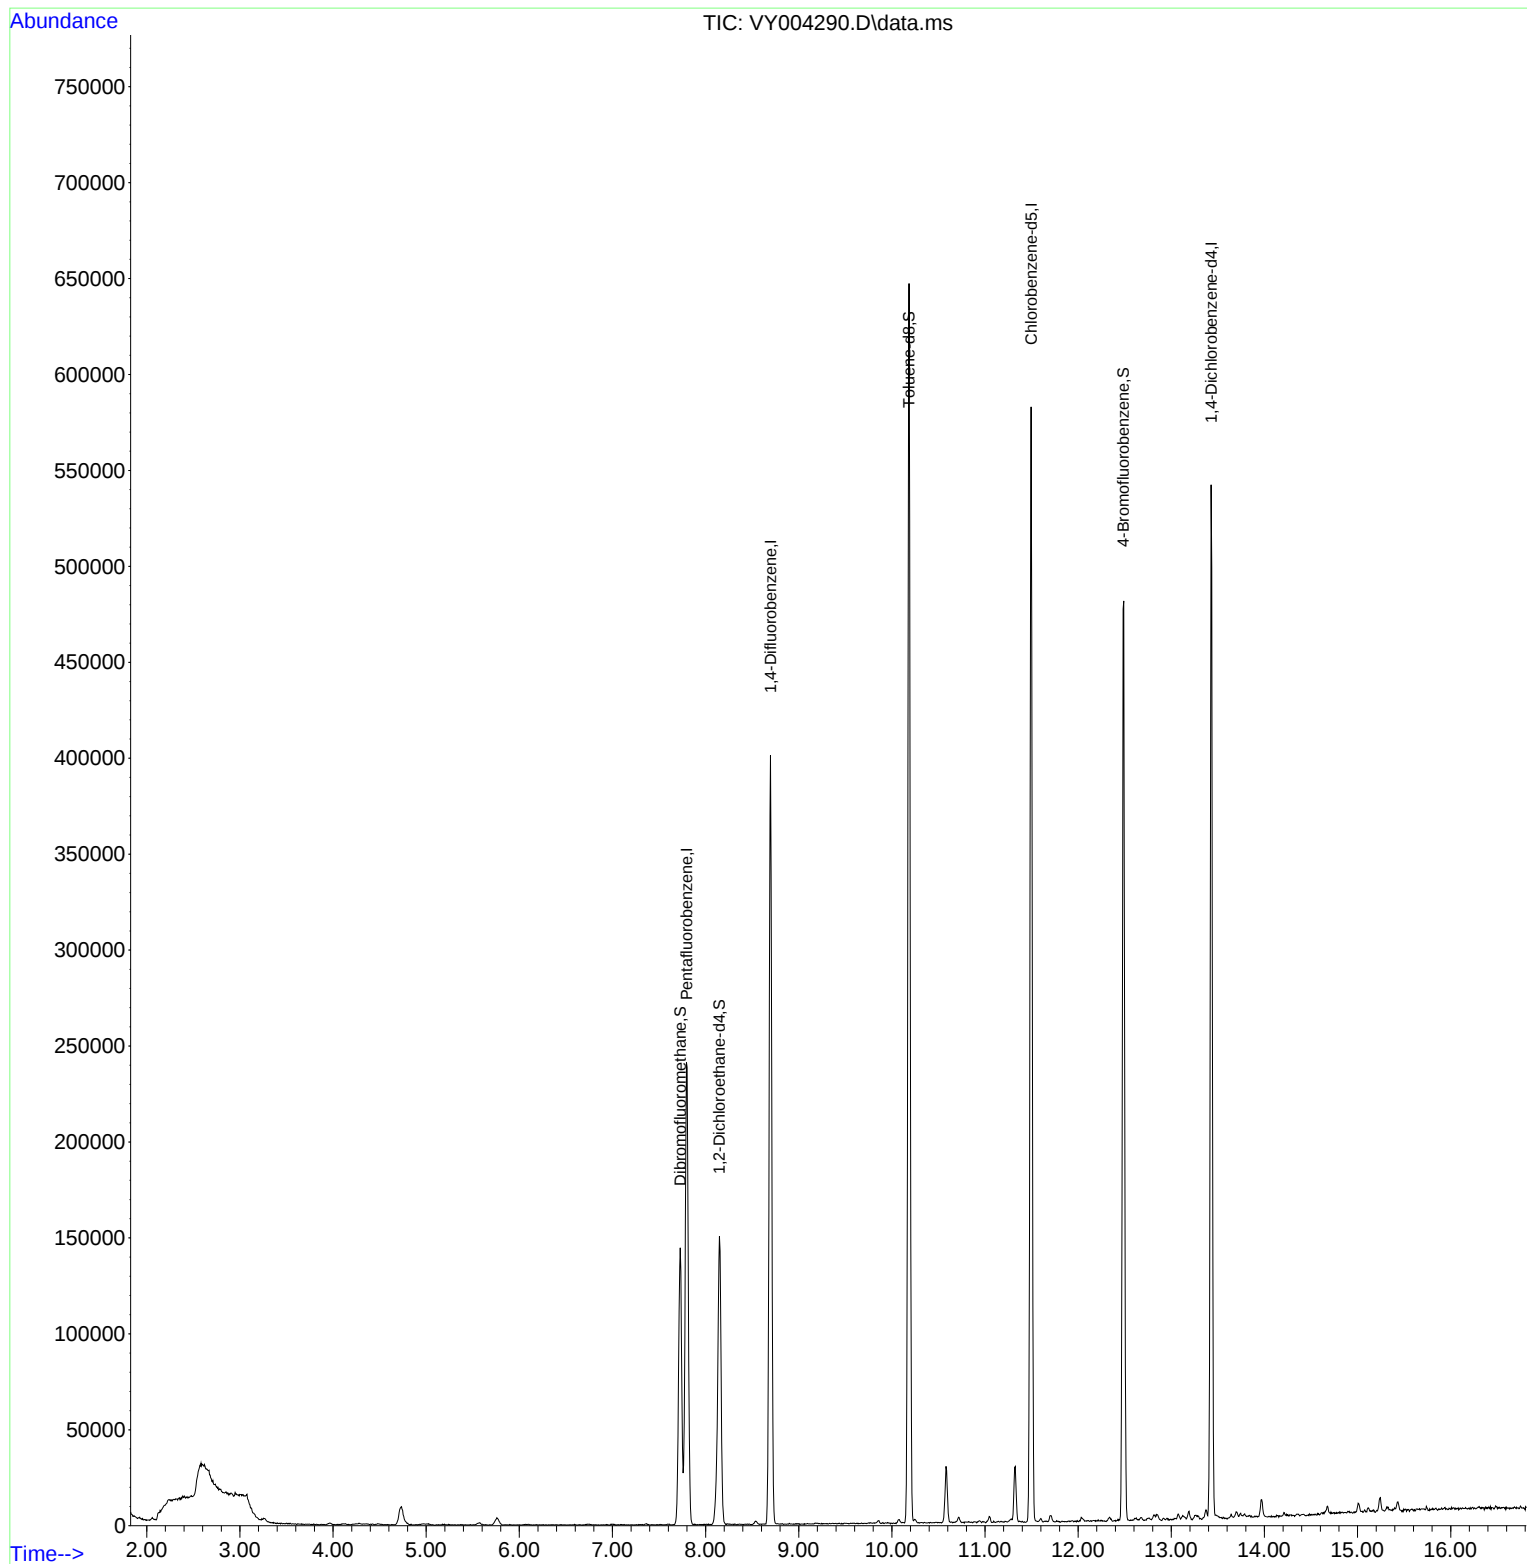


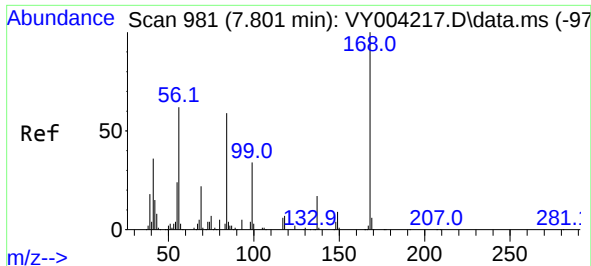

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.795 min Scan# 980
Delta R.T. -0.006 min
Lab File: VY004290.D
Acq: 06 Apr 2021 09:52




Instrument :
MSVOA_Y
ClientSampleId :
VY0406SBL01


Tgt Ion:168 Resp: 191135
Ion Ratio Lower Upper
168 100
99 54.5 42.6 64.0

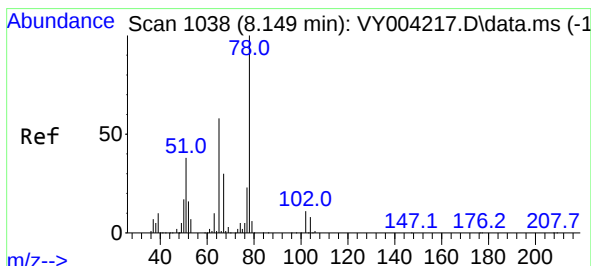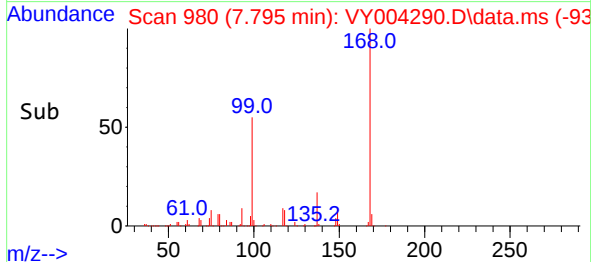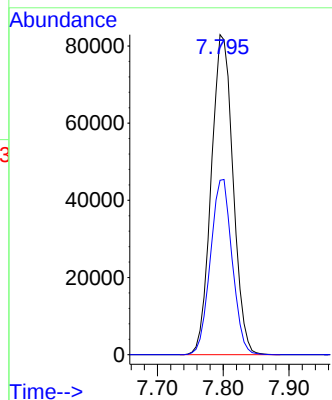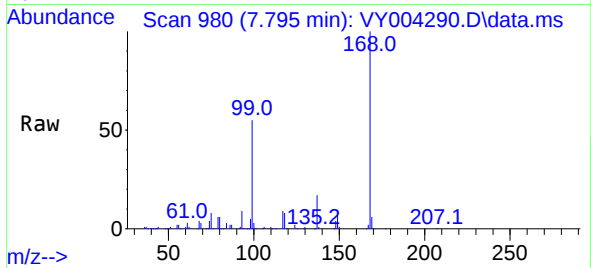

#33
1,2-Dichloroethane-d4
Concen: 61.71 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. -0.000 min
Lab File: VY004290.D
Acq: 06 Apr 2021 09:52

Tgt Ion: 65 Resp: 113382
Ion Ratio Lower Upper
65 100
67 52.1 0.0 103.2

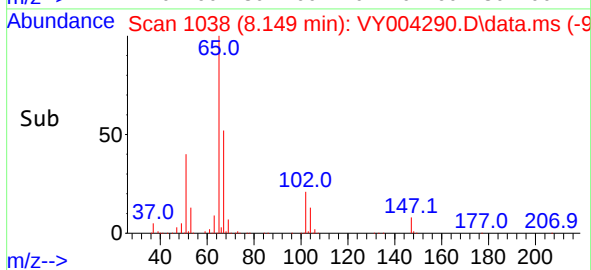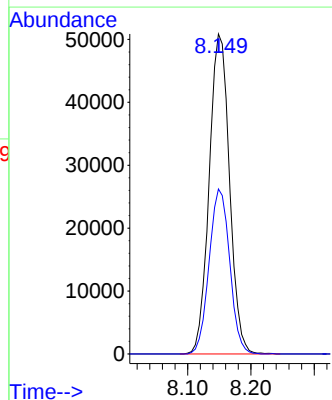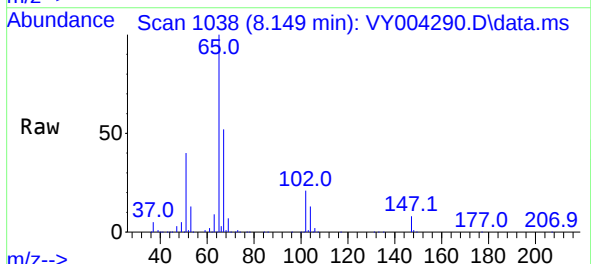




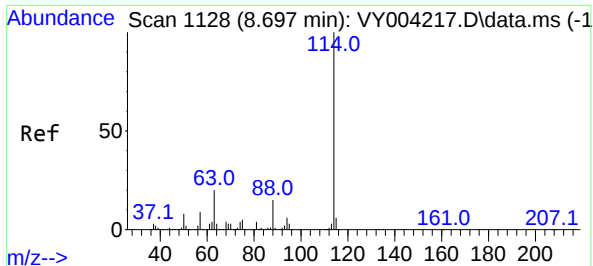


#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. 0.000 min
Lab File: VY004290.D
Acq: 06 Apr 2021 09:52

Instrument :
MSVOA_Y
ClientSampleId :
VY0406SBL01

Tgt Ion:114 Resp: 328233




Ion	Ratio	Lower	Upper
114	100		
63	20.1	0.0	40.4
88	15.7	0.0	30.8

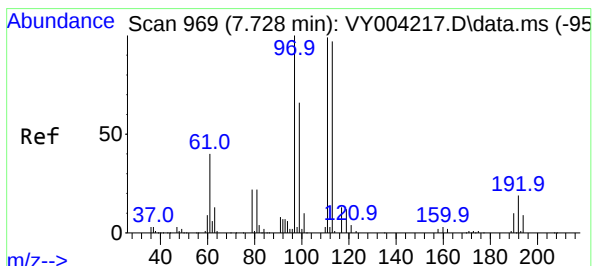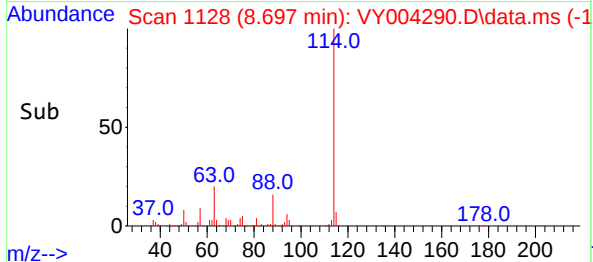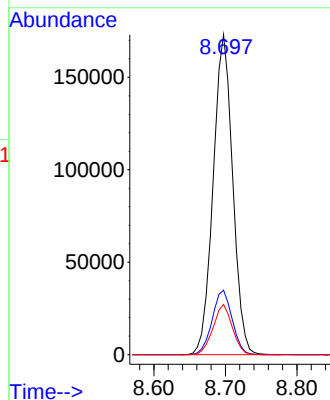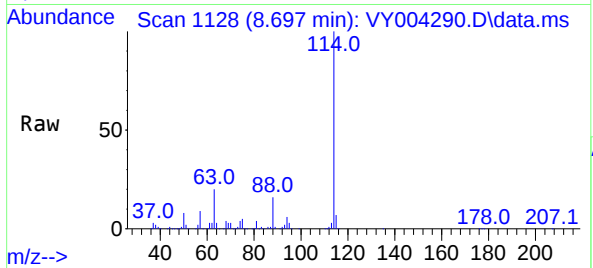


#35
Dibromofluoromethane
Concen: 54.87 ug/l
RT: 7.728 min Scan# 969
Delta R.T. -0.000 min
Lab File: VY004290.D
Acq: 06 Apr 2021 09:52

Tgt Ion:113 Resp: 100343

Ion	Ratio	Lower	Upper
113	100		
111	102.2	82.6	124.0
192	19.8	16.4	24.6


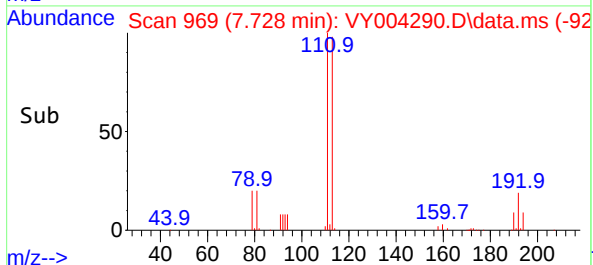
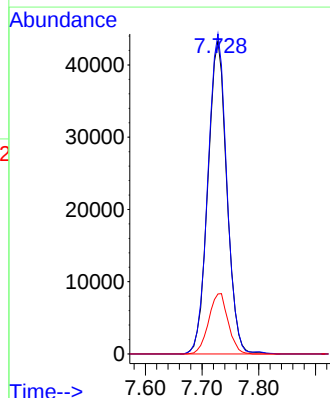
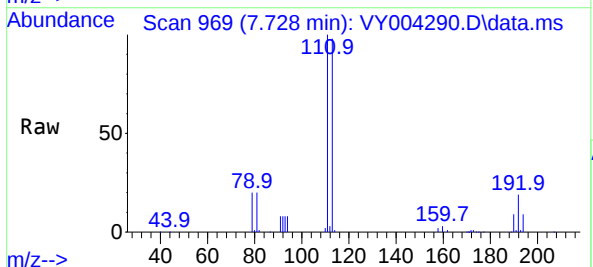


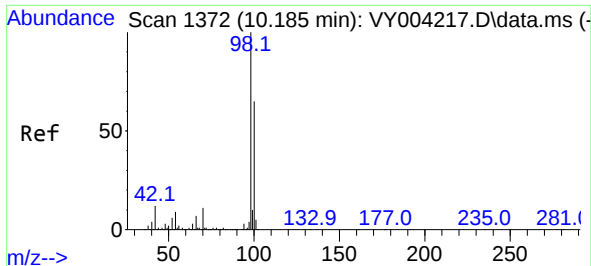

#50
Toluene-d8
Concen: 58.39 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. -0.000 min
Lab File: VY004290.D
Acq: 06 Apr 2021 09:52




Instrument :
MSVOA_Y
ClientSampleId :
VY0406SBL01


Tgt Ion: 98 Resp: 401642
Ion Ratio Lower Upper
98 100
100 64.7 52.5 78.7

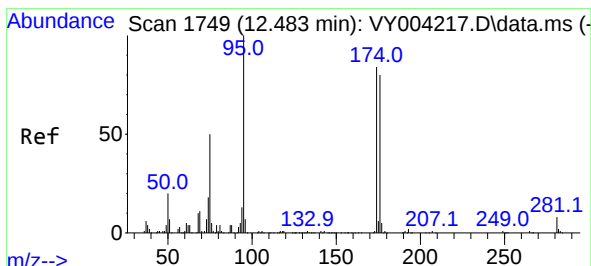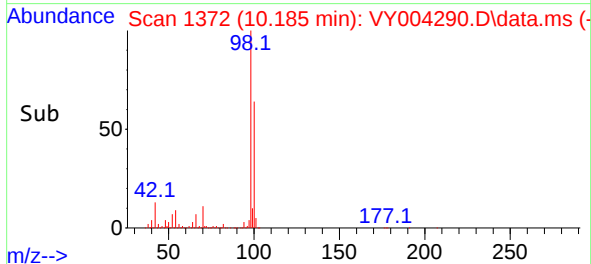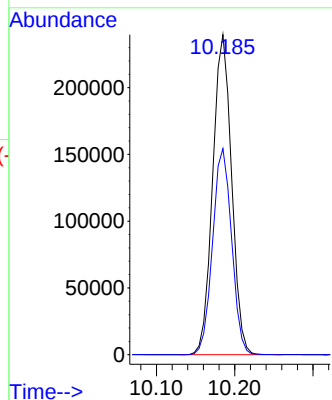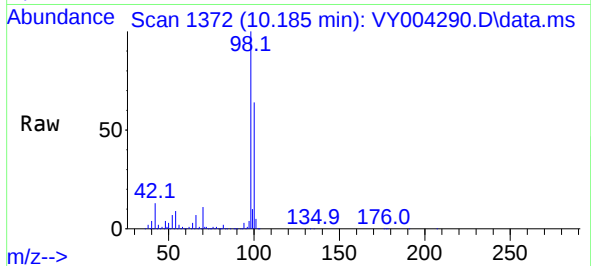

#62
4-Bromofluorobenzene
Concen: 55.37 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY004290.D
Acq: 06 Apr 2021 09:52

Tgt Ion: 95 Resp: 130544
Ion Ratio Lower Upper
95 100
174 84.6 0.0 171.4
176 80.9 0.0 165.6


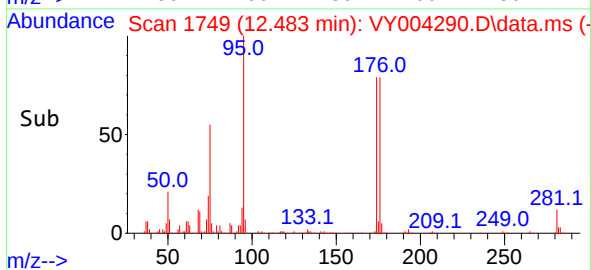
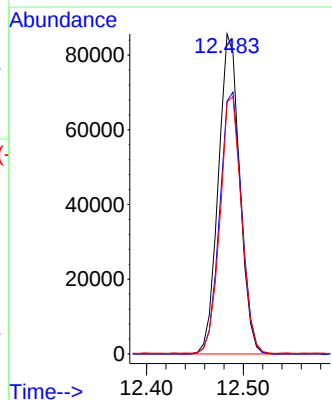
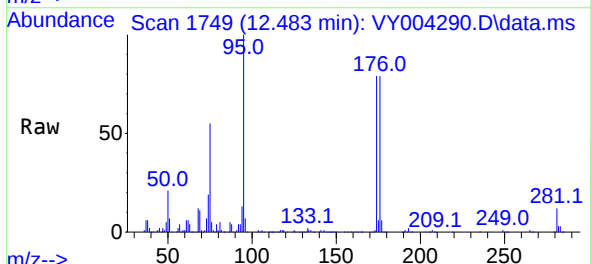


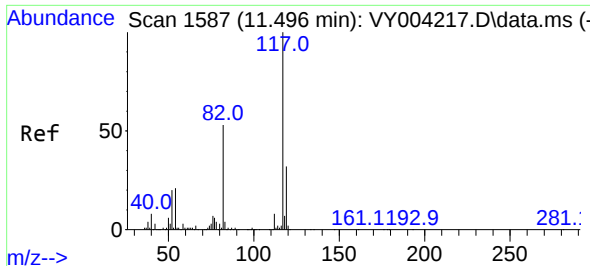

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.496 min Scan# 1587
Delta R.T. -0.000 min
Lab File: VY004290.D
Acq: 06 Apr 2021 09:52

Instrument :
MSVOA_Y
ClientSampleId :
VY0406SBL01

Tgt Ion:117 Resp: 298881
Ion Ratio Lower Upper
117 100
82 55.8 42.7 64.1
119 31.7 25.7 38.5

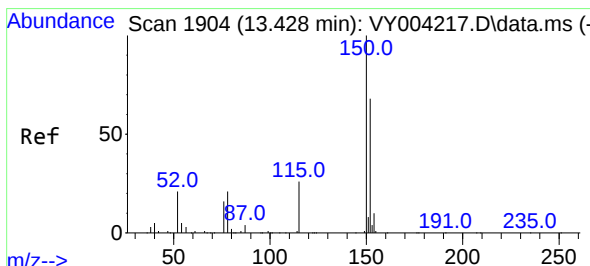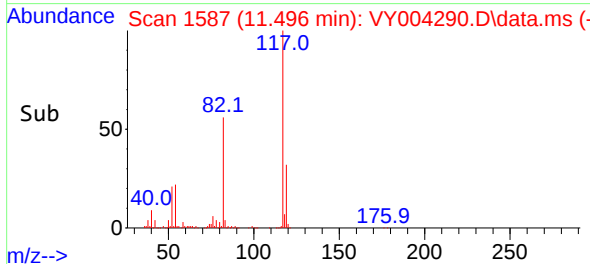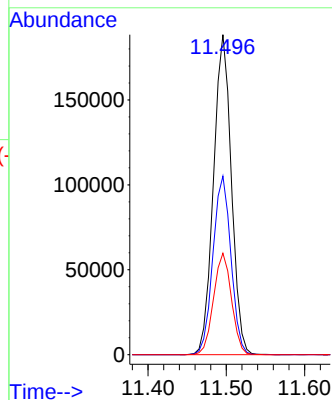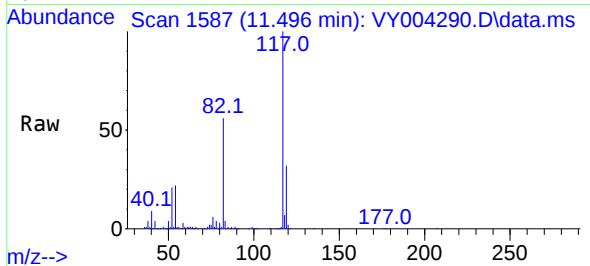

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY004290.D
Acq: 06 Apr 2021 09:52

Tgt Ion:152 Resp: 130476
Ion Ratio Lower Upper
152 100
115 59.4 29.0 87.1
150 159.7 0.0 347.4

