
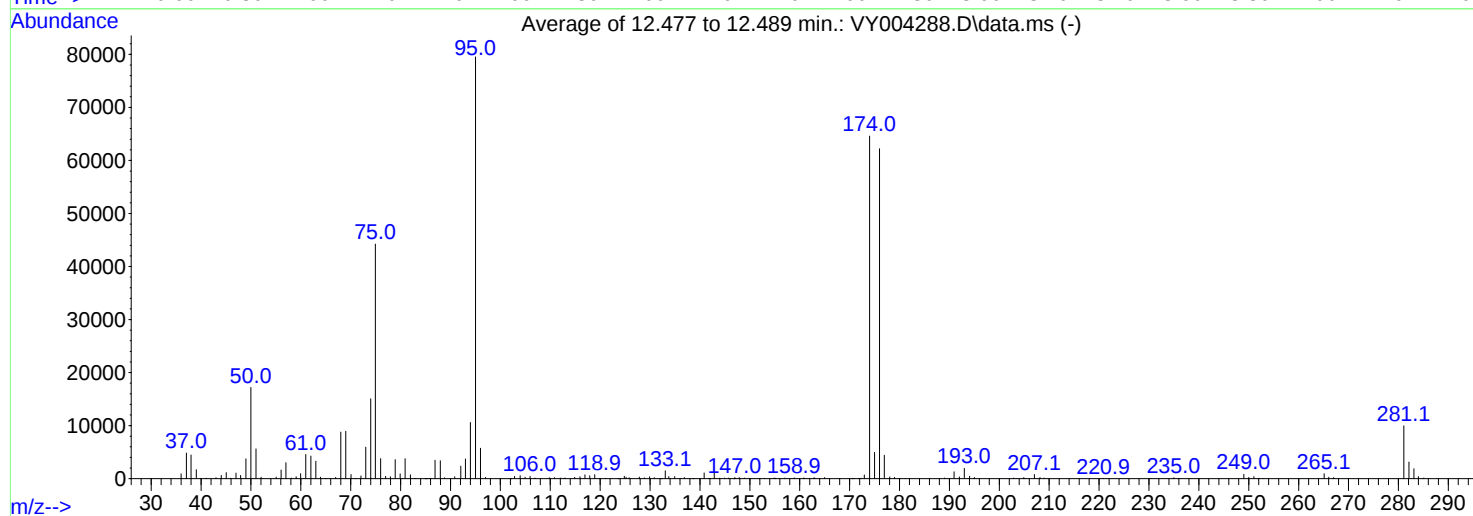


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY040621\  
Data File : VY004288.D  
Acq On : 06 Apr 2021 08:04  
Operator : SY/MD  
Sample : BFB  
Misc : 5.00g/5mL/MSVOA\_Y/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y032921S.M  
Title : SW846 8260  
Last Update : Tue Mar 30 06:38:14 2021

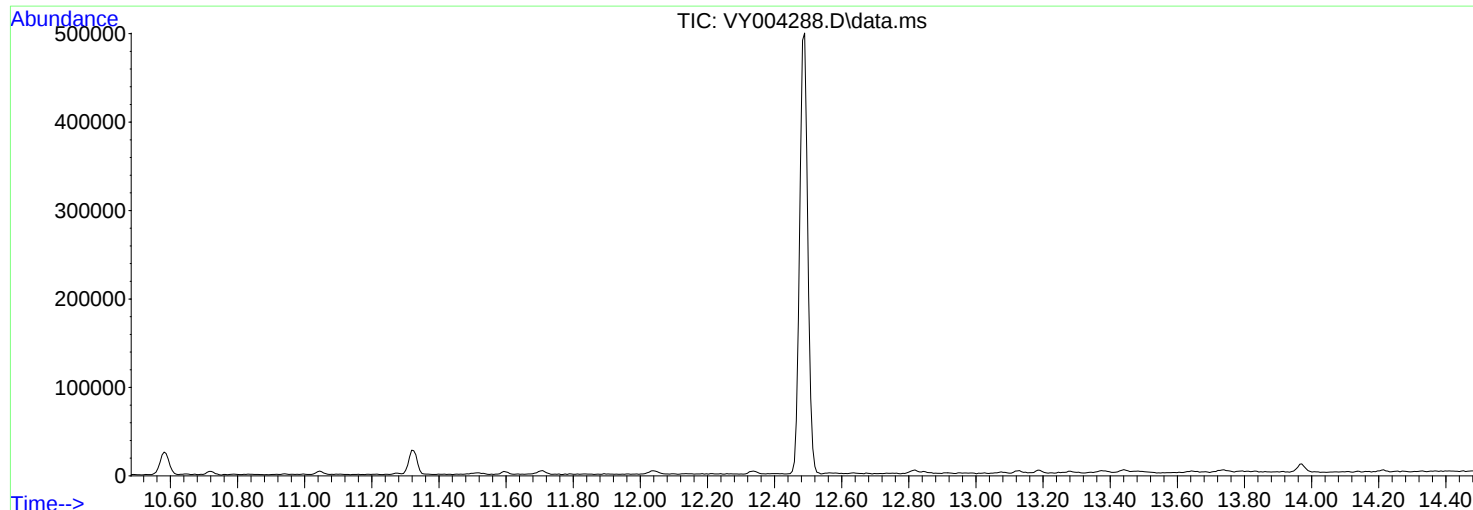

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 21.6  | 17191 | PASS      |
| 75     | 95      | 30     | 60     | 55.6  | 44238 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 79533 | PASS      |
| 96     | 95      | 5      | 9      | 7.2   | 5738  | PASS      |
| 173    | 174     | 0.00   | 2      | 1.1   | 687   | PASS      |
| 174    | 95      | 50     | 100    | 81.2  | 64592 | PASS      |
| 175    | 174     | 5      | 9      | 7.7   | 4943  | PASS      |
| 176    | 174     | 95     | 101    | 96.3  | 62199 | PASS      |
| 177    | 176     | 5      | 9      | 7.1   | 4406  | PASS      |