


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY040721\
Data File : VY004307.D
Acq On : 07 Apr 2021 09:55
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032921S.M
Title : SW846 8260
Last Update : Tue Mar 30 06:38:14 2021

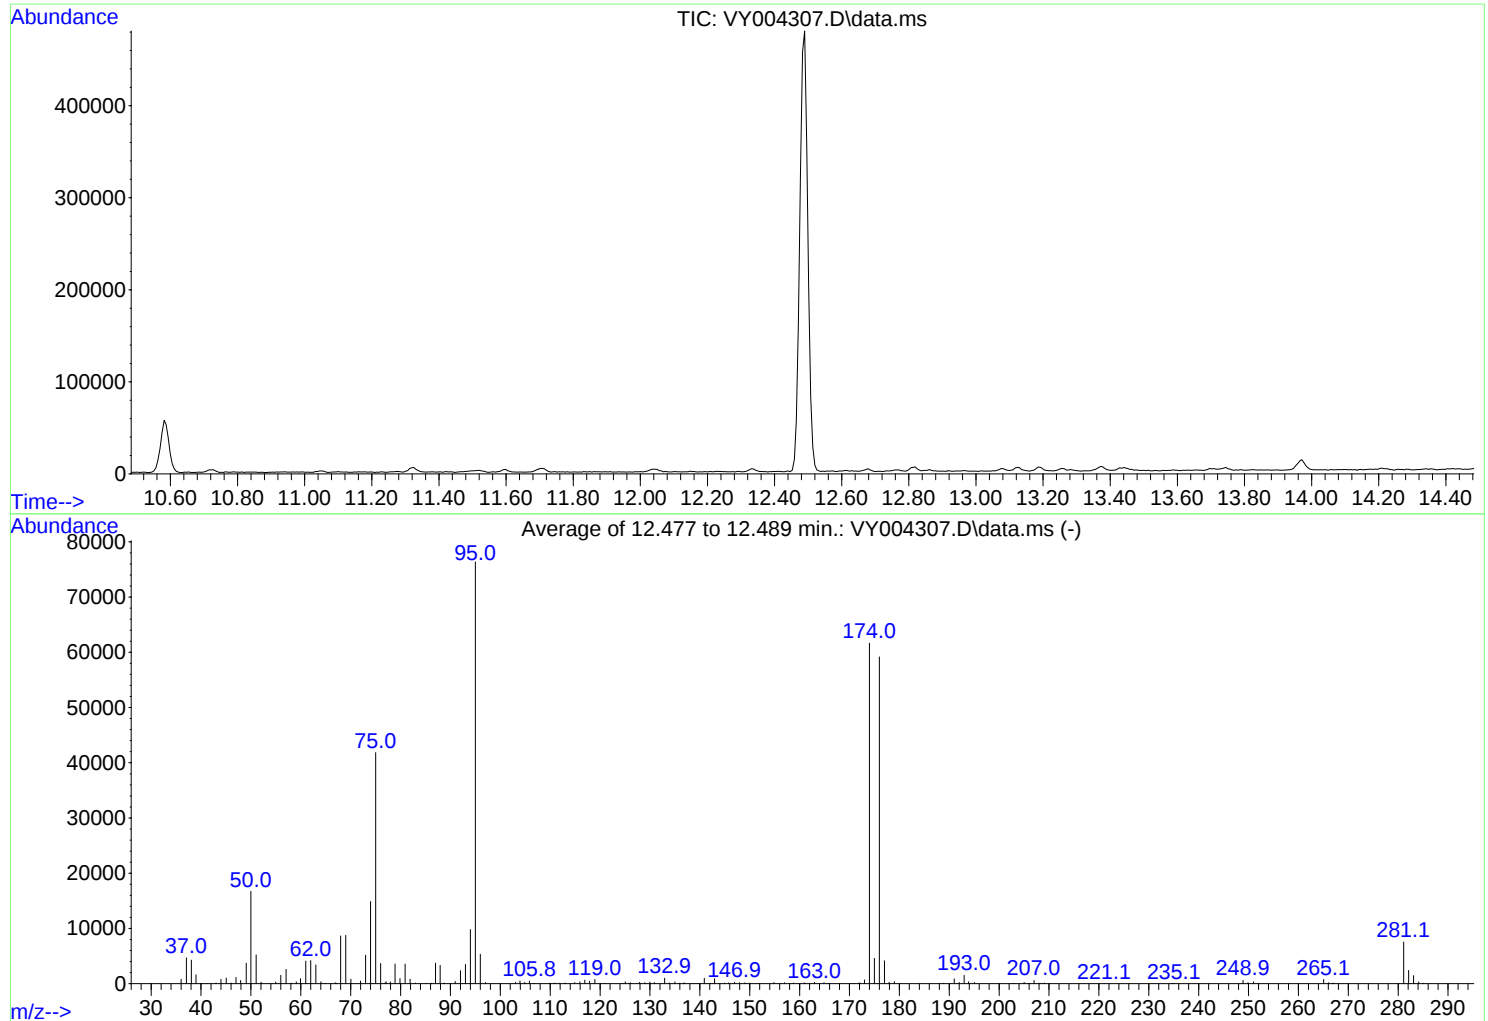

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.9	16713	PASS
75	95	30	60	54.8	41839	PASS
95	95	100	100	100.0	76381	PASS
96	95	5	9	7.0	5327	PASS
173	174	0.00	2	1.1	656	PASS
174	95	50	100	80.7	61667	PASS
175	174	5	9	7.4	4569	PASS
176	174	95	101	96.0	59182	PASS
177	176	5	9	7.0	4150	PASS