

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY040820\
 Data File : VY002255.D
 Acq On : 08 Apr 2020 17:18
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VIBLK

Quant Time: Apr 09 02:42:42 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y040820S.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 08 15:15:02 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.80	168	162623	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.70	114	304064	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.50	117	277039	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.43	152	129040	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.16	65	89856	49.69	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.38%	
35) Dibromofluoromethane	7.73	113	84180	46.53	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.06%	
50) Toluene-d8	10.19	98	345388	45.61	ug/l	0.00
Spiked Amount	50.000		Recovery	=	91.22%	
62) 4-Bromofluorobenzene	12.49	95	122927	49.20	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.40%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY040820\
Data File : VY002255.D
Acq On : 08 Apr 2020 17:18
Operator : SY/MD
Sample : VIBLK
Misc : 5.00G/5ML/MSVOA Y/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VIBLK

Quant Time: Apr 09 02:42:42 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y040820S.M
Quant Title : SW846 8260
QLast Update : Wed Apr 08 15:15:02 2020
Response via : Initial Calibration

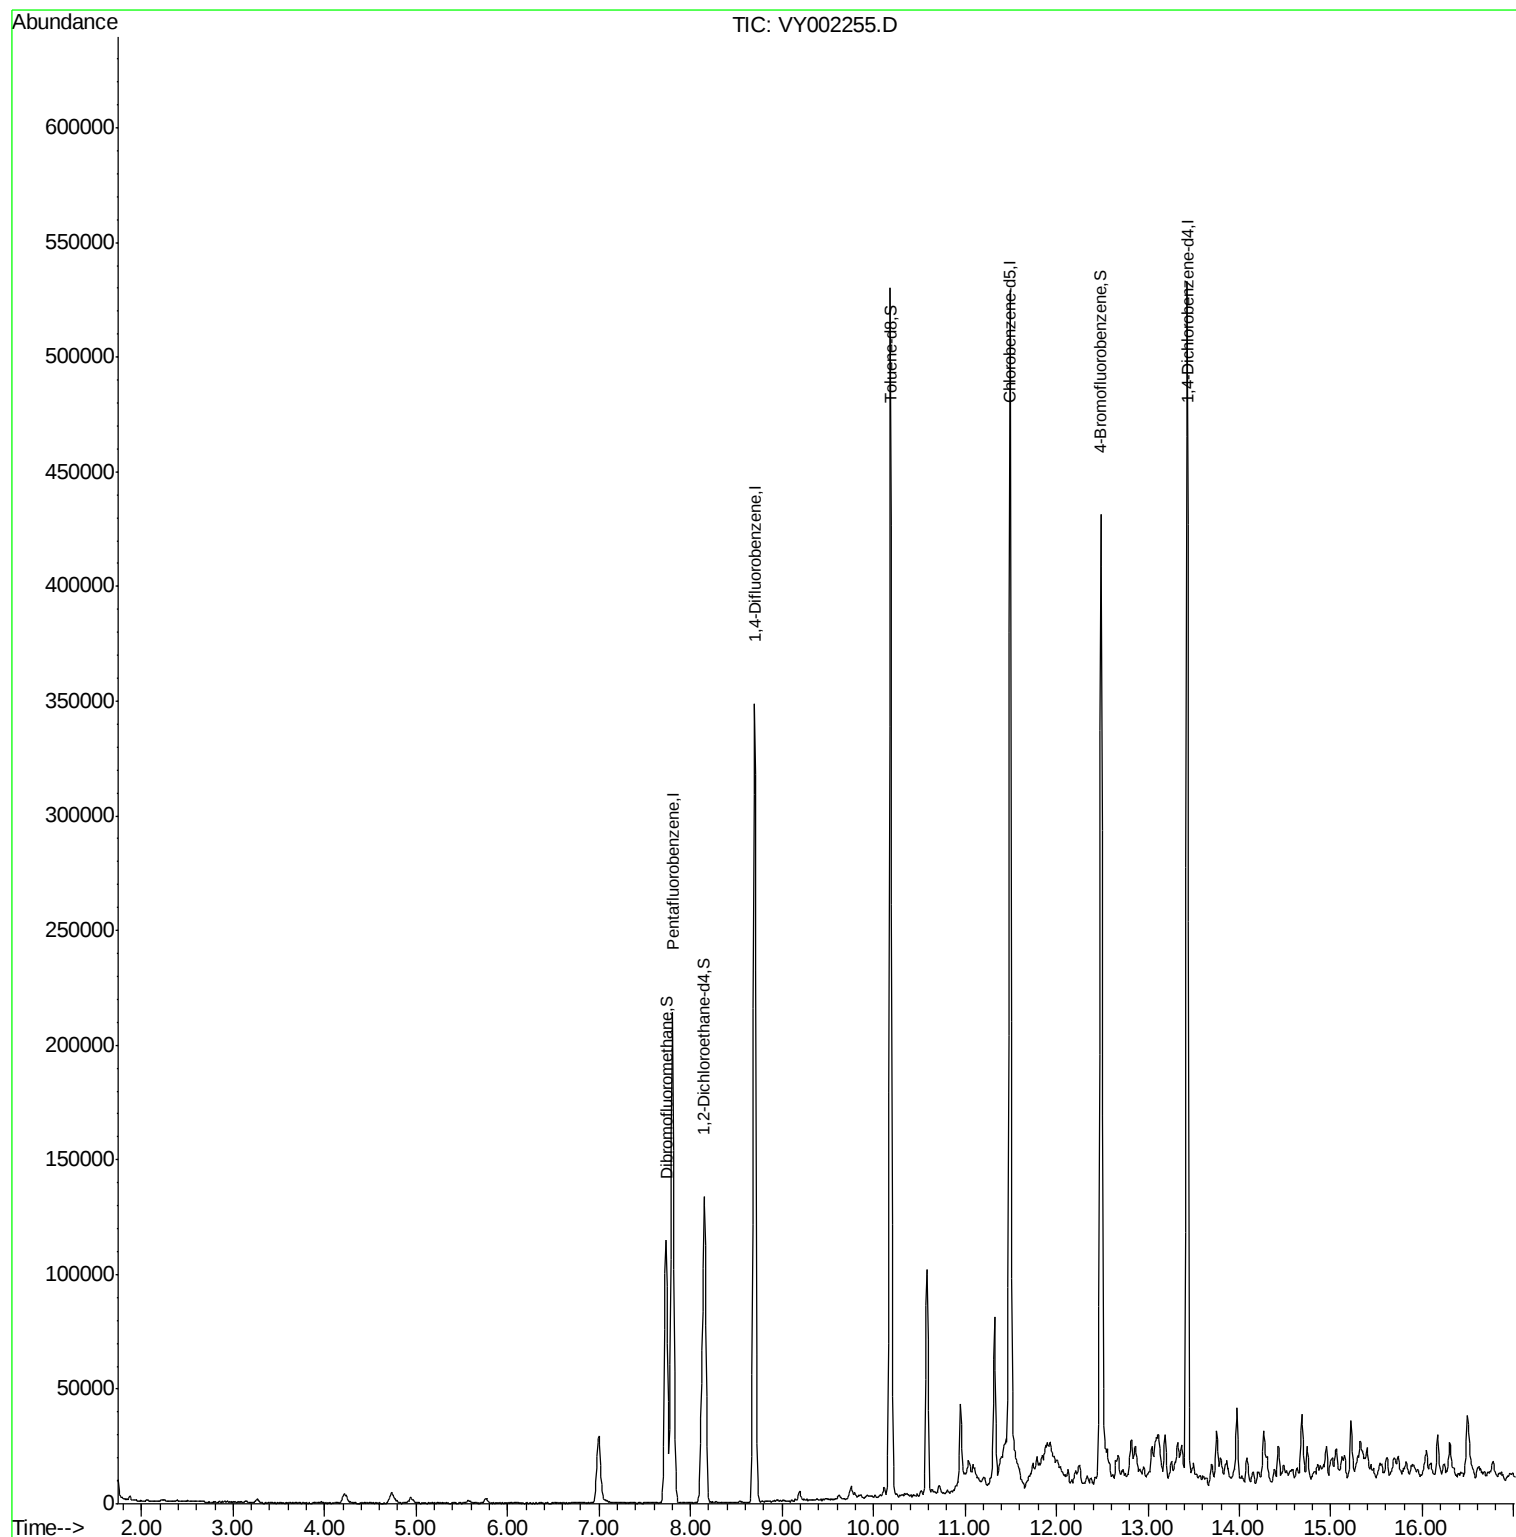

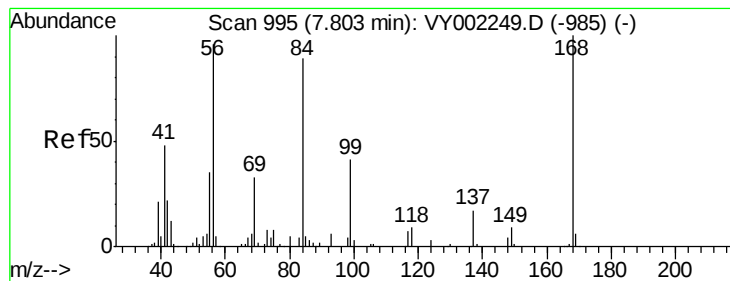

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.80 min Scan# 995

Delta R.T. 0.00 min

Lab File: VY002255.D

Acq: 08 Apr 2020 17:18

Instrument :

MSVOA_Y

ClientSampled :


VIBLK

Tot Ion:168 Resp: 162623




Ion Ratio Lower Upper

168 100

99 57.4 48.0 72.0

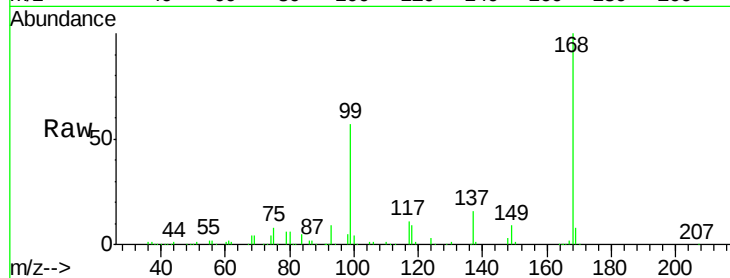

Abundance Ion 167.90 (167.60 to 168.60): VY002249.D (-985) (-)

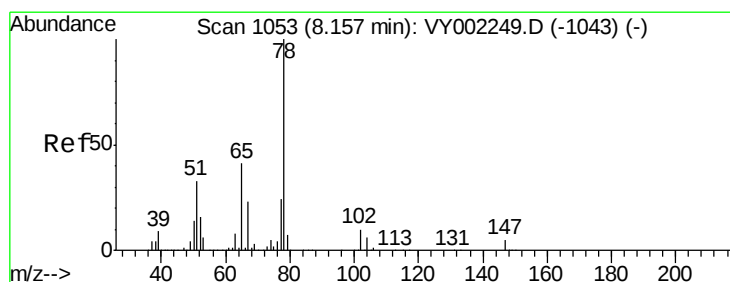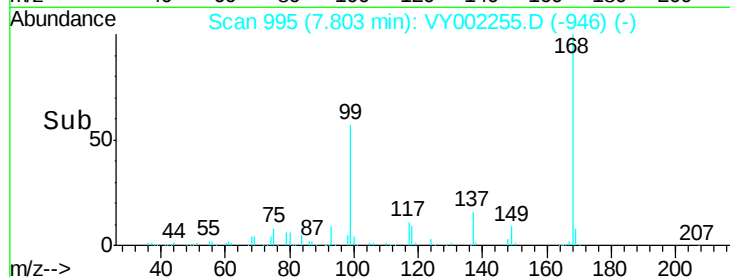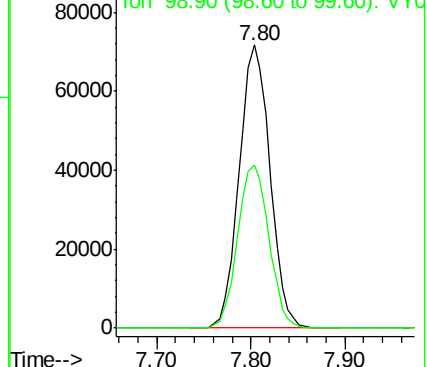

#33

1,2-Dichloroethane-d4

Concen: 49.686 ug/l

RT: 8.16 min Scan# 1053

Delta R.T. 0.00 min

Lab File: VY002255.D


Acq: 08 Apr 2020 17:18

Tgt Ion: 65 Resp: 89856



Ion Ratio Lower Upper


65 100

67 55.7 0.0 114.0

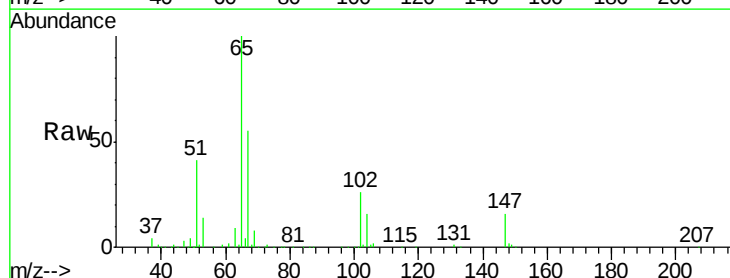

Abundance Ion 64.90 (64.60 to 65.60): VY002249.D (-1043) (-)

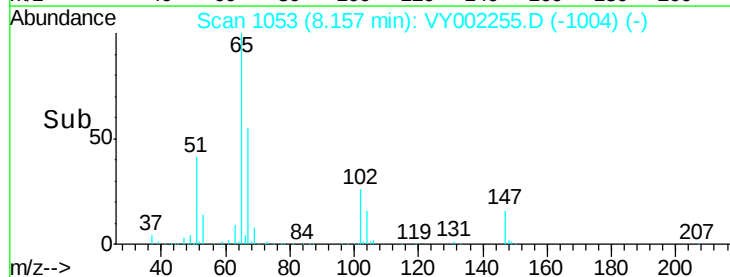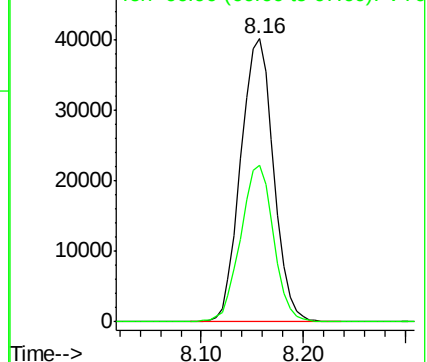

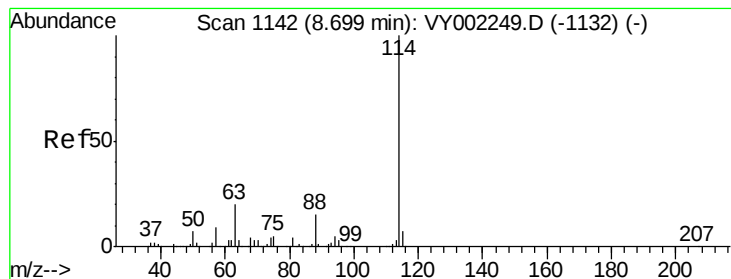

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.70 min Scan# 1142

Delta R.T. 0.00 min

Lab File: VY002255.D

Acq: 08 Apr 2020 17:18

Instrument :

MSVOA_Y

ClientSampleId :

VIBLK


Tot Ion:114 Resp: 304064

Ion Ratio Lower Upper

114 100

63 19.0 0.0 39.0




88 15.6 0.0 31.0

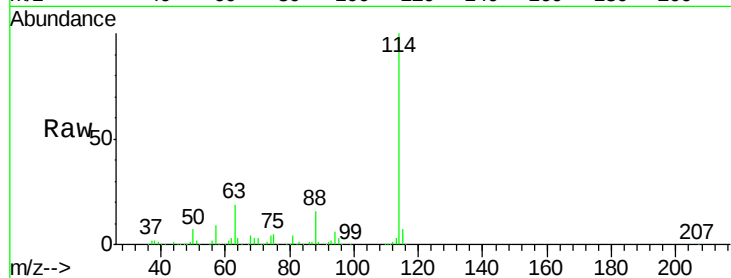

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VY0

Ion 87.90 (87.60 to 88.60): VY0

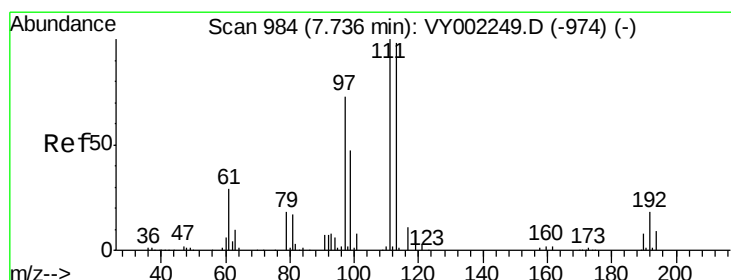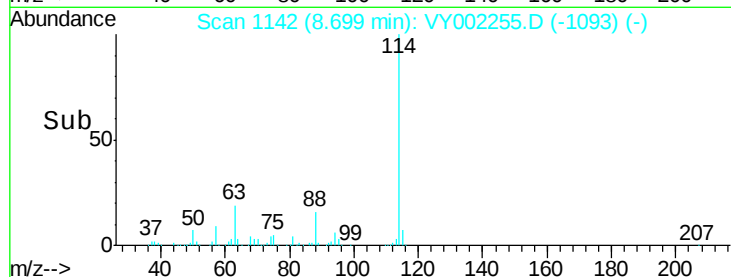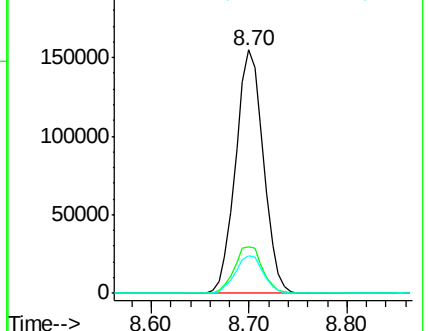

#35

Dibromofluoromethane

Concen: 46.527 ug/l

RT: 7.73 min Scan# 983

Delta R.T. -0.01 min

Lab File: VY002255.D

Acq: 08 Apr 2020 17:18


Tgt Ion:113 Resp: 84180

Ion Ratio Lower Upper

113 100

111 103.1 83.5 125.3



192 18.5 14.7 22.1

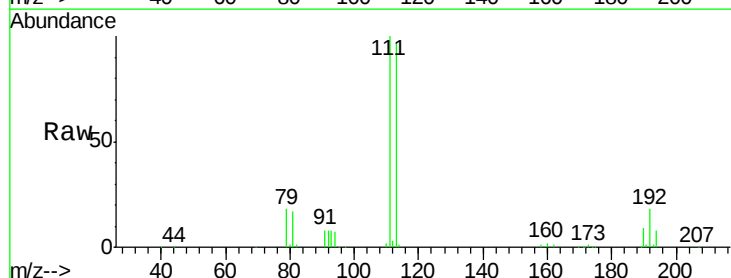


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



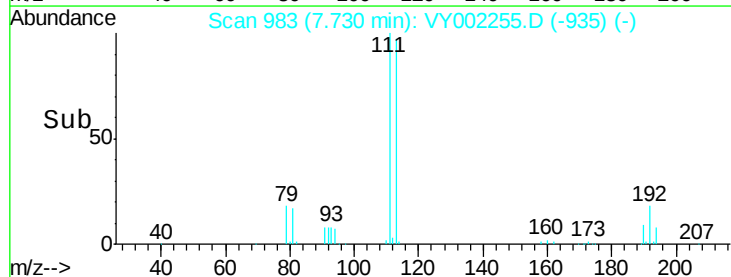
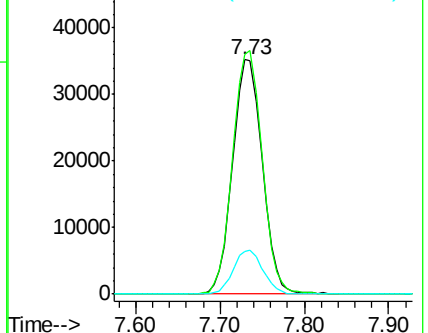


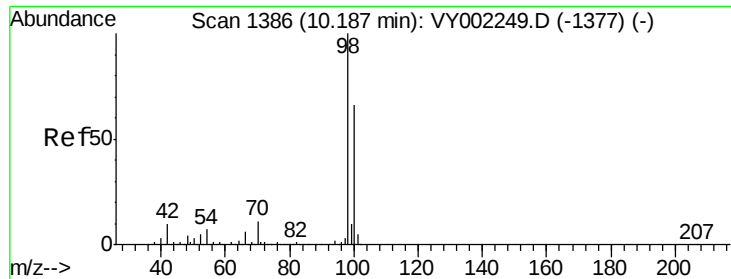

#50
Toluene-d8
Concen: 45.608 ug/l
RT: 10.19 min Scan# 1386
Delta R.T. 0.00 min
Lab File: VY002255.D
Acq: 08 Apr 2020 17:18




Instrument :
MSVOA_Y
ClientSampleId :
VIBLK


Tot Ion: 98 Resp: 345388
Ion Ratio Lower Upper
98 100
100 65.9 52.6 78.8

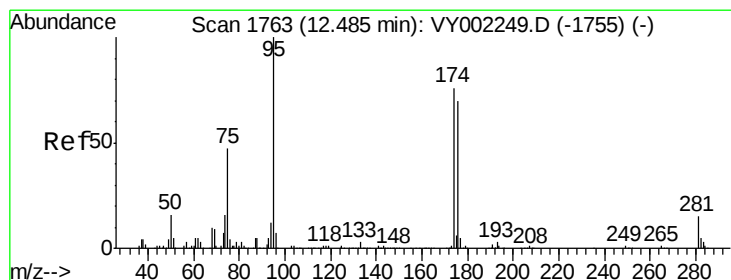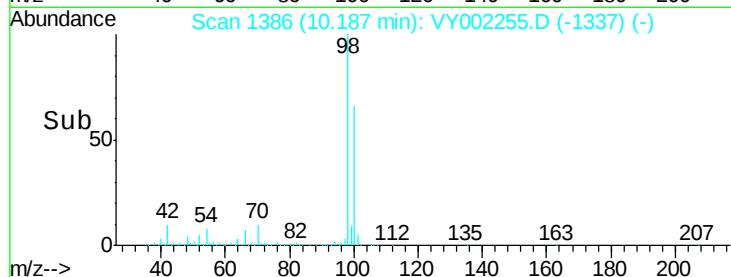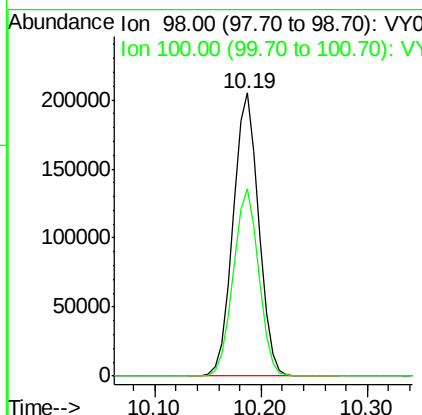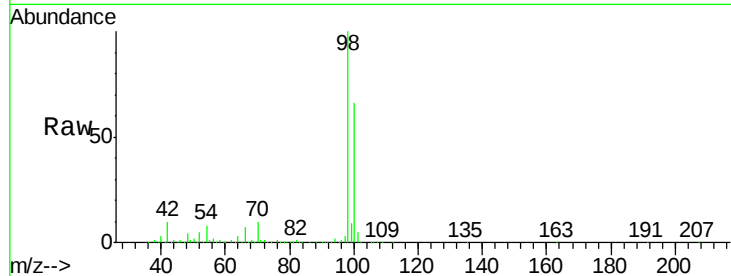

#62
4-Bromofluorobenzene
Concen: 49.202 ug/l
RT: 12.49 min Scan# 1763
Delta R.T. 0.00 min
Lab File: VY002255.D
Acq: 08 Apr 2020 17:18

Tgt Ion: 95 Resp: 122927
Ion Ratio Lower Upper
95 100
174 73.3 0.0 150.6
176 70.9 0.0 141.4

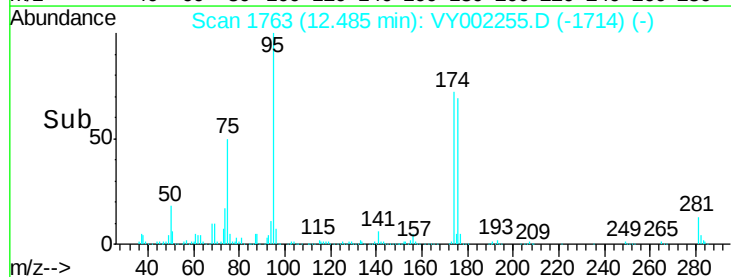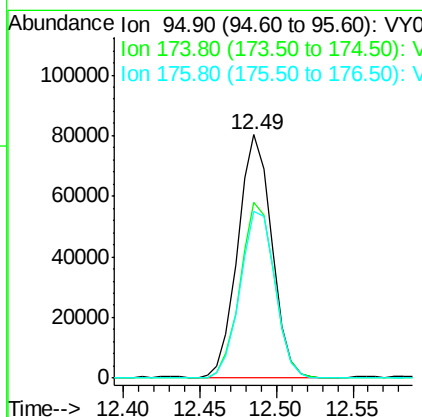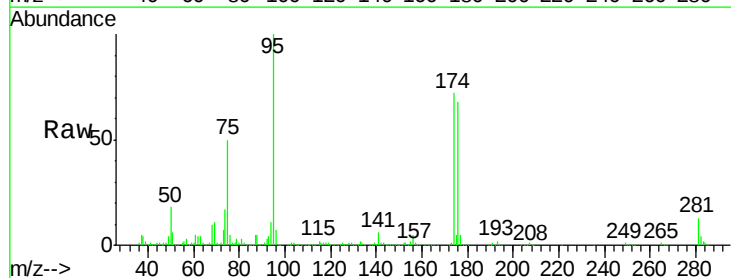


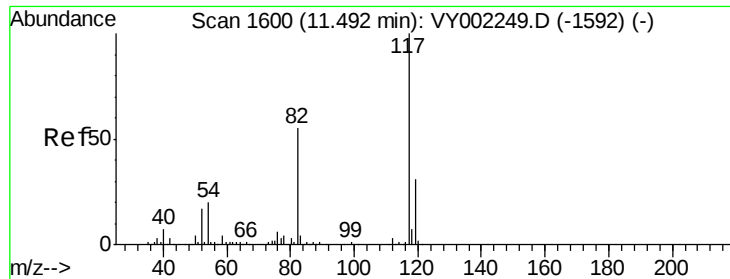




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.50 min Scan# 1601
Delta R.T. 0.01 min
Lab File: VY002255.D
Acq: 08 Apr 2020 17:18

Instrument :
MSVOA_Y
ClientSampleId :
VIBLK

Tot Ion:117 Resp: 277039
Ion Ratio Lower Upper
117 100
82 55.3 44.2 66.4
119 31.8 25.1 37.7

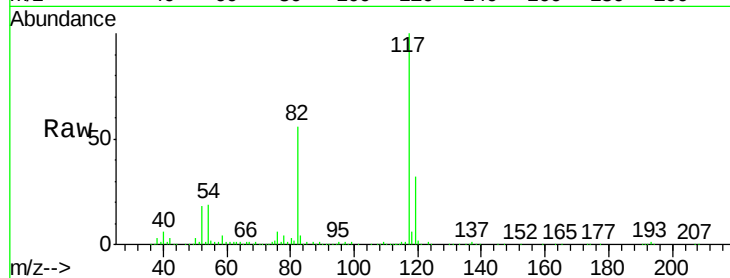


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VY0
Ion 118.90 (118.60 to 119.60): V

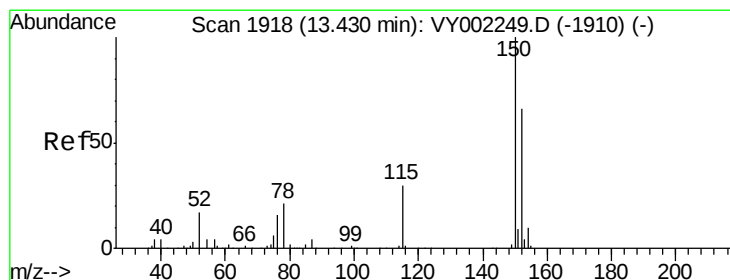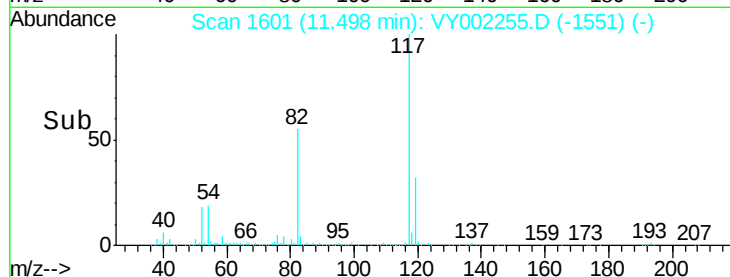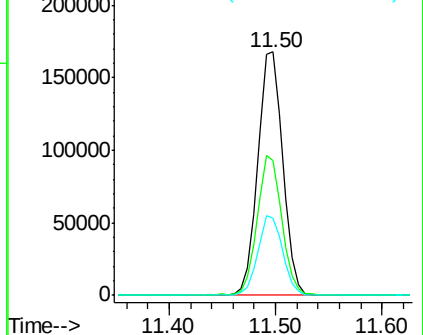

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.43 min Scan# 1918
Delta R.T. 0.00 min
Lab File: VY002255.D
Acq: 08 Apr 2020 17:18

Tgt Ion:152 Resp: 129040
Ion Ratio Lower Upper
152 100
115 61.3 30.7 92.1
150 158.5 0.0 350.6

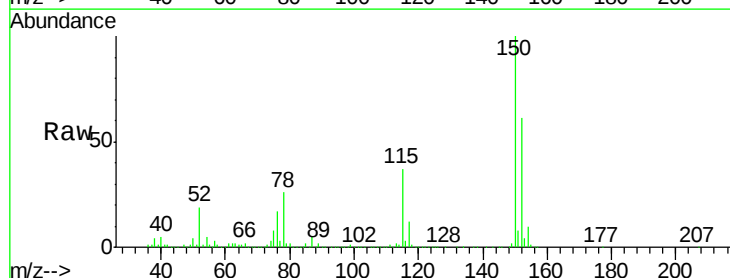

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

